


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF111417\
 Data File : BF100561.D
 Acq On : 15 Nov 2017 00:04
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 14 14:17:16 2017

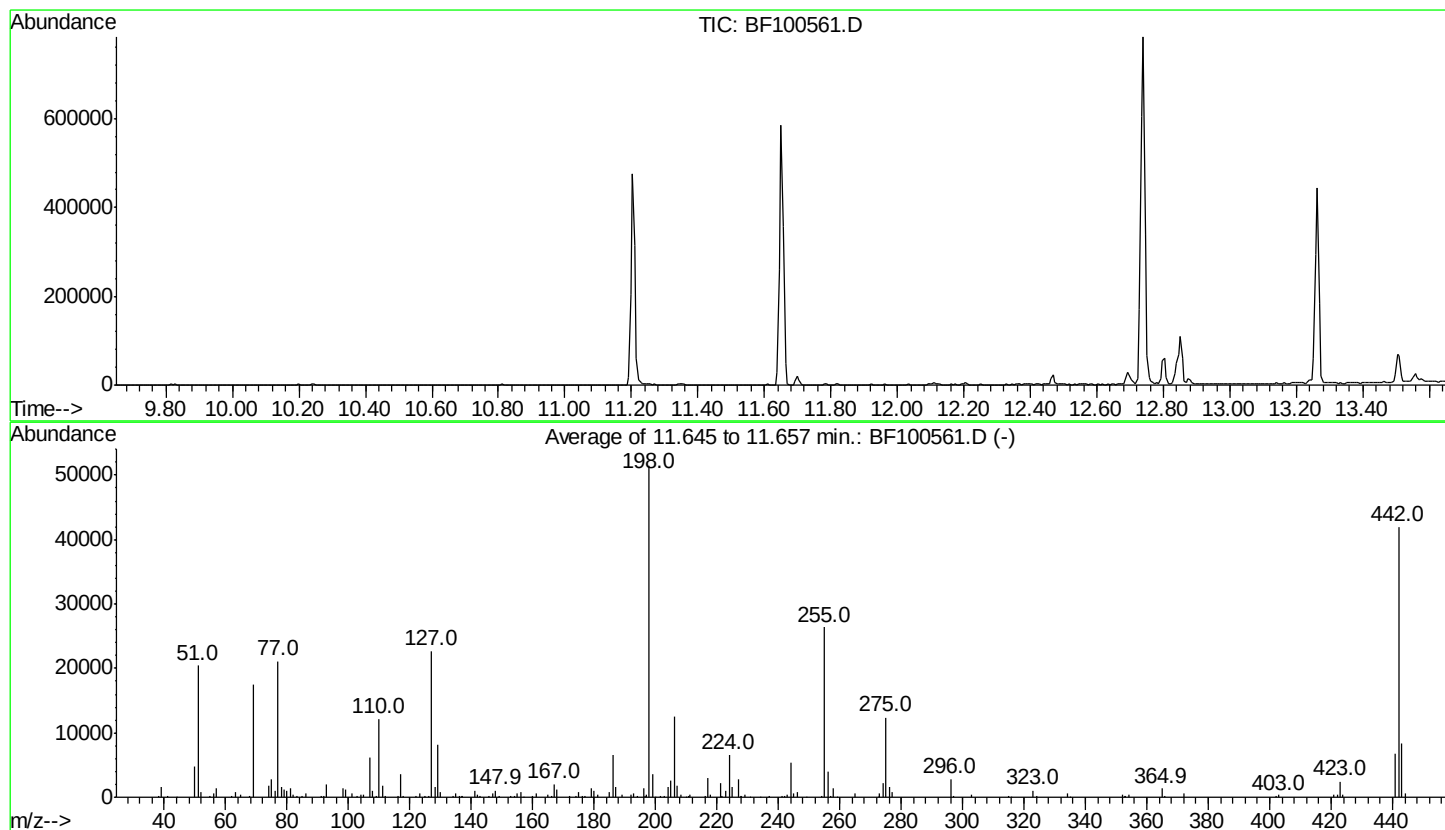

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	20394	PASS
68	69	0.00	2	1.5	265	PASS
69	198	0.00	100	33.9	17441	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	22729	PASS
197	198	0.00	2	0.8	412	PASS
198	198	100	100	100.0	51474	PASS
199	198	5	9	7.0	3616	PASS
275	198	10	60	24.1	12385	PASS
365	198	1	100	2.5	1304	PASS
441	443	0.01	100	80.4	6737	PASS
442	198	50	100	81.6	41990	PASS
443	442	15	24	19.9	8377	PASS