
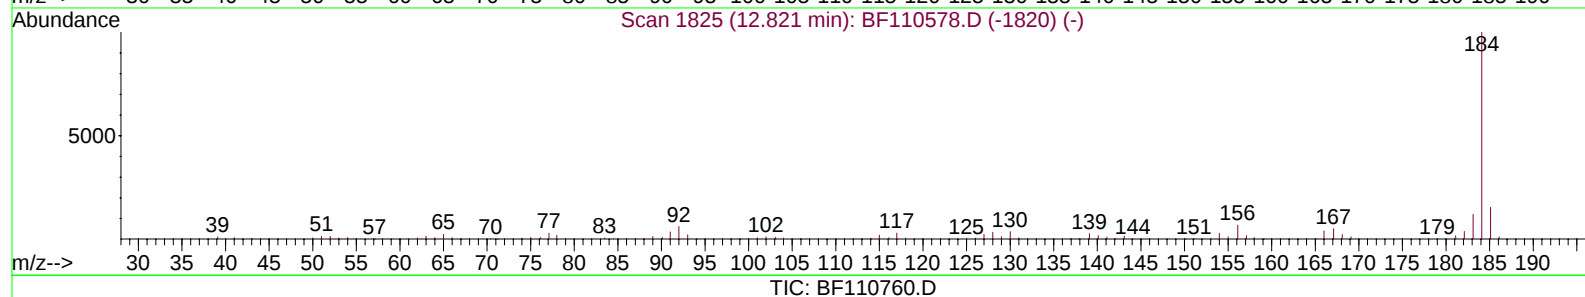
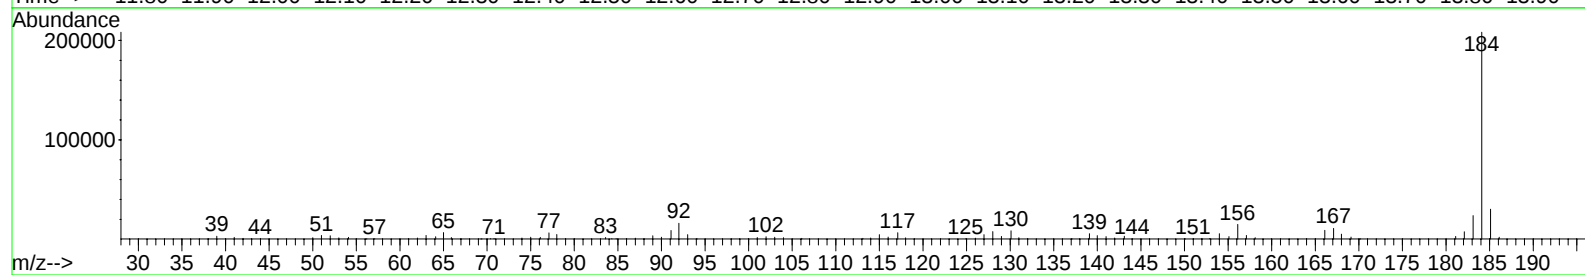


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111418\
 Data File : BF110760.D
 Acq On : 14 Nov 2018 13:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 17:13:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 12:43:10 2018
 Response via : Initial Calibration

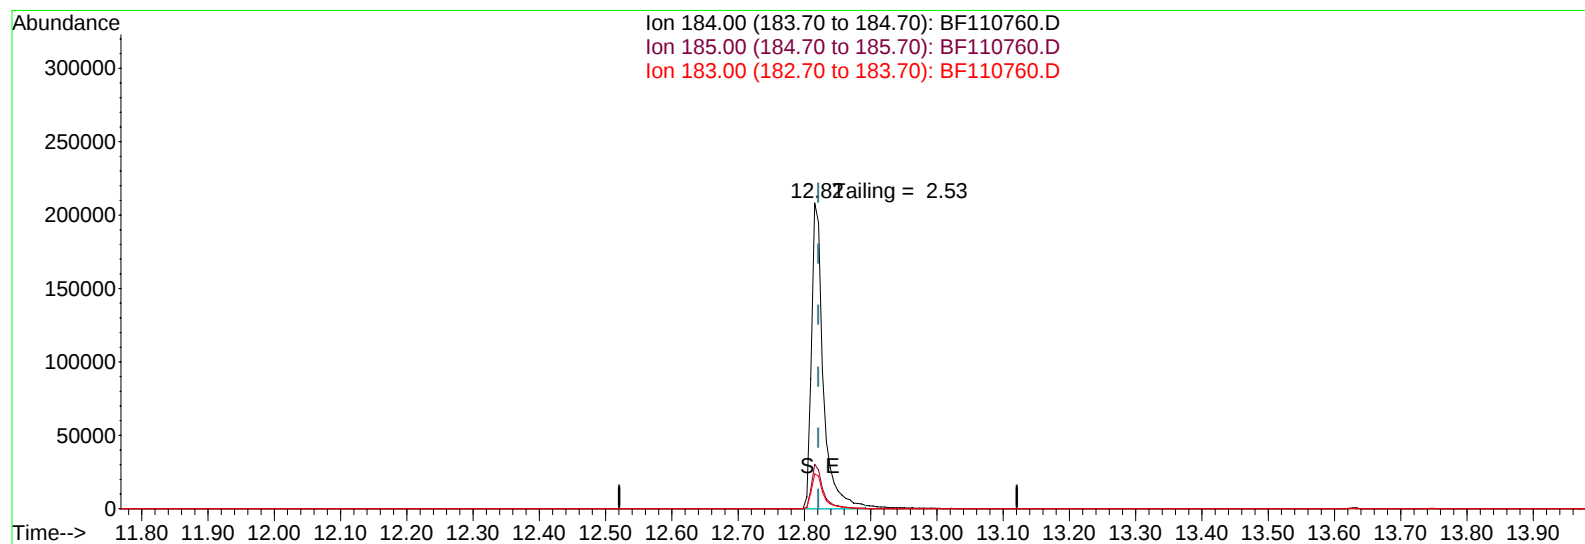

(77) Benzidine




12.816min (-0.005) 0.00ng

response 262967

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.54
183.00	11.80	11.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111418\
Data File : BF110760.D
Acq On : 14 Nov 2018 13:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 17:13:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

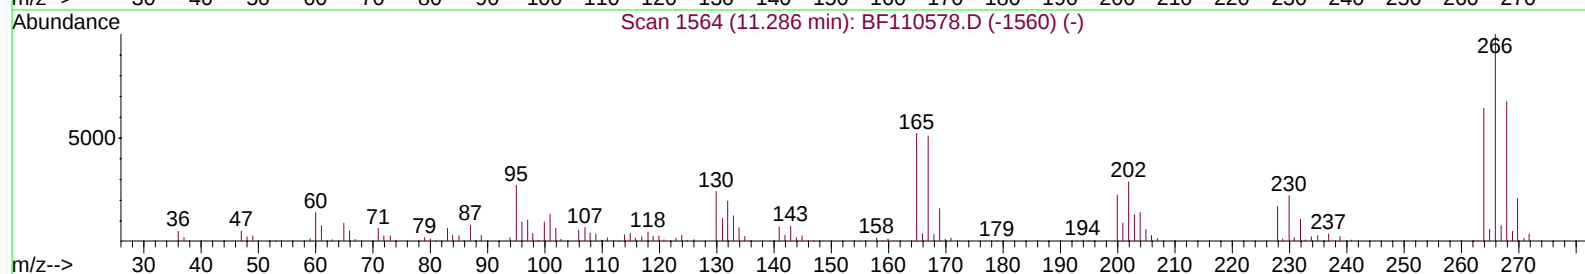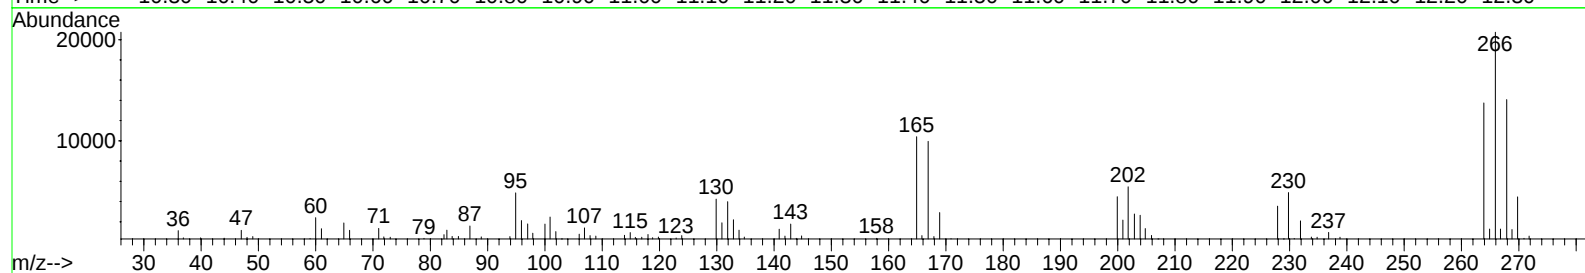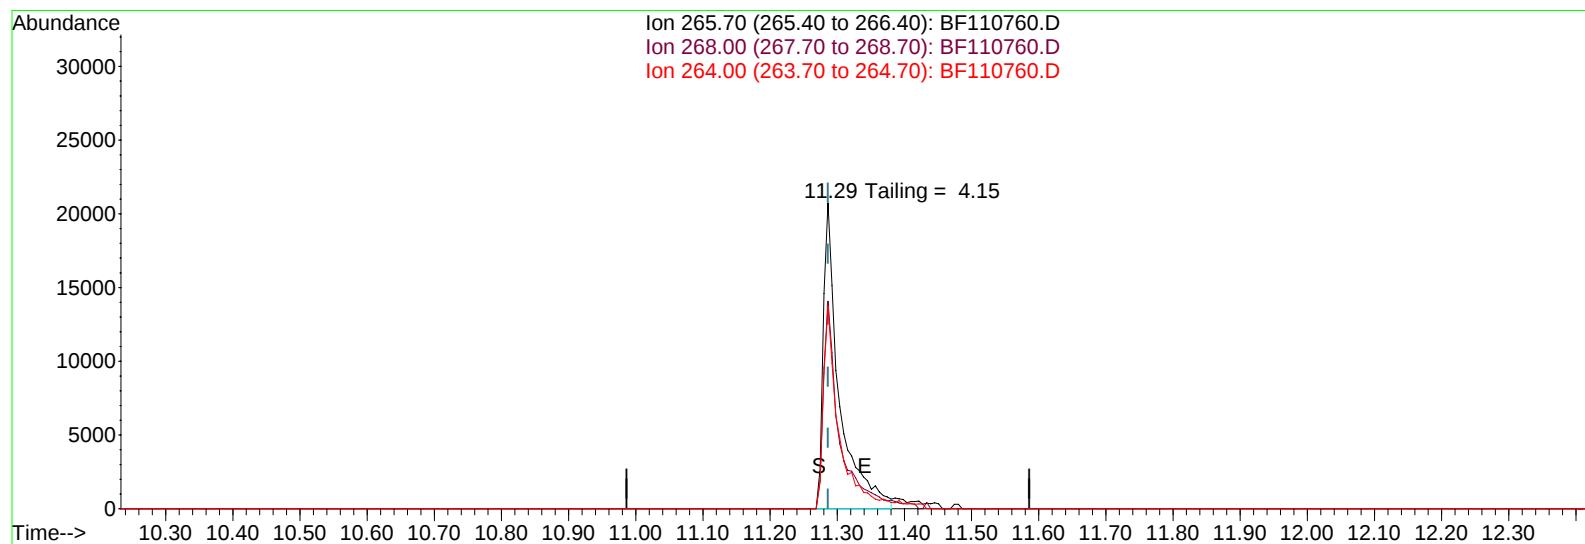

TIC: BF110760.D

(70) Pentachlorophenol (C)

11.286min (+0.000) 50949.44ng

response 35796

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	67.88
264.00	63.20	66.30
0.00	0.00	0.00