

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111418\
 Data File : BF110781.D
 Acq On : 14 Nov 2018 22:56
 Operator : JU/SJ
 Sample : PB114818BL
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB114818BL

Quant Time: Nov 15 06:21:22 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 13 12:43:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.94	152	72473	20.00	ng	0.00
21) Naphthalene-d8	8.22	136	293309	20.00	ng	0.00
39) Acenaphthene-d10	9.98	164	138190	20.00	ng	-0.01
64) Phenanthrene-d10	11.47	188	246352	20.00	ng	-0.01
76) Chrysene-d12	14.13	240	154806	20.00	ng	-0.01
87) Perylene-d12	15.66	264	141631	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.57	112	561115	125.76	ng	0.00
7) Phenol-d6	6.57	99	707577	124.02	ng	0.00
23) Nitrobenzene-d5	7.51	82	442415	86.87	ng	0.00
42) 2,4,6-Tribromophenol	10.77	330	158168	113.59	ng	-0.01
45) 2-Fluorobiphenyl	9.30	172	852670	88.12	ng	0.00
79) Terphenyl-d14	13.06	244	688562	83.30	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF111418\
Data File : BF110781.D
Acq On : 14 Nov 2018 22:56
Operator : JU/SJ
Sample : PB114818BL
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB114818BL

Quant Time: Nov 15 06:21:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

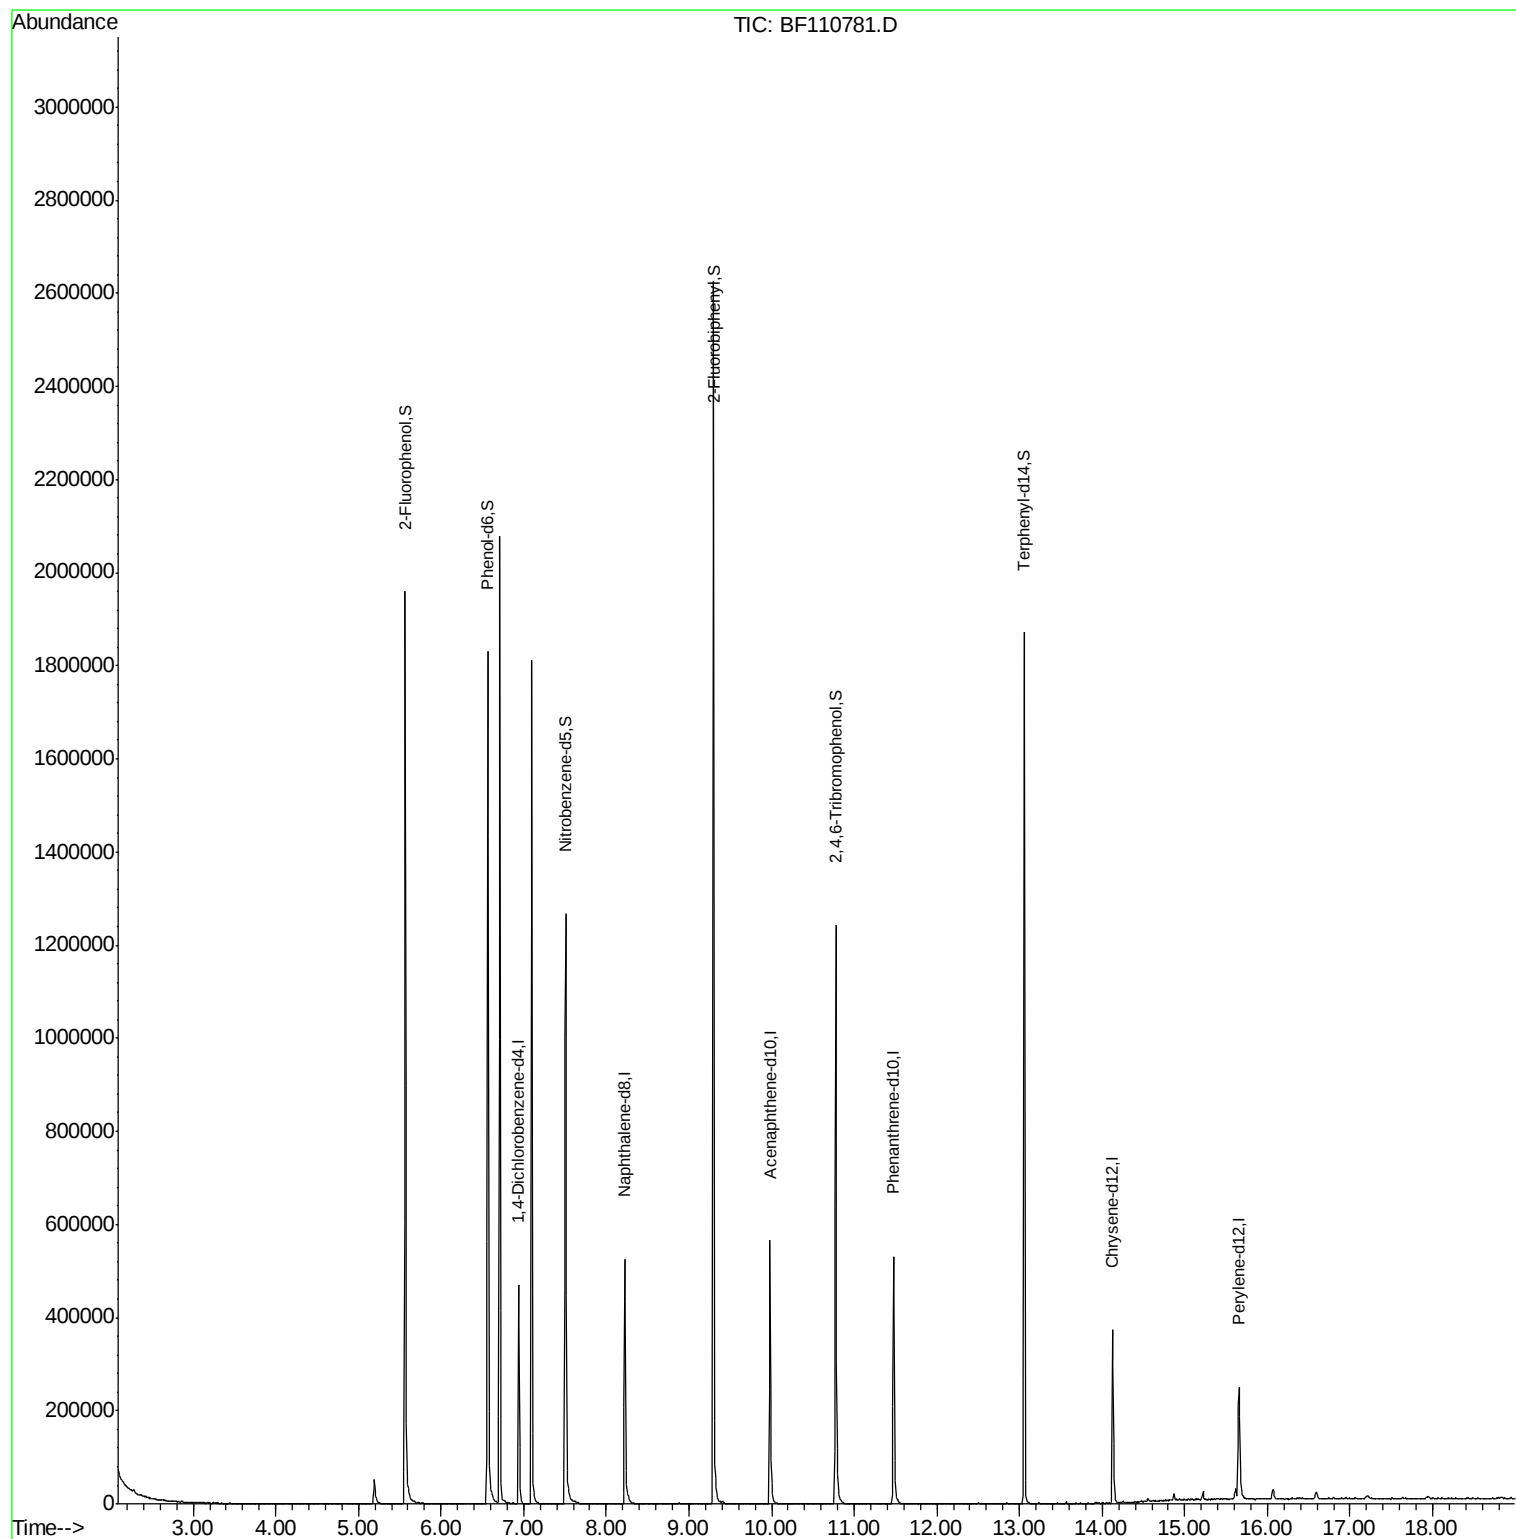




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.94 min Scan# 825
 Delta R.T. -0.01 min
 Lab File: BF110781.D
 Acq: 14 Nov 2018 22:56

Instrument :
 BNA_F
 ClientSampleId :
 PB114818BL

Tot Ion:152 Resp: 72473
 Ion Ratio Lower Upper
 152 100
 150 157.3 122.7 184.1
 115 62.8 49.1 73.7

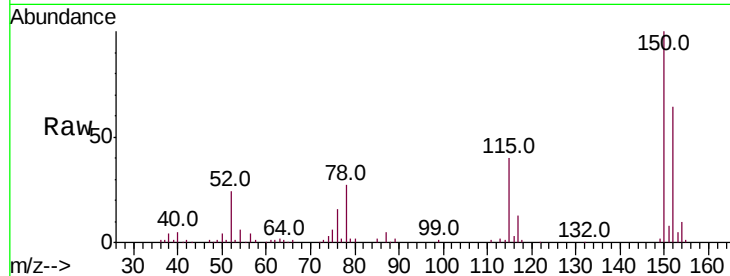


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

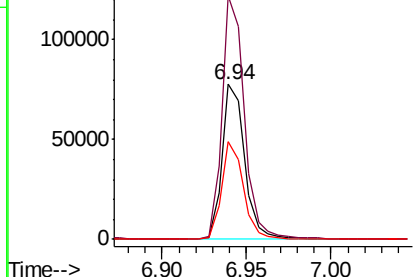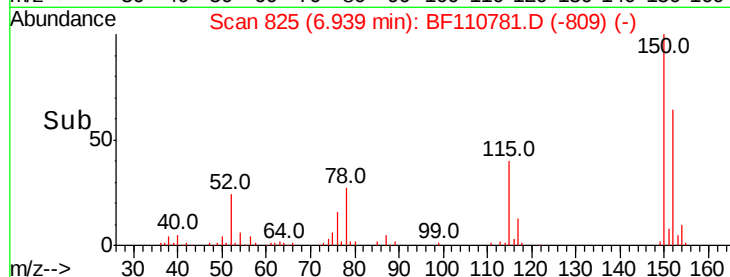



#5

2-Fluorophenol
 Concen: 125.761 ng
 RT: 5.57 min Scan# 592
 Delta R.T. 0.01 min
 Lab File: BF110781.D
 Acq: 14 Nov 2018 22:56

Tgt Ion:112 Resp: 561115
 Ion Ratio Lower Upper
 112 100
 64 59.7 44.1 66.1
 63 31.7 23.7 35.5

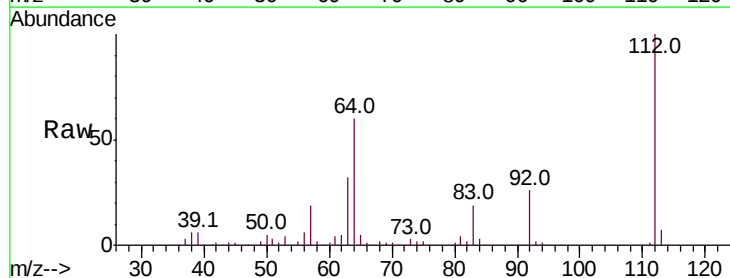

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

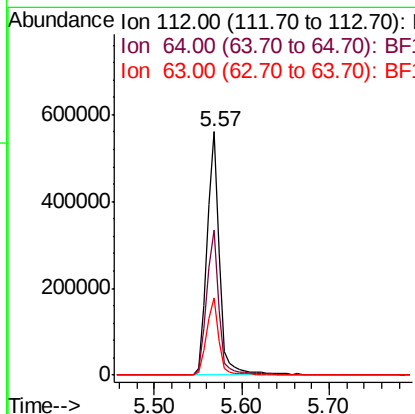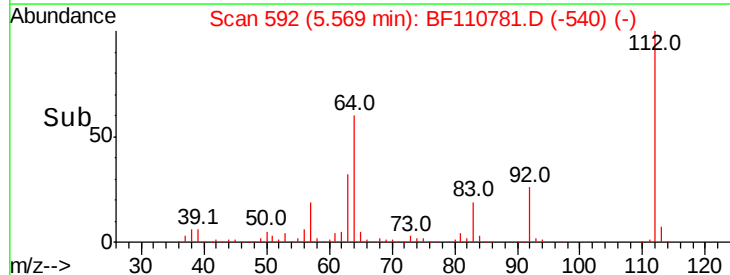



#7

Phenol-d6

Concen: 124.016 ng

RT: 6.57 min Scan# 762

Delta R.T. -0.01 min

Lab File: BF110781.D

Acq: 14 Nov 2018 22:56

Instrument :

BNA_F

ClientSampleId :

PB114818BL


Tot Ion: 99 Resp: 707577

Ion Ratio Lower Upper




99 100

42 20.0 15.8 23.6

71 35.9 28.0 42.0

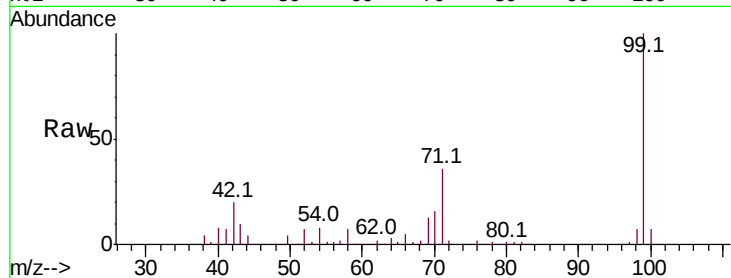

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

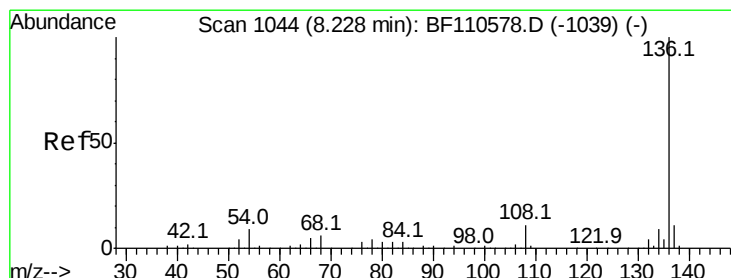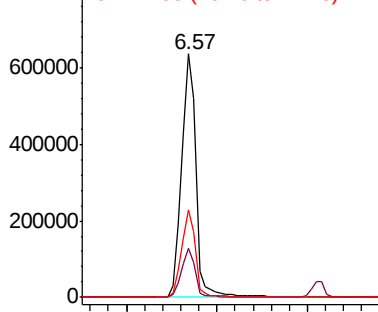

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.22 min Scan# 1043

Delta R.T. -0.01 min

Lab File: BF110781.D

Acq: 14 Nov 2018 22:56

Tgt Ion: 136 Resp: 293309


Ion Ratio Lower Upper

136 100



137 10.9 8.8 13.2

54 8.4 5.4 8.2#

68 5.0 4.2 6.2

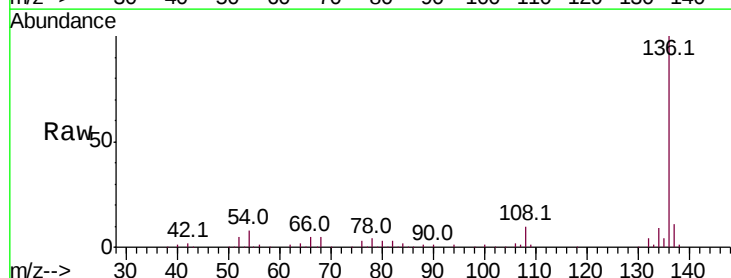

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

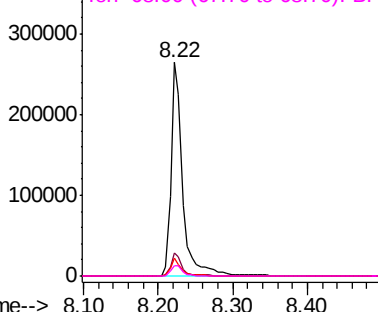







#23
Nitrobenzene-d5
Concen: 86.866 ng
RT: 7.51 min Scan# 922
Delta R.T. -0.01 min
Lab File: BF110781.D
Acq: 14 Nov 2018 22:56

Instrument :
BNA_F
ClientSampled :
PB114818BL

Tot Ion: 82 Resp: 442415
Ion Ratio Lower Upper
82 100
128 46.2 34.2 51.2
54 52.3 38.6 58.0

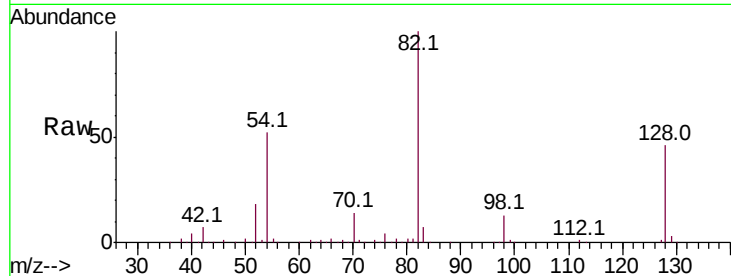


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

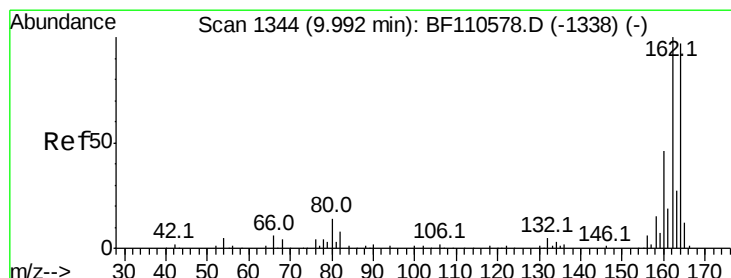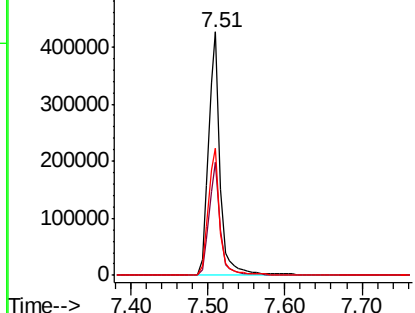




#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.98 min Scan# 1342
Delta R.T. -0.01 min
Lab File: BF110781.D
Acq: 14 Nov 2018 22:56

Tgt Ion:164 Resp: 138190
Ion Ratio Lower Upper
164 100
162 103.2 83.0 124.6
160 45.0 37.0 55.6

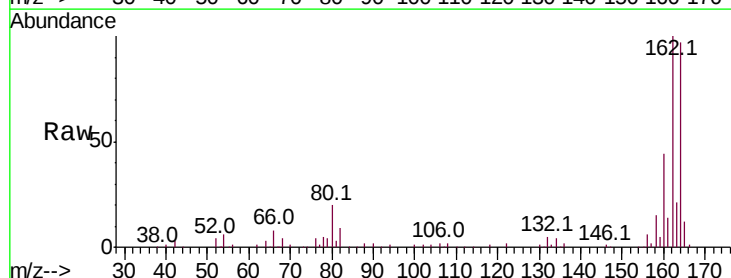

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

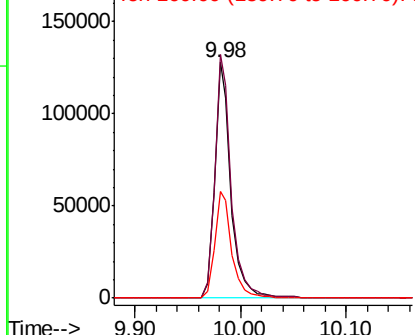


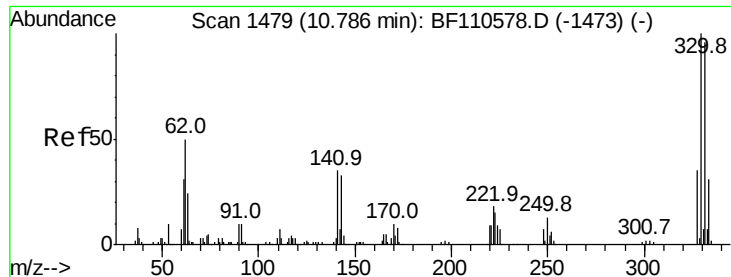




#42
 2,4,6-Tribromophenol
 Concen: 113.591 ng
 RT: 10.77 min Scan# 1477
 Delta R.T. -0.01 min
 Lab File: BF110781.D
 Acq: 14 Nov 2018 22:56

Instrument :
 BNA_F
 ClientSampleId :
 PB114818BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.1	77.1	115.7
141	36.7	27.0	40.4

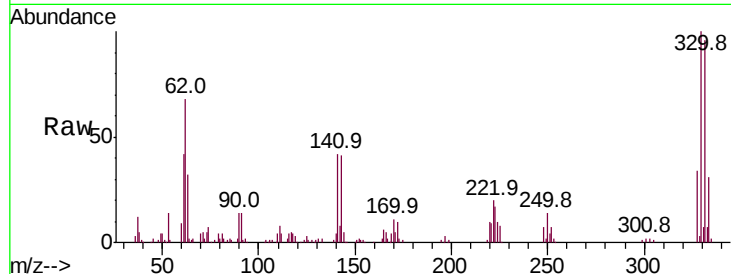


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

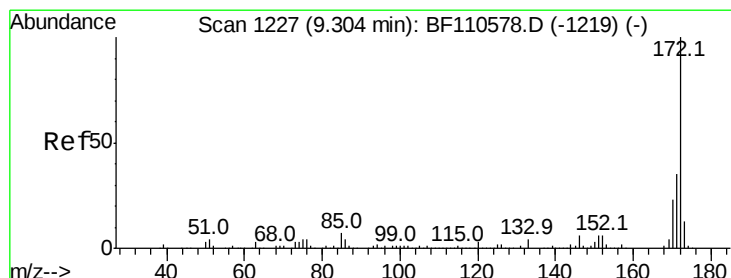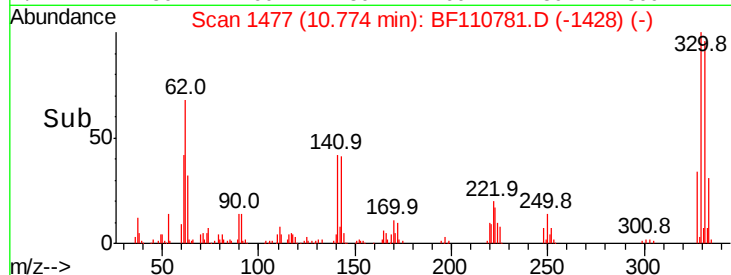
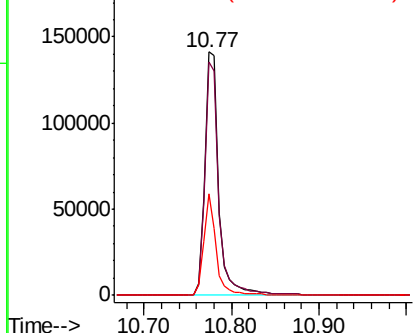



#45
 2-Fluorobiphenyl
 Concen: 88.123 ng
 RT: 9.30 min Scan# 1226
 Delta R.T. -0.01 min
 Lab File: BF110781.D
 Acq: 14 Nov 2018 22:56

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.3	28.6	43.0
170	23.8	19.7	29.5

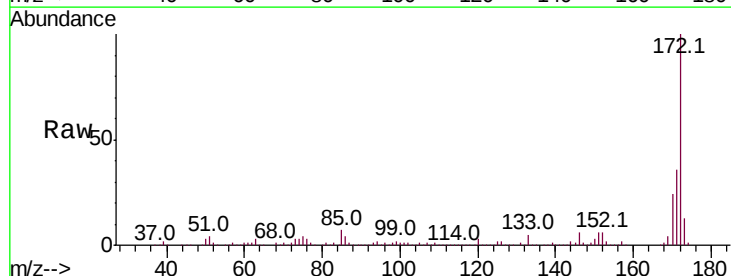

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

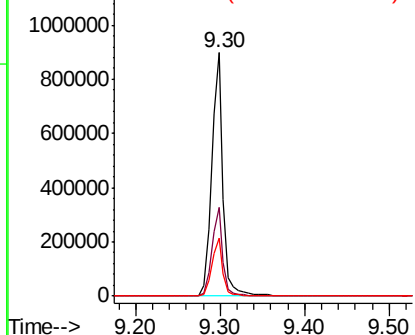


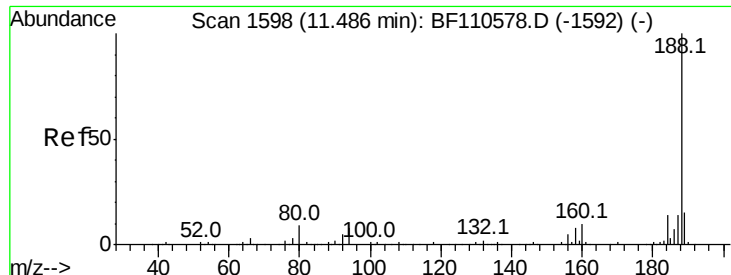




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.47 min Scan# 1596
Delta R.T. -0.01 min
Lab File: BF110781.D
Acq: 14 Nov 2018 22:56

Instrument :
BNA_F
ClientSampleId :
PB114818BL

Tot Ion:188 Resp: 246352
Ion Ratio Lower Upper
188 100
94 9.5 7.2 10.8
80 9.8 7.9 11.9

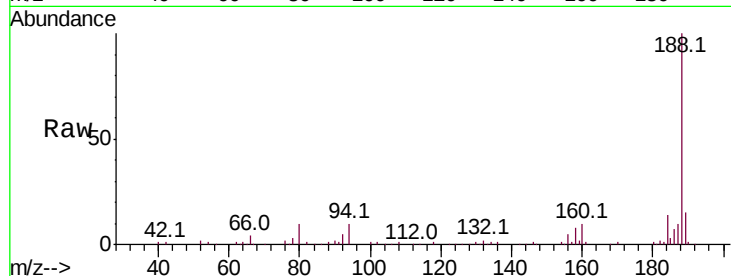


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

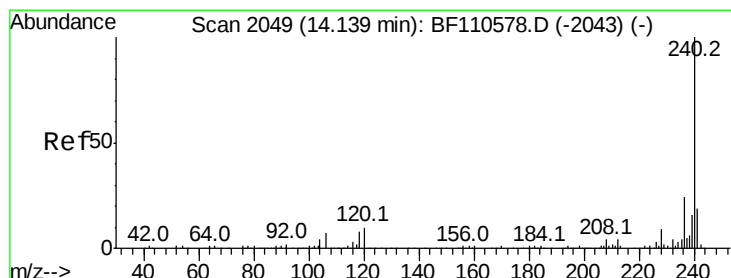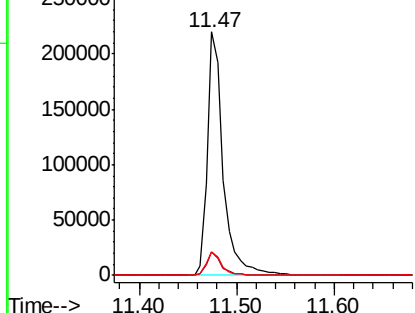




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.13 min Scan# 2047
Delta R.T. -0.01 min
Lab File: BF110781.D
Acq: 14 Nov 2018 22:56

Tgt Ion:240 Resp: 154806
Ion Ratio Lower Upper
240 100
120 12.0 8.3 12.5
236 24.6 21.2 31.8

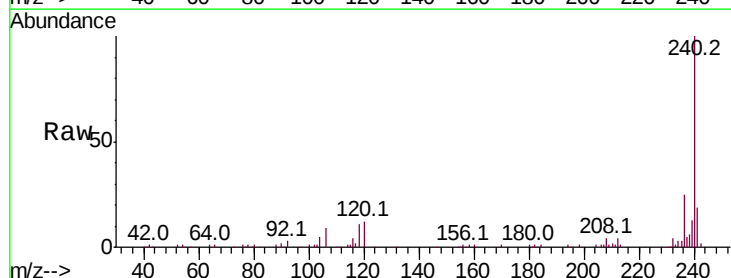

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

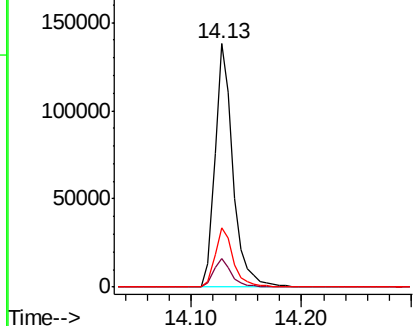

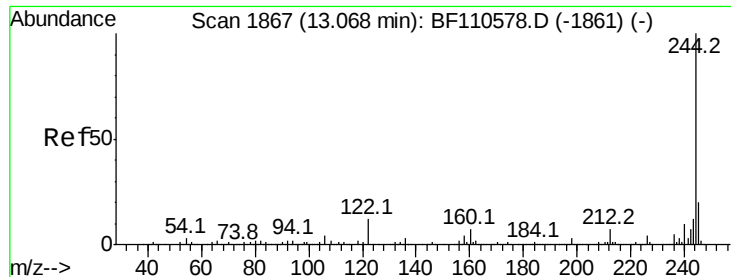

#79

Terphenyl-d14

Concen: 83.299 ng

RT: 13.06 min Scan# 1866

Delta R.T. -0.01 min

Lab File: BF110781.D

Acq: 14 Nov 2018 22:56

Instrument :

BNA_F

ClientSampleId :

PB114818BL


Tot Ion:244 Resp: 688562

Ion Ratio Lower Upper

244 100

212 6.7 5.8 8.8




122 10.5 8.7 13.1

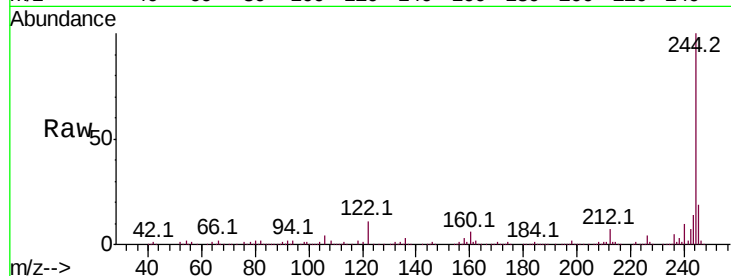

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

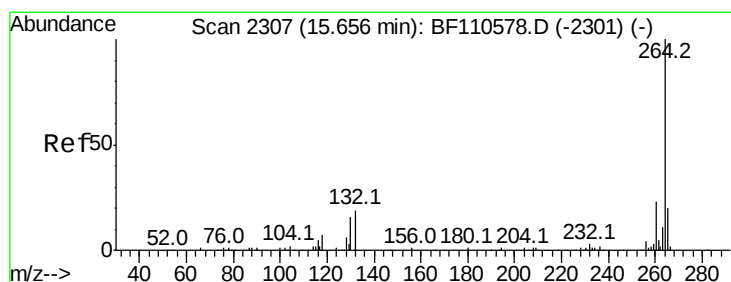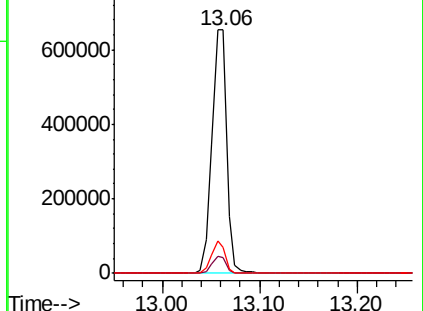

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.66 min Scan# 2307

Delta R.T. 0.00 min

Lab File: BF110781.D

Acq: 14 Nov 2018 22:56


Tgt Ion:264 Resp: 141631

Ion Ratio Lower Upper

264 100

260 23.7 18.7 28.1

265 22.4 16.7 25.1

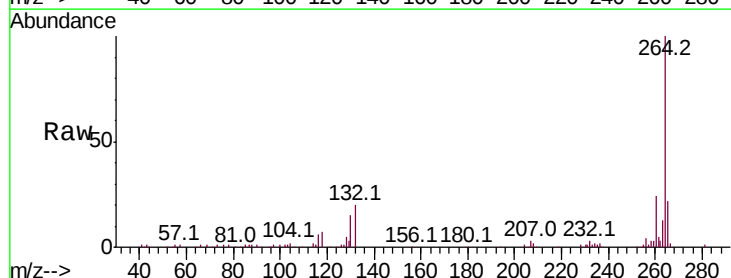

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

