


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111422\
Data File : BF131219.D
Acq On : 14 Nov 2022 10:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110922.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Nov 12 00:03:31 2022

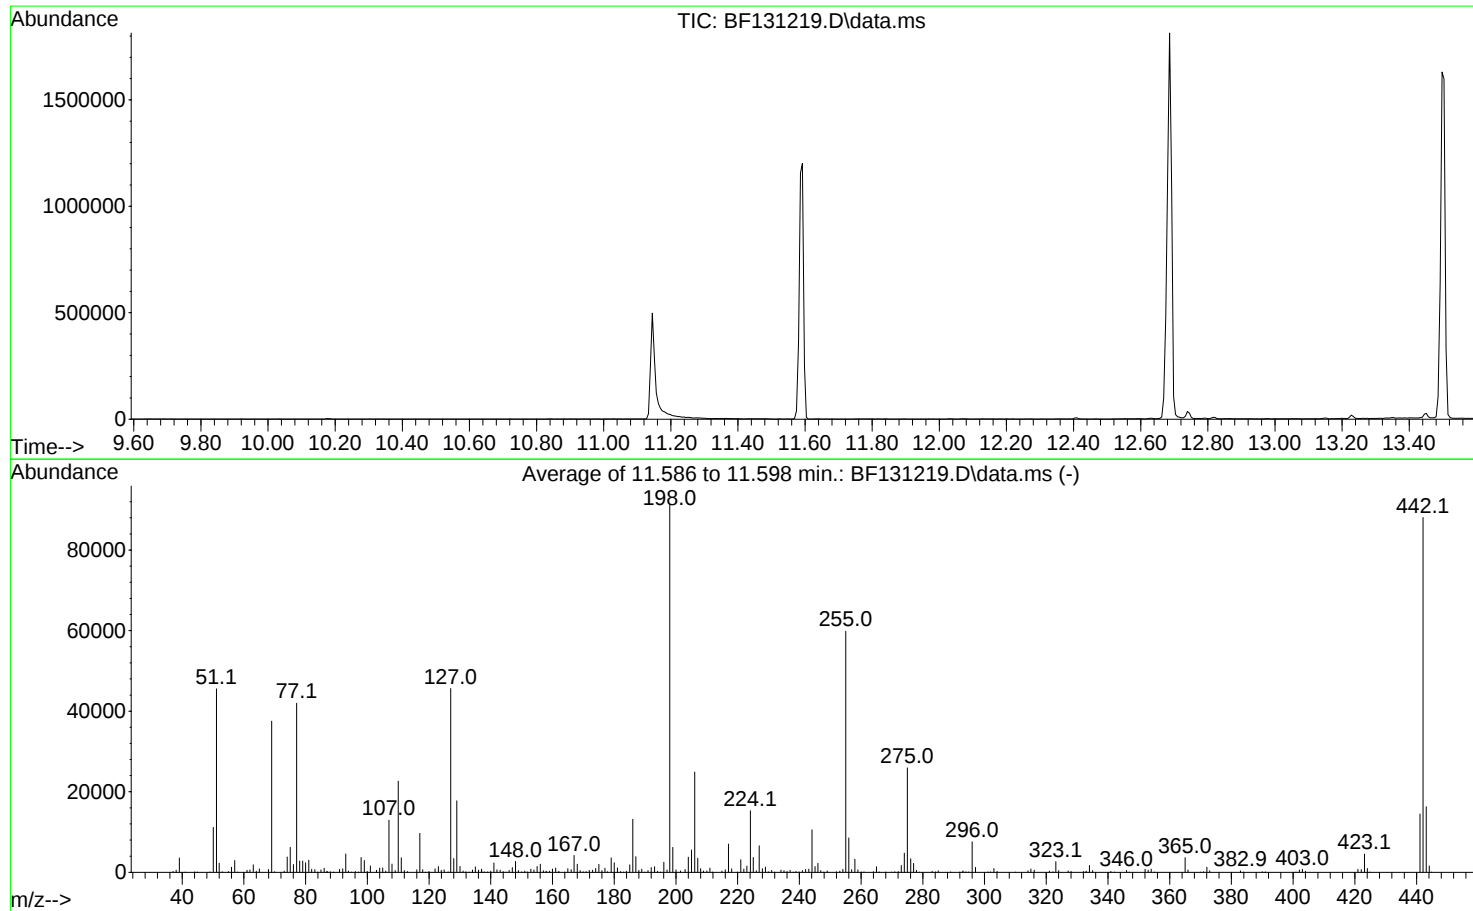

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1609

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	45544	PASS
68	69	0.00	2	1.8	680	PASS
69	198	0.00	100	41.1	37542	PASS
70	69	0.00	2	0.4	151	PASS
127	198	10	80	49.9	45609	PASS
197	198	0.00	2	0.6	580	PASS
198	198	100	100	100.0	91331	PASS
199	198	5	9	6.7	6162	PASS
275	198	10	60	28.4	25919	PASS
365	198	1	100	4.0	3643	PASS
441	198	0.01	100	15.8	14466	PASS
442	442	50	100	100.0	88083	PASS
443	442	15	24	18.5	16270	PASS