
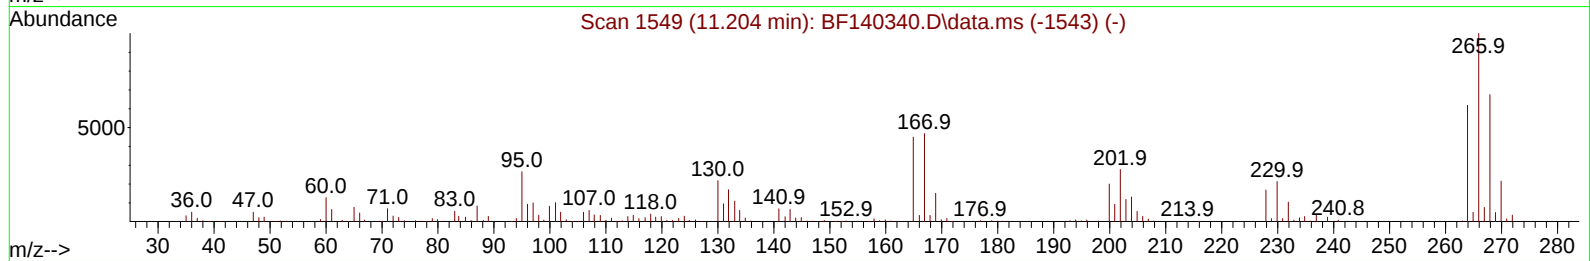
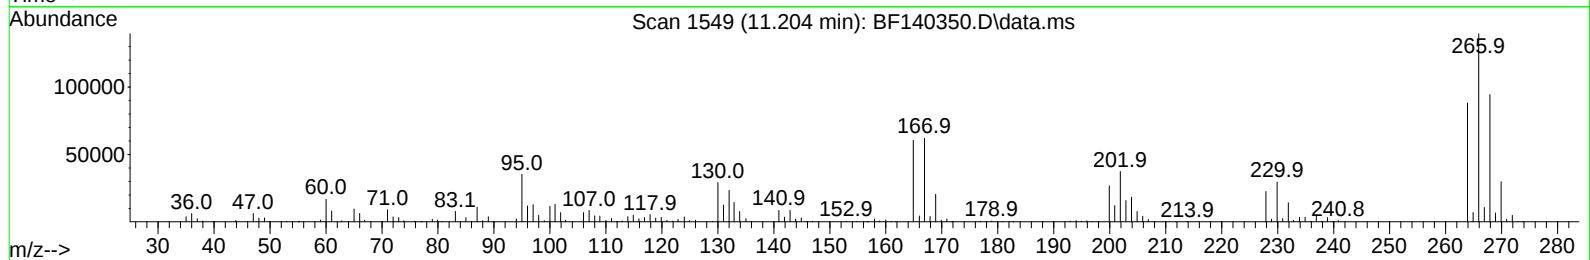


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140350.D
Acq On : 14 Nov 2024 08:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 10:48:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

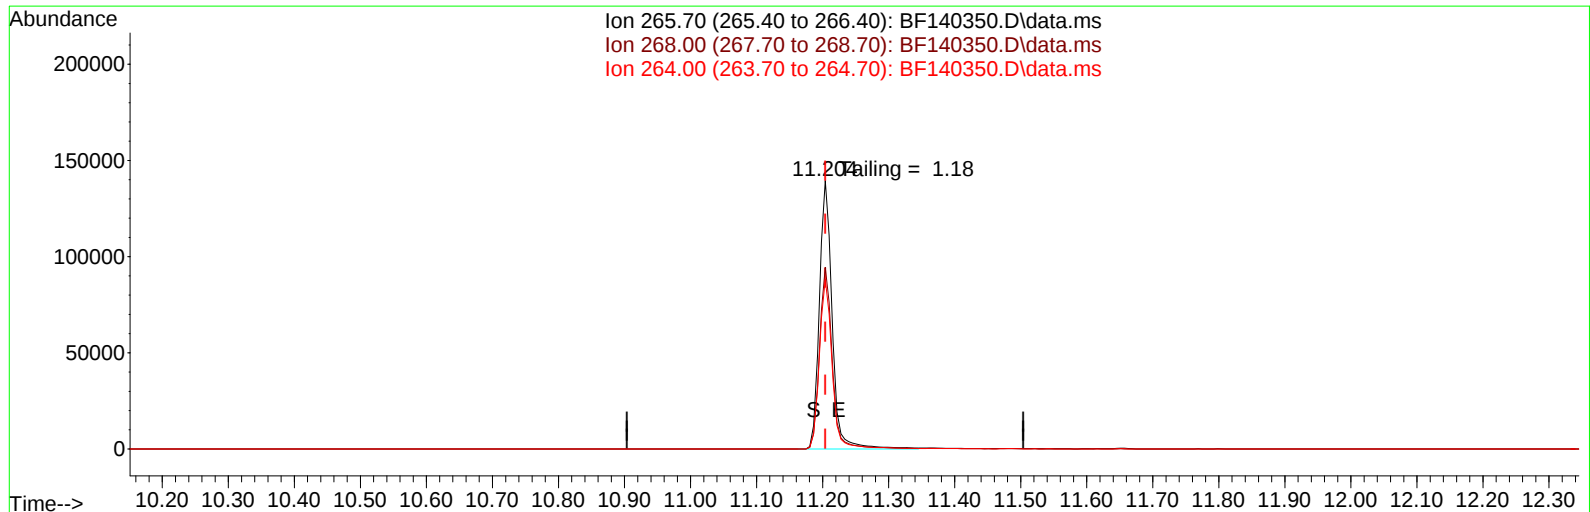

TIC: BF140350.D\data.ms

(70) Pentachlorophenol (C)




11.204min (-0.000) 30509.82 ng

response 188723

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.69
264.00	62.90	63.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140350.D
Acq On : 14 Nov 2024 08:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 14 10:48:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

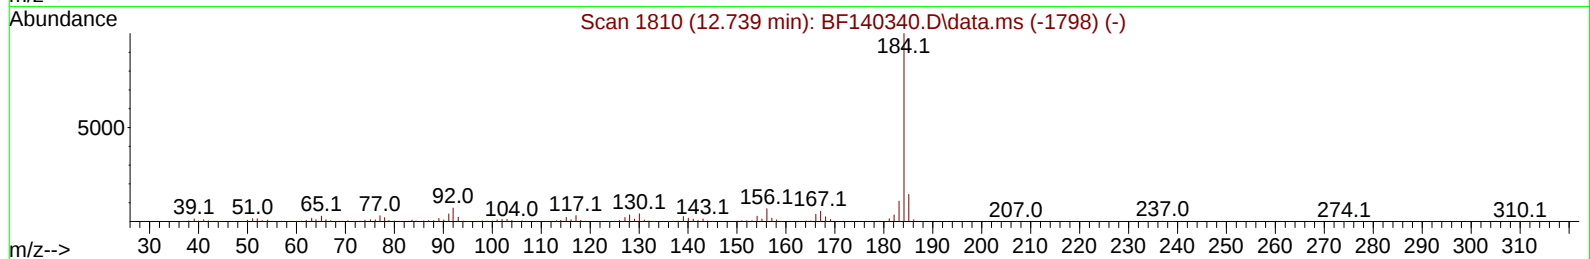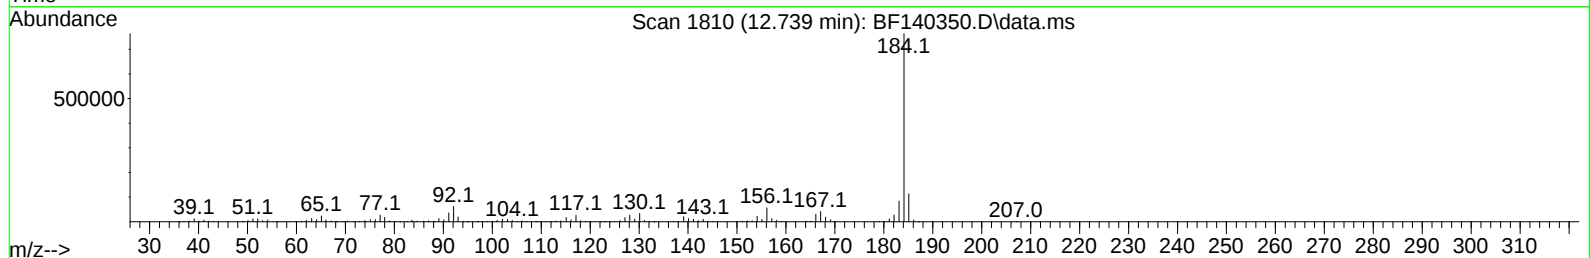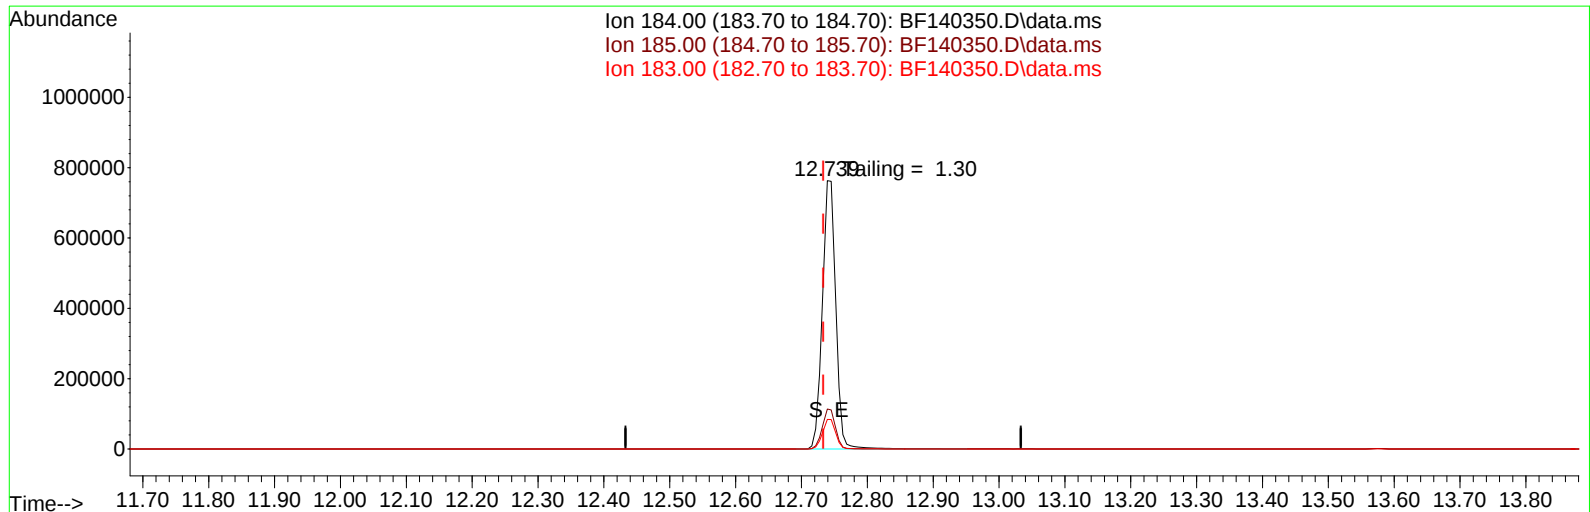

TIC: BF140350.D\data.ms

(77) Benzidine**12.739min (+ 0.006) 49755.95 ng****response 1078960**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.90
183.00	10.80	11.03
0.00	0.00	0.00