

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
 Data File : BF140376.D
 Acq On : 14 Nov 2024 21:28
 Operator : RC/JU
 Sample : P4796-01RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-1RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.140	3	8	19	rVB	689584	1095114	47.92%	6.312%
2	2.252	21	27	33	rBV	35405	59903	2.62%	0.345%
3	5.087	501	509	522	rBV	125834	181963	7.96%	1.049%
4	5.504	574	580	598	rBV	1483904	1960230	85.78%	11.299%
5	6.516	746	752	768	rVB	1559915	2046640	89.56%	11.797%
6	6.875	808	813	818	rBV	575462	698112	30.55%	4.024%
7	7.434	902	908	913	rBV	1010146	1276986	55.88%	7.361%
8	7.687	946	951	960	rBV	42481	58944	2.58%	0.340%
9	8.157	1025	1031	1044	rBV	667386	879084	38.47%	5.067%
10	9.228	1207	1213	1218	rBV	1873313	2285254	100.00%	13.173%
11	9.910	1323	1329	1334	rBV	722174	886596	38.80%	5.110%
12	10.622	1445	1450	1457	rBV	124965	156682	6.86%	0.903%
13	10.698	1458	1463	1479	rVV	800293	1043299	45.65%	6.014%
14	11.398	1577	1582	1590	rBV	589700	764655	33.46%	4.408%
15	11.922	1666	1671	1683	rBV3	87064	182652	7.99%	1.053%
16	12.622	1784	1790	1801	rBV2	155150	433326	18.96%	2.498%
17	12.710	1802	1805	1817	rVB5	36528	83348	3.65%	0.480%
18	12.839	1823	1827	1833	rVB	55422	79332	3.47%	0.457%
19	12.980	1846	1851	1857	rBV	1344804	1770528	77.48%	10.206%
20	13.892	2002	2006	2016	rVB3	47974	91312	4.00%	0.526%
21	14.039	2024	2031	2042	rBV	491173	787464	34.46%	4.539%
22	15.098	2207	2211	2219	rBV	43818	91807	4.02%	0.529%
23	15.533	2280	2285	2295	rVB	268690	435397	19.05%	2.510%




Sum of corrected areas: 17348628

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140376.D
Acq On : 14 Nov 2024 21:28
Operator : RC/JU
Sample : P4796-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

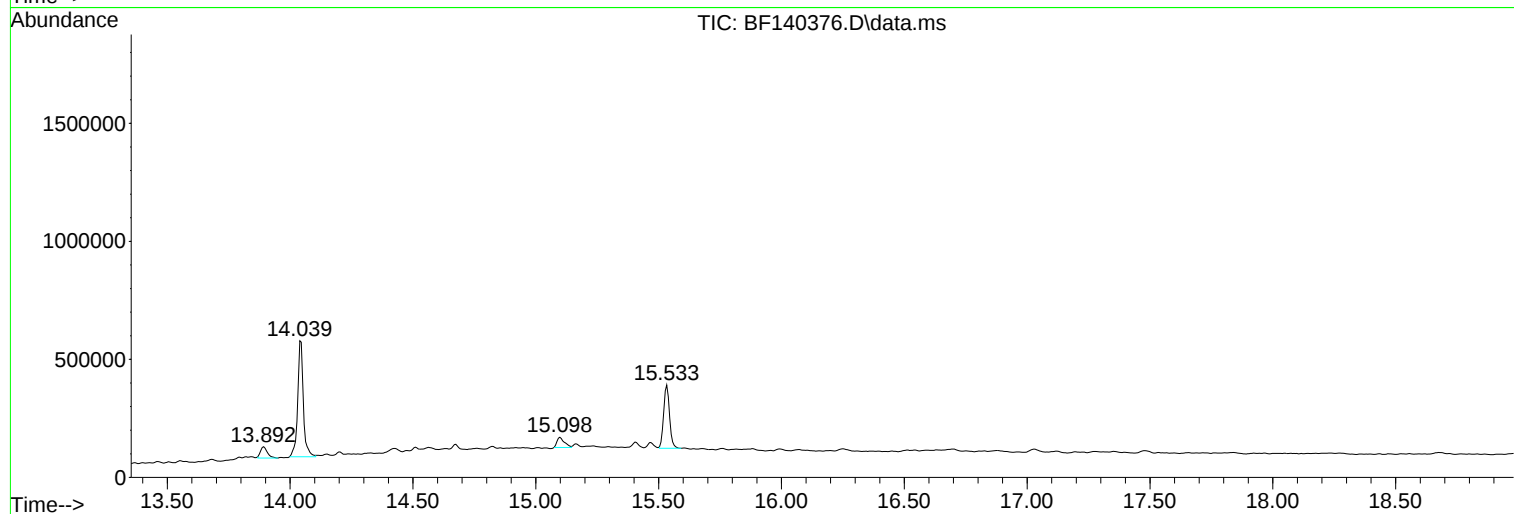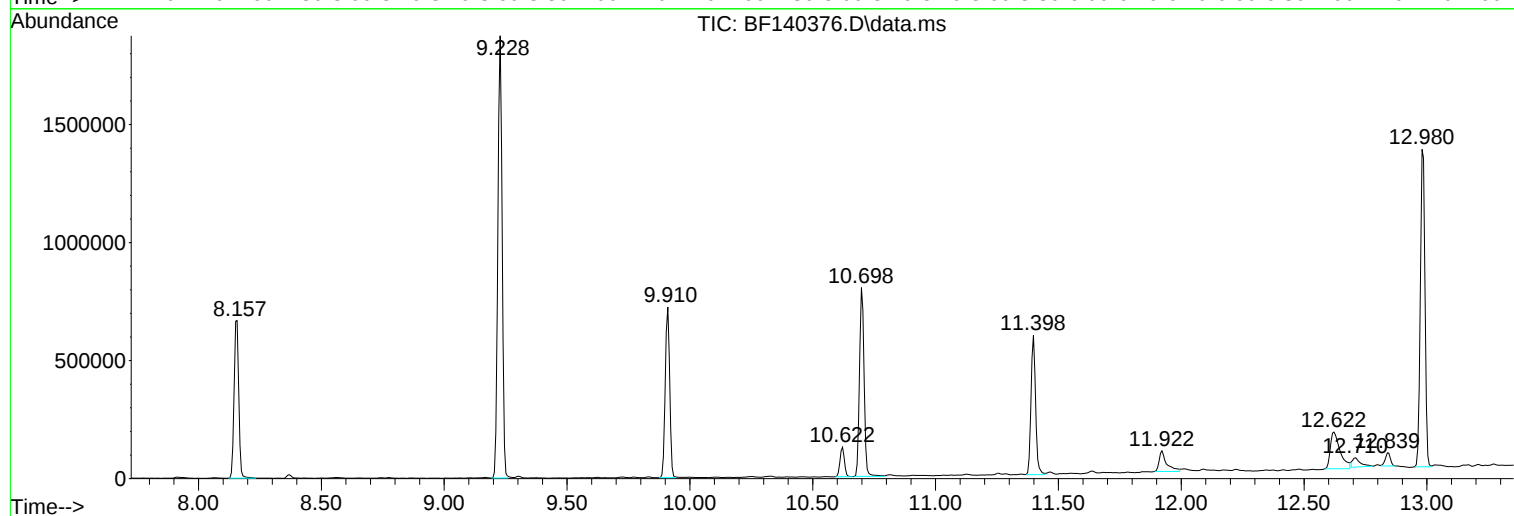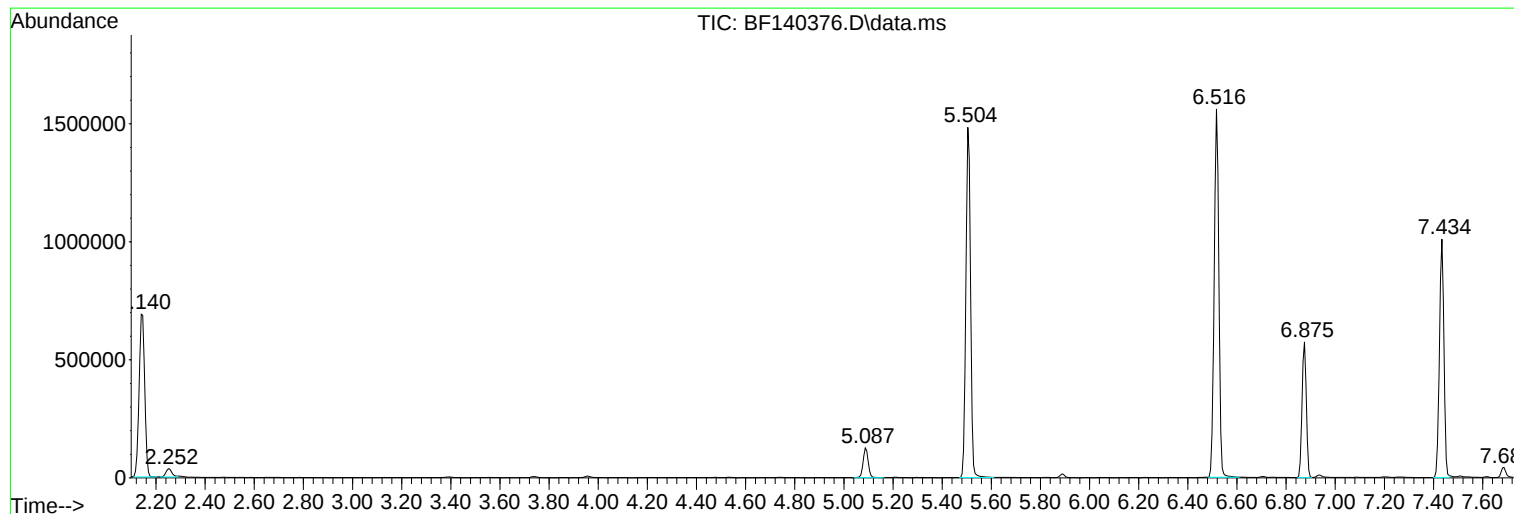

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140376.D
Acq On : 14 Nov 2024 21:28
Operator : RC/JU
Sample : P4796-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140376.D
Acq On : 14 Nov 2024 21:28
Operator : RC/JU
Sample : P4796-01RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-1RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------