

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
 Data File : BF140380.D
 Acq On : 14 Nov 2024 23:13
 Operator : RC/JU
 Sample : P4795-01RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LAW-23-00189RE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140380.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.146	3	9	20	rVB	894143	1379338	46.37%	5.734%
2	2.252	21	27	33	rBV	47522	84815	2.85%	0.353%
3	5.093	501	510	520	rBV	162438	248272	8.35%	1.032%
4	5.510	575	581	598	rBV	1895157	2595265	87.25%	10.789%
5	5.893	638	646	653	rBV	22179	32101	1.08%	0.133%
6	6.522	748	753	770	rVB	1927887	2683578	90.22%	11.157%
7	6.875	808	813	819	rBV	618185	748640	25.17%	3.112%
8	6.940	819	824	829	rBV3	22913	40138	1.35%	0.167%
9	7.434	899	908	917	rBV	1310062	1764990	59.34%	7.338%
10	7.687	945	951	959	rBV	61197	83954	2.82%	0.349%
11	8.157	1026	1031	1041	rVB	734773	933973	31.40%	3.883%
12	9.228	1207	1213	1218	rBV	2387901	2974524	100.00%	12.366%
13	9.775	1302	1306	1310	rBV	38583	56865	1.91%	0.236%
14	9.910	1324	1329	1334	rBV	721523	909468	30.58%	3.781%
15	10.316	1395	1398	1403	rBV3	45803	58891	1.98%	0.245%
16	10.622	1446	1450	1454	rBV	173733	232378	7.81%	0.966%
17	10.704	1459	1464	1469	rBV	1046871	1407117	47.31%	5.850%
18	10.822	1481	1484	1491	rBV	127298	189091	6.36%	0.786%
19	11.404	1579	1583	1592	rBV	569754	955380	32.12%	3.972%
20	11.933	1670	1673	1679	rVB3	585420	793067	26.66%	3.297%
21	12.992	1849	1853	1859	rVB	1628943	2105698	70.79%	8.754%
22	14.045	2029	2032	2039	rVB2	468333	727139	24.45%	3.023%
23	14.969	2185	2189	2194	rVB	278550	371551	12.49%	1.545%
24	15.098	2208	2211	2218	rVV	110916	202708	6.81%	0.843%
25	15.163	2218	2222	2225	rVV	246913	354774	11.93%	1.475%
26	15.204	2225	2229	2245	rVB2	391902	808593	27.18%	3.362%
27	15.539	2281	2286	2300	rVB	283883	520784	17.51%	2.165%
28	15.757	2319	2323	2335	rVB	148356	263063	8.84%	1.094%
29	15.998	2358	2364	2370	rVB	286781	527783	17.74%	2.194%




Sum of corrected areas: 24053938

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140380.D
Acq On : 14 Nov 2024 23:13
Operator : RC/JU
Sample : P4795-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LAW-23-00189RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

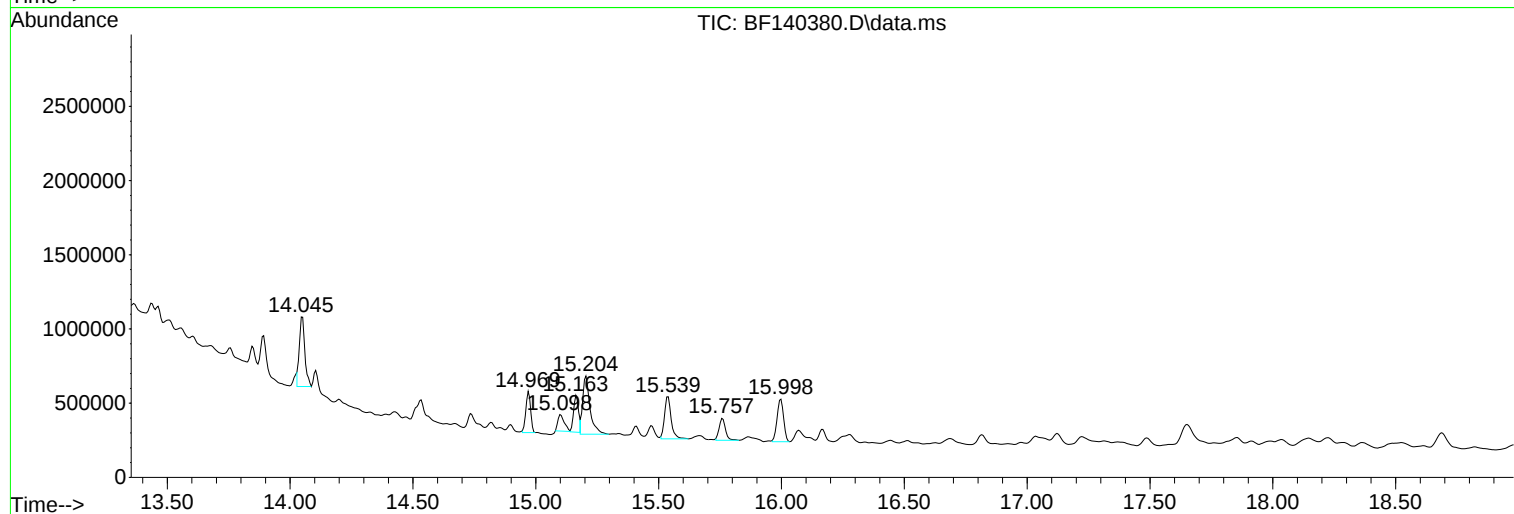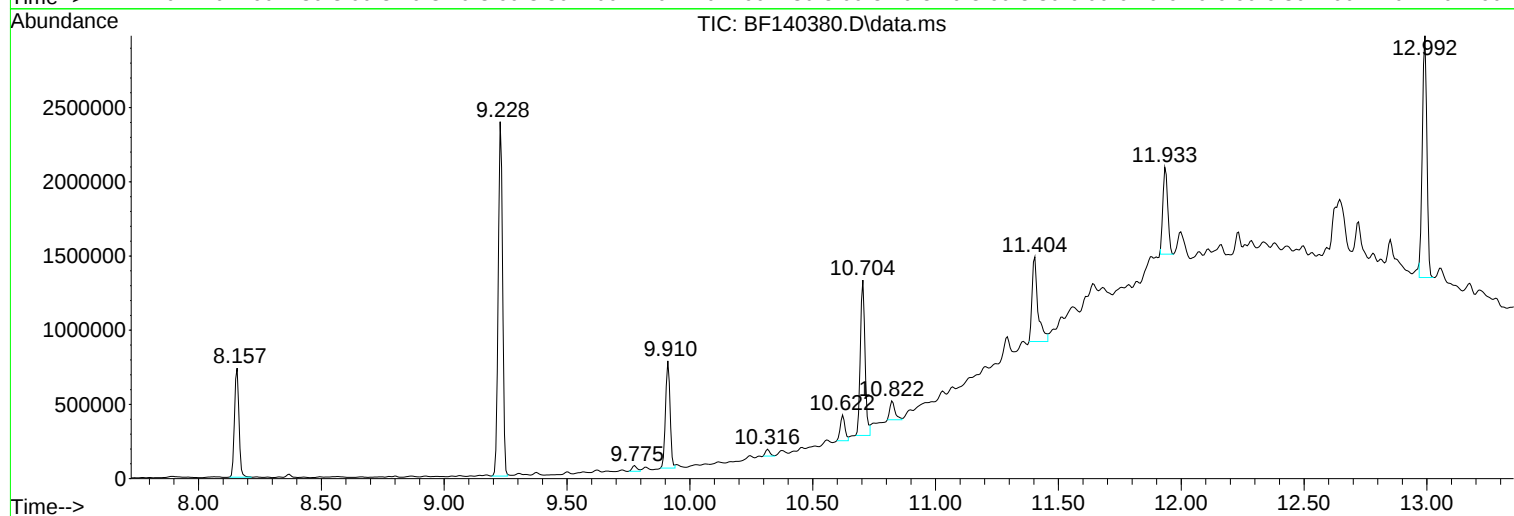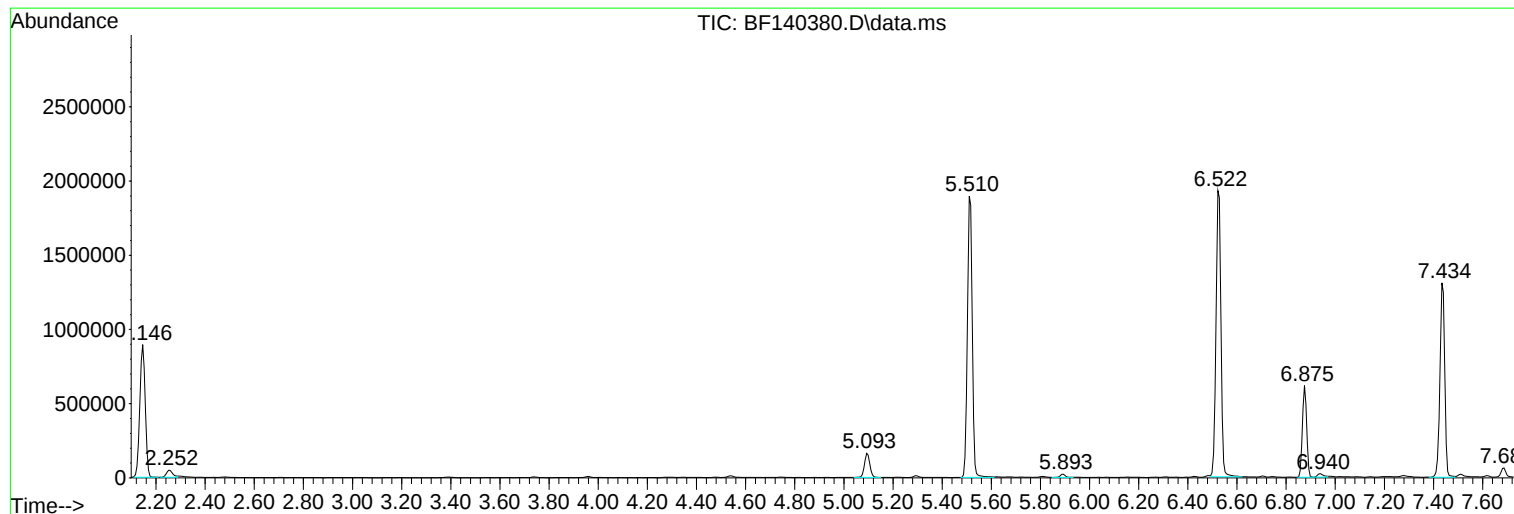

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140380.D
Acq On : 14 Nov 2024 23:13
Operator : RC/JU
Sample : P4795-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LAW-23-00189RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111424\
Data File : BF140380.D
Acq On : 14 Nov 2024 23:13
Operator : RC/JU
Sample : P4795-01RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LAW-23-00189RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------