
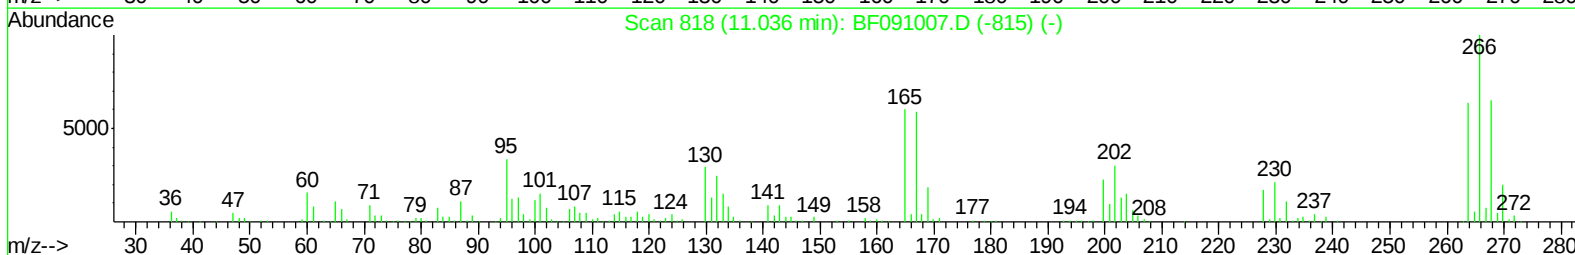
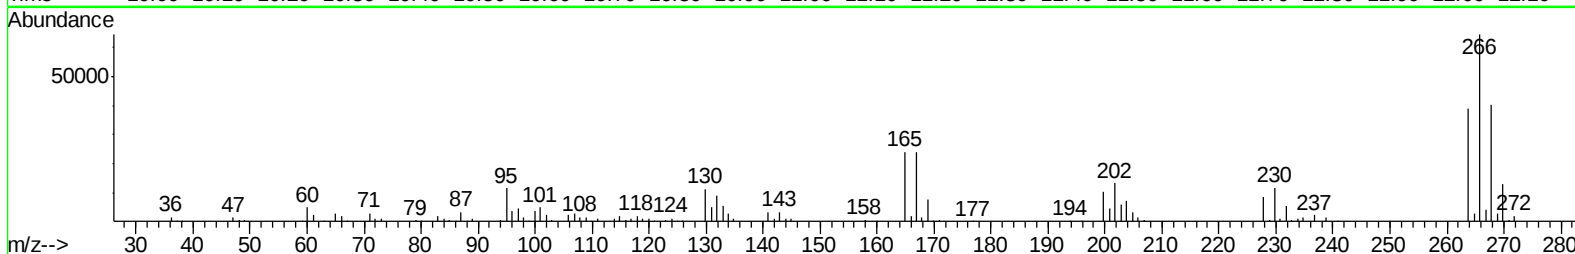


Data Path : Z:\HPCHEM1\BNA F\DATA\BF111516\
Data File : BF091166.D
Acq On : 15 Nov 2016 8:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 17:13:27 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

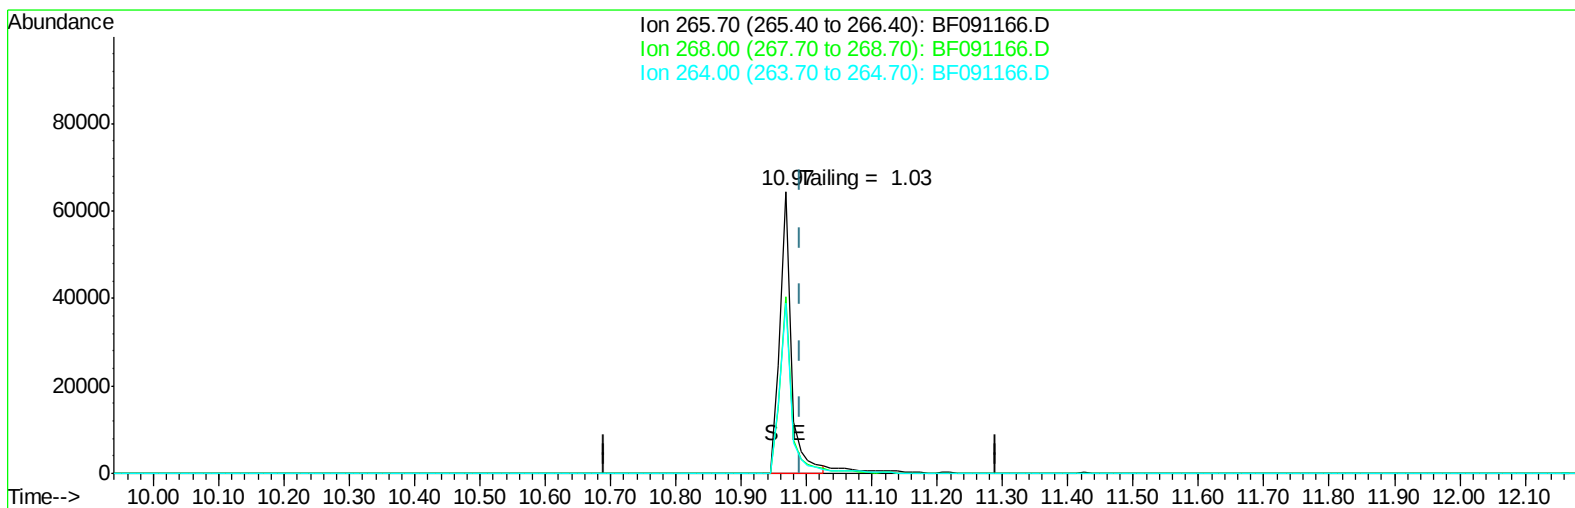

TIC: BF091166.D

(69) Pentachlorophenol (C)




10.968min (-0.023) 32560.02ng

response 82885

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	62.75
264.00	63.90	60.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111516\
Data File : BF091166.D
Acq On : 15 Nov 2016 8:50
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 15 17:13:27 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

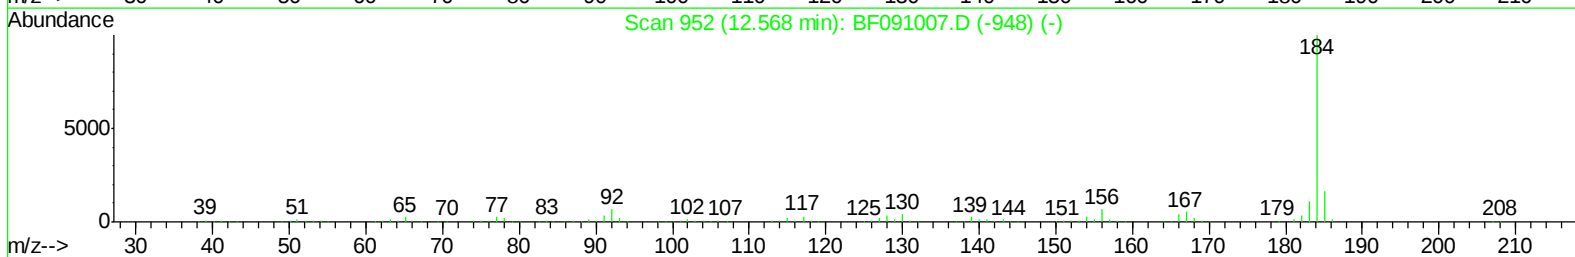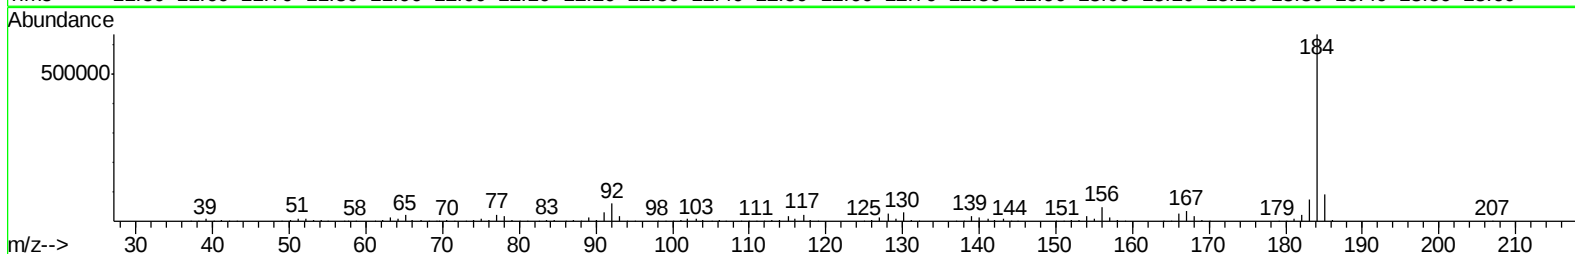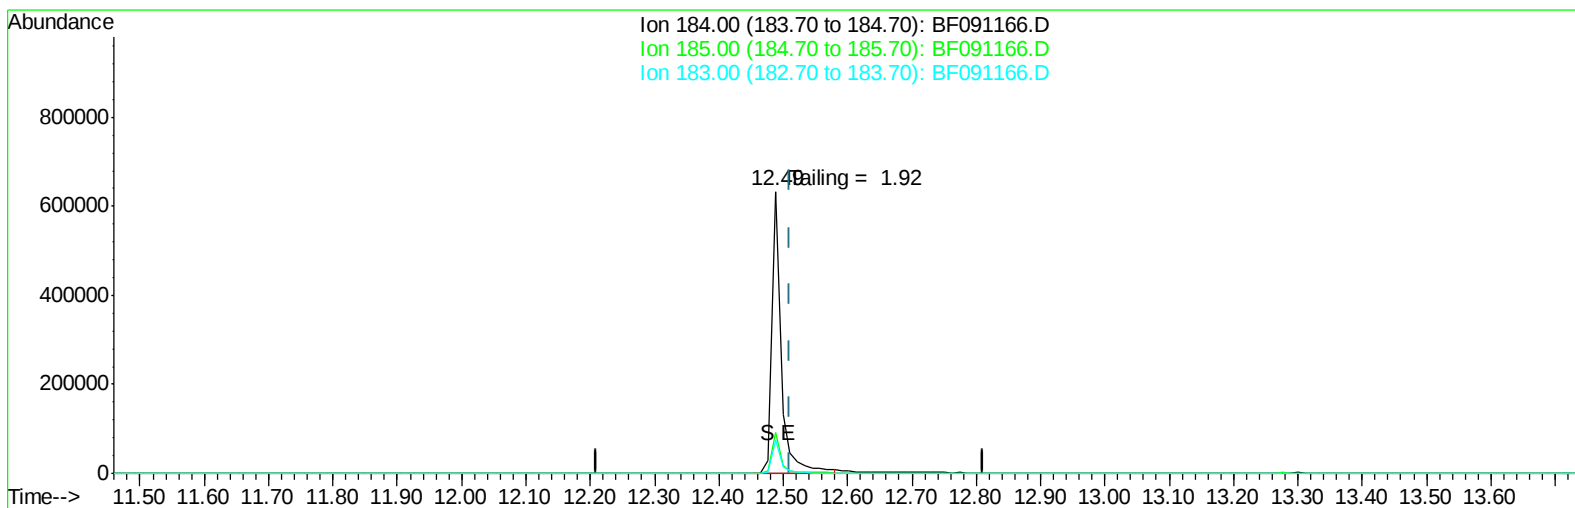

TIC: BF091166.D

(76) Benzidine

12.488min (-0.023) 40256.36ng

response 663720

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.78
183.00	10.90	11.64
0.00	0.00	0.00