
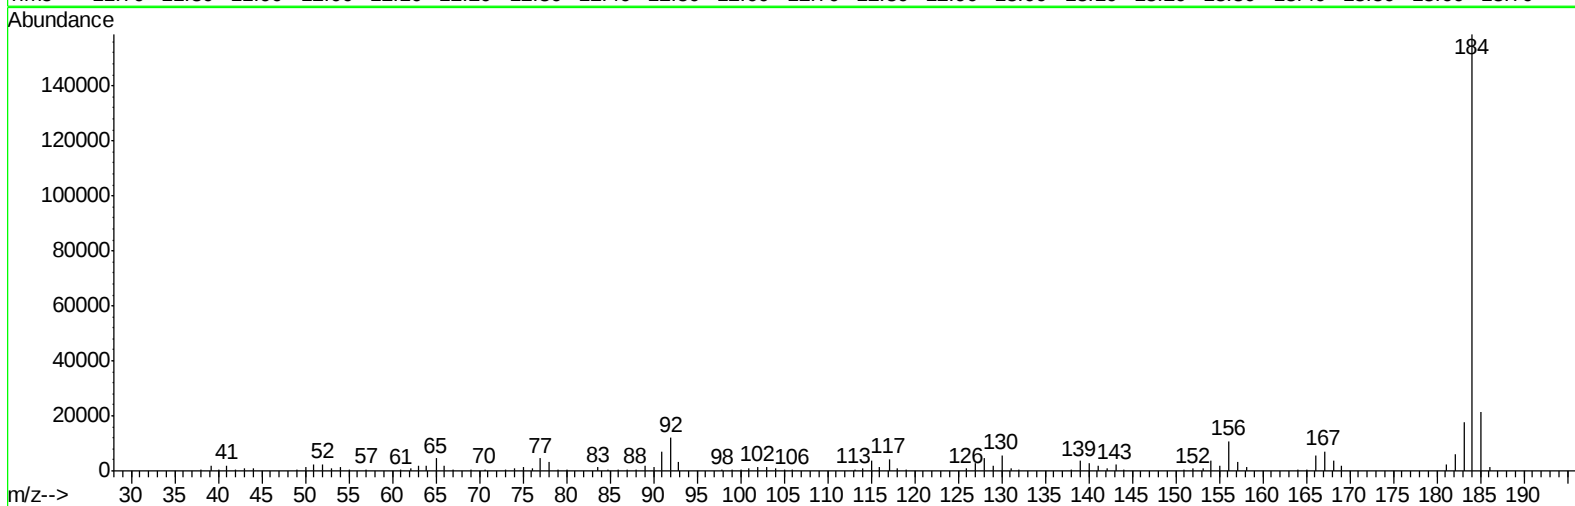


Data Path : Z:\HPCHEM1\BNA F\DATA\BF111517\
Data File : BF100577.D
Acq On : 15 Nov 2017 9:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 07:27:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 13:27:38 2017
Response via : Initial Calibration

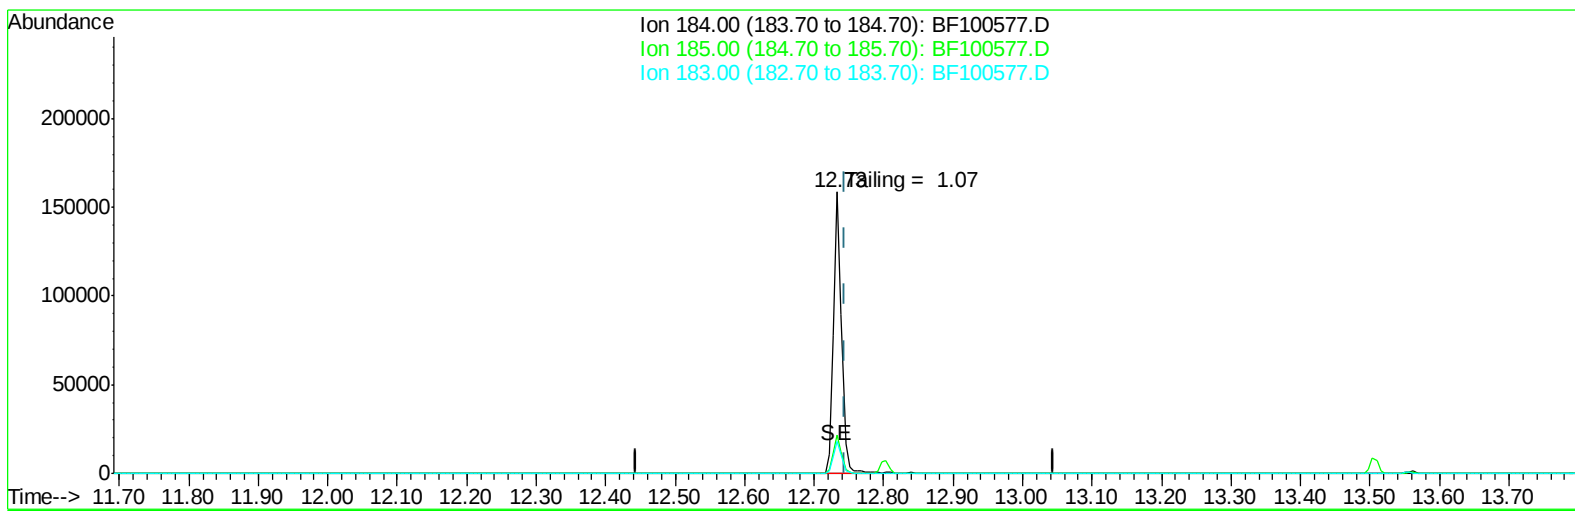

TIC: BF100577.D

(76) Benzidine



12.733min (-0.012) 0.00ng

response 128595

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.62
183.00	11.60	11.15
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111517\
Data File : BF100577.D
Acq On : 15 Nov 2017 9:16
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 07:27:46 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 13:27:38 2017
Response via : Initial Calibration

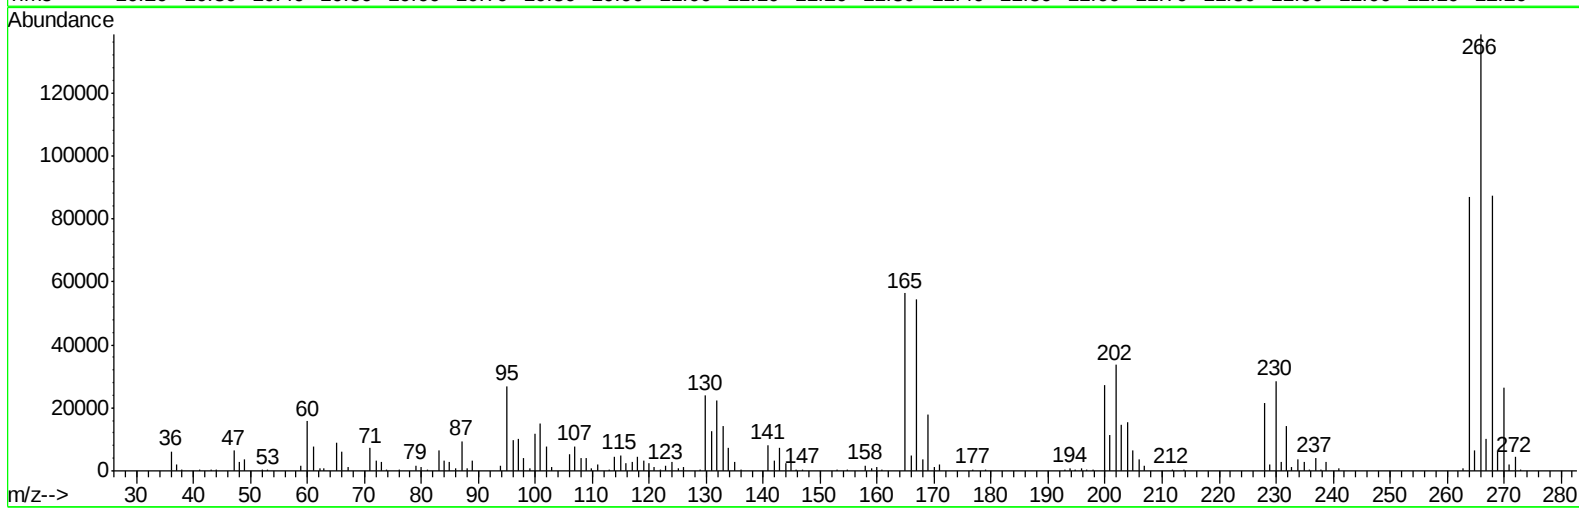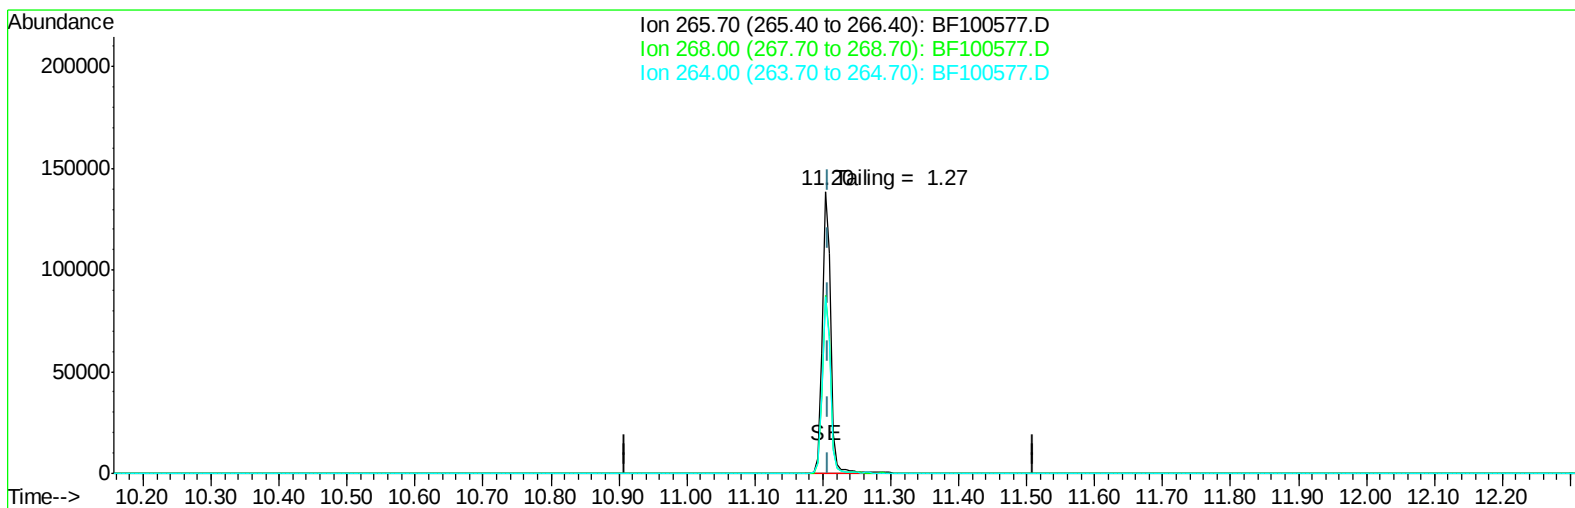

TIC: BF100577.D

(69) Pentachlorophenol (C)

11.204min (-0.006) 34046.70ng

response 123172

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.20
264.00	61.90	62.88
0.00	0.00	0.00