
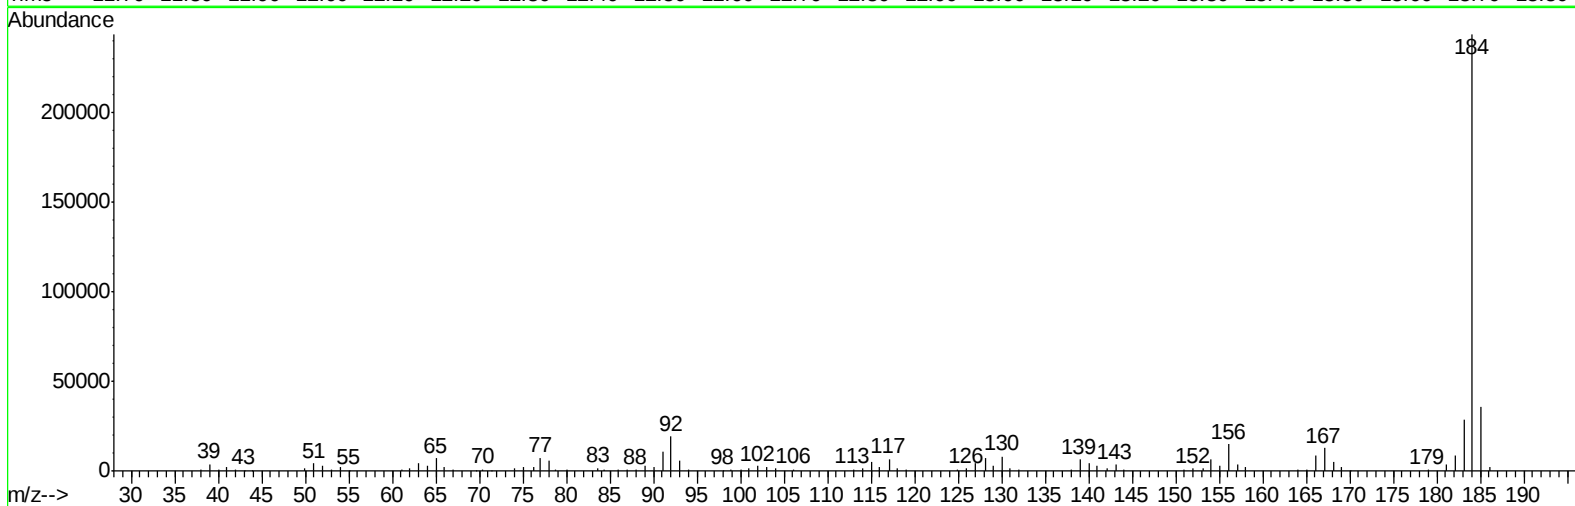


Data Path : Z:\HPCHEM1\BNA F\DATA\BF111517\
Data File : BF100601.D
Acq On : 15 Nov 2017 21:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 07:28:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 13:27:38 2017
Response via : Initial Calibration

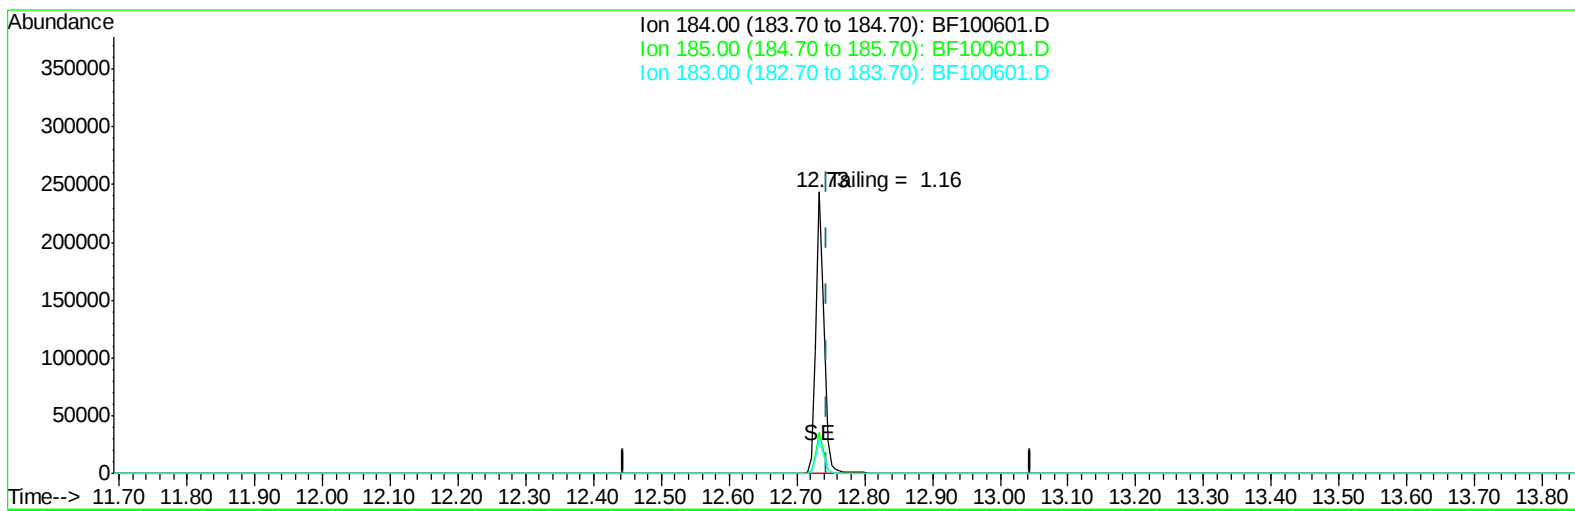

TIC: BF100601.D

(76) Benzidine



12.733min (-0.012) 0.00ng

response 200580

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.70
183.00	11.60	11.73
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111517\
Data File : BF100601.D
Acq On : 15 Nov 2017 21:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 07:28:48 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 13:27:38 2017
Response via : Initial Calibration

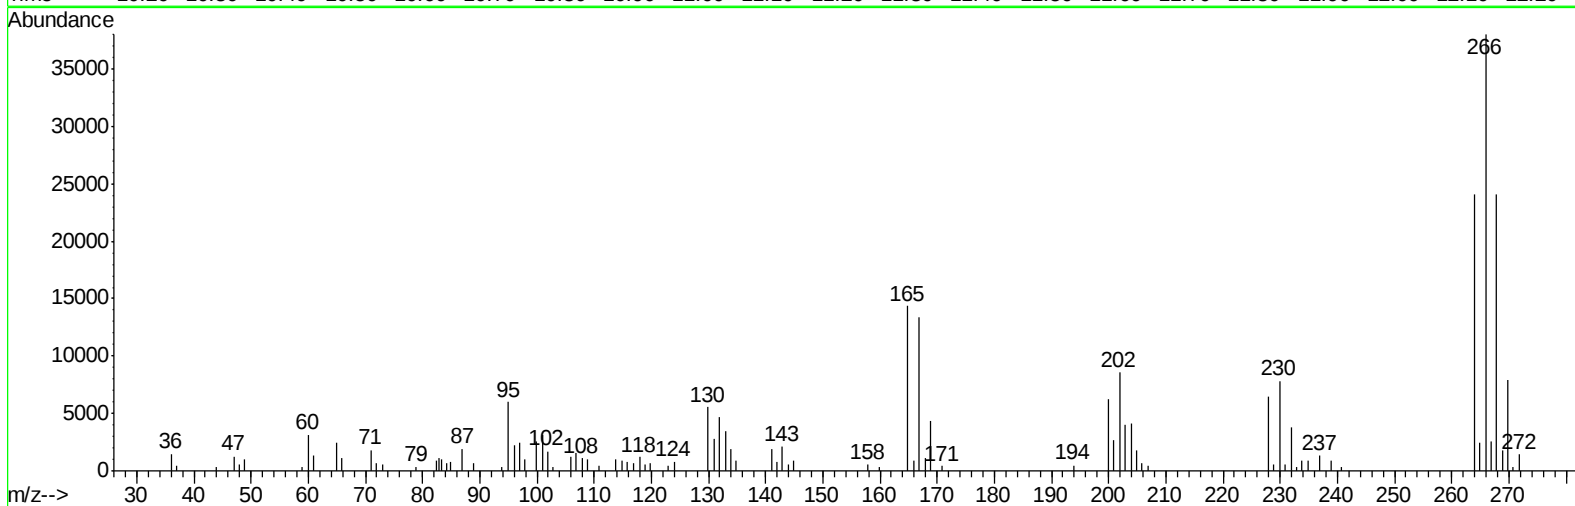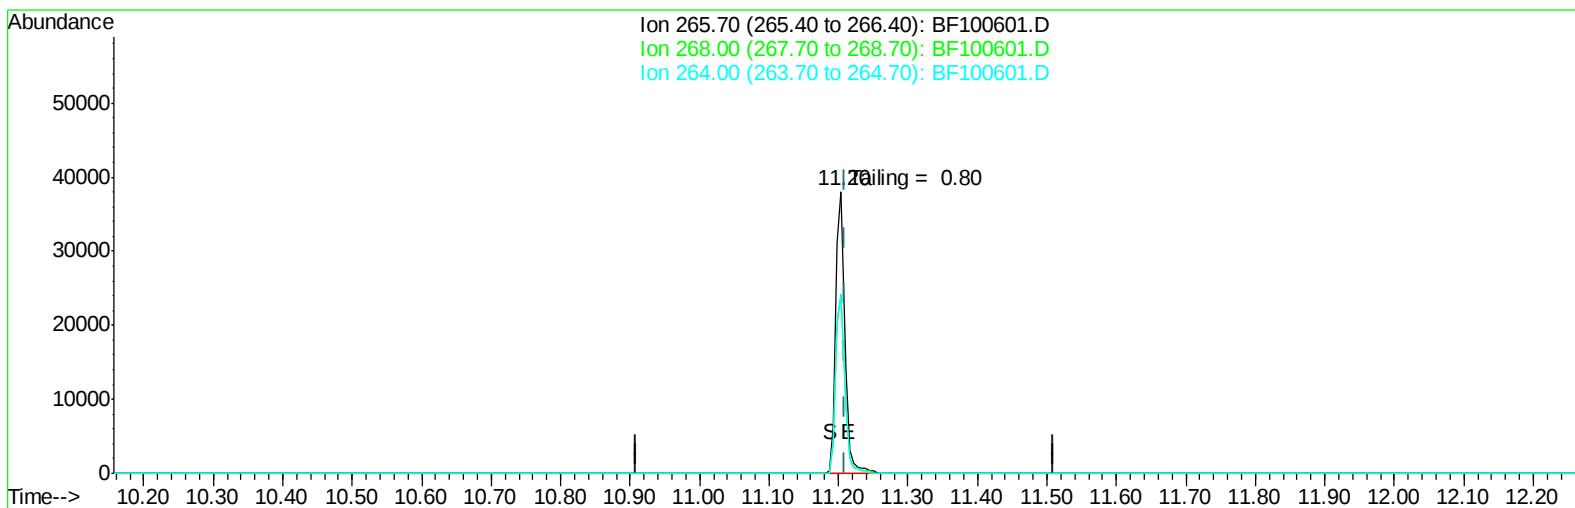

TIC: BF100601.D

(69) Pentachlorophenol (C)

11.204min (-0.006) 18246.64ng

response 34326

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.43
264.00	61.90	63.40
0.00	0.00	0.00