

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111517\
 Data File : BF100612.D
 Acq On : 16 Nov 2017 3:00
 Operator : SJ/JU
 Sample : I6426-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 110917-JETT-F-D-S

Quant Time: Nov 16 06:44:54 2017
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 15 13:27:38 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	115644	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	444481	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	199265	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	351747	20.00	ng	0.00
75) Chrysene-d12	14.04	240	222003	20.00	ng	-0.01
86) Perylene-d12	15.51	264	231853	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	275498	38.19	ng	0.00
7) Phenol-d6	6.50	99	210919	23.71	ng	-0.02
23) Nitrobenzene-d5	7.45	82	614990	91.48	ng	0.00
41) 2,4,6-Tribromophenol	10.70	330	172787	85.10	ng	-0.01
44) 2-Fluorobiphenyl	9.24	172	1149377	87.83	ng	0.00
78) Terphenyl-d14	12.99	244	855681	88.56	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.63	163	39409	2.590	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111517\
Data File : BF100612.D
Acq On : 16 Nov 2017 3:00
Operator : SJ/JU
Sample : I6426-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
110917-JETT-F-D-S

Quant Time: Nov 16 06:44:54 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 15 13:27:38 2017
Response via : Initial Calibration




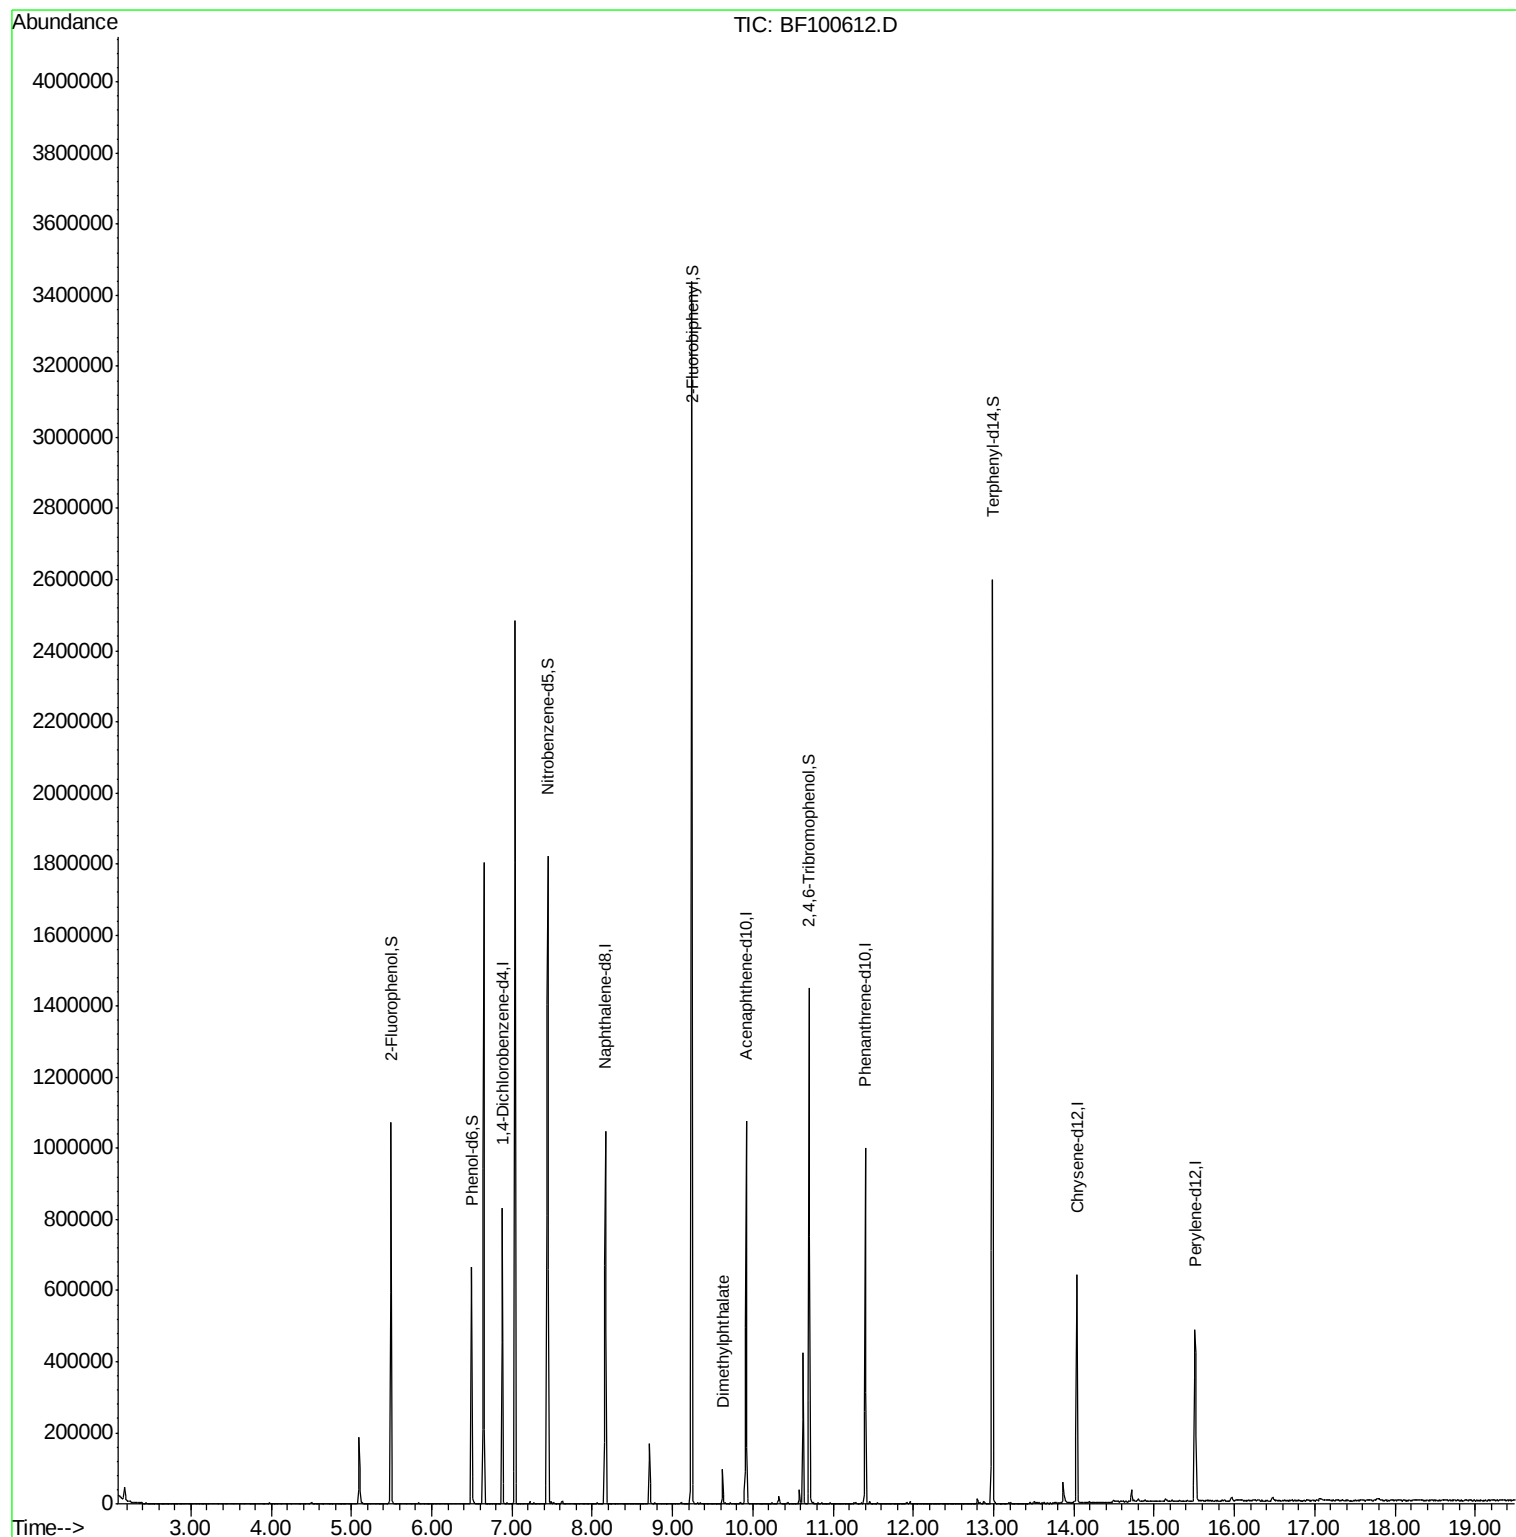


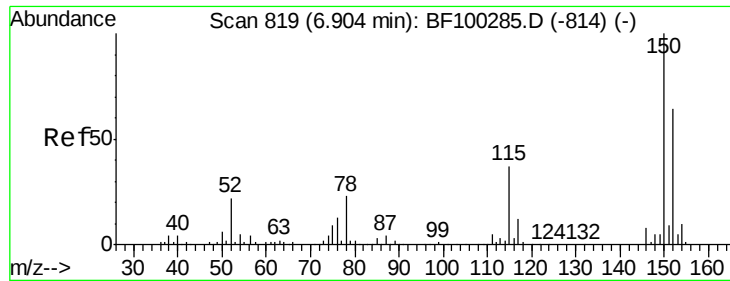

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.88 min Scan# 815
 Delta R.T. -0.01 min
 Lab File: BF100612.D
 Acq: 16 Nov 2017 3:00




Instrument :
 BNA_F
 ClientSampleId :
 110917-JETT-F-D-S


Tgt Ion:152 Resp: 115644
 Ion Ratio Lower Upper
 152 100
 150 152.7 124.6 186.8
 115 57.7 50.1 75.1

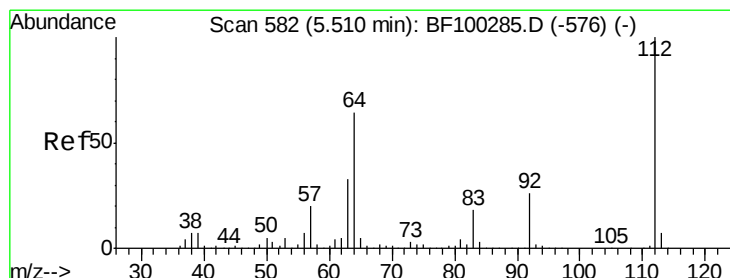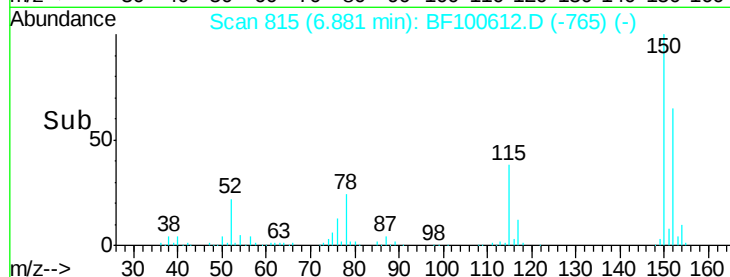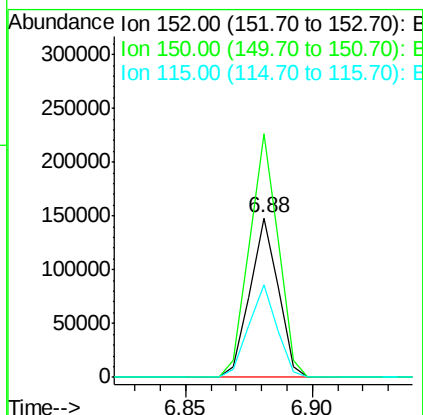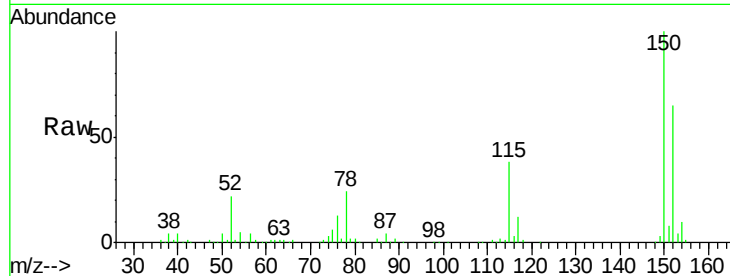

#5
 2-Fluorophenol
 Concen: 38.188 ng
 RT: 5.49 min Scan# 579
 Delta R.T. -0.01 min
 Lab File: BF100612.D
 Acq: 16 Nov 2017 3:00

Tgt Ion:112 Resp: 275498
 Ion Ratio Lower Upper
 112 100
 64 60.4 47.9 71.9
 63 30.6 23.7 35.5

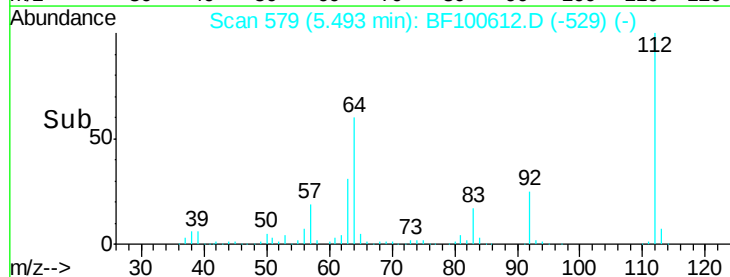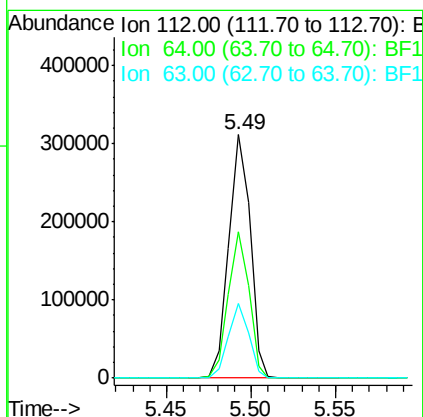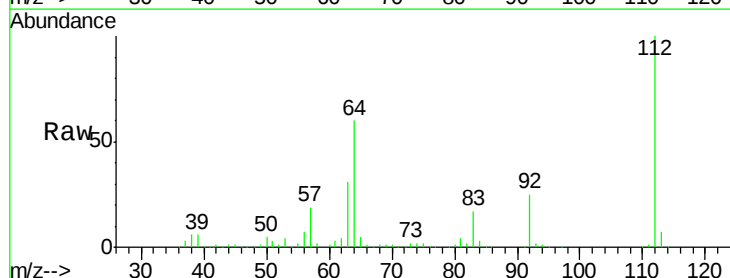

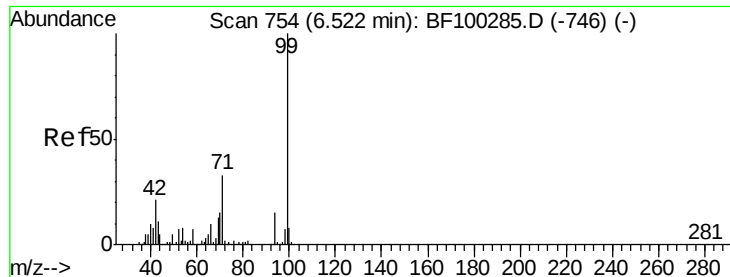

#7

Phenol-d6

Concen: 23.709 ng

RT: 6.50 min Scan# 750

Delta R.T. -0.02 min

Lab File: BF100612.D

Acq: 16 Nov 2017 3:00

Instrument :

BNA_F

ClientSampleId :

110917-JETT-F-D-S





Tgt Ion: 99 Resp: 210919

Ion Ratio Lower Upper

99 100

42 17.3 14.5 21.7

71 30.1 25.4 38.0

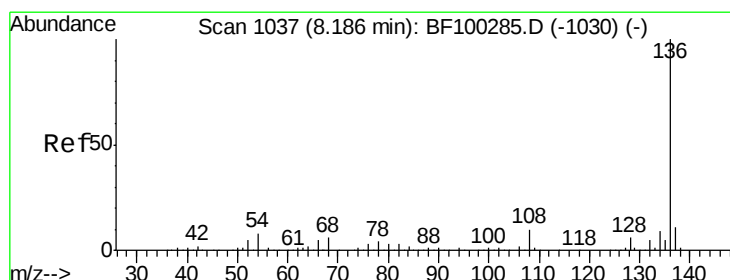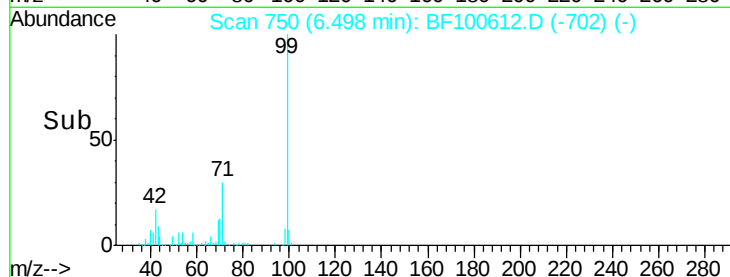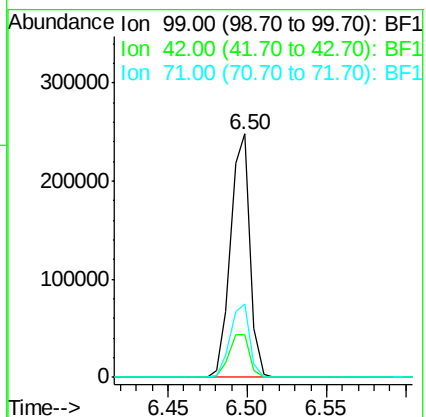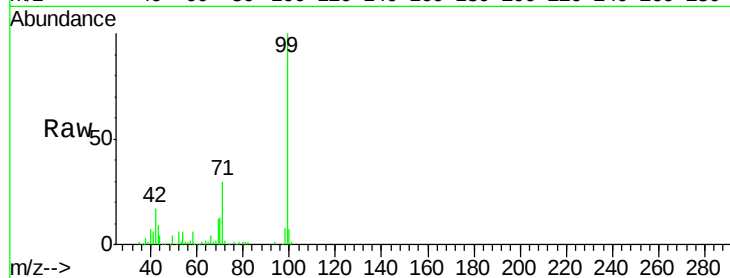

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1033

Delta R.T. -0.01 min

Lab File: BF100612.D

Acq: 16 Nov 2017 3:00

Tgt Ion: 136 Resp: 444481




Ion Ratio Lower Upper


136 100

137 10.7 8.9 13.3

54 8.2 6.6 9.8

68 6.0 5.0 7.4

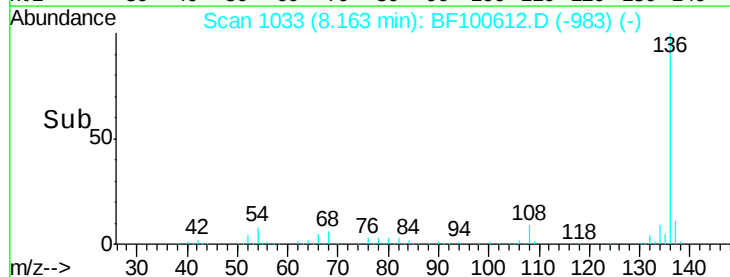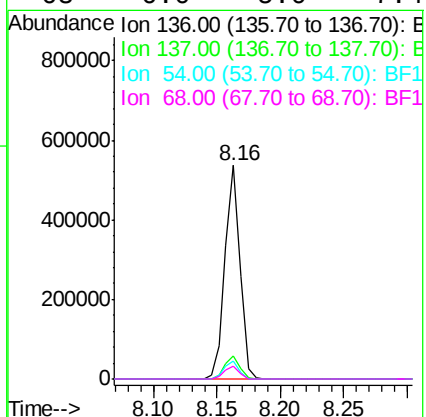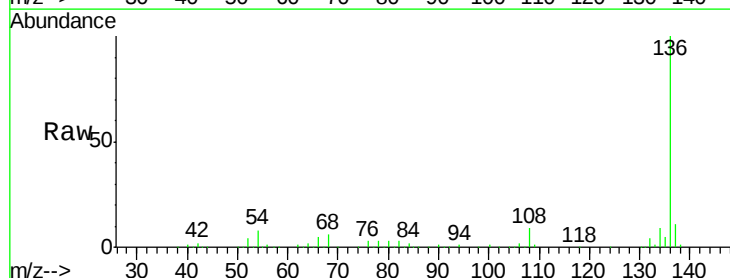


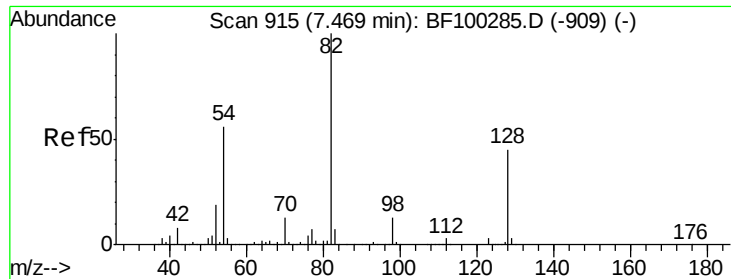




#23
 Nitrobenzene-d5
 Concen: 91.475 ng
 RT: 7.45 min Scan# 911
 Delta R.T. -0.01 min
 Lab File: BF100612.D
 Acq: 16 Nov 2017 3:00

Instrument :
 BNA_F
 ClientSampleId :
 110917-JETT-F-D-S

Tgt Ion	Ratio	Lower	Upper
82	100		
128	46.8	36.1	54.1
54	53.0	41.4	62.2

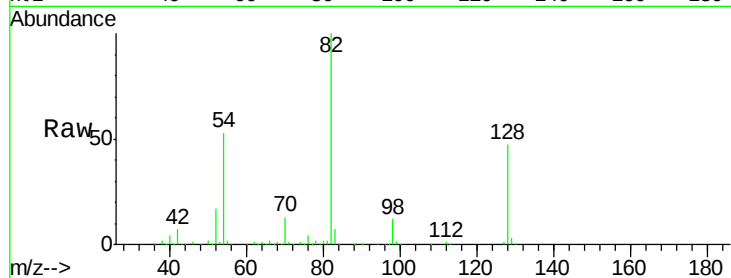


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

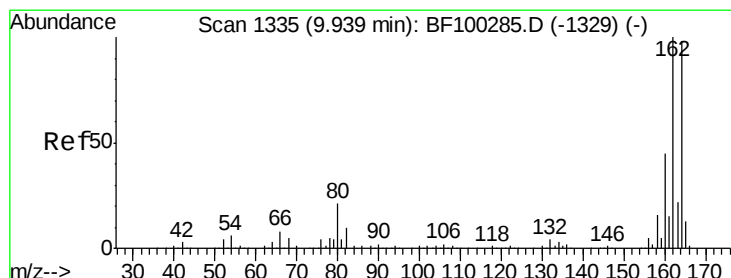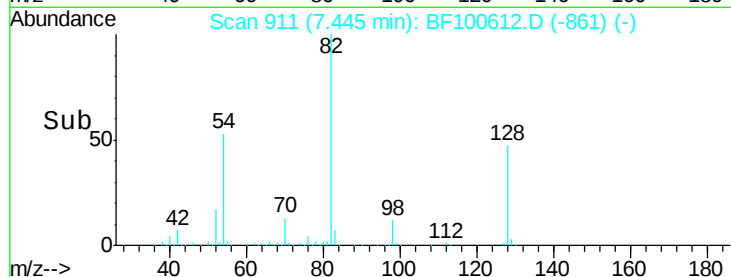
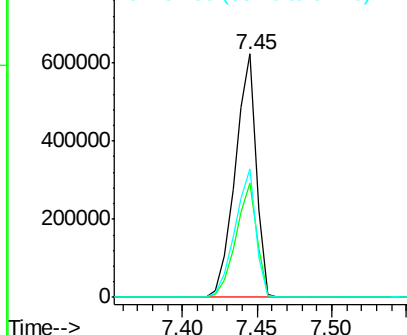



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.01 min
 Lab File: BF100612.D
 Acq: 16 Nov 2017 3:00

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.2	86.1	129.1
160	47.1	38.3	57.5

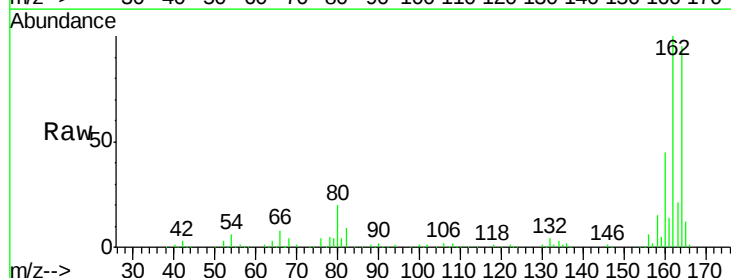

Abundance Ion 164.00 (163.70 to 164.70): BF1
 Ion 162.00 (161.70 to 162.70): BF1
 Ion 160.00 (159.70 to 160.70): BF1



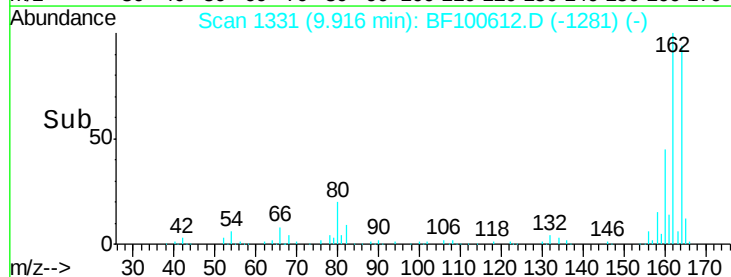
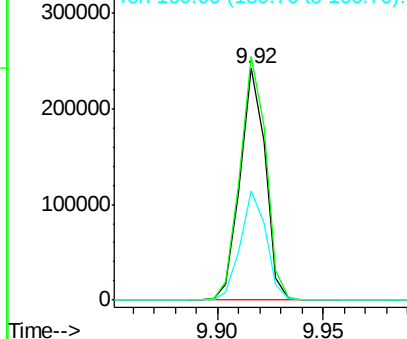


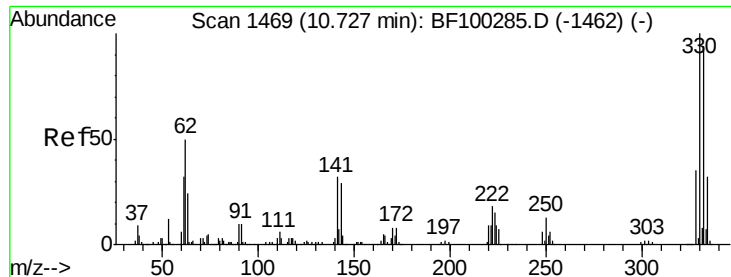

#41
 2,4,6-Tribromophenol
 Concen: 85.095 ng
 RT: 10.70 min Scan# 1465
 Delta R.T. -0.01 min
 Lab File: BF100612.D
 Acq: 16 Nov 2017 3:00




Instrument :
 BNA_F
 ClientSampleId :
 110917-JETT-F-D-S


Tgt Ion:330 Resp: 172787
 Ion Ratio Lower Upper
 330 100
 332 98.1 77.0 115.6
 141 28.6 29.9 44.9#

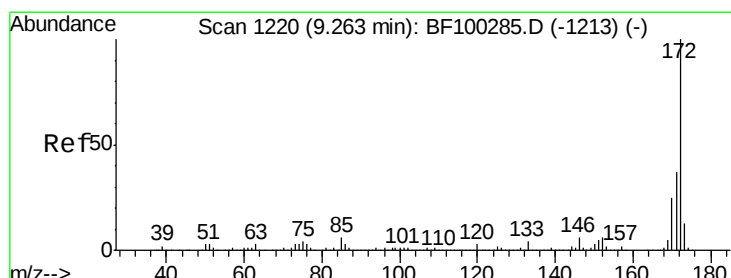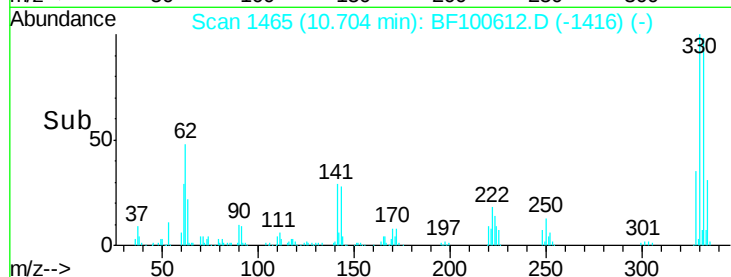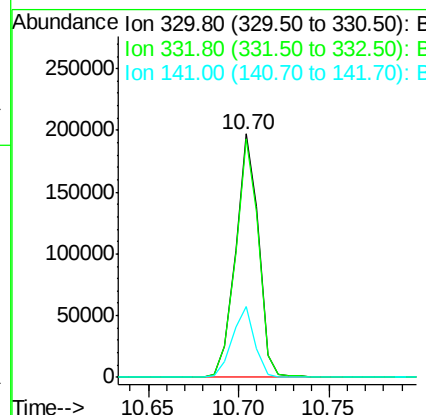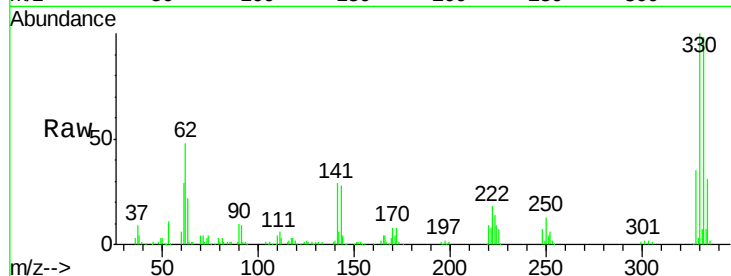

#44
 2-Fluorobiphenyl
 Concen: 87.831 ng
 RT: 9.24 min Scan# 1216
 Delta R.T. -0.01 min
 Lab File: BF100612.D
 Acq: 16 Nov 2017 3:00

Tgt Ion:172 Resp: 1149377
 Ion Ratio Lower Upper
 172 100
 171 36.0 29.7 44.5
 170 24.0 19.6 29.4

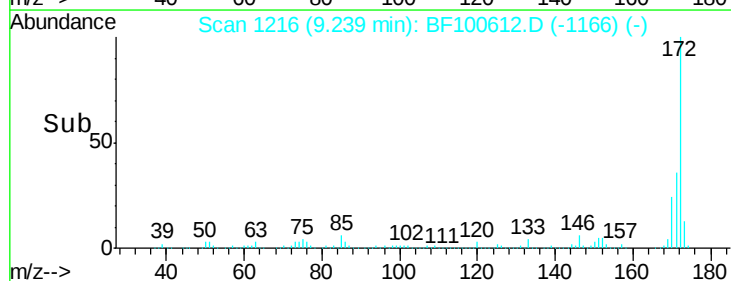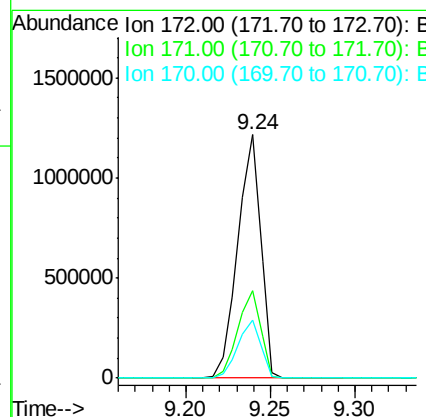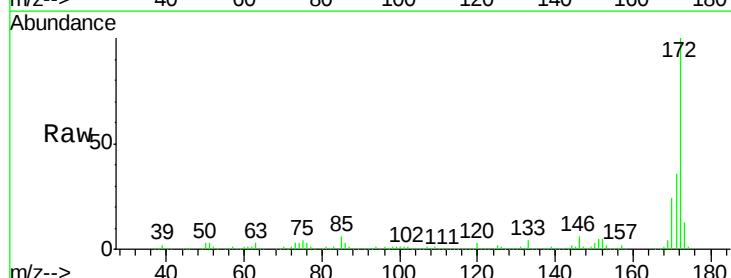


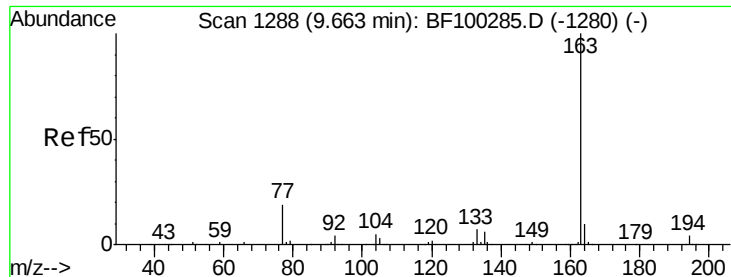




#49
Dimethylphthalate
Concen: 2.590 ng
RT: 9.63 min Scan# 1282
Delta R.T. -0.02 min
Lab File: BF100612.D
Acq: 16 Nov 2017 3:00

Instrument :
BNA_F
ClientSampleId :
110917-JETT-F-D-S

Tgt Ion:163 Resp: 39409
Ion Ratio Lower Upper
163 100
194 3.6 2.7 4.1
164 10.8 8.2 12.2

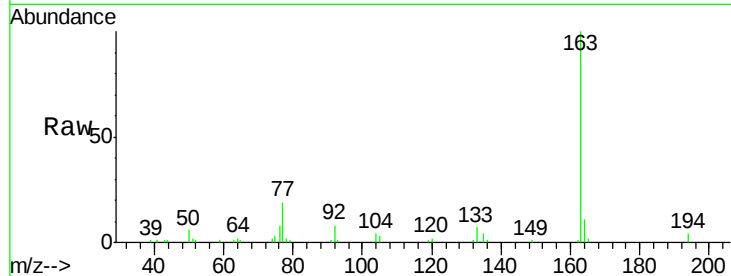


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

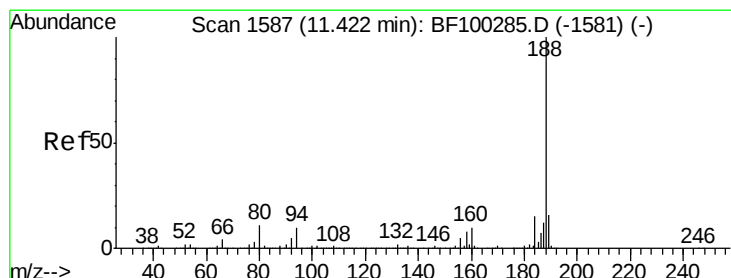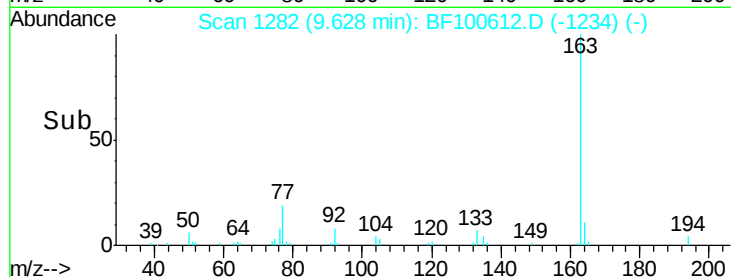
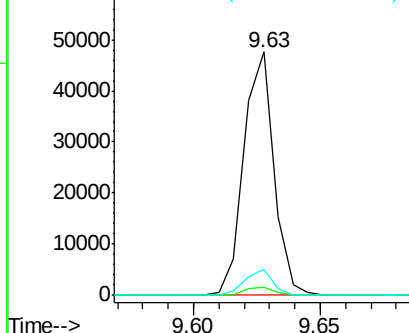



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. -0.01 min
Lab File: BF100612.D
Acq: 16 Nov 2017 3:00

Tgt Ion:188 Resp: 351747
Ion Ratio Lower Upper
188 100
94 8.8 8.5 12.7
80 10.1 9.2 13.8

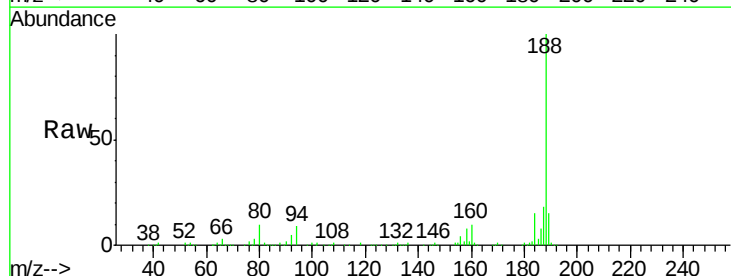

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1



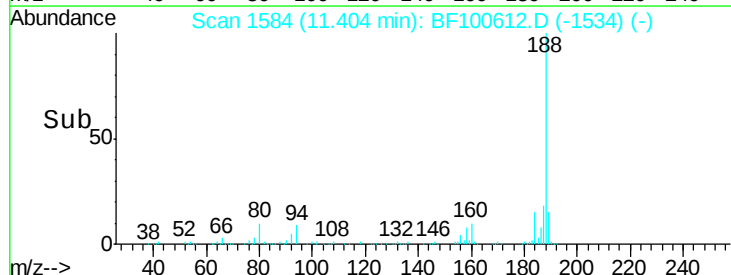
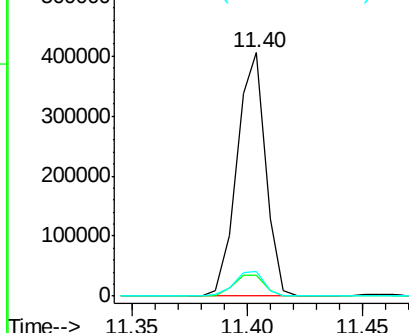


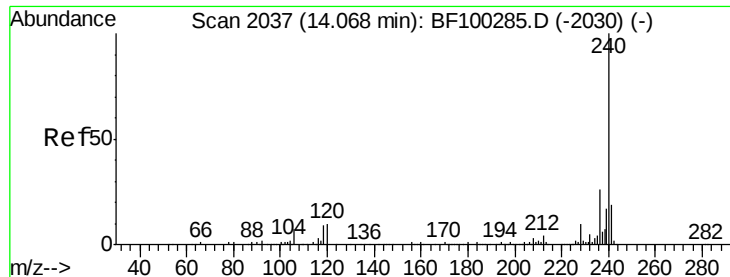

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.04 min Scan# 2032
Delta R.T. -0.01 min
Lab File: BF100612.D
Acq: 16 Nov 2017 3:00




Instrument :
BNA_F
ClientSampleId :
110917-JETT-F-D-S


Tgt Ion:240 Resp: 222003
Ion Ratio Lower Upper
240 100
120 10.1 9.5 14.3
236 25.5 20.7 31.1

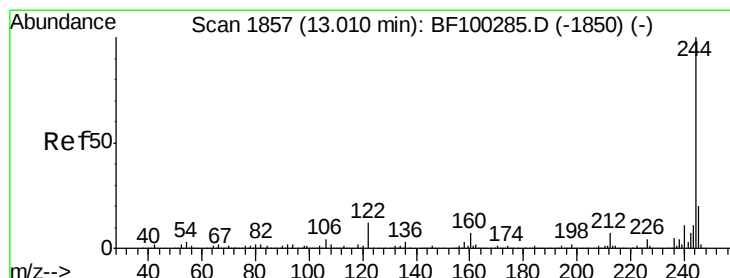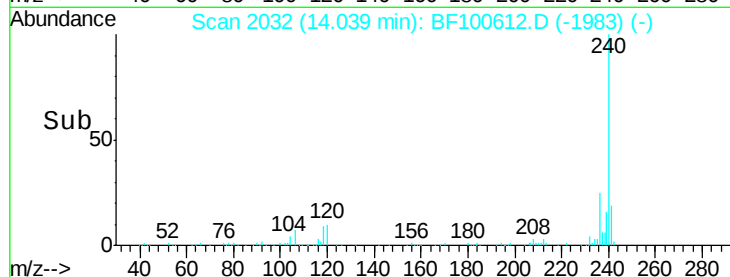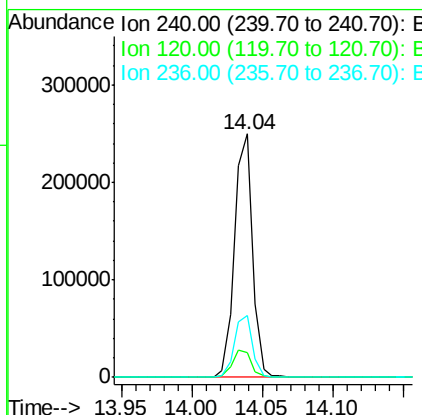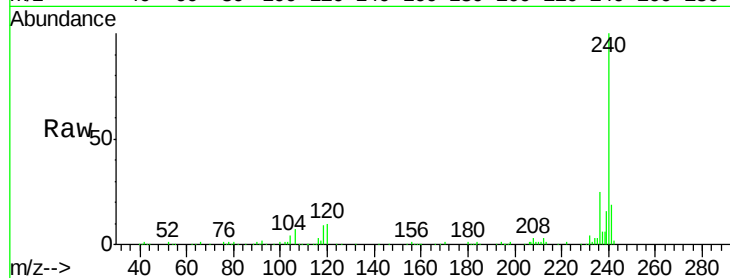

#78
Terphenyl-d14
Concen: 88.562 ng
RT: 12.99 min Scan# 1853
Delta R.T. -0.01 min
Lab File: BF100612.D
Acq: 16 Nov 2017 3:00

Tgt Ion:244 Resp: 855681
Ion Ratio Lower Upper
244 100
212 7.1 5.4 8.0
122 11.4 11.0 16.4

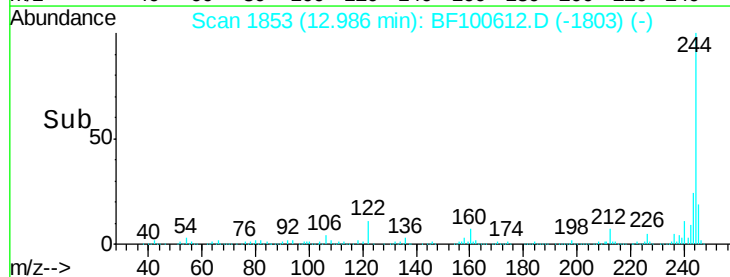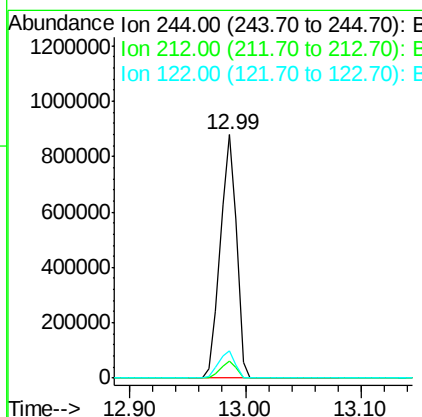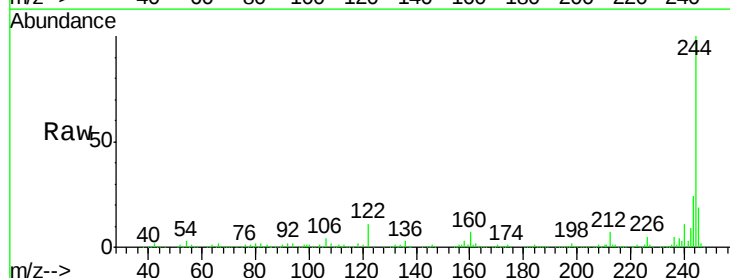


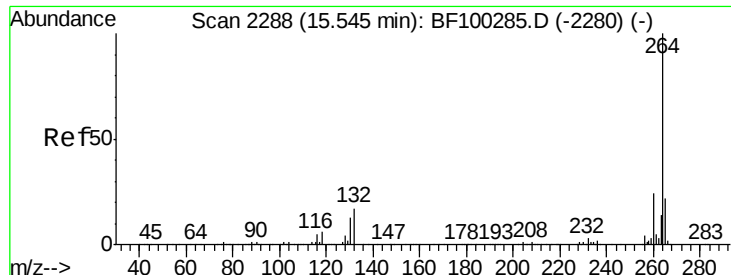

#86
Perylene-d12
Concen: 20.000 ng
RT: 15.51 min Scan# 2282
Delta R.T. -0.01 min
Lab File: BF100612.D
Acq: 16 Nov 2017 3:00

Instrument :
BNA_F
ClientSampleId :
110917-JETT-F-D-S

Tgt Ion	Ratio	Lower	Upper
264	100		
260	22.5	19.2	28.8
265	21.6	17.5	26.3

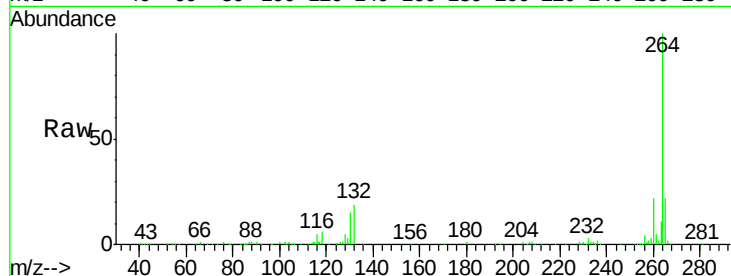

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

