


Data Path : Z:\HPCHEM1\BNA_F\Data\BF111517\
 Data File : BF100577.D
 Acq On : 15 Nov 2017 9:16
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 15 13:27:38 2017

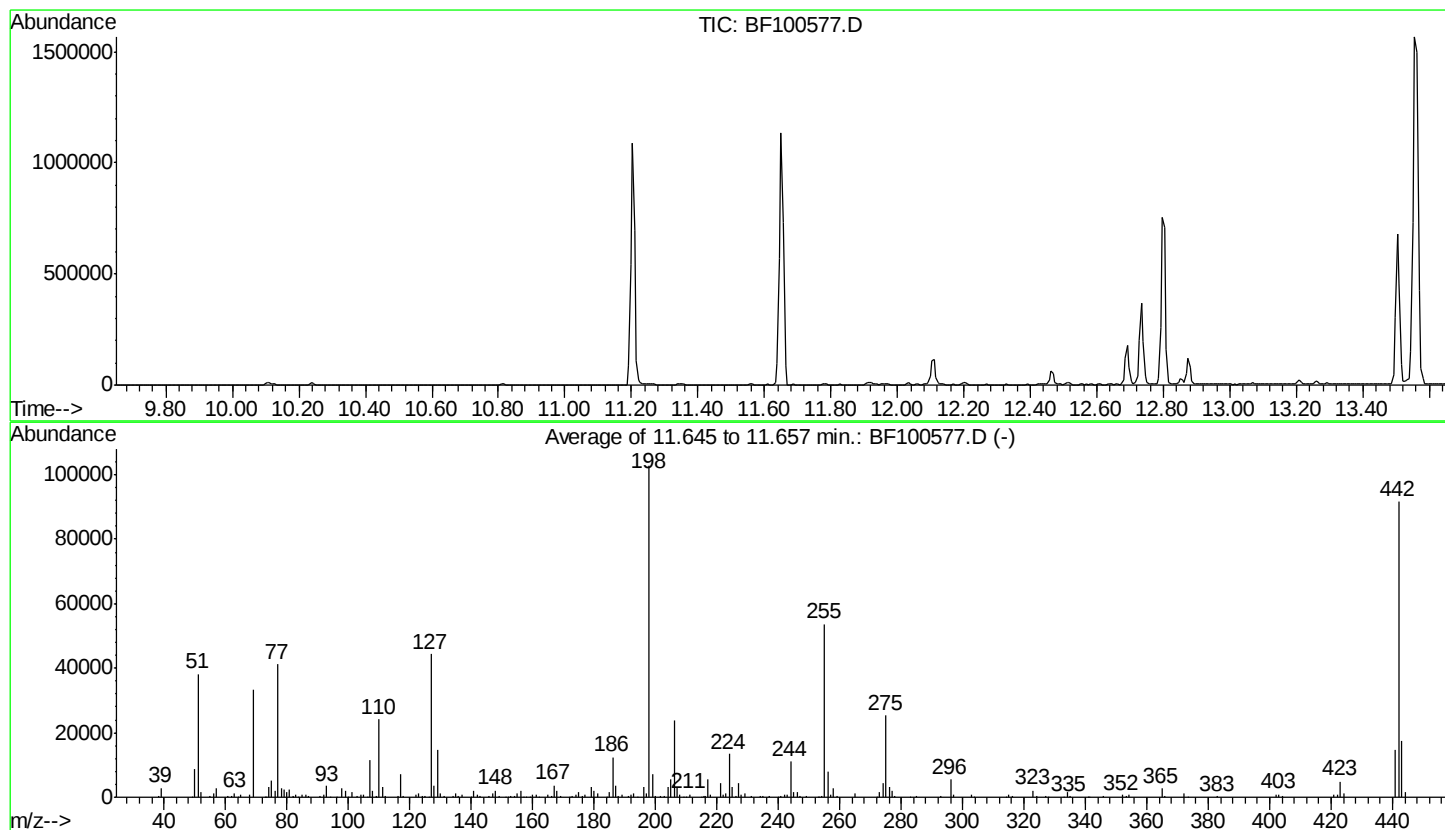

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	38152	PASS
68	69	0.00	2	2.0	676	PASS
69	198	0.00	100	32.3	33216	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	43.2	44373	PASS
197	198	0.00	2	1.1	1095	PASS
198	198	100	100	100.0	102813	PASS
199	198	5	9	6.8	7001	PASS
275	198	10	60	24.5	25234	PASS
365	198	1	100	2.7	2729	PASS
441	443	0.01	100	83.8	14716	PASS
442	198	50	100	89.1	91578	PASS
443	442	15	24	19.2	17558	PASS