


Data Path : Z:\HPCHEM1\BNA_F\Data\BF111517\
 Data File : BF100601.D
 Acq On : 15 Nov 2017 21:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 15 13:27:38 2017

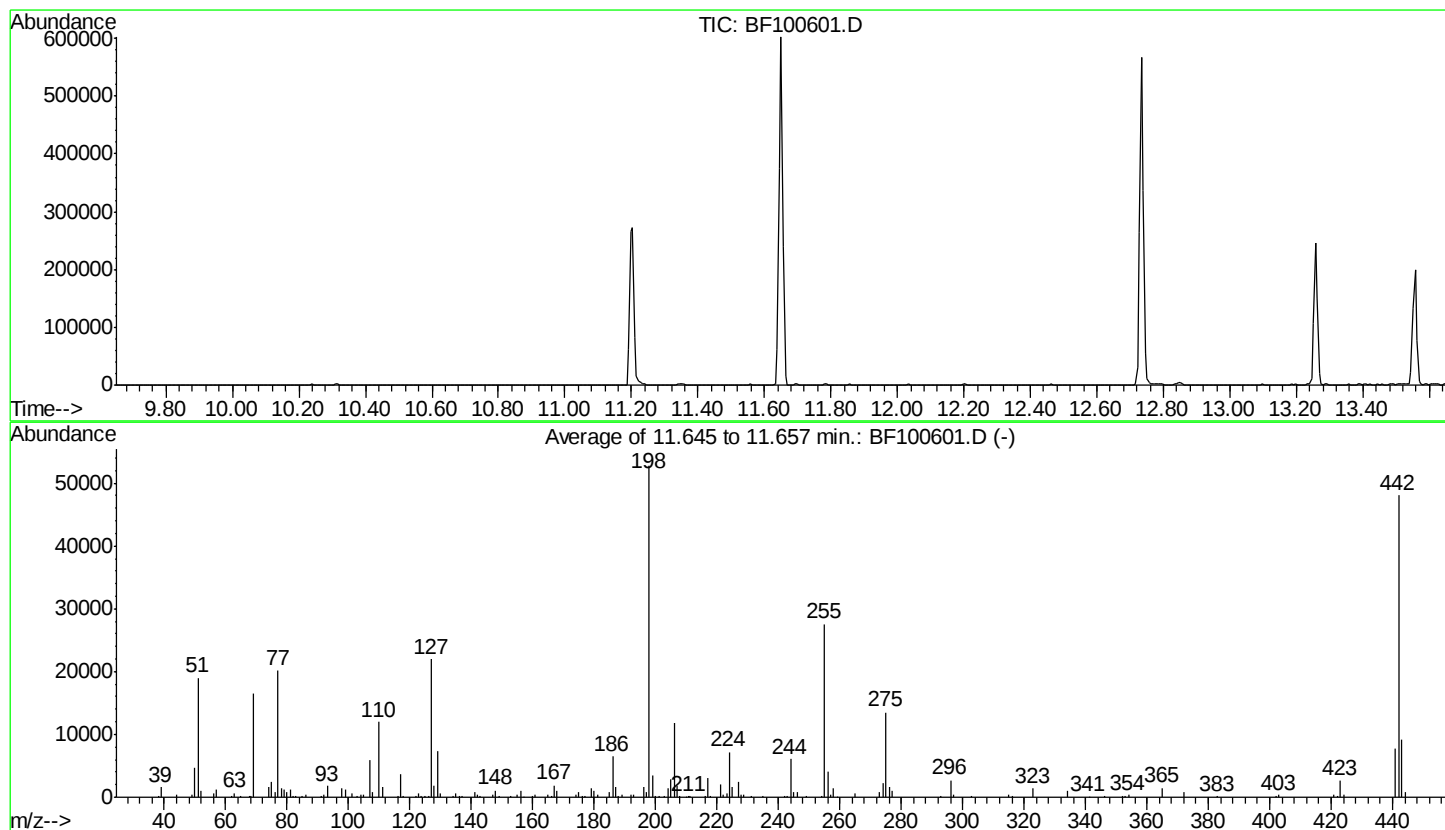

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.9	18952	PASS
68	69	0.00	2	1.4	235	PASS
69	198	0.00	100	31.2	16453	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.6	21933	PASS
197	198	0.00	2	1.5	778	PASS
198	198	100	100	100.0	52778	PASS
199	198	5	9	6.6	3502	PASS
275	198	10	60	25.7	13549	PASS
365	198	1	100	2.9	1521	PASS
441	443	0.01	100	84.3	7811	PASS
442	198	50	100	91.1	48066	PASS
443	442	15	24	19.3	9271	PASS