
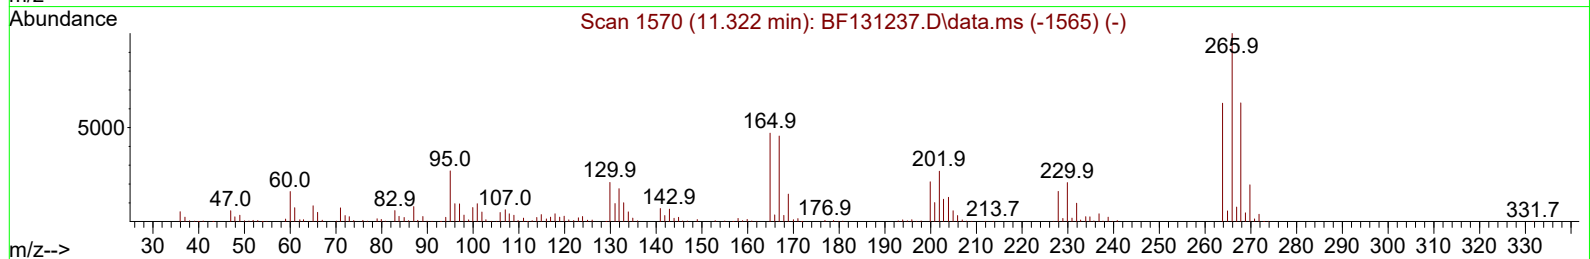
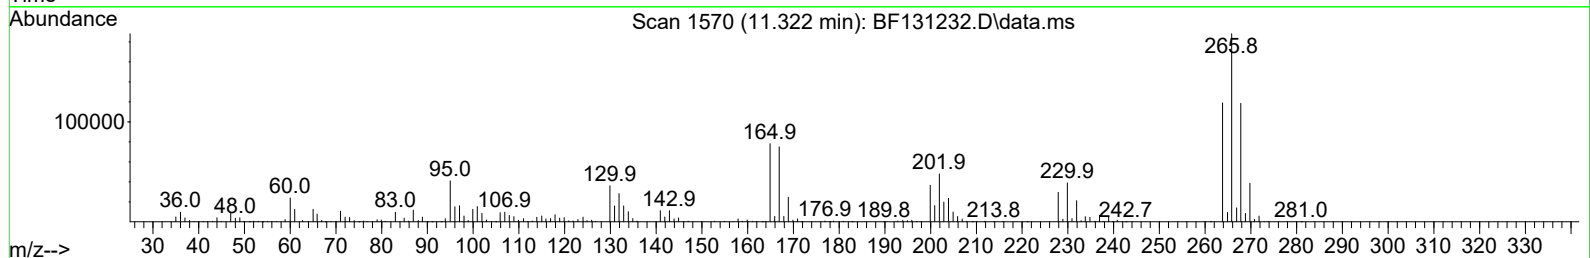


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111522\
Data File : BF131232.D
Acq On : 15 Nov 2022 15:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 04:36:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 01:15:55 2022
Response via : Initial Calibration

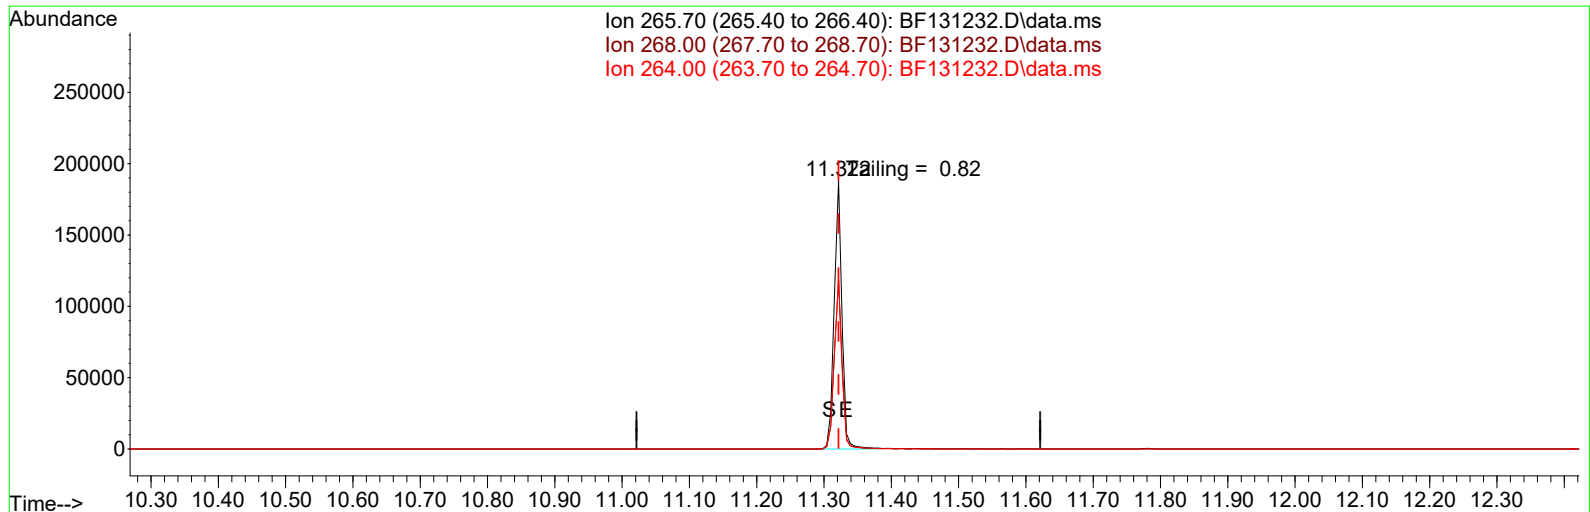

TIC: BF131232.D\data.ms

(70) Pentachlorophenol (C)




11.322min (+ 0.000) 25911.58 ng

response 152994

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.99
264.00	63.00	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111522\
 Data File : BF131232.D
 Acq On : 15 Nov 2022 15:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 04:36:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 01:15:55 2022
 Response via : Initial Calibration

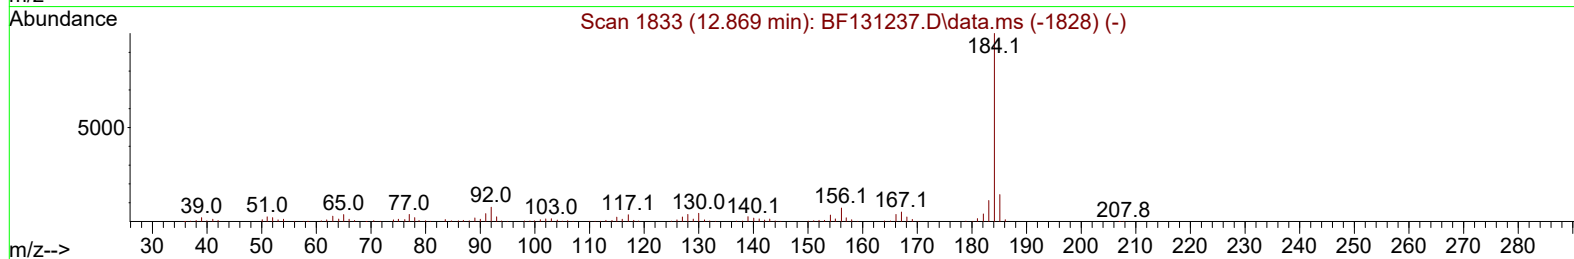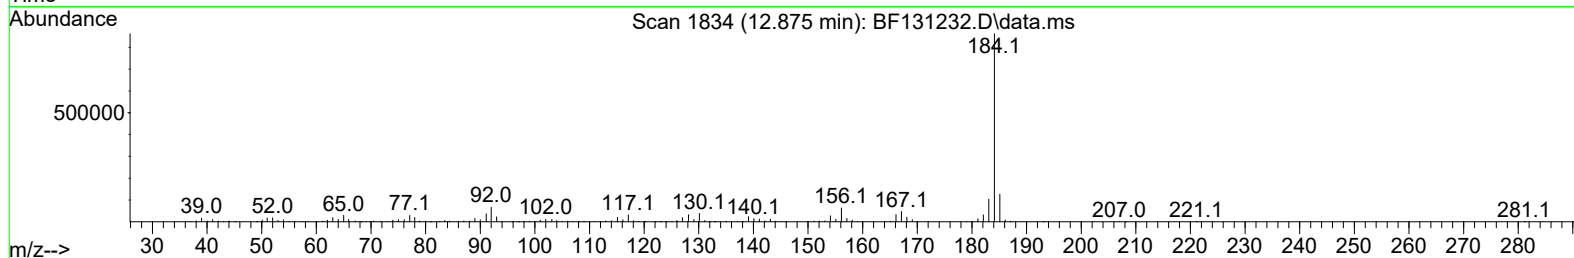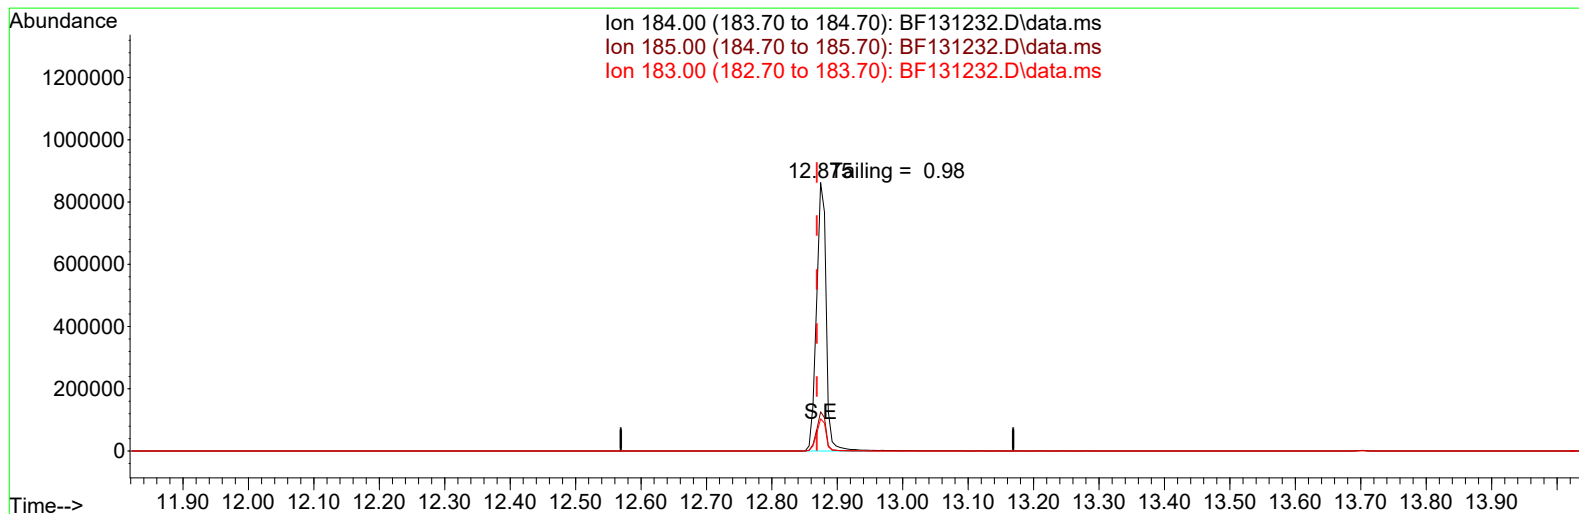

TIC: BF131232.D\data.ms

(77) Benzidine

12.875min (+ 0.006) 0.00 ng

response 890422

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.65
183.00	11.20	12.00
0.00	0.00	0.00