


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111522\
 Data File : BF131232.D
 Acq On : 15 Nov 2022 15:07
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 16 06:35:36 2022

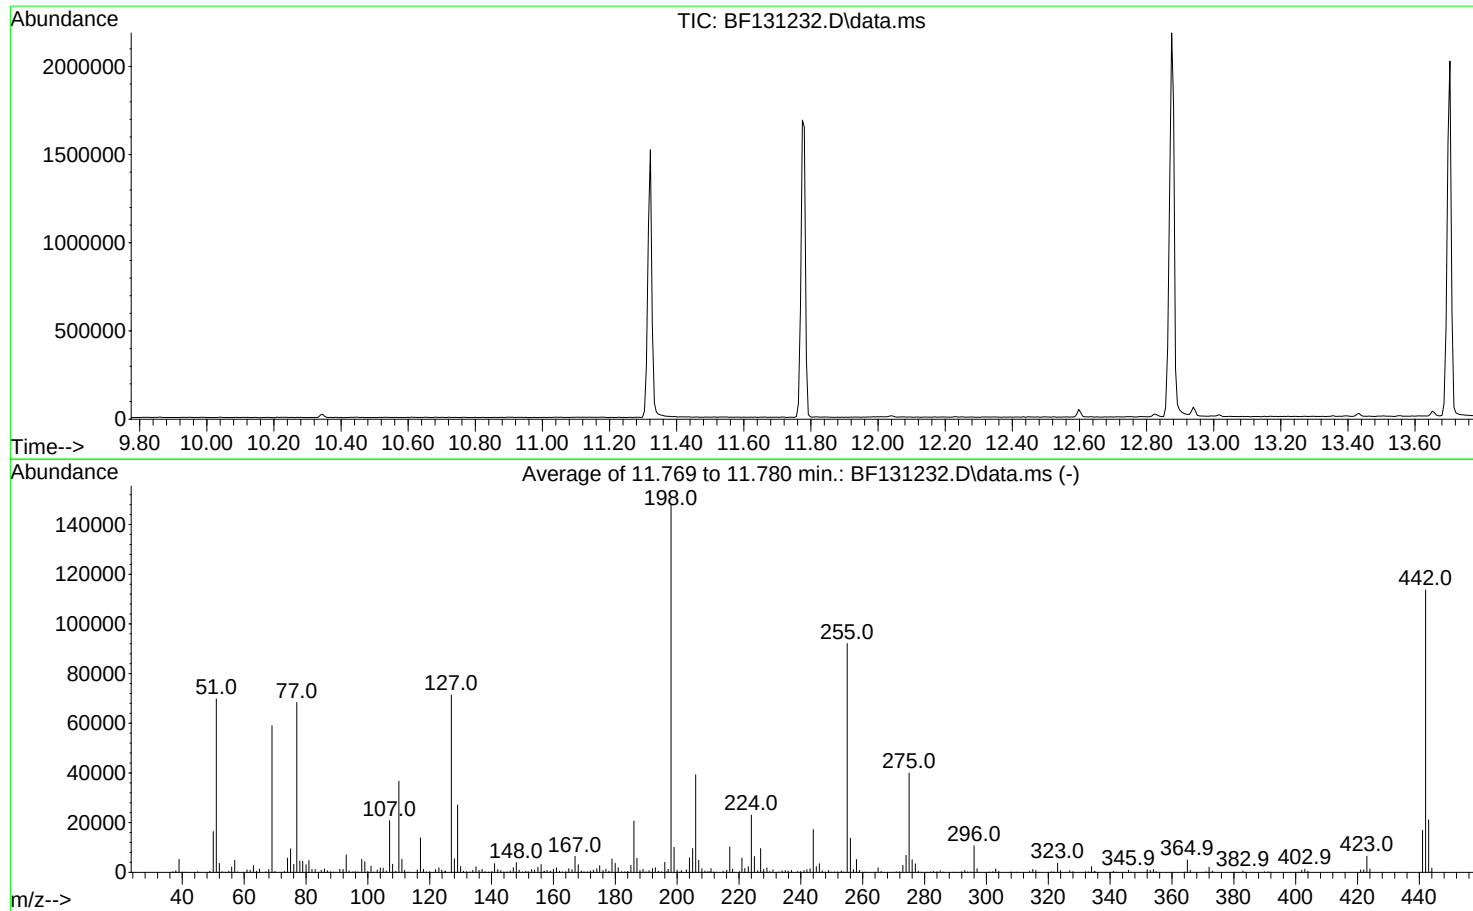




AutoFind: Scans 1646, 1647, 1648; Background Corrected with Scan 1641

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	69792	PASS
68	69	0.00	2	2.0	1163	PASS
69	198	0.00	100	39.8	58979	PASS
70	69	0.00	2	0.7	391	PASS
127	198	10	80	48.2	71347	PASS
197	198	0.00	2	0.8	1222	PASS
198	198	100	100	100.0	148107	PASS
199	198	5	9	6.8	10062	PASS
275	198	10	60	27.0	39956	PASS
365	198	1	100	3.4	5000	PASS
441	198	0.01	100	11.4	16859	PASS
442	442	50	100	100.0	113675	PASS
443	442	15	24	18.6	21093	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111522\
Data File : BF131232.D
Acq On : 15 Nov 2022 15:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 16 04:36:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 01:15:55 2022
Response via : Initial Calibration

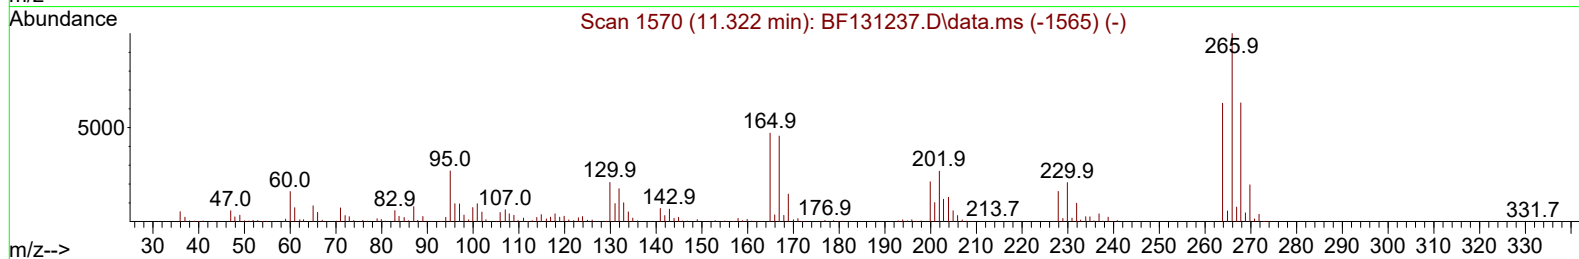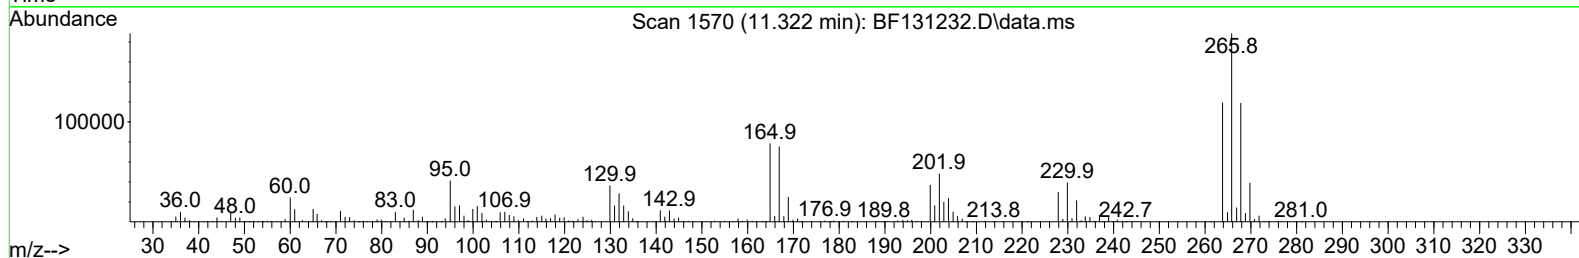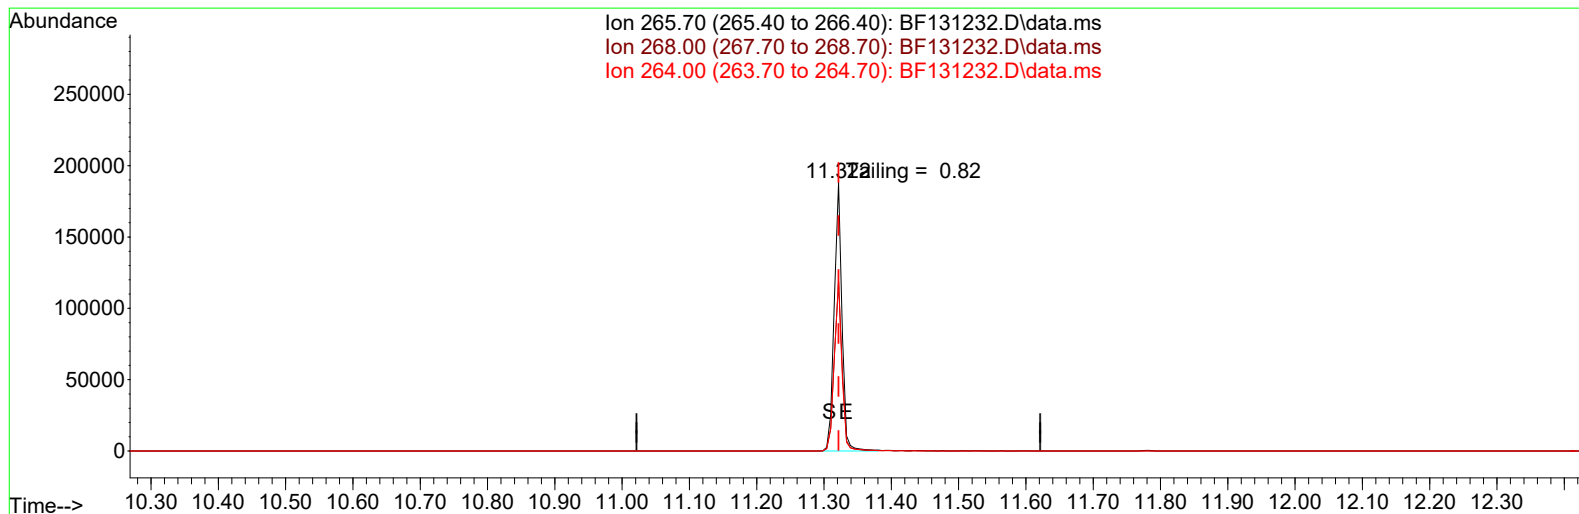

TIC: BF131232.D\data.ms

(70) Pentachlorophenol (C)

11.322min (+ 0.000) 25911.58 ng




response 152994

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.99
264.00	63.00	63.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111522\
Data File : BF131232.D
Acq On : 15 Nov 2022 15:07
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 16 04:36:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 01:15:55 2022
Response via : Initial Calibration

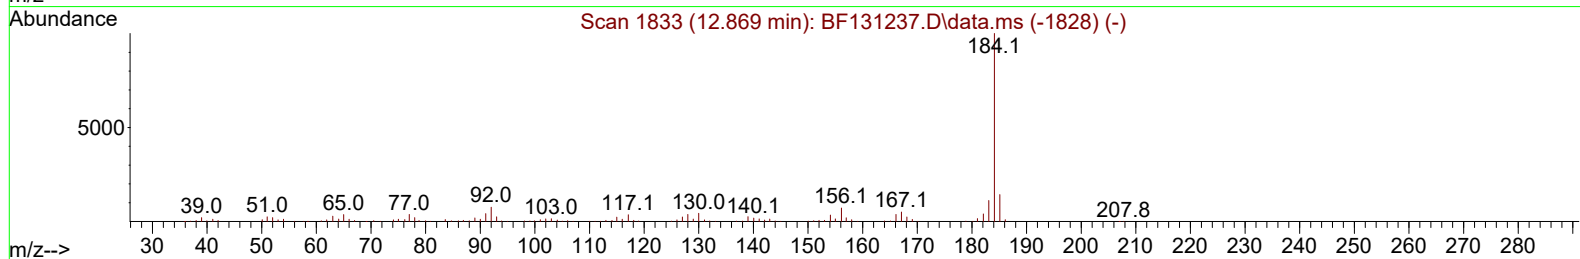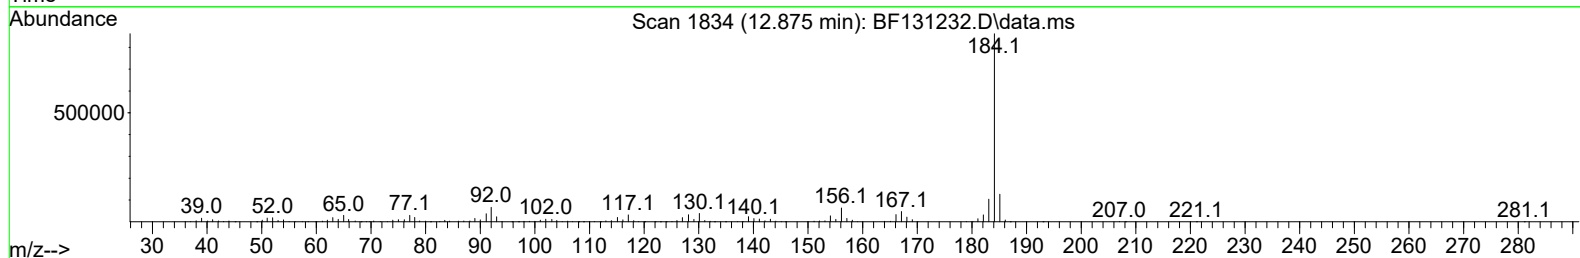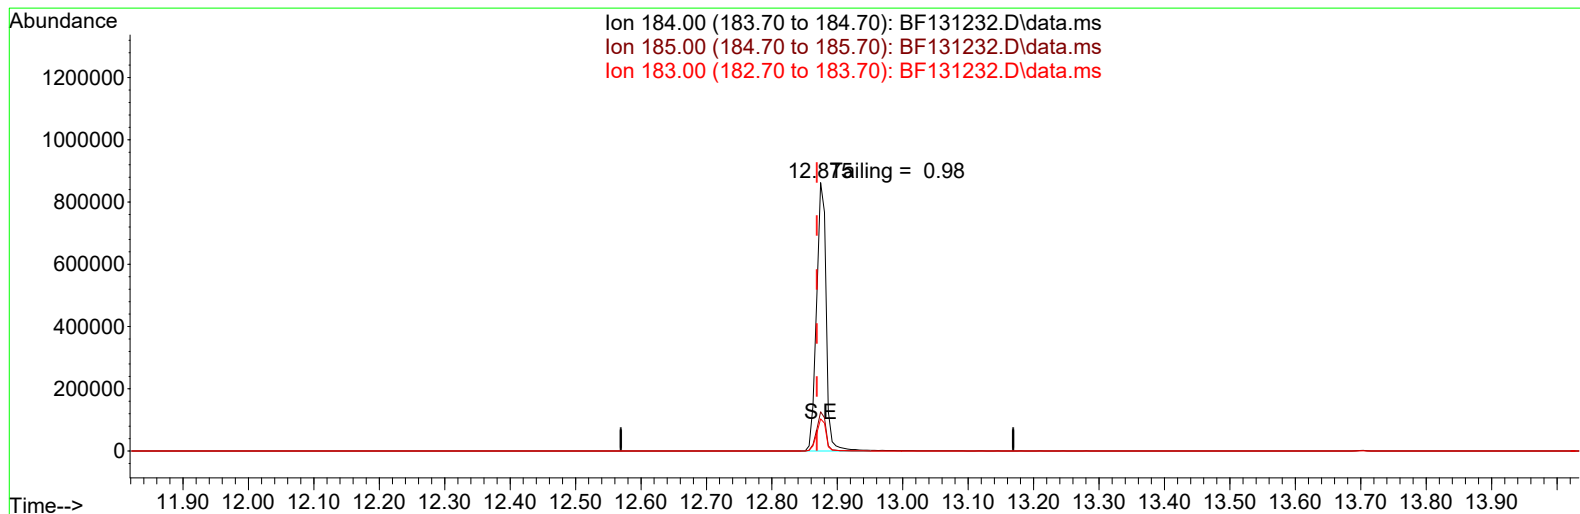

TIC: BF131232.D\data.ms

(77) Benzidine

12.875min (+ 0.006) 0.00 ng

response 890422

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.65
183.00	11.20	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/15/2022	BNA_F	<u>BF131232.D</u>
Compound Name	Response	Retention Time
DDT	294639	13.704
DDD	3324	13.433
DDE	0	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3324	297963	1.12

Instrument :
BNA_F
ClientSampleId :
DFTPP