

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111615\
 Data File : BF082948.D
 Acq On : 16 Nov 2015 19:59
 Operator : UM/IZ
 Sample : G4429-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 111315-A263-F-D-S

Quant Time: Nov 17 07:34:10 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Nov 07 02:32:49 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.78	152	223780	20.00	ng	-0.07
21) Naphthalene-d8	8.06	136	820615	20.00	ng	-0.08
38) Acenaphthene-d10	9.82	164	469593	20.00	ng	-0.07
63) Phenanthrene-d10	11.30	188	826583	20.00	ng	-0.08
75) Chrysene-d12	13.94	240	872118	20.00	ng	-0.08
86) Perylene-d12	15.35	264	692811	20.00	ng	-0.11
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	493836	34.34	ng	-0.06
7) Phenol-d6	6.43	99	484349	25.33	ng	-0.05
23) Nitrobenzene-d5	7.34	82	1373072	72.81	ng	-0.07
41) 2,4,6-Tribromophenol	10.61	330	348375	64.70	ng	-0.07
44) 2-Fluorobiphenyl	9.15	172	1987483	60.66	ng	-0.07
78) Terphenyl-d14	12.90	244	2355557	64.06	ng	-0.07


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111615\
Data File : BF082948.D
Acq On : 16 Nov 2015 19:59
Operator : UM/IZ
Sample : G4429-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
111315-A263-F-D-S

Quant Time: Nov 17 07:34:10 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Nov 07 02:32:49 2015
Response via : Initial Calibration

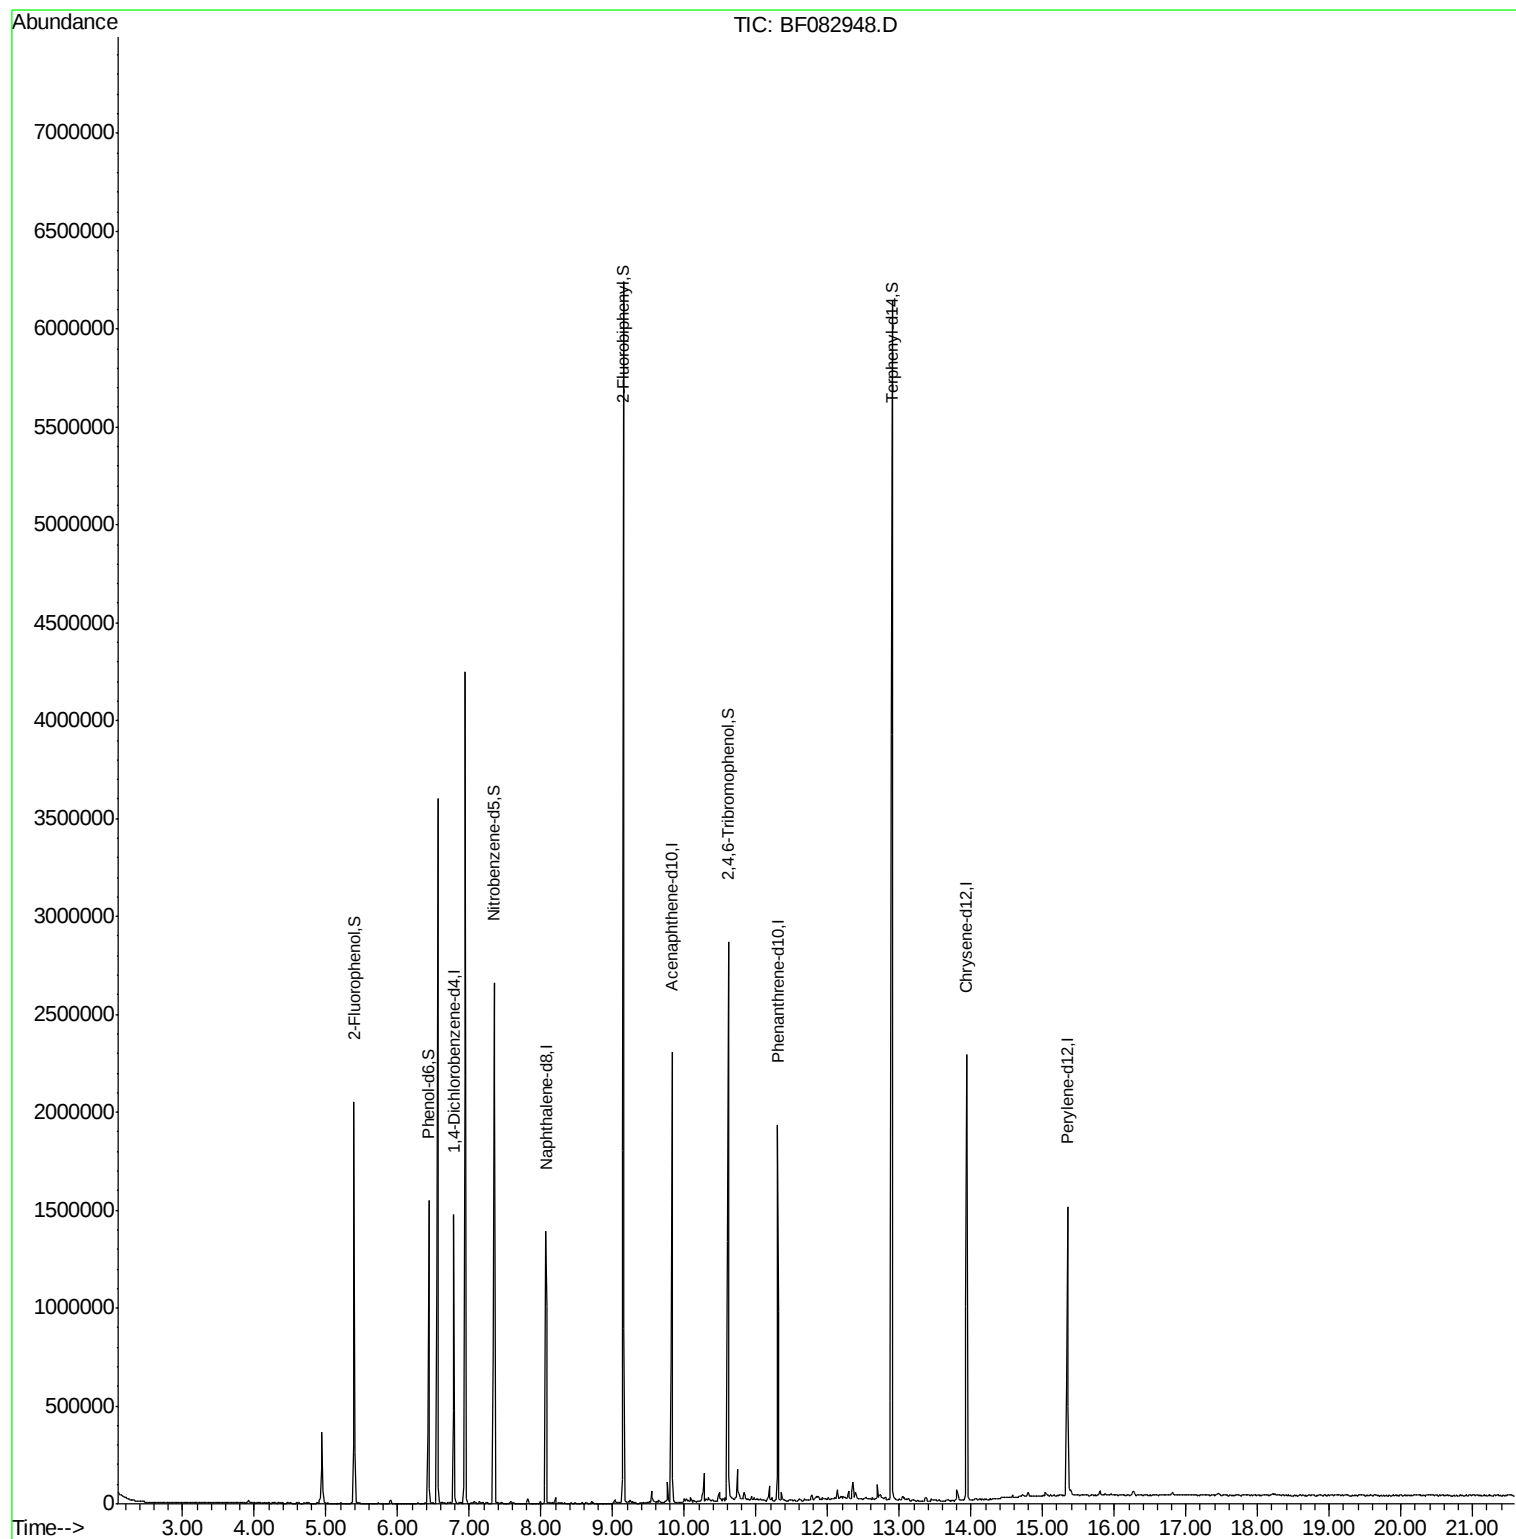




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.78 min Scan# 411
Delta R.T. -0.07 min
Lab File: BF082948.D
Acq: 16 Nov 2015 19:59

Instrument :
BNA_F
ClientSampleId :
111315-A263-F-D-S

Tot Ion:152 Resp: 223780
Ion Ratio Lower Upper
152 100
150 154.5 127.0 190.4
115 59.7 47.0 70.6

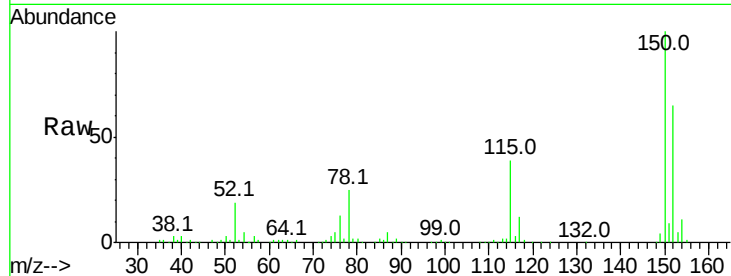


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

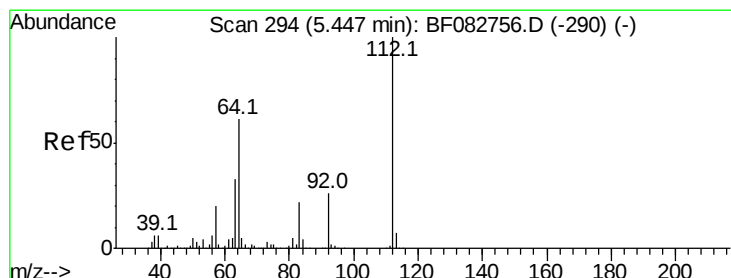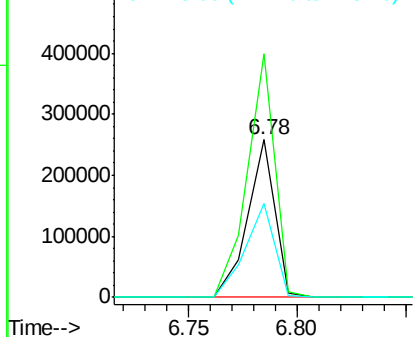



#5


2-Fluorophenol
Concen: 34.34 ng
RT: 5.39 min Scan# 289
Delta R.T. -0.06 min
Lab File: BF082948.D
Acq: 16 Nov 2015 19:59

Tgt Ion:112 Resp: 493836
Ion Ratio Lower Upper
112 100
64 66.8 48.9 73.3
63 33.4 28.1 42.1

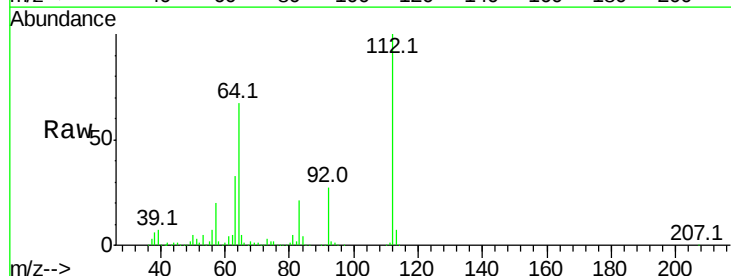

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

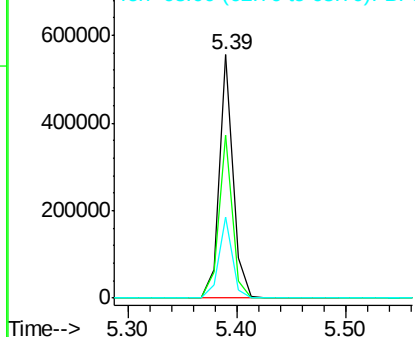

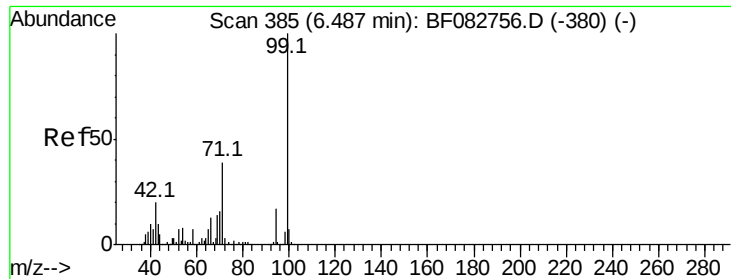

#7

Phenol-d6

Concen: 25.33 ng

RT: 6.43 min Scan# 380

Delta R.T. -0.05 min

Lab File: BF082948.D

Acq: 16 Nov 2015 19:59

Instrument :

BNA_F

ClientSampleId :

111315-A263-F-D-S





Tot Ion: 99 Resp: 484349

Ion Ratio Lower Upper

99 100

42 16.8 19.2 28.8#

71 34.2 35.0 52.4#

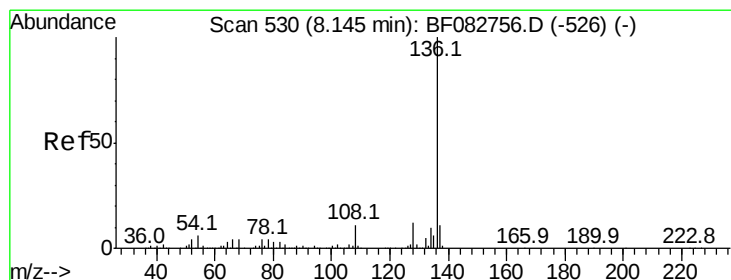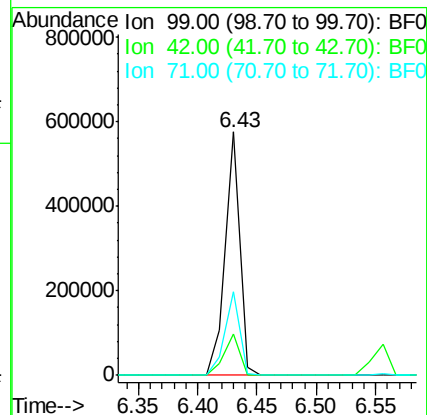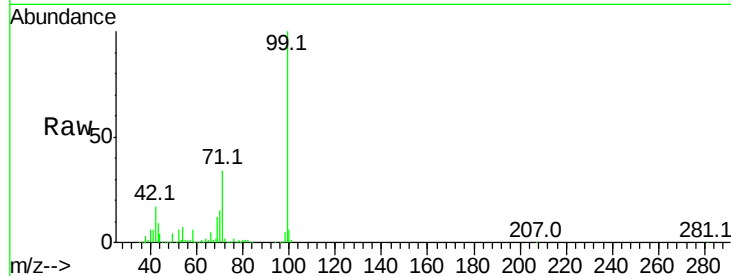

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.06 min Scan# 523

Delta R.T. -0.08 min

Lab File: BF082948.D

Acq: 16 Nov 2015 19:59

Tgt Ion: 136 Resp: 820615




Ion Ratio Lower Upper


136 100

137 11.6 9.1 13.7

54 11.5 9.1 13.7

68 7.5 4.8 7.2#

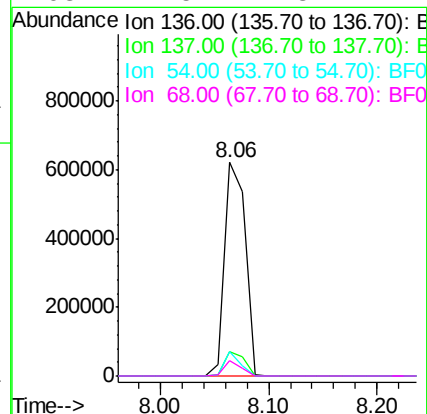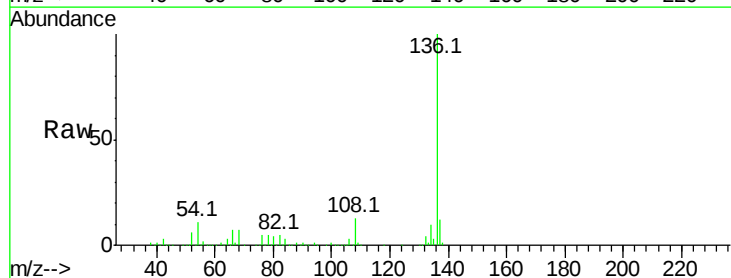

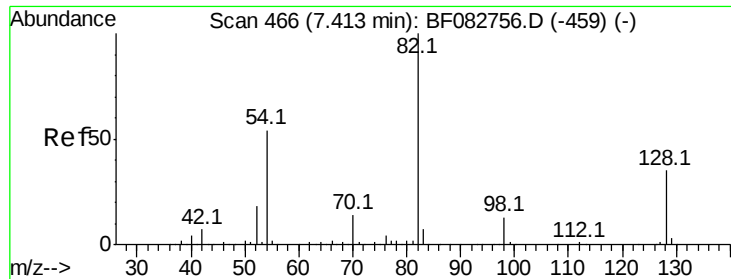


#23
 Nitrobenzene-d5
 Concen: 72.81 ng
 RT: 7.34 min Scan# 460
 Delta R.T. -0.07 min
 Lab File: BF082948.D
 Acq: 16 Nov 2015 19:59




Instrument :
 BNA_F
 ClientSampleId :
 111315-A263-F-D-S

Tot Ion: 82 Resp: 1373072

Ion	Ratio	Lower	Upper
82	100		
128	35.9	26.8	40.2
54	53.5	45.7	68.5

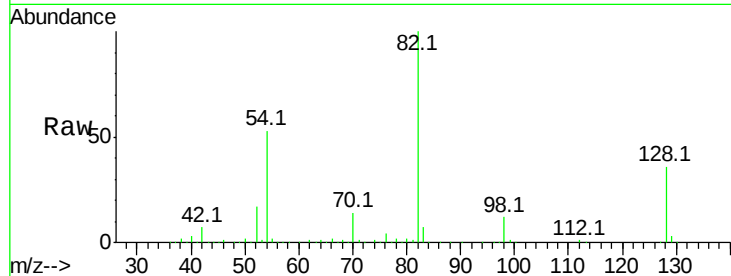


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

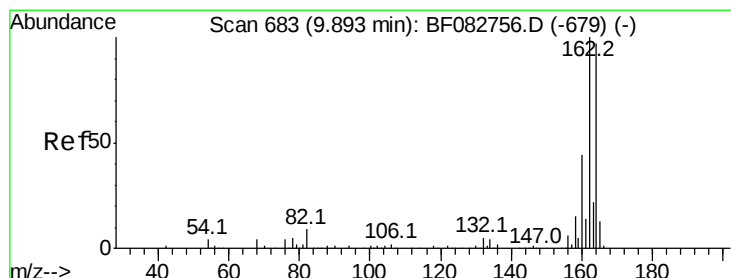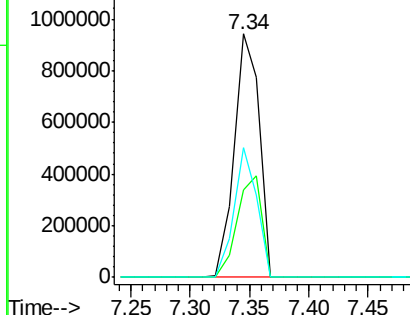



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.82 min Scan# 677
 Delta R.T. -0.07 min
 Lab File: BF082948.D
 Acq: 16 Nov 2015 19:59


Tgt Ion: 164 Resp: 469593

Ion	Ratio	Lower	Upper
164	100		
162	102.3	84.9	127.3
160	45.3	37.5	56.3

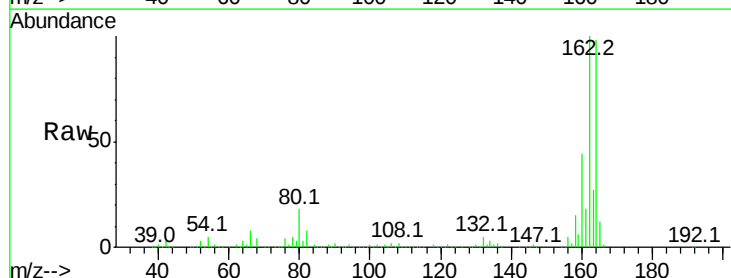

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

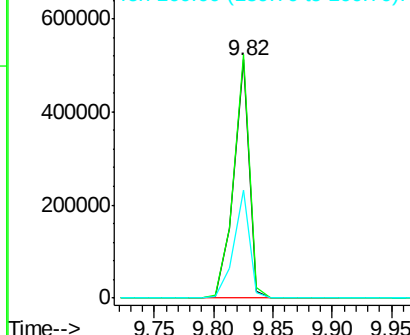







#41
 2,4,6-Tribromophenol
 Concen: 64.70 ng
 RT: 10.61 min Scan# 746
 Delta R.T. -0.07 min
 Lab File: BF082948.D
 Acq: 16 Nov 2015 19:59

Instrument :
 BNA_F
 ClientSampleId :
 111315-A263-F-D-S

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.6	76.6	114.8
141	40.0	41.2	61.8#

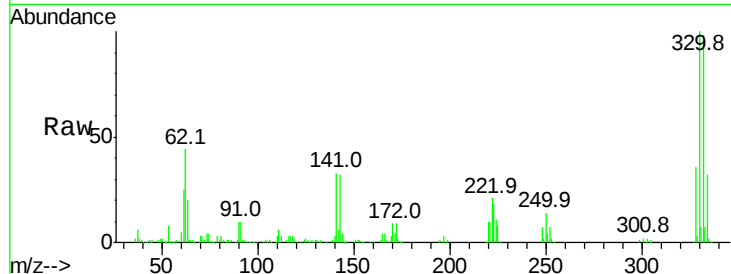


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

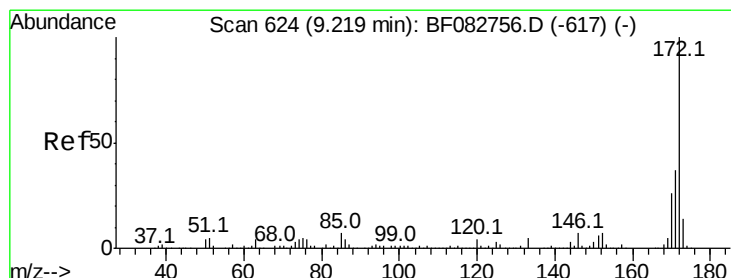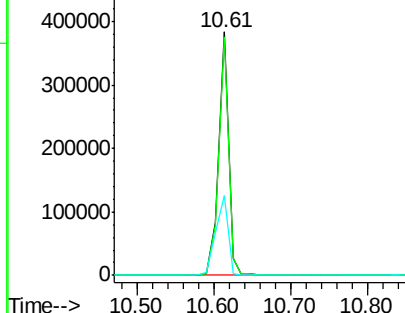




#44
 2-Fluorobiphenyl
 Concen: 60.66 ng
 RT: 9.15 min Scan# 618
 Delta R.T. -0.07 min
 Lab File: BF082948.D
 Acq: 16 Nov 2015 19:59

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.2	30.8	46.2
170	25.6	21.2	31.8

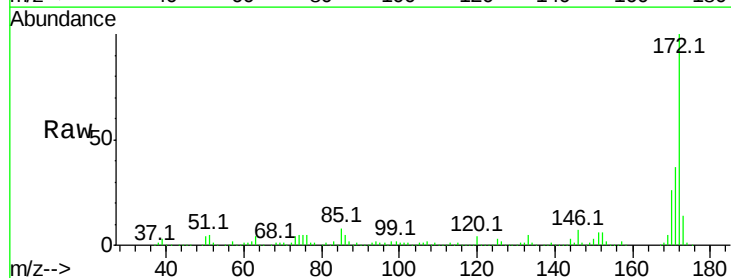

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



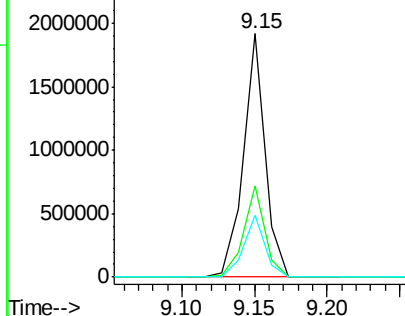



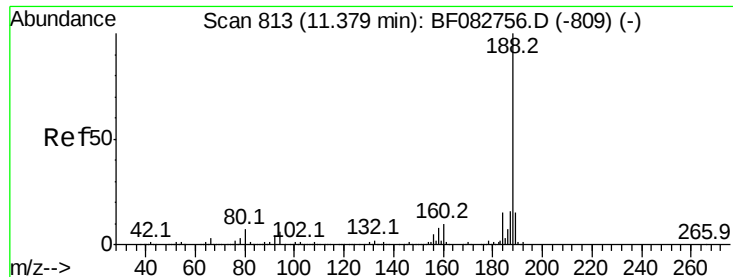

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.30 min Scan# 806
Delta R.T. -0.08 min
Lab File: BF082948.D
Acq: 16 Nov 2015 19:59




Instrument :
BNA_F
ClientSampleId :
111315-A263-F-D-S


Tot Ion:188 Resp: 826583
Ion Ratio Lower Upper
188 100
94 11.7 6.1 9.1#
80 13.3 7.0 10.6#

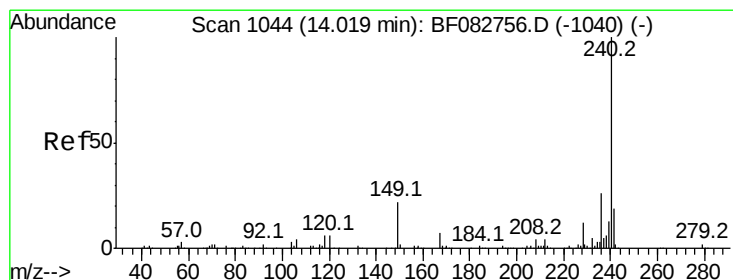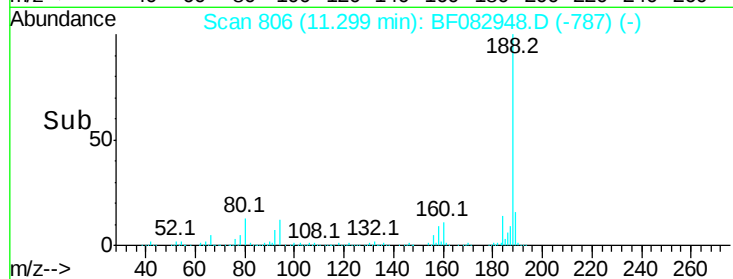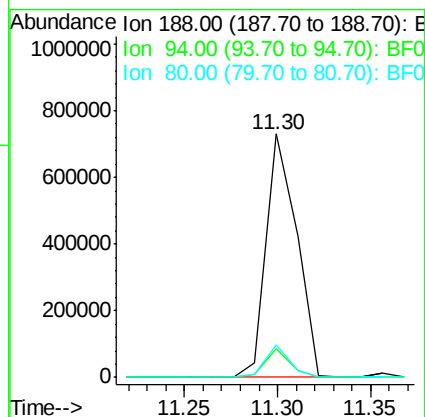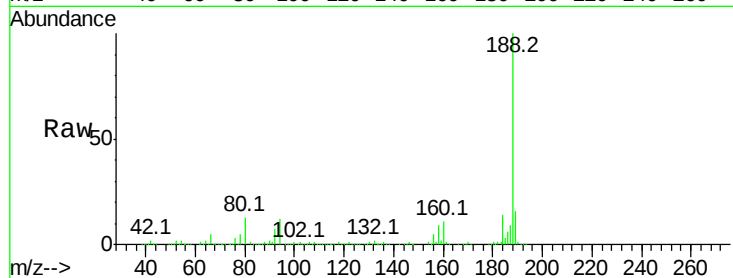

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.94 min Scan# 1037
Delta R.T. -0.08 min
Lab File: BF082948.D
Acq: 16 Nov 2015 19:59

Tgt Ion:240 Resp: 872118
Ion Ratio Lower Upper
240 100
120 7.3 10.9 16.3#
236 26.2 21.6 32.4

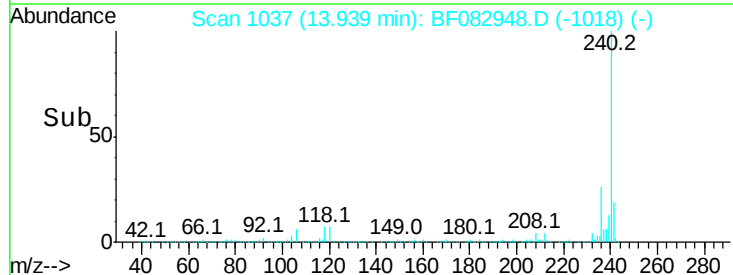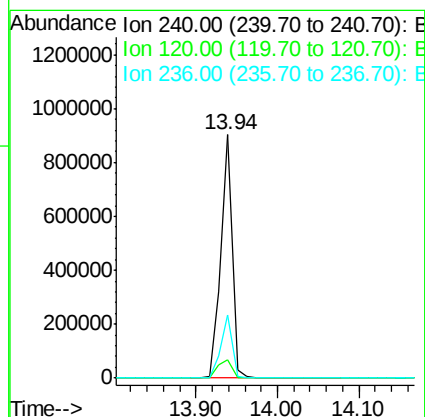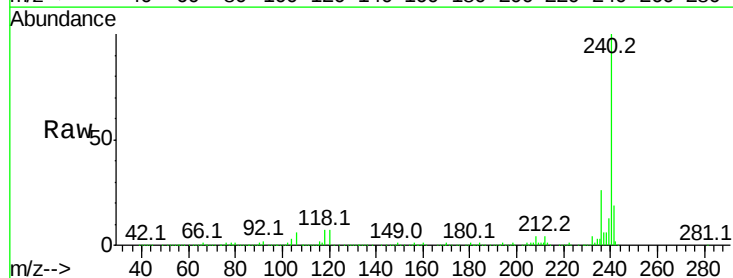



#78

Terphenyl-d14

Concen: 64.06 ng

RT: 12.90 min Scan# 946

Delta R.T. -0.07 min

Lab File: BF082948.D

Acq: 16 Nov 2015 19:59

Instrument :

BNA_F

ClientSampleId :

111315-A263-F-D-S


Tot Ion:244 Resp: 2355557

Ion Ratio Lower Upper

244 100

212 8.1 7.6 11.4




122 8.3 11.3 16.9#

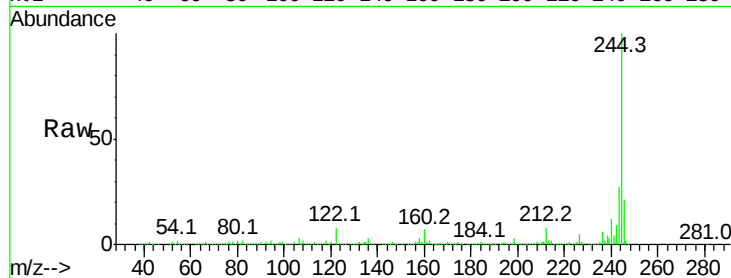

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

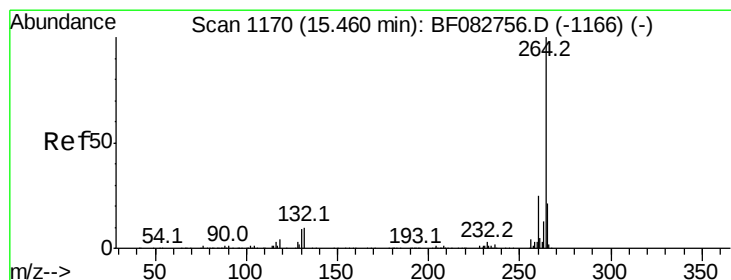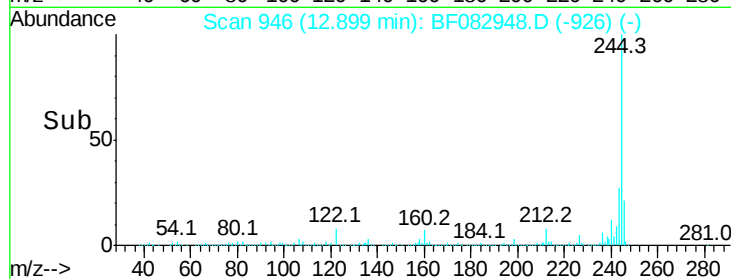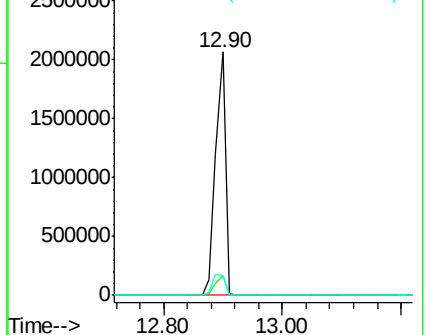

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.35 min Scan# 1160

Delta R.T. -0.11 min

Lab File: BF082948.D

Acq: 16 Nov 2015 19:59


Tgt Ion:264 Resp: 692811

Ion Ratio Lower Upper

264 100

260 24.6 19.8 29.6

265 21.8 17.4 26.0

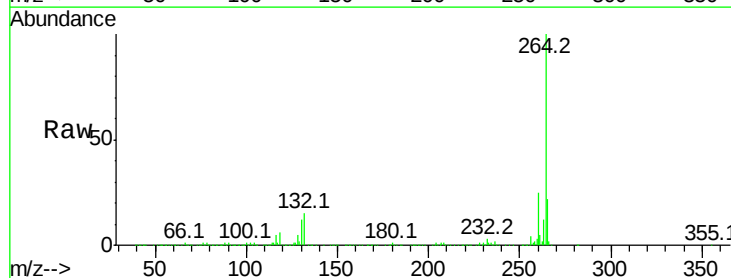

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

