


Data Path : Z:\HPCHEM1\BNA F\Data\BF111615\
 Data File : BF082940.D
 Acq On : 16 Nov 2015 13:22
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 18 13:32:32 2015

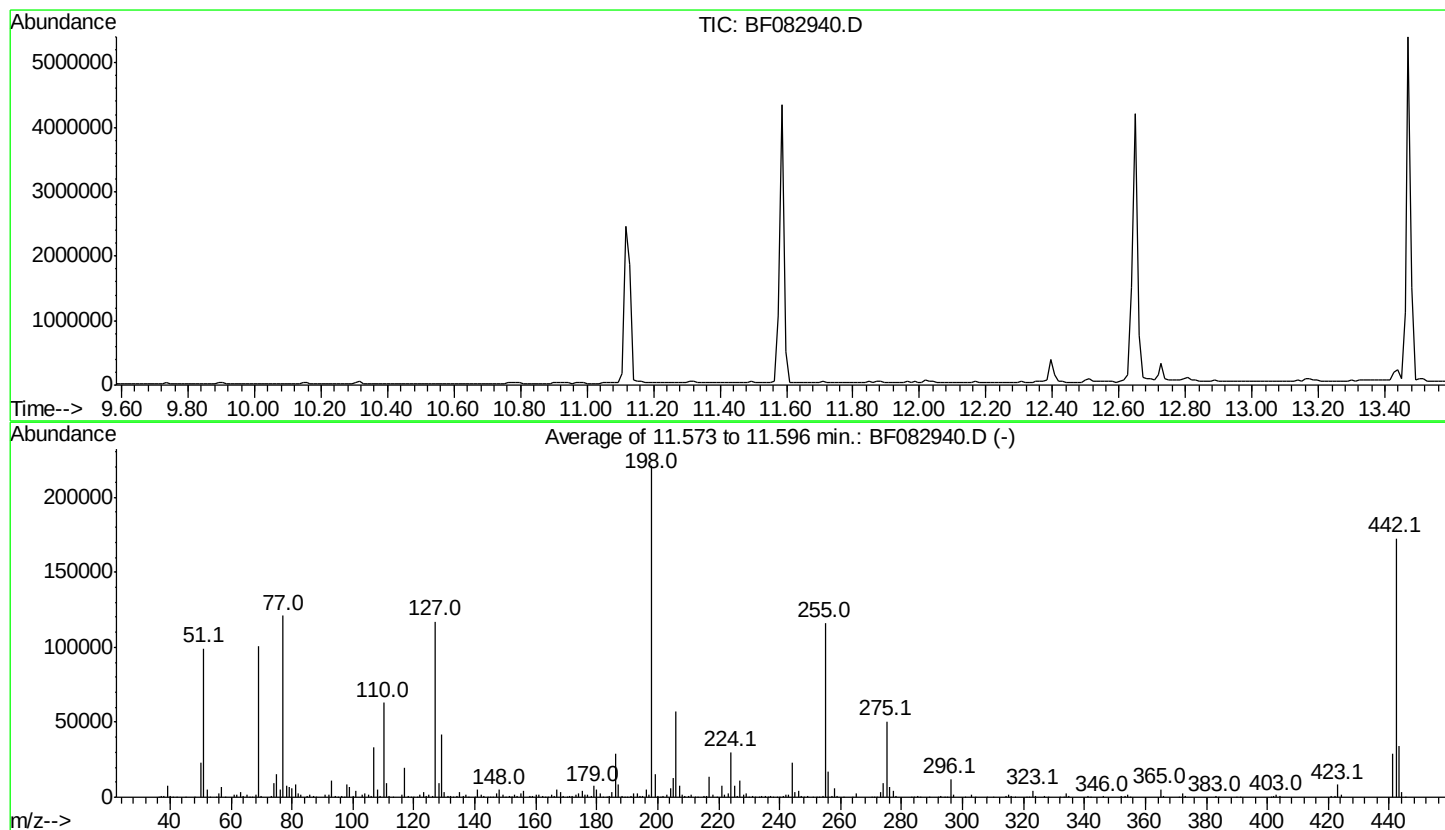

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	99395	PASS
68	69	0.00	2	1.7	1677	PASS
69	198	0.00	100	45.6	100781	PASS
70	69	0.00	2	0.6	576	PASS
127	198	10	80	52.9	116970	PASS
197	198	0.00	2	0.6	1385	PASS
198	198	100	100	100.0	221056	PASS
199	198	5	9	6.8	15124	PASS
275	198	10	60	22.8	50496	PASS
365	198	1	100	2.5	5421	PASS
441	442	0.01	24	16.6	28659	PASS
442	198	50	100	78.1	172728	PASS
443	442	15	24	19.8	34256	PASS