


Data Path : Z:\HPCHEM1\BNA F\DATA\BF111615\
 Data File : BF082958.D
 Acq On : 17 Nov 2015 00:50
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 18 13:32:32 2015

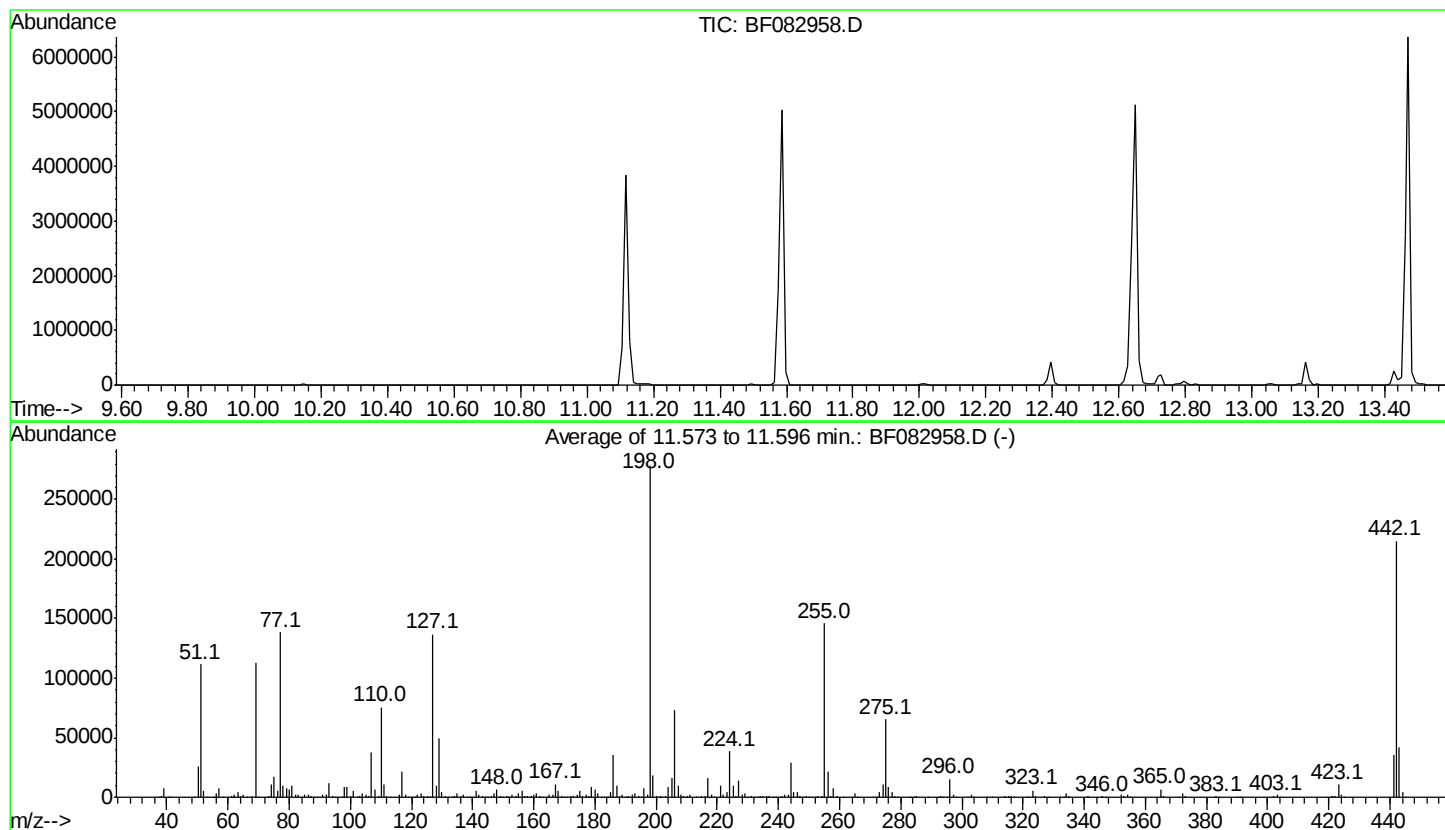

AutoFind: Scans 830, 831, 832; Background Corrected with Scan 826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	111319	PASS
68	69	0.00	2	1.4	1607	PASS
69	198	0.00	100	40.4	112554	PASS
70	69	0.00	2	0.4	475	PASS
127	198	10	80	49.1	136594	PASS
197	198	0.00	2	0.6	1690	PASS
198	198	100	100	100.0	278461	PASS
199	198	5	9	6.7	18726	PASS
275	198	10	60	23.5	65544	PASS
365	198	1	100	2.3	6483	PASS
441	442	0.01	24	16.4	35340	PASS
442	198	50	100	77.4	215496	PASS
443	442	15	24	19.6	42317	PASS