
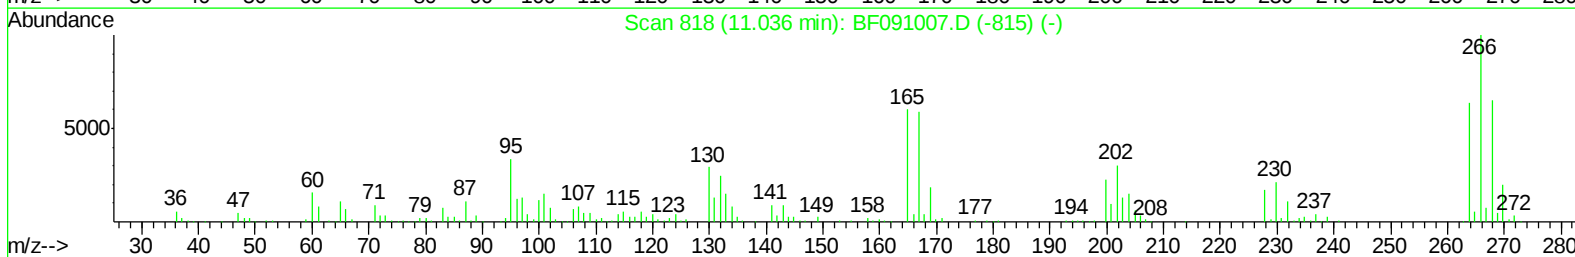
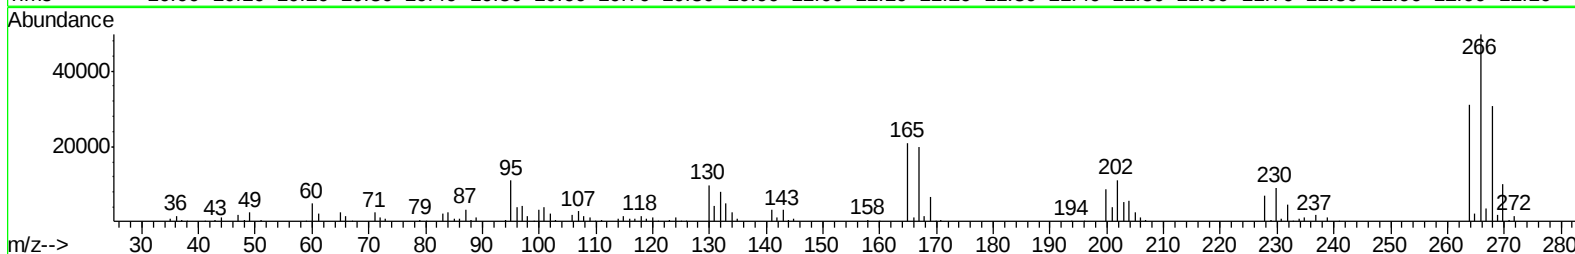


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111616\
Data File : BF091186.D
Acq On : 16 Nov 2016 13:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 07:47:13 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 00:05:11 2016
Response via : Initial Calibration

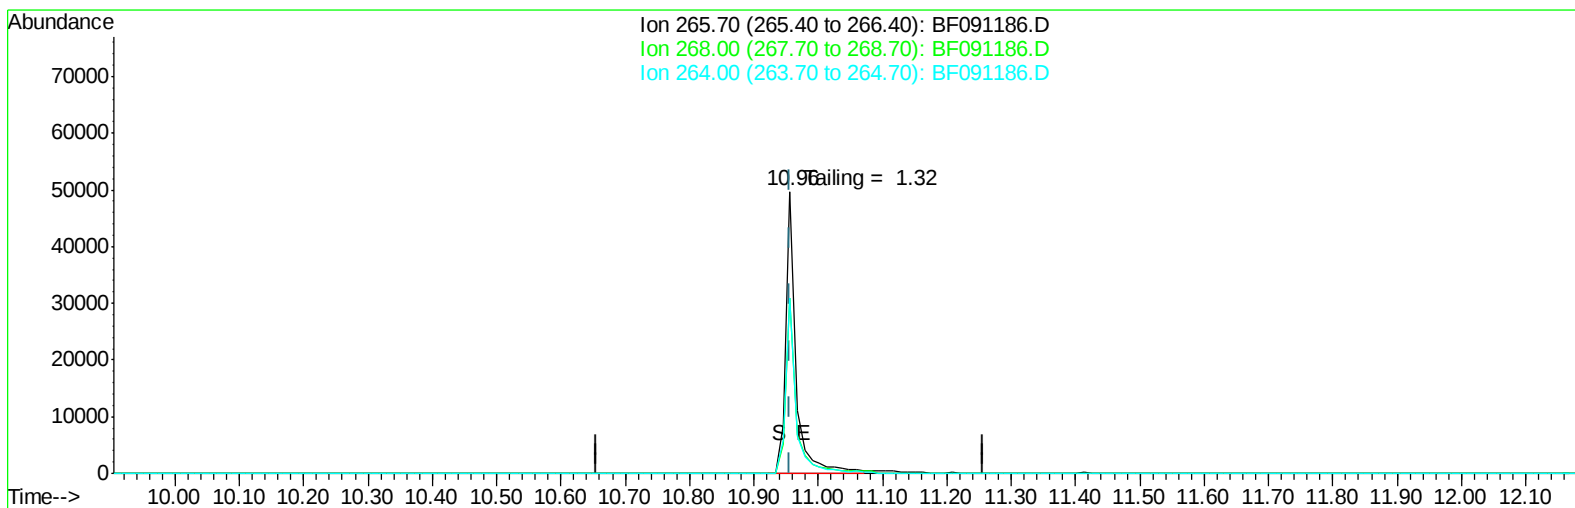

TIC: BF091186.D

(69) Pentachlorophenol (C)




10.956min (-0.000) 0.00ng

response 58996

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	62.19
264.00	63.90	62.48
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111616\
Data File : BF091186.D
Acq On : 16 Nov 2016 13:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 07:47:13 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 17 00:05:11 2016
Response via : Initial Calibration

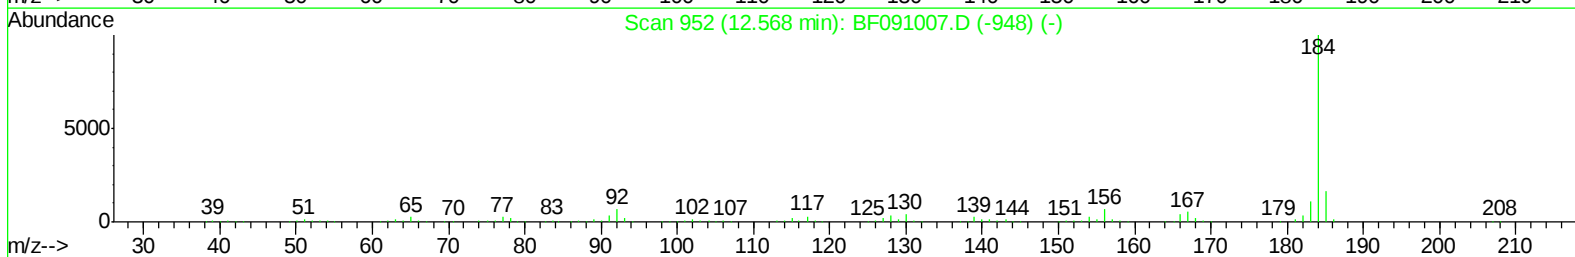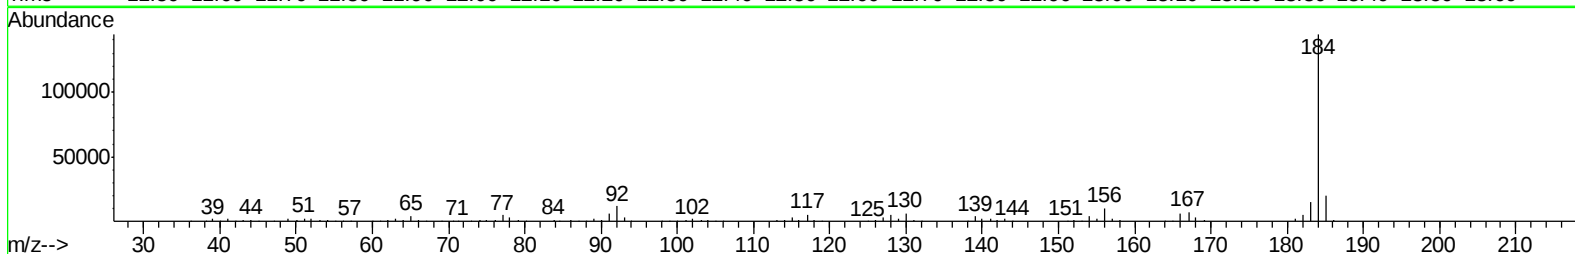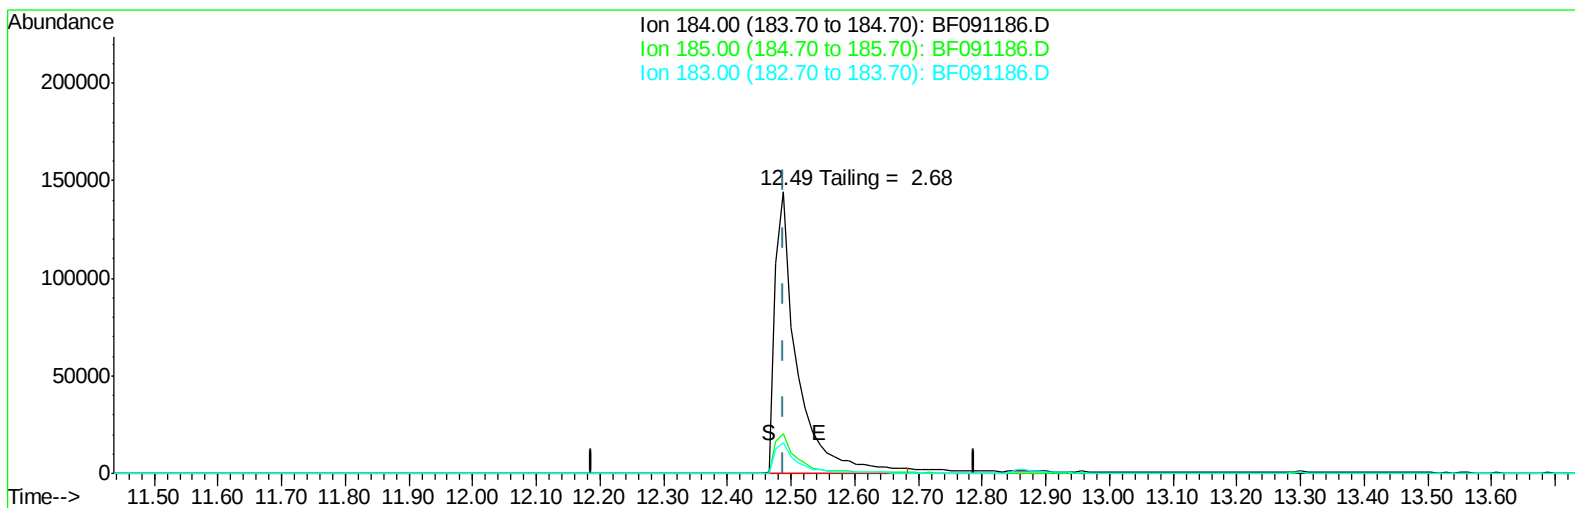

TIC: BF091186.D

(76) Benzidine

12.488min (-0.000) 0.00ng

response 353890

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	13.99
183.00	10.90	10.78
0.00	0.00	0.00