

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111616\
 Data File : BF091197.D
 Acq On : 16 Nov 2016 19:27
 Operator : UM/SJ
 Sample : H5636-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 C19043041

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.750	265	268	280	rBV	346736	641731	8.29%	1.348%
2	5.207	305	308	322	rBV	1534654	2641251	34.12%	5.547%
3	6.270	399	401	409	rBV	1695468	1717007	22.18%	3.606%
4	6.384	409	411	414	rBV	4084151	4373436	56.50%	9.184%
5	6.613	430	431	443	rBV2	872459	1205626	15.58%	2.532%
6	6.773	443	445	448	rBV	4481575	4532185	58.55%	9.518%
7	7.196	479	482	484	rBV	3503243	4049349	52.32%	8.504%
8	7.904	542	544	547	rBV	1578179	1616873	20.89%	3.395%
9	8.327	579	581	595	rVB	88669	180944	2.34%	0.380%
10	8.990	636	639	642	rBV	5784153	6786381	87.68%	14.251%
11	9.390	672	674	679	rVB	231163	214457	2.77%	0.450%
12	9.653	695	697	700	rBV	1603202	1961850	25.35%	4.120%
13	10.088	730	735	738	rBV4	90311	230644	2.98%	0.484%
14	10.453	764	767	769	rBV	3737563	4286978	55.39%	9.003%
15	10.579	776	778	785	rVB	101695	127422	1.65%	0.268%
16	11.025	815	817	818	rBV	106566	92724	1.20%	0.195%
17	11.139	825	827	829	rBV	2273877	1996787	25.80%	4.193%
18	11.448	852	854	857	rVB	96665	98934	1.28%	0.208%
19	12.728	963	966	969	rBV	4999416	7740145	100.00%	16.254%
20	13.642	1043	1046	1055	rBV	75669	122410	1.58%	0.257%
21	13.768	1055	1057	1060	rBV	1587068	1712054	22.12%	3.595%
22	15.139	1175	1177	1180	rBV	1116822	1289945	16.67%	2.709%


Sum of corrected areas: 47619133

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111616\
Data File : BF091197.D
Acq On : 16 Nov 2016 19:27
Operator : UM/SJ
Sample : H5636-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C19043041

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

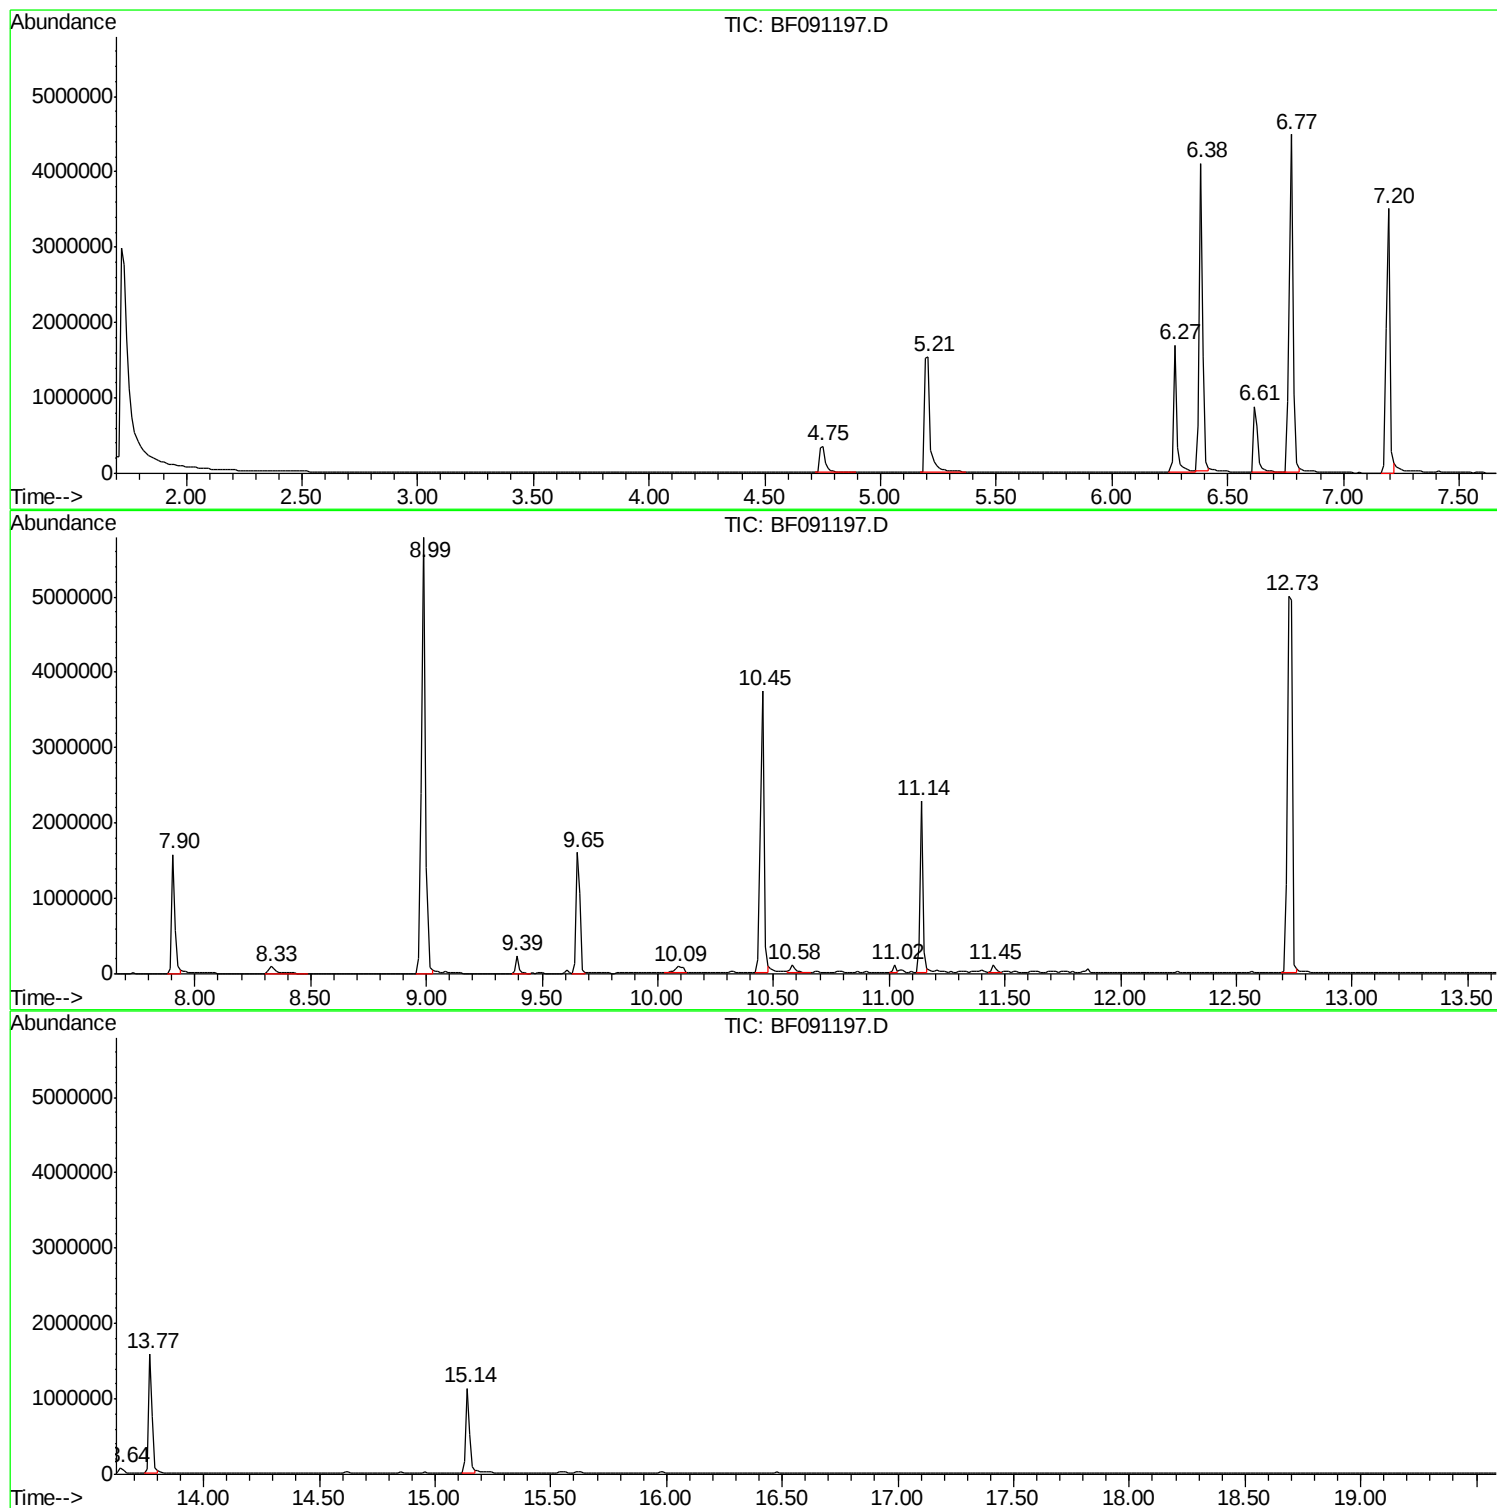

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111616\
Data File : BF091197.D
Acq On : 16 Nov 2016 19:27
Operator : UM/SJ
Sample : H5636-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C19043041










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.75	10.65 ng	641731	1,4-Dichlorobenzene-d4	6.61

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
3			Acetone	58	C3H6O	000067-64-1	9
4			5-Hexen-2-one	98	C6H10O	000109-49-9	9
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

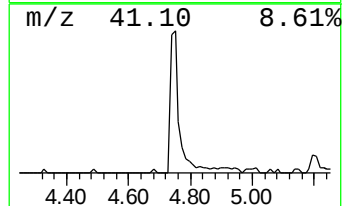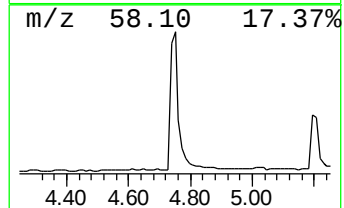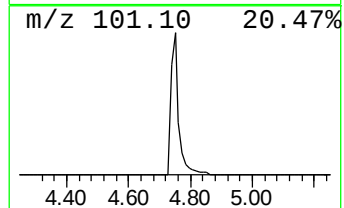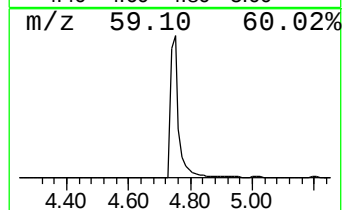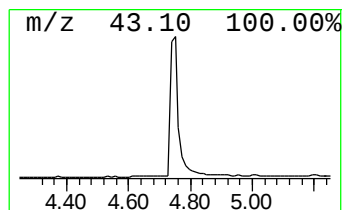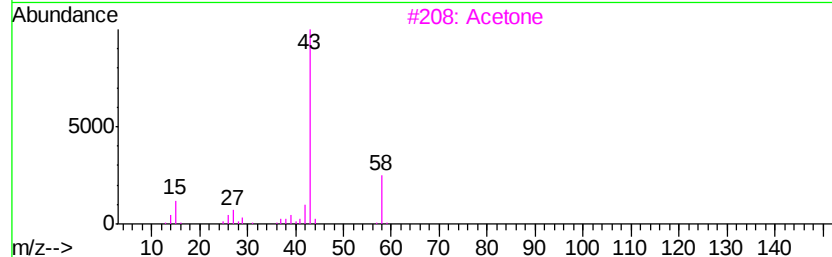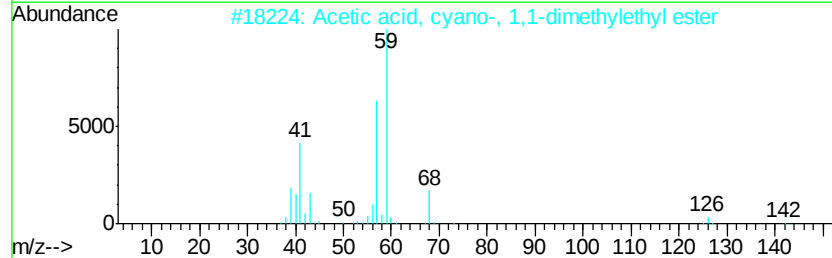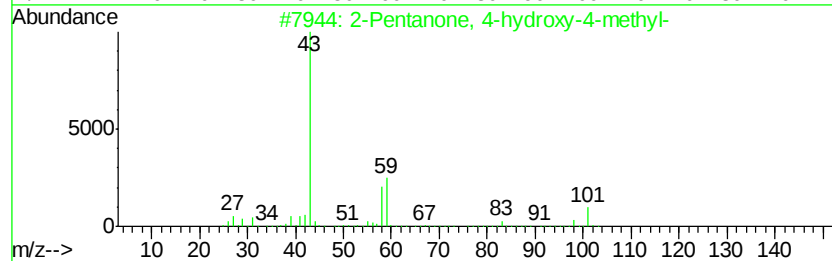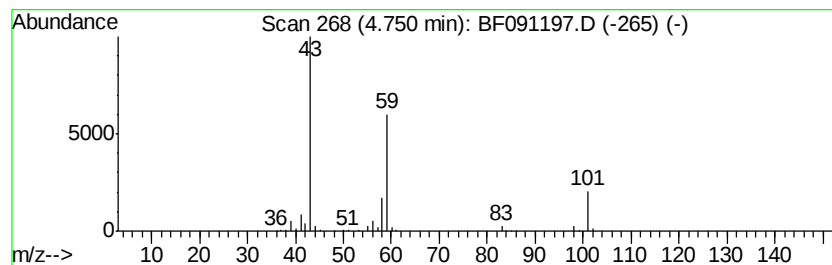

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111616\
Data File : BF091197.D
Acq On : 16 Nov 2016 19:27
Operator : UM/SJ
Sample : H5636-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C19043041







Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.38 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.38	72.55 ng	4373440	1,4-Dichlorobenzene-d4	6.61

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

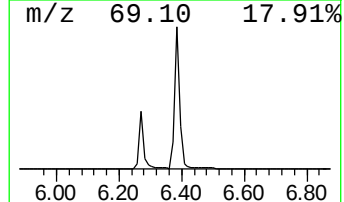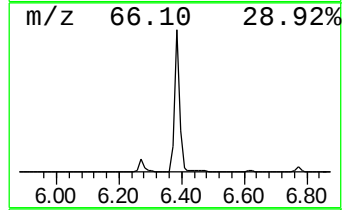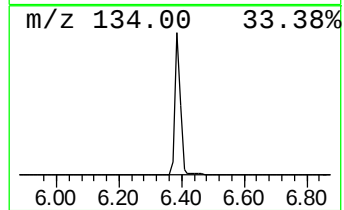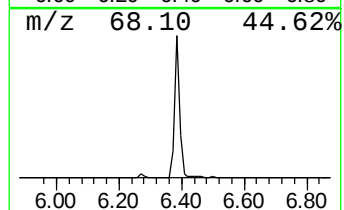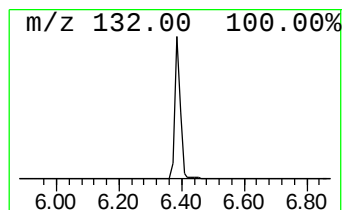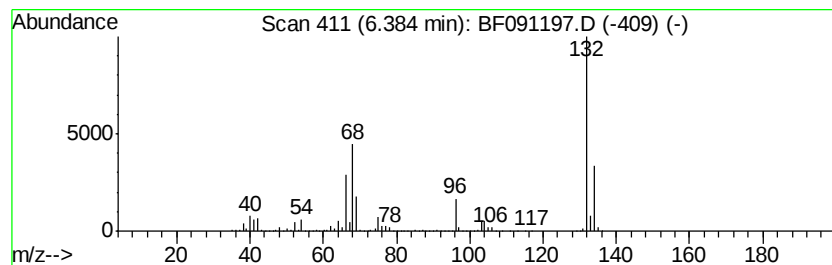

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111616\
Data File : BF091197.D
Acq On : 16 Nov 2016 19:27
Operator : UM/SJ
Sample : H5636-06
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
C19043041

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.75	10.7	ng	641731	1	6.61	1205630	20.0
unknown6.38	6.38	72.5	ng	4373440	1	6.61	1205630	20.0