


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111616\
Data File : BF091186.D
Acq On : 16 Nov 2016 13:53
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 08 12:59:29 2016

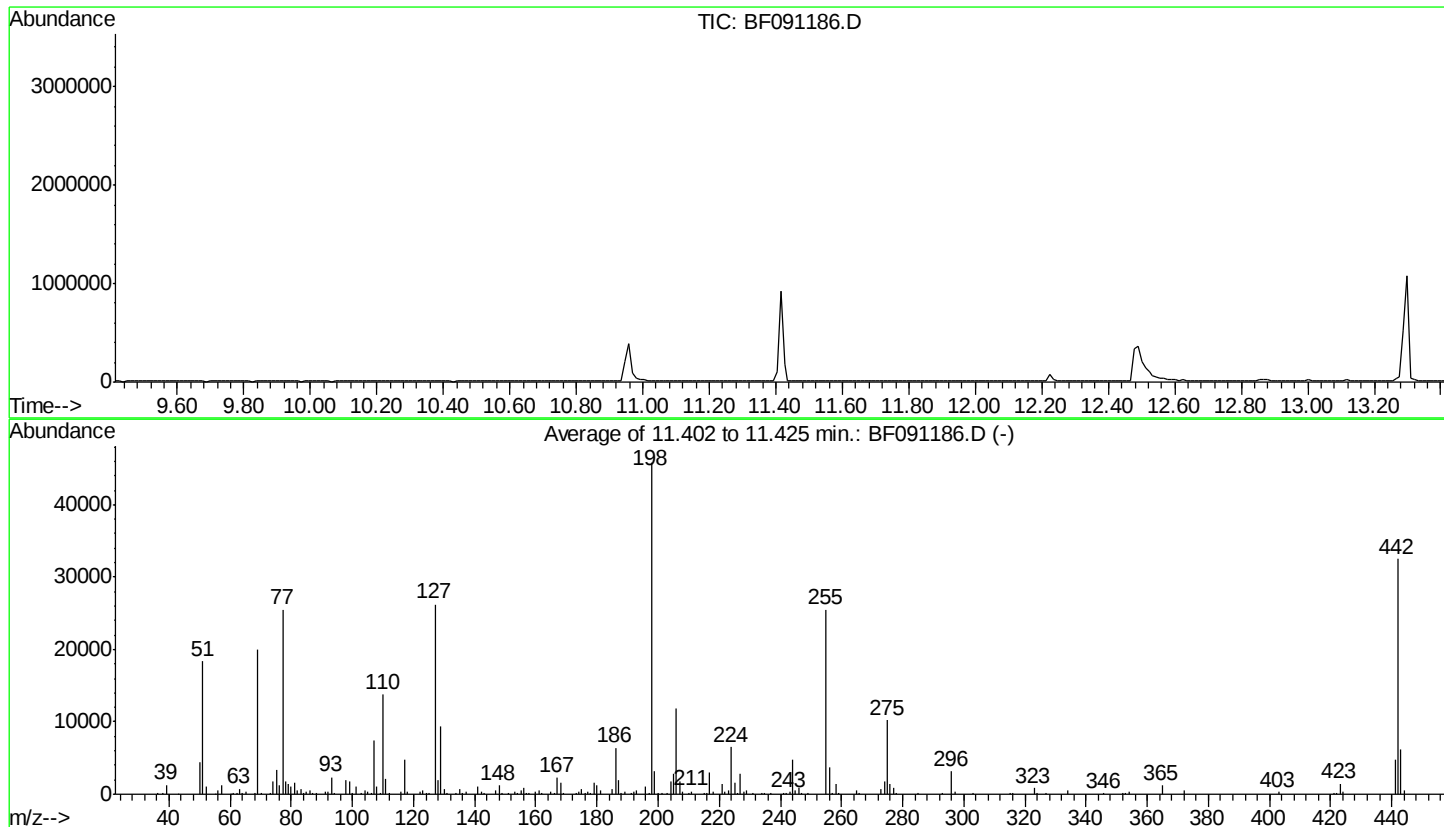

AutoFind: Scans 850, 851, 852; Background Corrected with Scan 847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	18334	PASS
68	69	0.00	2	1.0	210	PASS
69	198	0.00	100	43.8	20068	PASS
70	69	0.00	2	0.7	133	PASS
127	198	10	80	57.3	26266	PASS
197	198	0.00	2	0.3	123	PASS
198	198	100	100	100.0	45815	PASS
199	198	5	9	6.9	3184	PASS
275	198	10	60	22.4	10257	PASS
365	198	1	100	2.6	1207	PASS
441	442	0.01	24	14.8	4809	PASS
442	198	50	100	70.9	32490	PASS
443	442	15	24	19.0	6166	PASS