
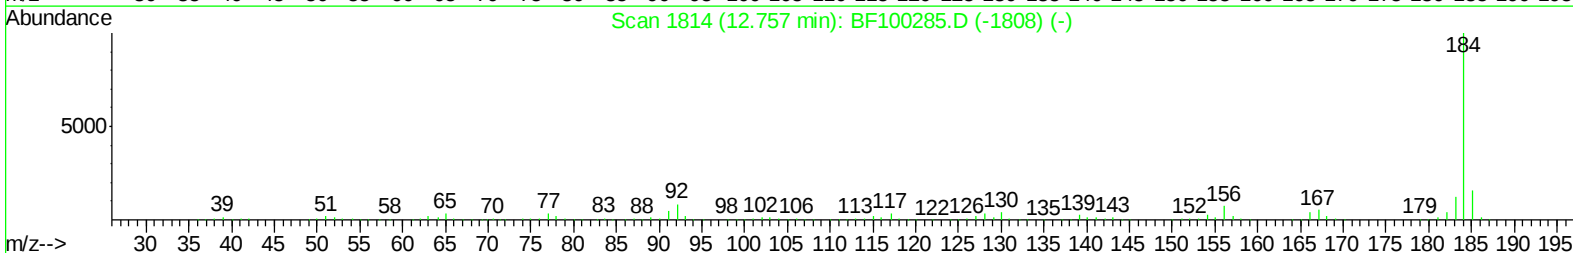
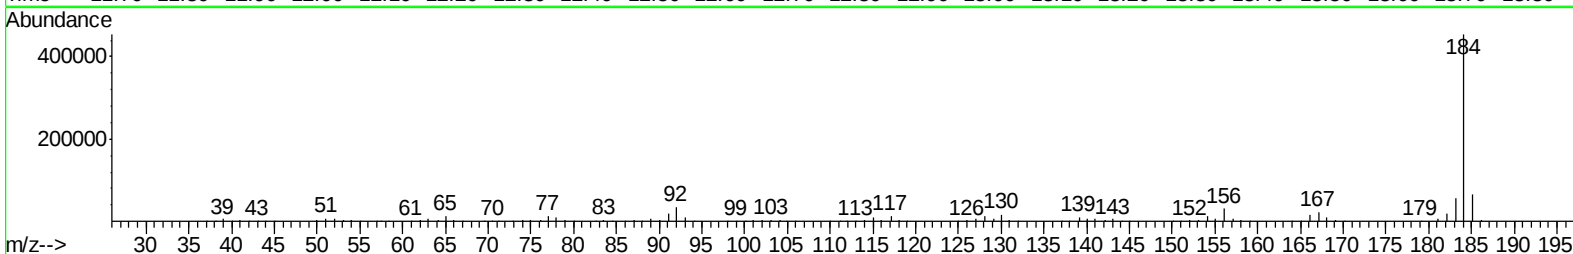


Data File : BF100617.D
Acq On : 16 Nov 2017 8:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 06:08:27 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 12:15:03 2017
Response via : Initial Calibration

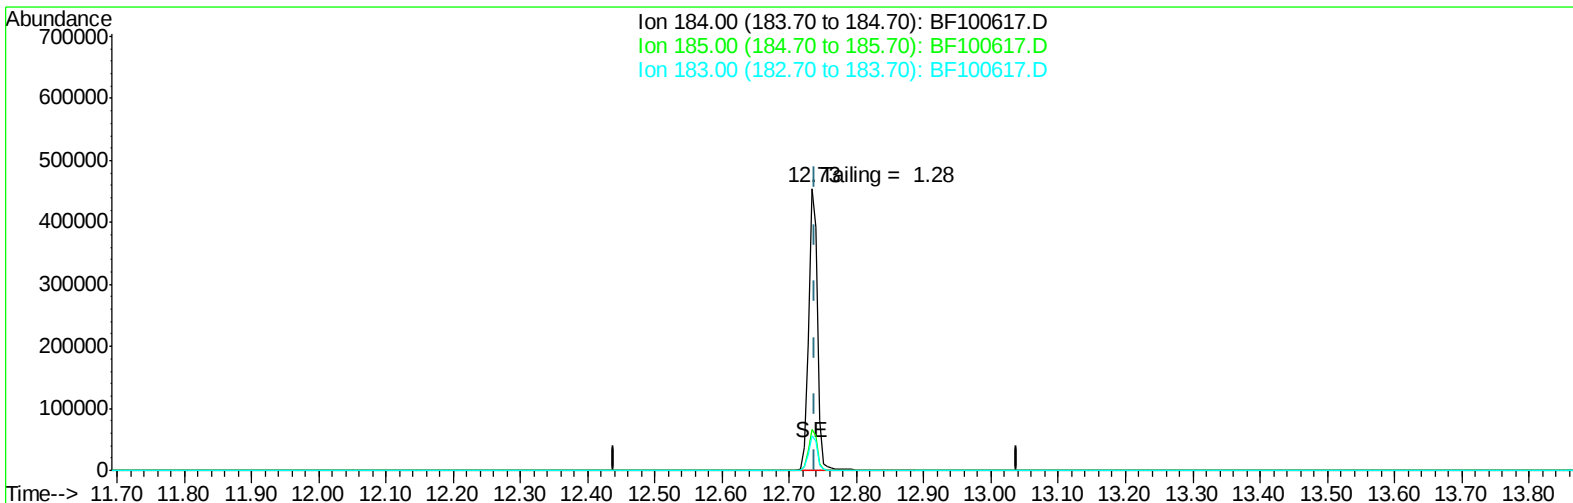

TIC: BF100617.D

(76) Benzidine




12.733min (-0.006) 0.00ng

response 425682

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.42
183.00	11.60	12.09
0.00	0.00	0.00

Data File : BF100617.D
Acq On : 16 Nov 2017 8:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 06:08:27 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 12:15:03 2017
Response via : Initial Calibration

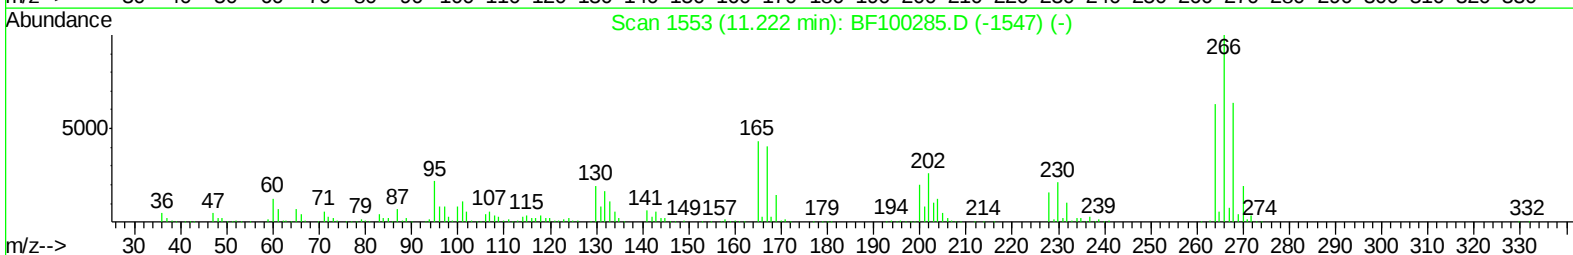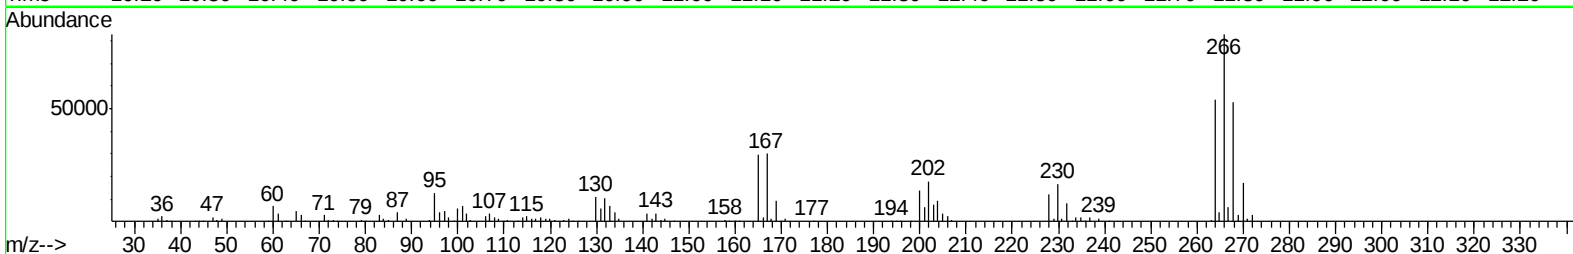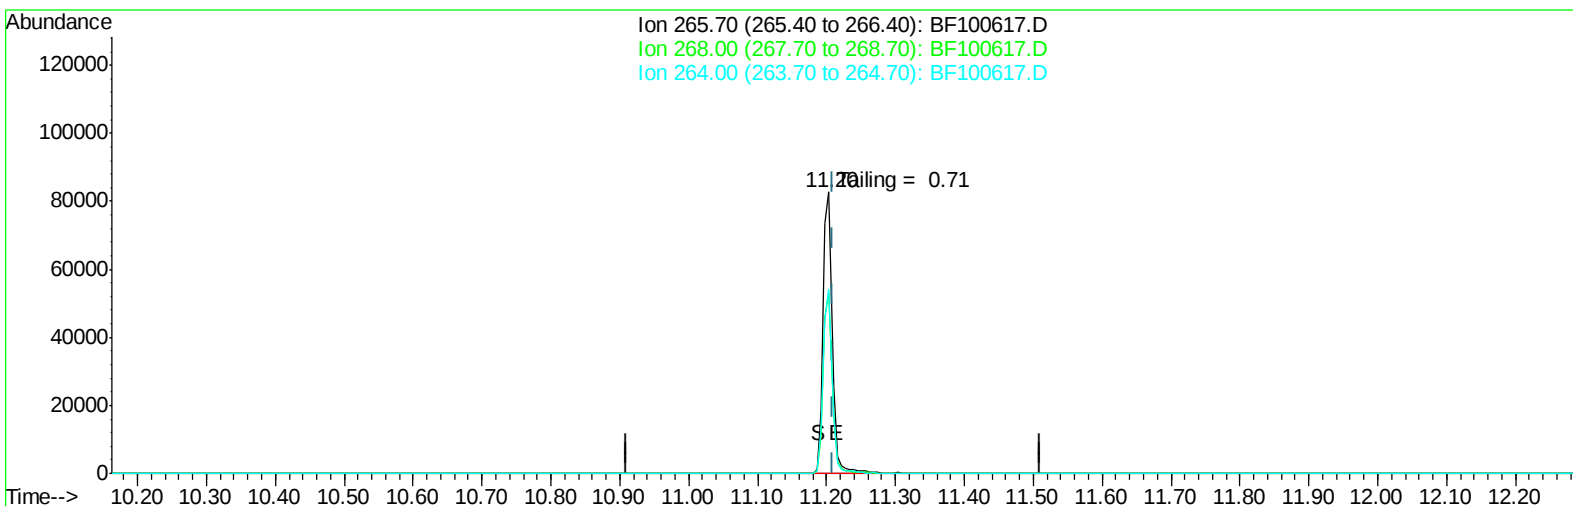

TIC: BF100617.D

(69) Pentachlorophenol (C)

11.204min (-0.006) 55827.02ng

response 75850

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.17
264.00	61.90	65.29
0.00	0.00	0.00