
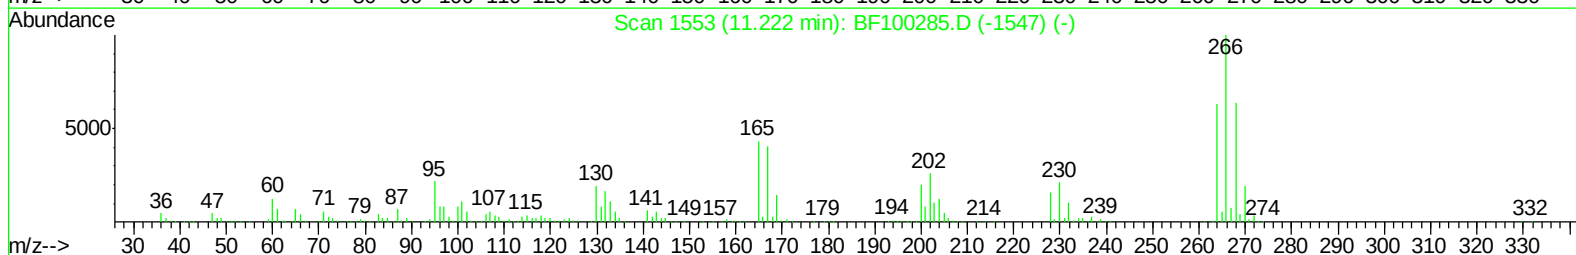
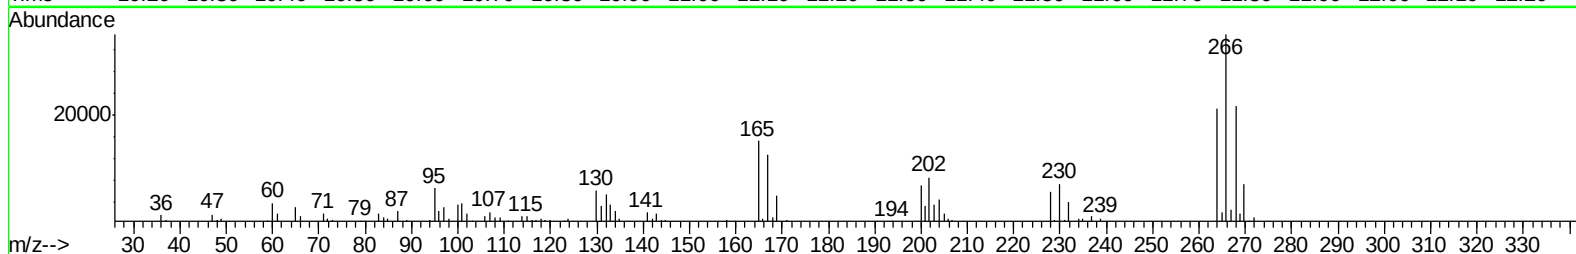


Data File : BF100643.D
Acq On : 16 Nov 2017 21:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 06:10:15 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 12:15:03 2017
Response via : Initial Calibration

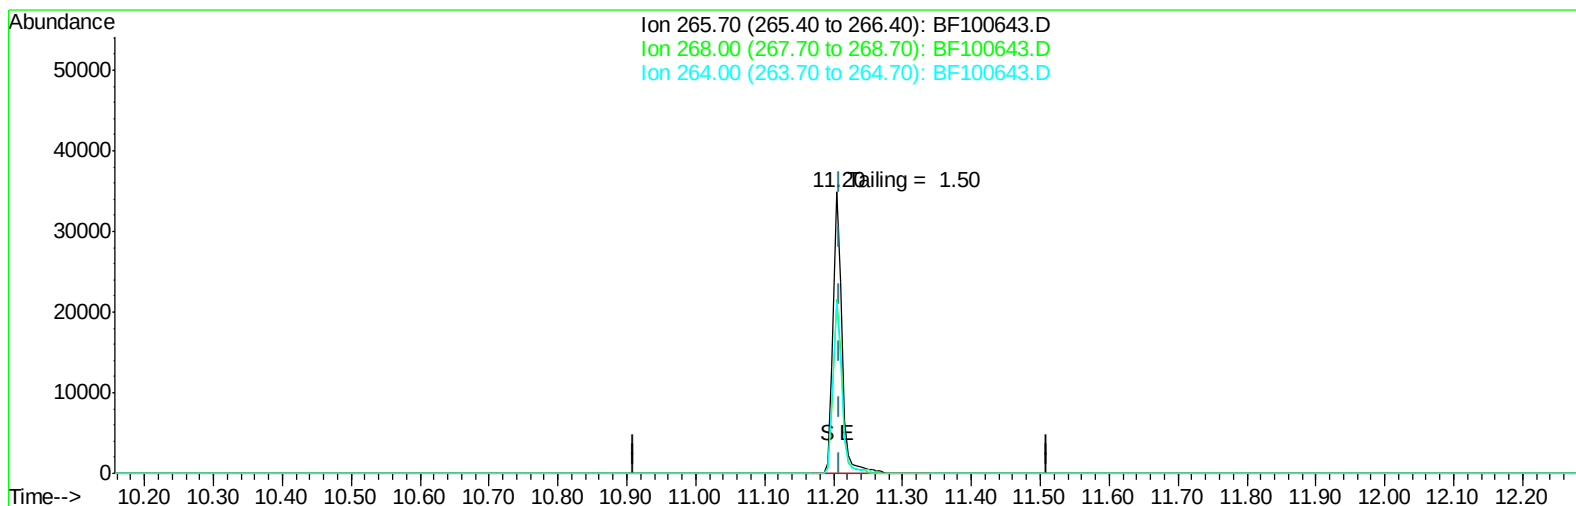

TIC: BF100643.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 33383.77ng

response 30596

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.05
264.00	61.90	60.70
0.00	0.00	0.00

Data File : BF100643.D
Acq On : 16 Nov 2017 21:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 17 06:10:15 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 12:15:03 2017
Response via : Initial Calibration

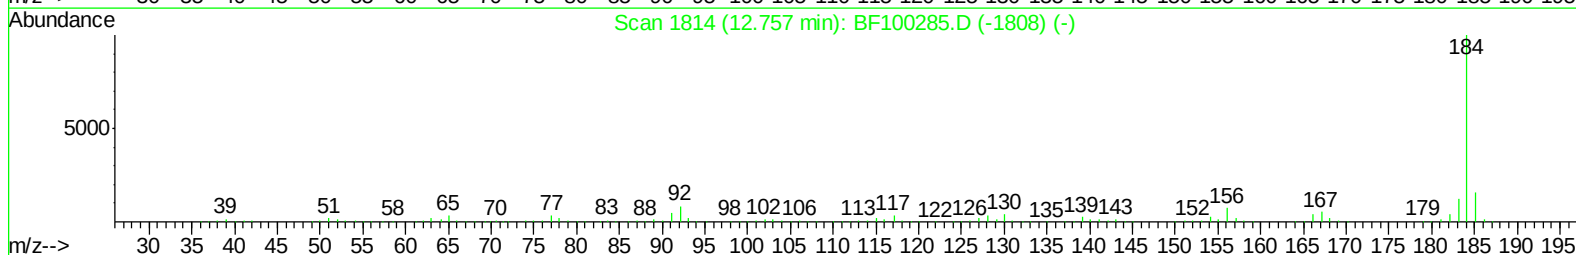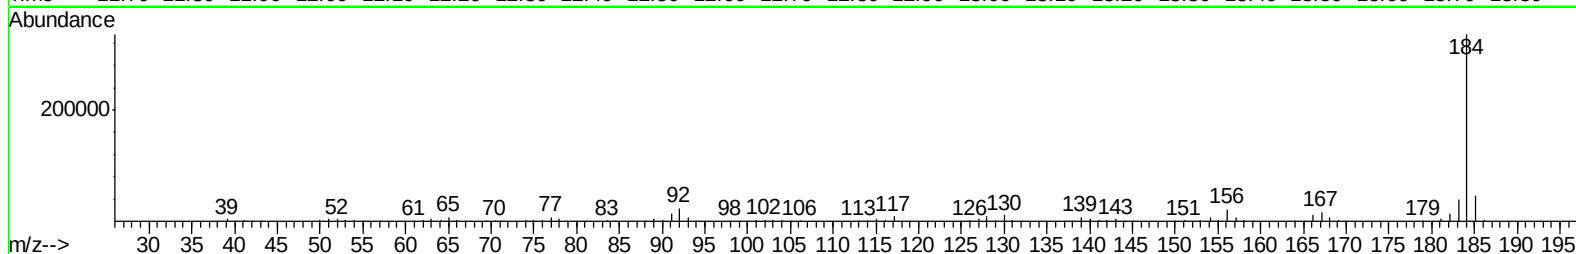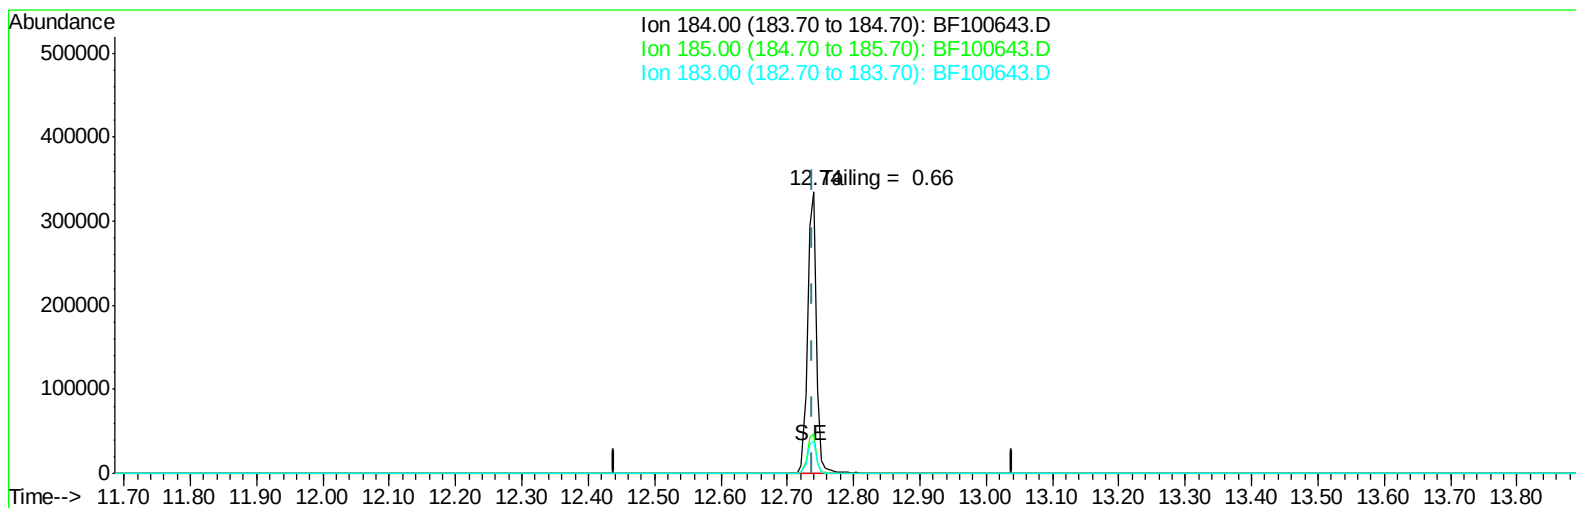

TIC: BF100643.D

(76) Benzidine

12.739min (-0.000) 0.00ng

response 308119

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.10
183.00	11.60	11.59
0.00	0.00	0.00