

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111617\
 Data File : BF100652.D
 Acq On : 17 Nov 2017 1:53
 Operator : SJ/JU
 Sample : I6490-05
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 111417-TIDO-E-D-B

Quant Time: Nov 17 03:05:55 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 16 12:15:03 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	108424	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	416782	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	182086	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	287763	20.00	ng	0.00
75) Chrysene-d12	14.04	240	224773	20.00	ng	0.00
86) Perylene-d12	15.52	264	217082	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.50	112	271423	40.13	ng	0.00
7) Phenol-d6	6.50	99	211117	25.31	ng	-0.01
23) Nitrobenzene-d5	7.45	82	555916	88.18	ng	0.00
41) 2,4,6-Tribromophenol	10.70	330	123122	66.36	ng	0.00
44) 2-Fluorobiphenyl	9.24	172	1036057	86.64	ng	0.00
78) Terphenyl-d14	12.99	244	690462	70.58	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111617\
Data File : BF100652.D
Acq On : 17 Nov 2017 1:53
Operator : SJ/JU
Sample : I6490-05
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
111417-TIDO-E-D-B

Quant Time: Nov 17 03:05:55 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 16 12:15:03 2017
Response via : Initial Calibration

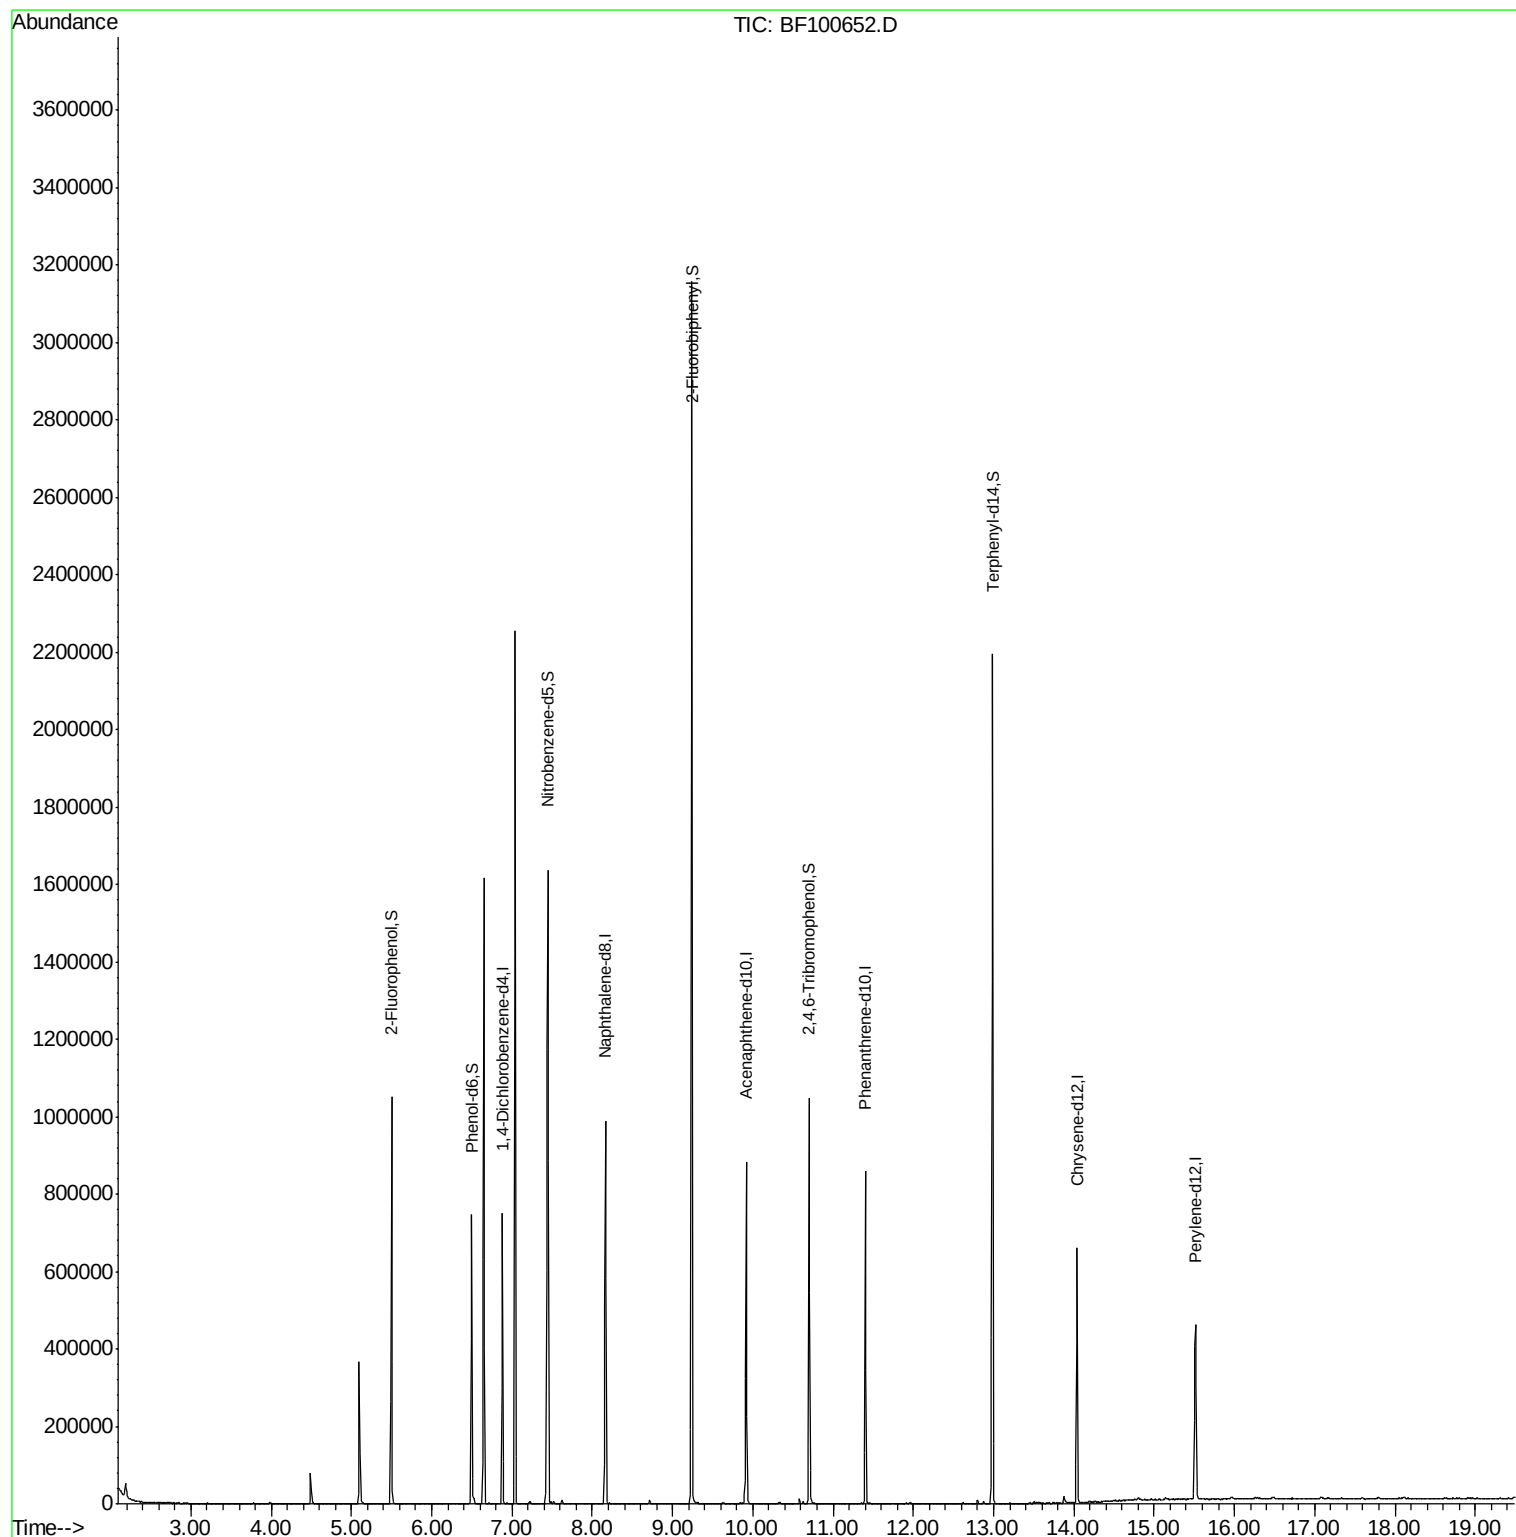




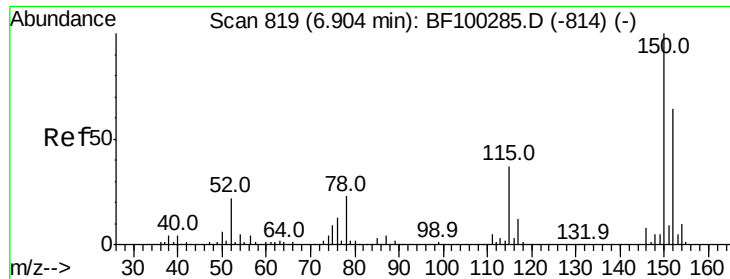


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.88 min Scan# 815
Delta R.T. -0.01 min
Lab File: BF100652.D
Acq: 17 Nov 2017 1:53

Instrument :
BNA_F
ClientSampleId :
111417-TIDO-E-D-B




Tot Ion:152 Resp: 108424
Ion Ratio Lower Upper
152 100
150 157.5 124.6 186.8
115 61.0 50.1 75.1

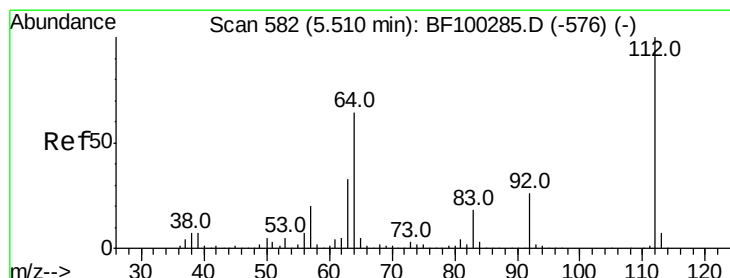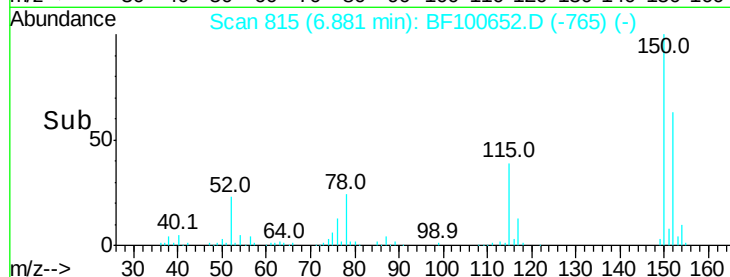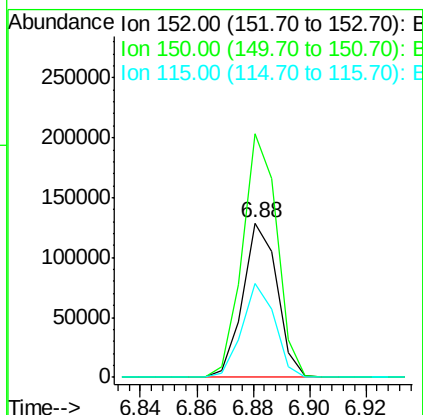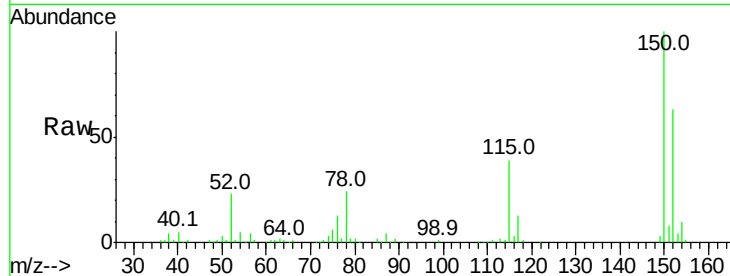


#5

2-Fluorophenol
Concen: 40.128 ng
RT: 5.50 min Scan# 580
Delta R.T. 0.00 min
Lab File: BF100652.D
Acq: 17 Nov 2017 1:53

Tgt Ion:112 Resp: 271423
Ion Ratio Lower Upper
112 100
64 58.4 47.9 71.9
63 27.9 23.7 35.5

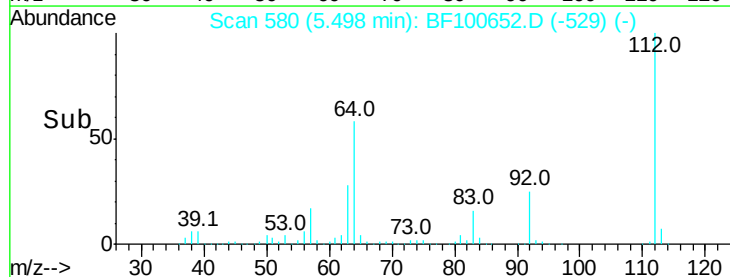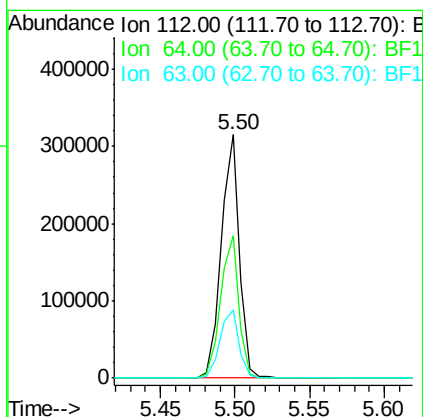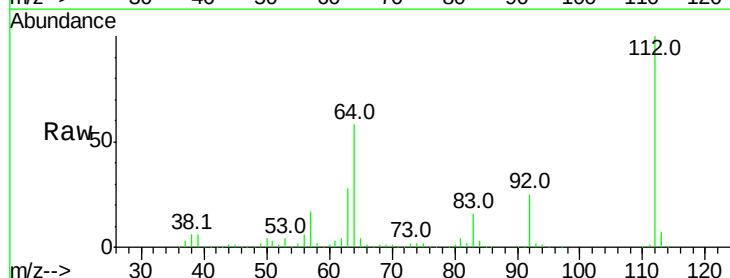

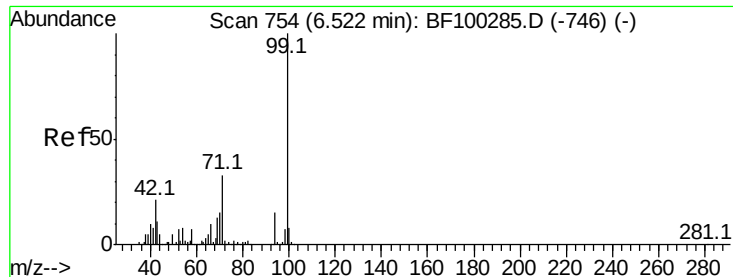

#7

Phenol-d6

Concen: 25.312 ng

RT: 6.50 min Scan# 750

Delta R.T. -0.01 min

Lab File: BF100652.D

Acq: 17 Nov 2017 1:53

Instrument :

BNA_F

ClientSampleId :

111417-TIDO-E-D-B


Tot Ion: 99 Resp: 211117

Ion Ratio Lower Upper




99 100

42 17.7 14.5 21.7

71 31.4 25.4 38.0

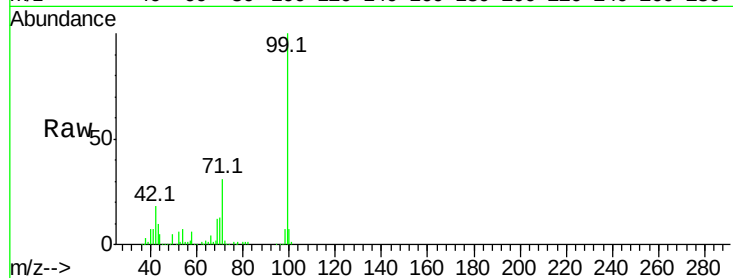

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

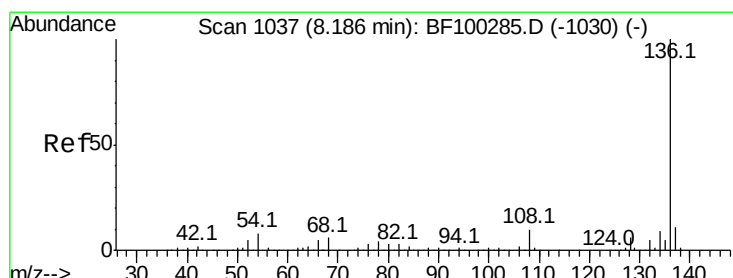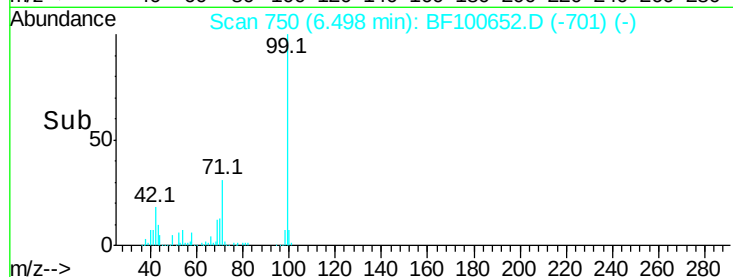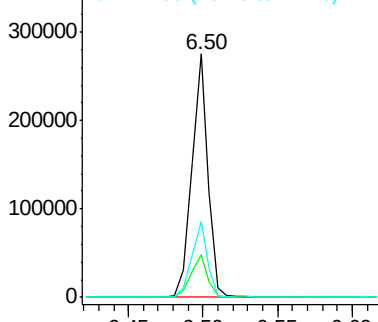

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1033

Delta R.T. -0.01 min

Lab File: BF100652.D

Acq: 17 Nov 2017 1:53

Tgt Ion: 136 Resp: 416782


Ion Ratio Lower Upper

136 100



137 11.3 8.9 13.3


54 8.5 6.6 9.8

68 5.9 5.0 7.4

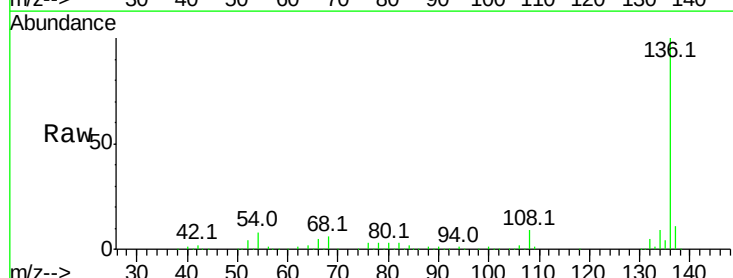

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

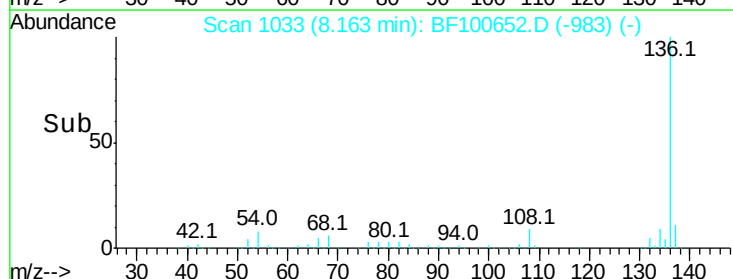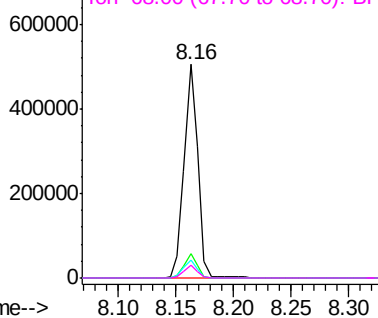


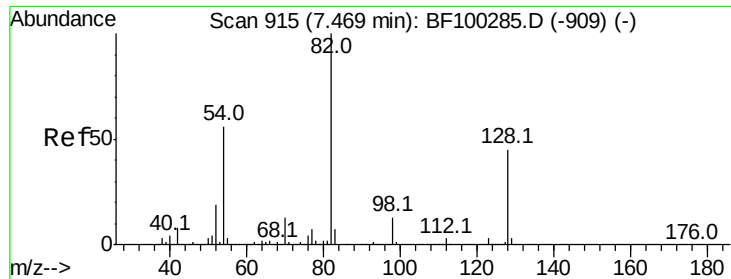




#23
 Nitrobenzene-d5
 Concen: 88.184 ng
 RT: 7.45 min Scan# 911
 Delta R.T. -0.01 min
 Lab File: BF100652.D
 Acq: 17 Nov 2017 1:53

Instrument :
 BNA_F
 ClientSampleId :
 111417-TIDO-E-D-B

Tot Ion: 82 Resp: 555916
 Ion Ratio Lower Upper
 82 100
 128 46.1 36.1 54.1
 54 53.3 41.4 62.2

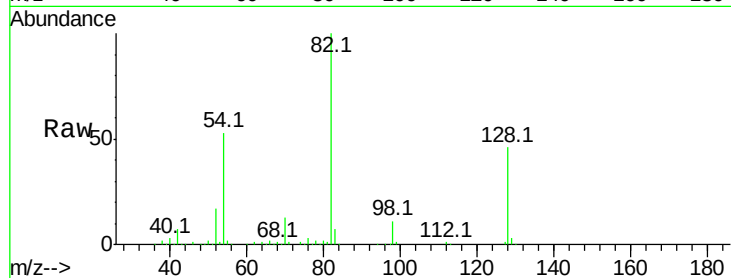


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

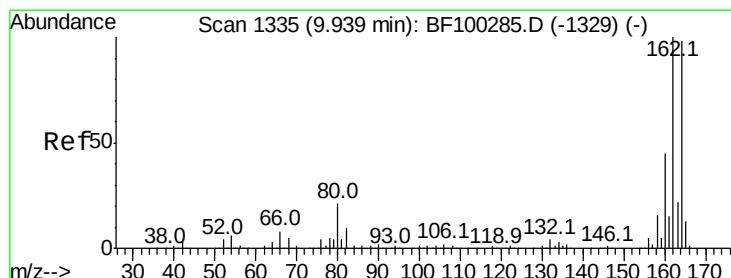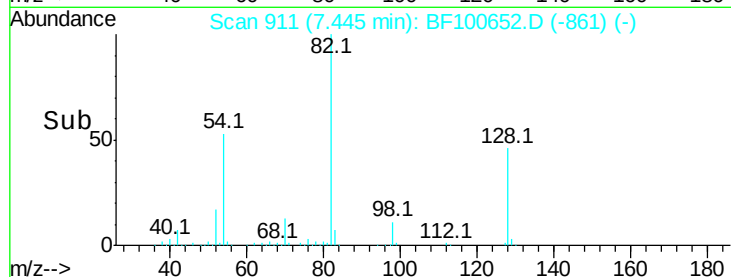
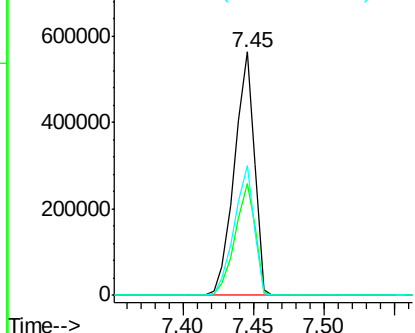



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.01 min
 Lab File: BF100652.D
 Acq: 17 Nov 2017 1:53

Tgt Ion: 164 Resp: 182086
 Ion Ratio Lower Upper
 164 100
 162 102.2 86.1 129.1
 160 44.4 38.3 57.5

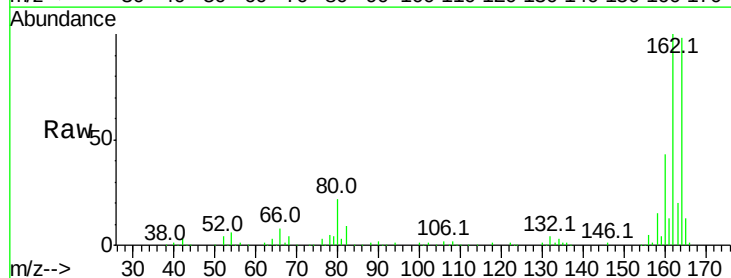

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

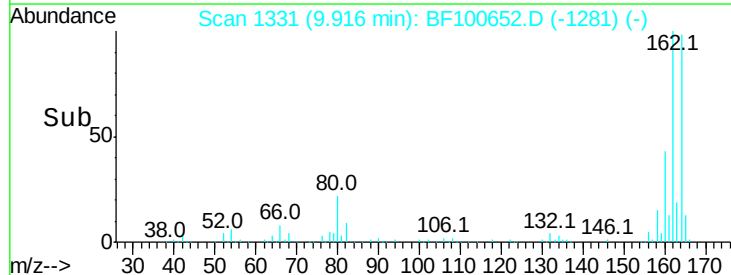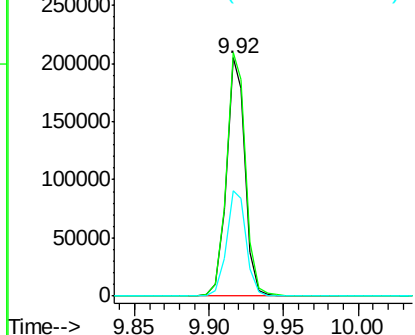


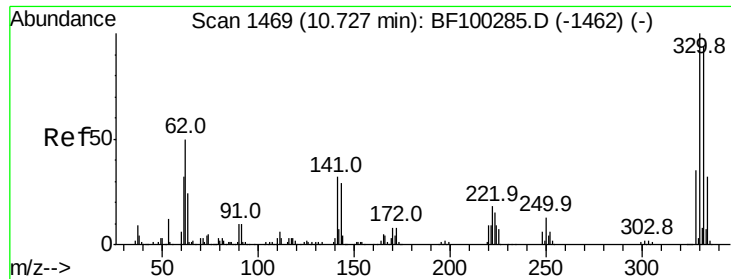




#41
 2,4,6-Tribromophenol
 Concen: 66.357 ng
 RT: 10.70 min Scan# 1465
 Delta R.T. -0.01 min
 Lab File: BF100652.D
 Acq: 17 Nov 2017 1:53

Instrument :
 BNA_F
 ClientSampleId :
 111417-TIDO-E-D-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.9	77.0	115.6
141	28.7	29.9	44.9#

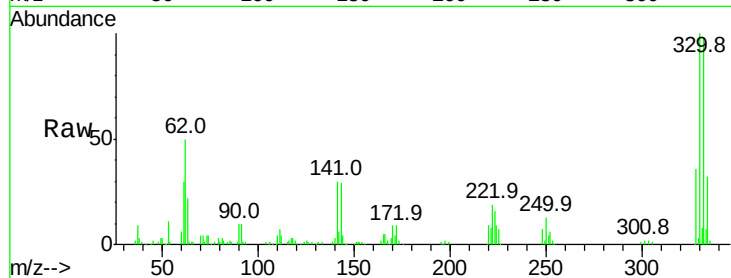


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

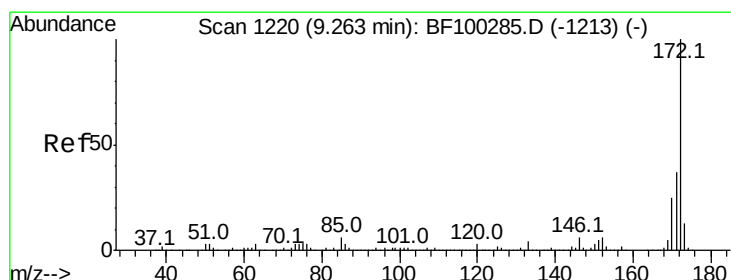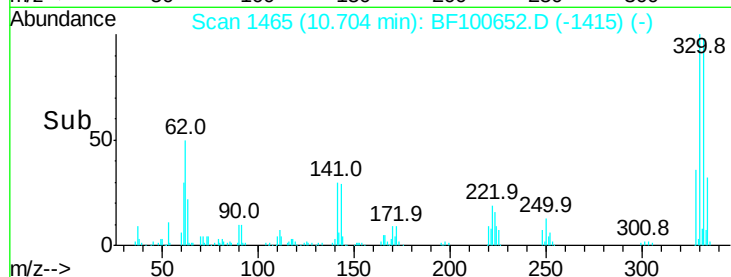
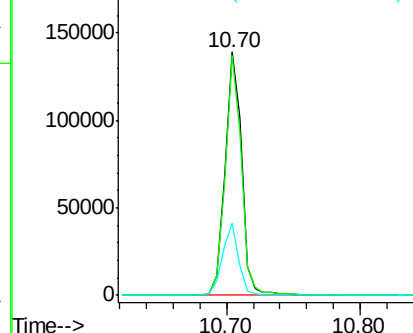



#44
 2-Fluorobiphenyl
 Concen: 86.641 ng
 RT: 9.24 min Scan# 1216
 Delta R.T. 0.00 min
 Lab File: BF100652.D
 Acq: 17 Nov 2017 1:53

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.7	29.7	44.5
170	24.2	19.6	29.4

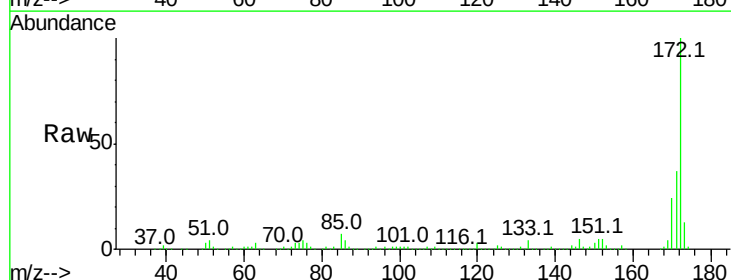

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



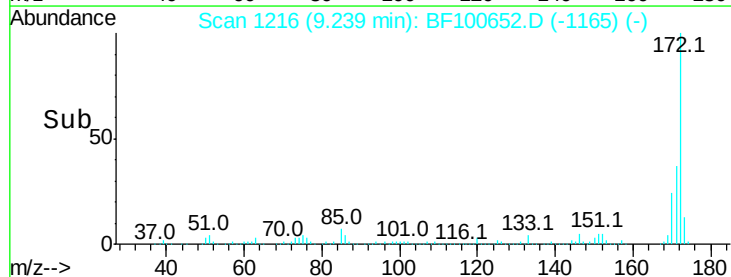
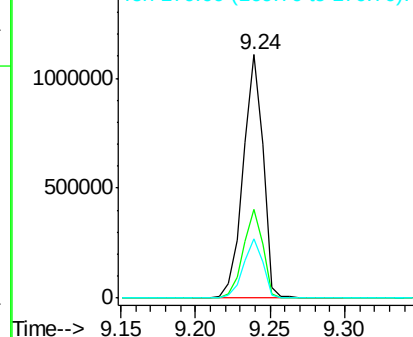


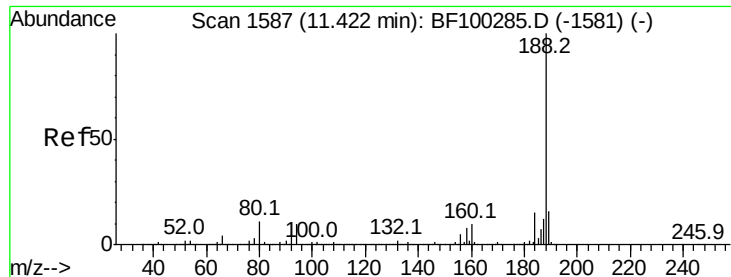

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.40 min Scan# 1584
Delta R.T. 0.00 min
Lab File: BF100652.D
Acq: 17 Nov 2017 1:53




Instrument :
BNA_F
ClientSampleId :
111417-TIDO-E-D-B


Tot Ion	Ratio	Lower	Upper
188	100		
94	8.9	8.5	12.7
80	9.1	9.2	13.8#

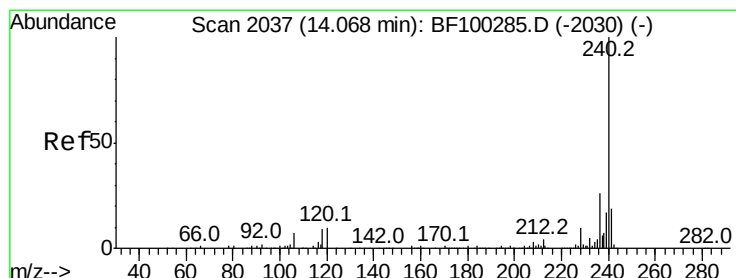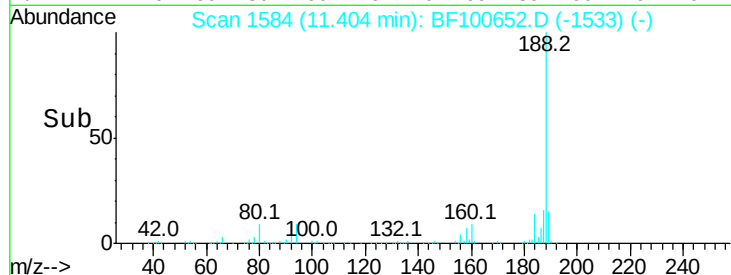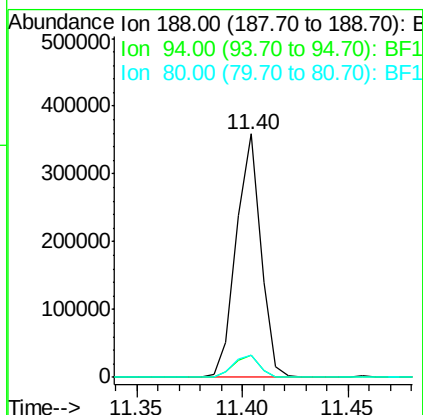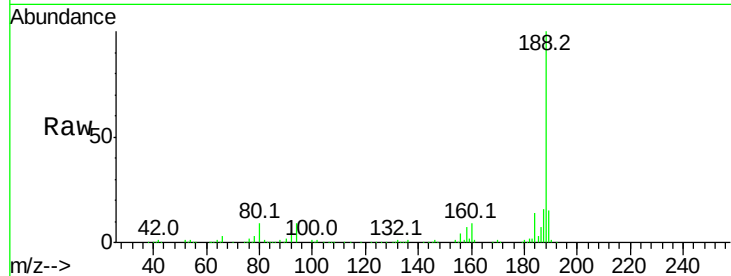

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.04 min Scan# 2032
Delta R.T. -0.01 min
Lab File: BF100652.D
Acq: 17 Nov 2017 1:53

Tgt Ion	Ratio	Lower	Upper
240	100		
120	11.4	9.5	14.3
236	24.7	20.7	31.1

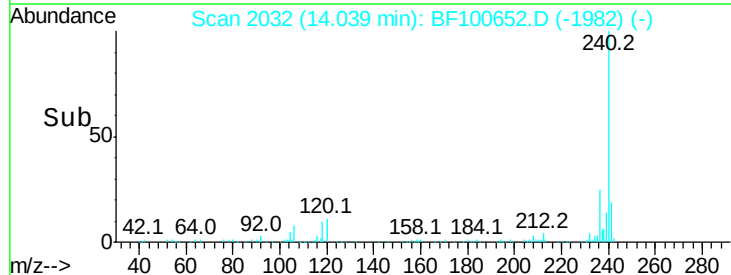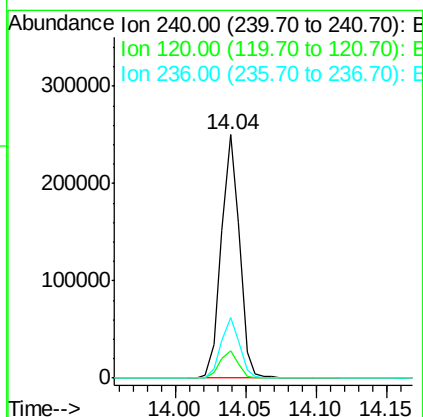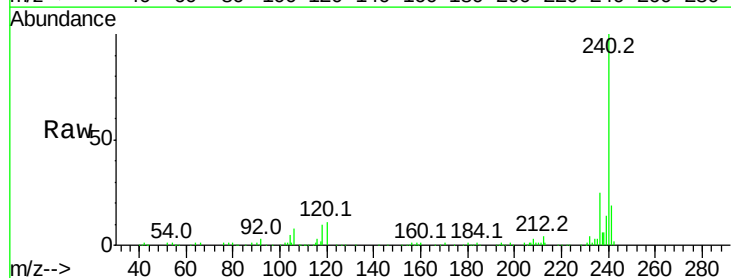

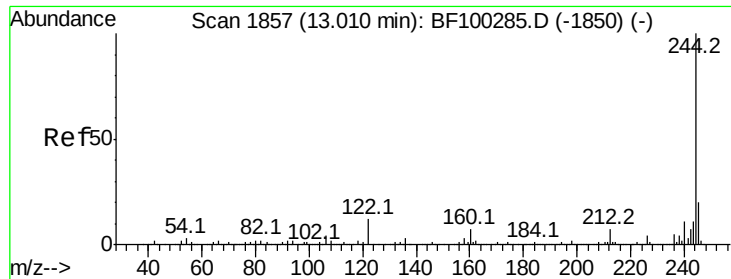

#78

Terphenyl-d14

Concen: 70.581 ng

RT: 12.99 min Scan# 1853

Delta R.T. -0.01 min

Lab File: BF100652.D

Acq: 17 Nov 2017 1:53

Instrument :

BNA_F

ClientSampleId :

111417-TIDO-E-D-B


Tot Ion:244 Resp: 690462

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0




122 11.8 11.0 16.4

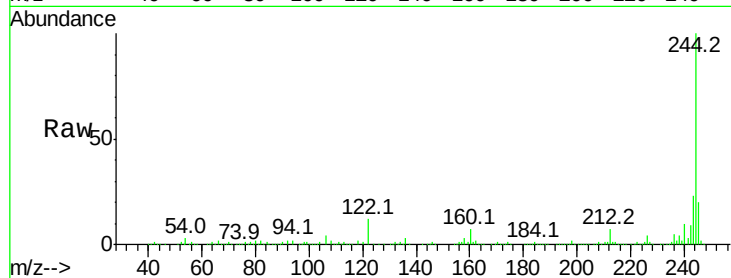

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

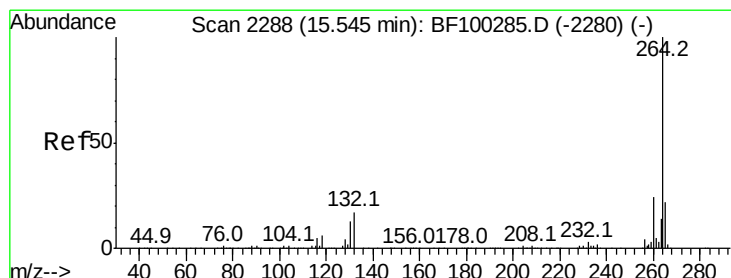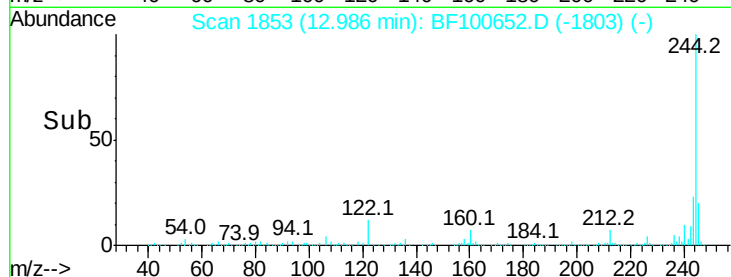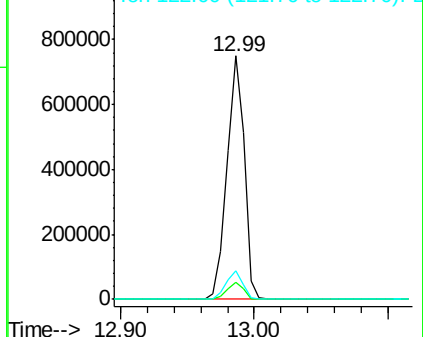

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.52 min Scan# 2283

Delta R.T. 0.00 min

Lab File: BF100652.D

Acq: 17 Nov 2017 1:53


Tgt Ion:264 Resp: 217082

Ion Ratio Lower Upper

264 100

260 23.0 19.2 28.8

265 21.5 17.5 26.3

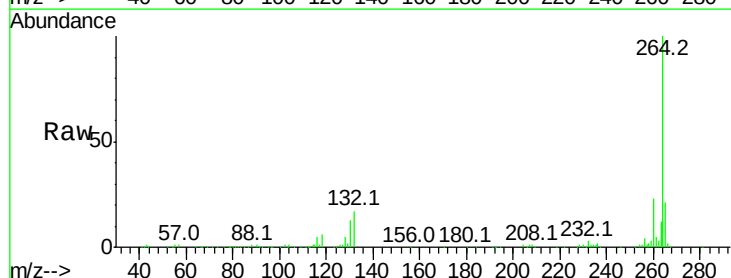

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

