


Data Path : Z:\HPCHEM1\BNA F\DATA\BF111617\
 Data File : BF100617.D
 Acq On : 16 Nov 2017 8:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Nov 16 12:15:03 2017

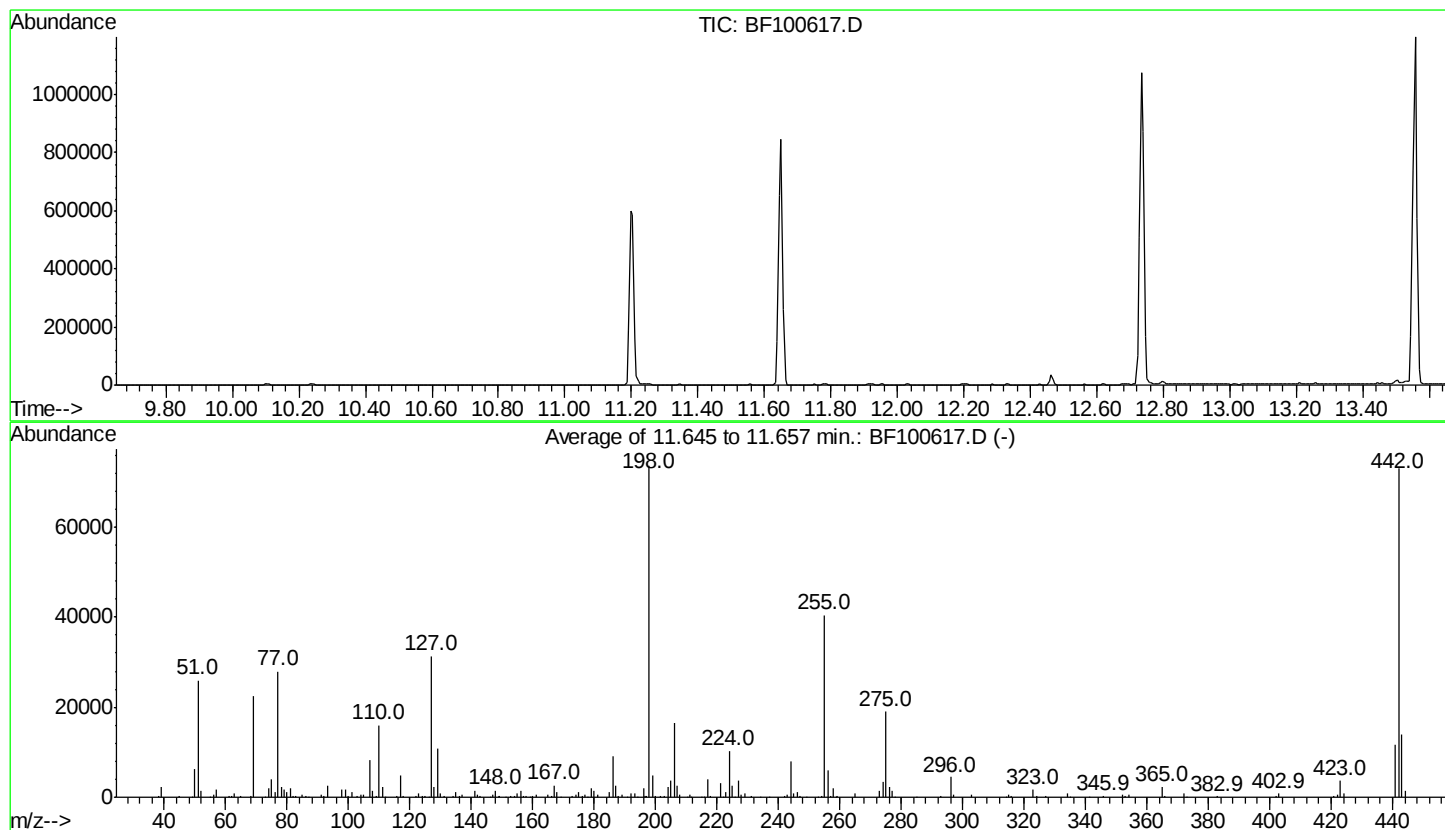

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	25893	PASS
68	69	0.00	2	1.8	405	PASS
69	198	0.00	100	30.6	22516	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.6	31361	PASS
197	198	0.00	2	0.4	288	PASS
198	198	100	100	100.0	73661	PASS
199	198	5	9	6.7	4972	PASS
275	198	10	60	25.8	18978	PASS
365	198	1	100	3.1	2304	PASS
441	443	0.01	100	83.3	11734	PASS
442	198	50	100	99.3	73120	PASS
443	442	15	24	19.3	14078	PASS