
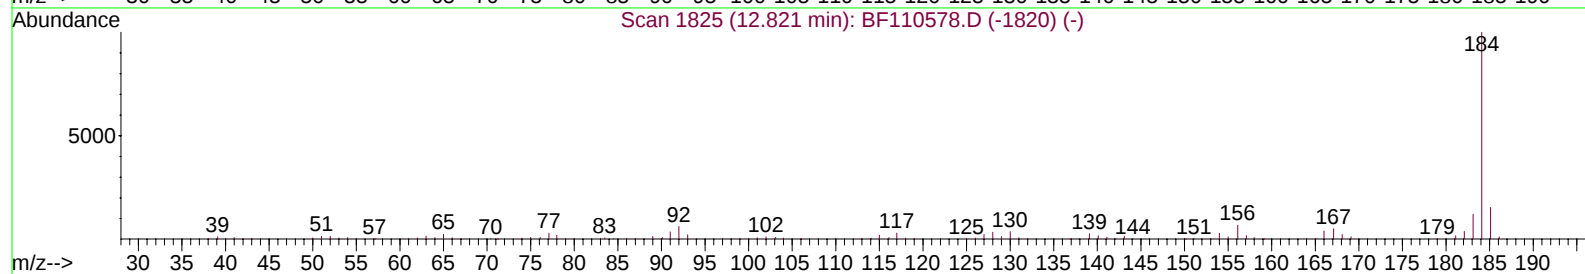
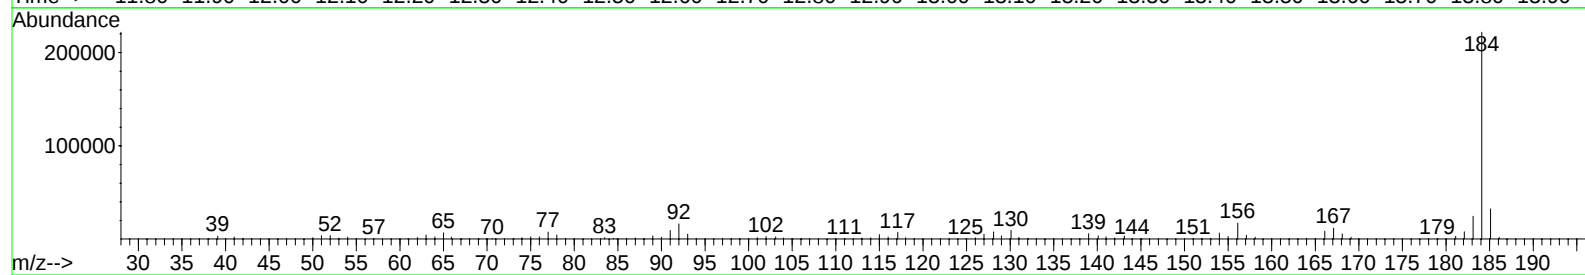


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111618\
Data File : BF110808.D
Acq On : 16 Nov 2018 10:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 16:58:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

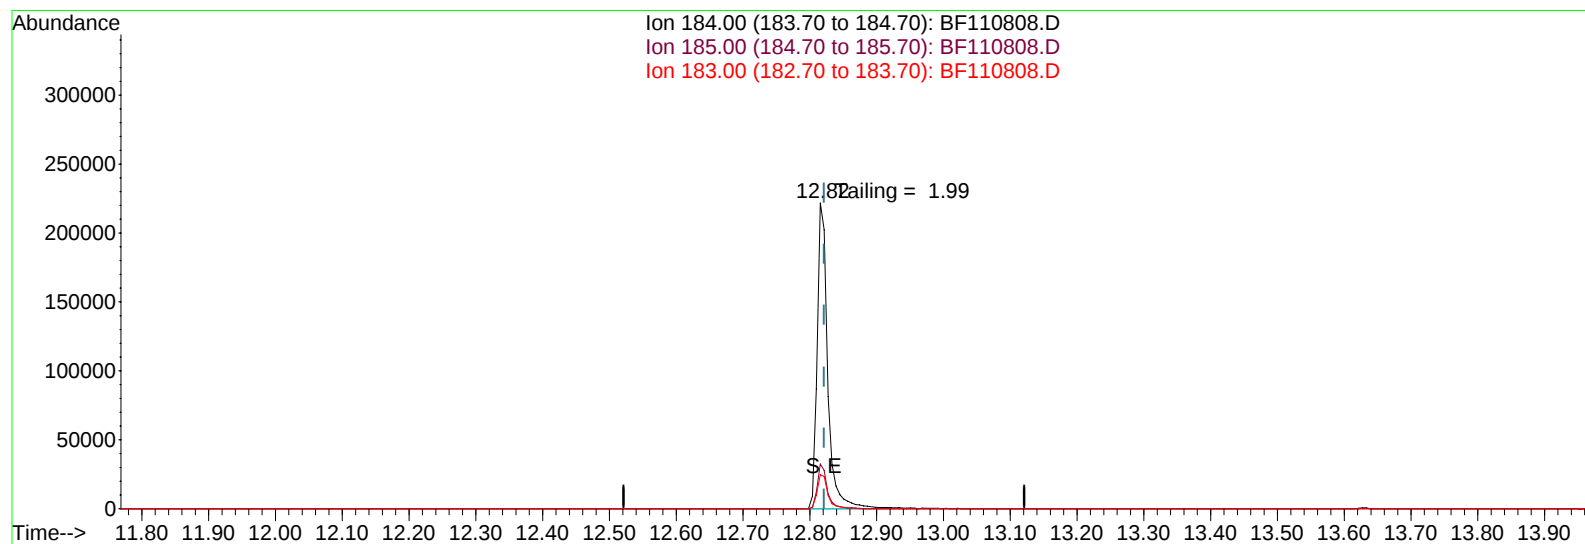

TIC: BF110808.D

(77) Benzidine




12.816min (-0.005) 0.00ng

response 245743

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.68
183.00	11.80	11.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF111618\
Data File : BF110808.D
Acq On : 16 Nov 2018 10:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 16:58:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF110818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 13 12:43:10 2018
Response via : Initial Calibration

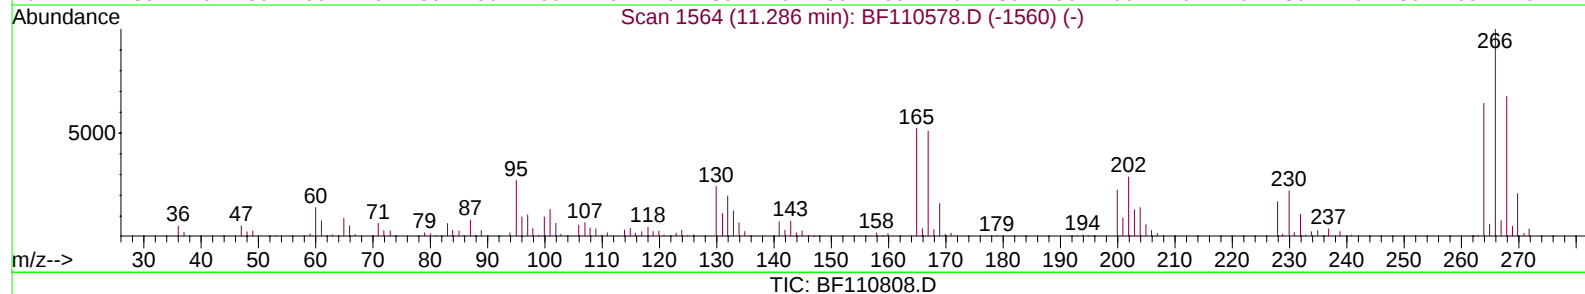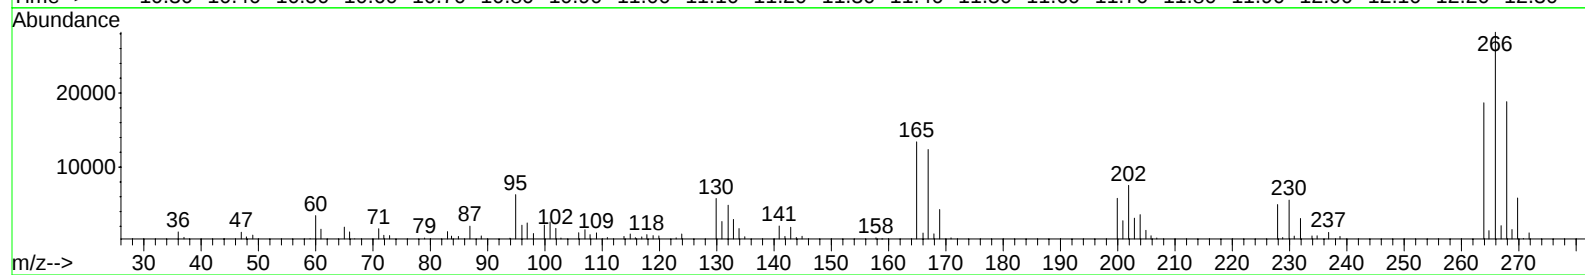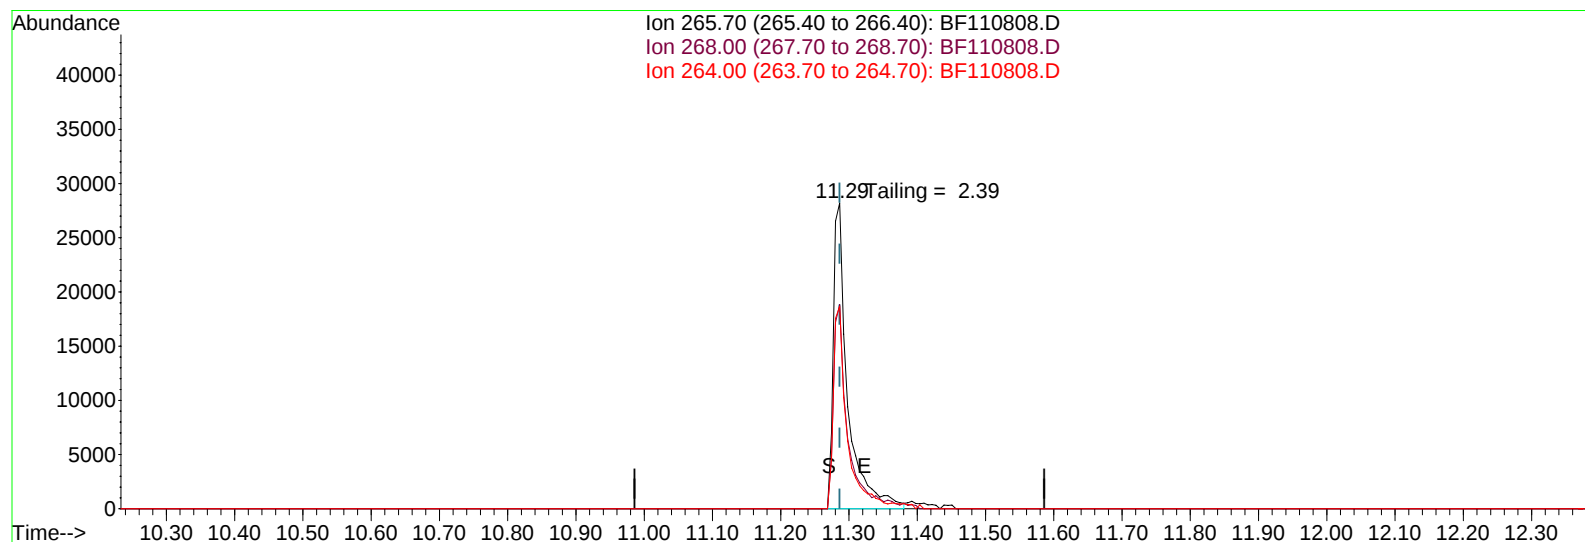

(70) Pentachlorophenol (C)

11.286min (+0.000) 60644.03ng

response 41099

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	66.76
264.00	63.20	66.22
0.00	0.00	0.00