


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111618\
 Data File : BF110808.D
 Acq On : 16 Nov 2018 10:54
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Nov 13 12:43:10 2018

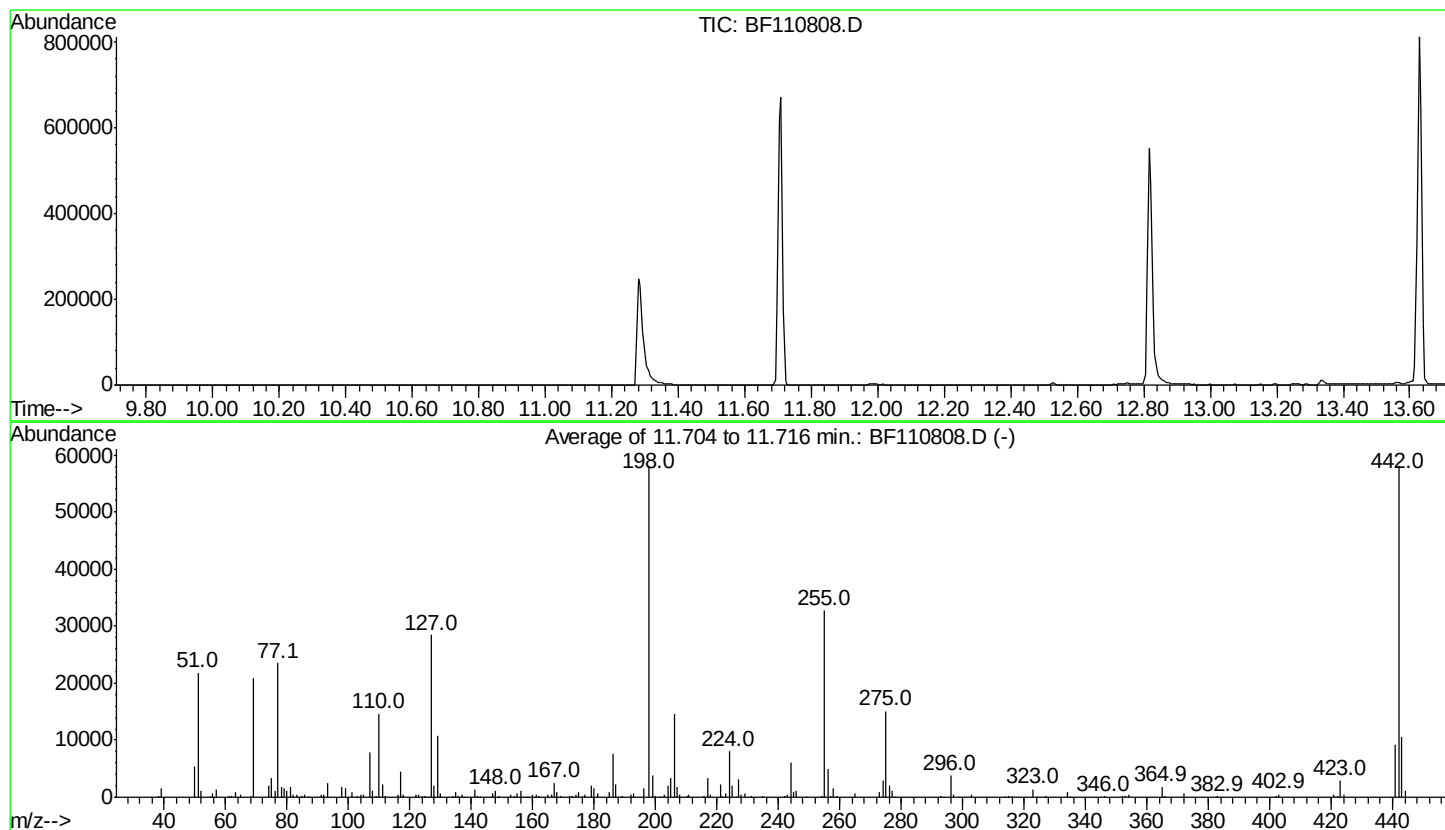

AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	21862	PASS
68	69	0.00	2	1.5	303	PASS
69	198	0.00	100	35.8	20785	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	28424	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58125	PASS
199	198	5	9	6.7	3872	PASS
275	198	10	60	26.0	15087	PASS
365	198	1	100	3.3	1903	PASS
441	198	0.01	100	16.0	9277	PASS
442	198	50	100	99.9	58093	PASS
443	442	15	24	18.0	10447	PASS