
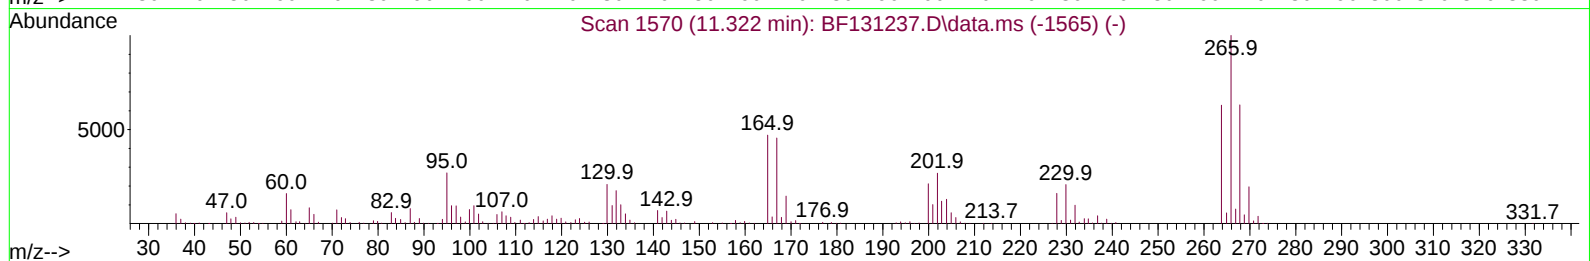
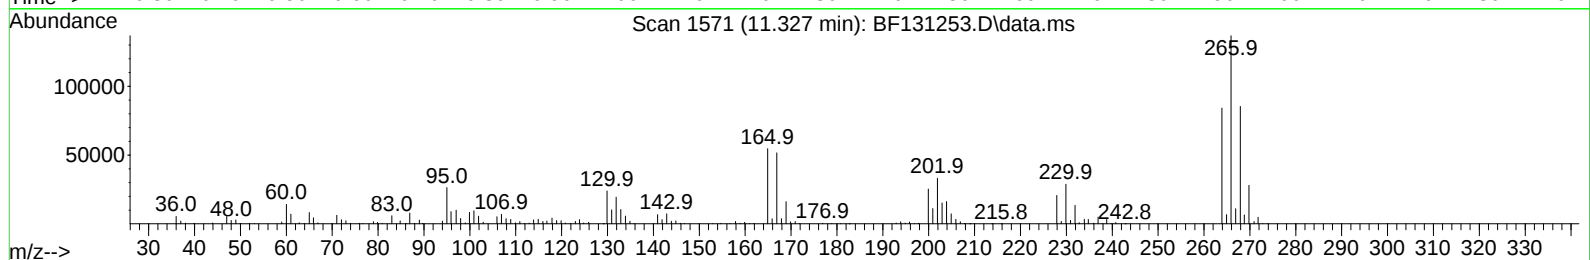


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
 Data File : BF131253.D
 Acq On : 16 Nov 2022 08:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 15:10:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 06:35:36 2022
 Response via : Initial Calibration

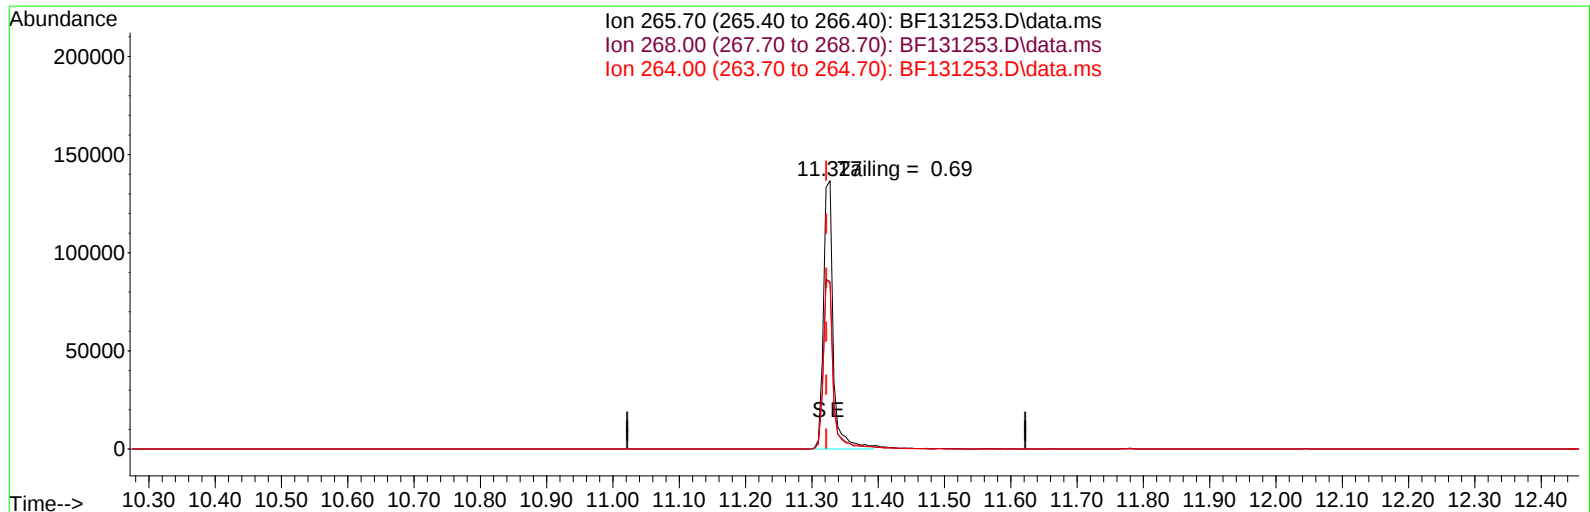

TIC: BF131253.D\data.ms

(70) Pentachlorophenol (C)




11.327min (+ 0.006) 325256.22 ng

response 142525

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.45
264.00	63.00	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
Data File : BF131253.D
Acq On : 16 Nov 2022 08:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 16 15:10:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 16 06:35:36 2022
Response via : Initial Calibration

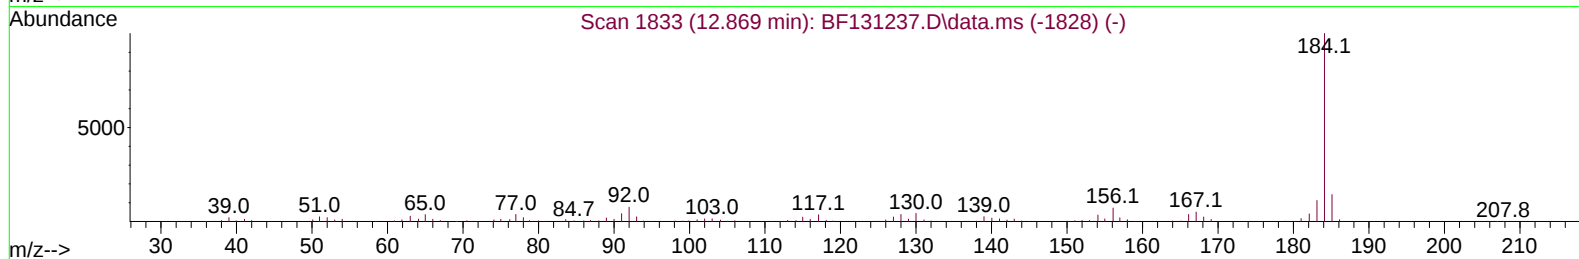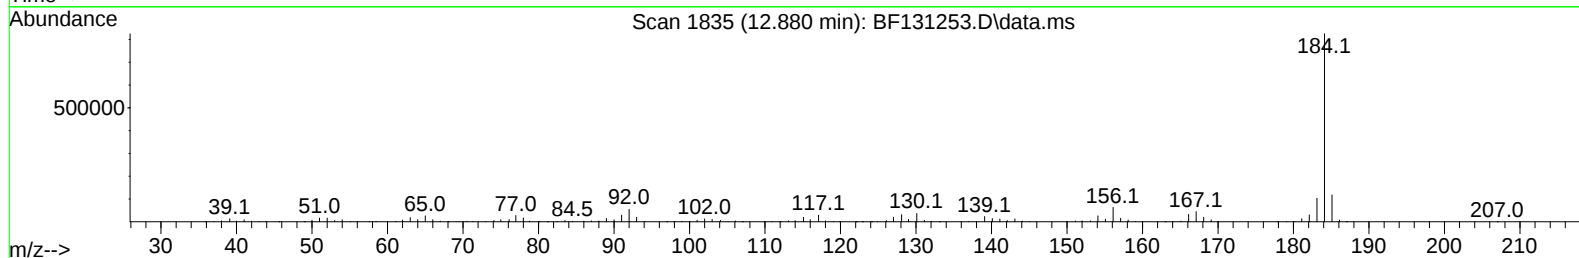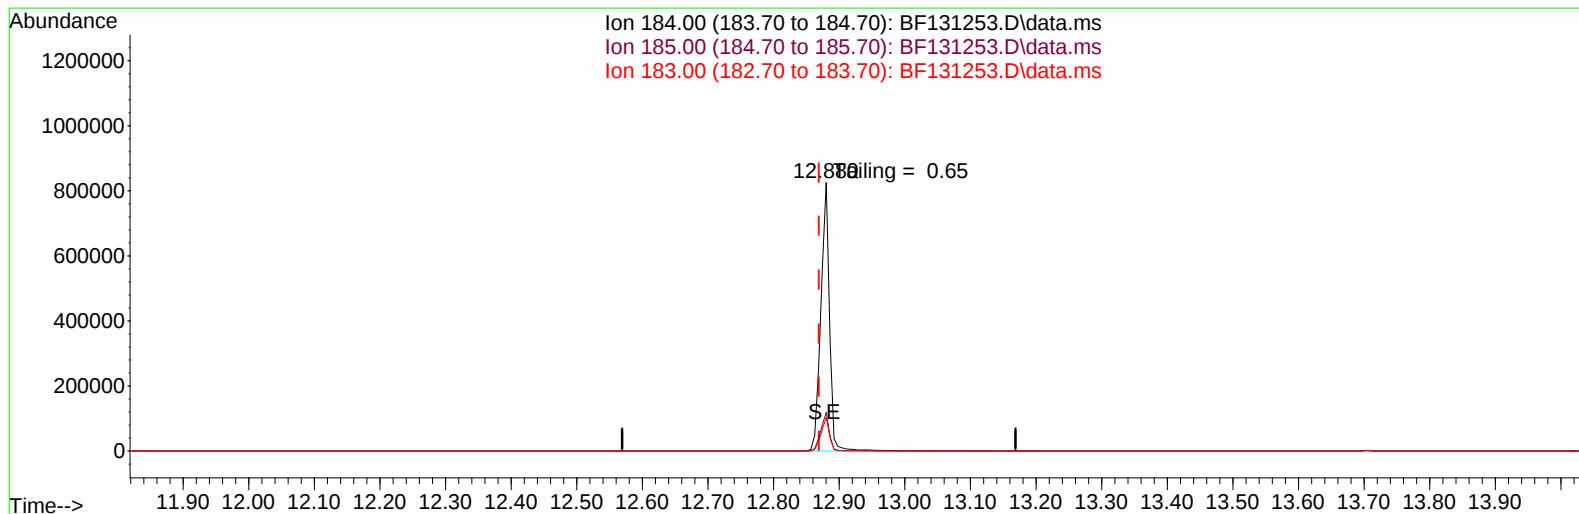

TIC: BF131253.D\data.ms

(77) Benzidine**12.880min (+ 0.011) 264531.36 ng****response 753953**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.36
183.00	11.20	12.53
0.00	0.00	0.00