

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
 Data File : BF131265.D
 Acq On : 16 Nov 2022 15:04
 Operator : CG\JU
 Sample : PB149098BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB149098BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF131265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.334	34	42	47	rVB	66781	90230	2.69%	0.461%
2	5.204	524	530	536	rBV	759047	925515	27.55%	4.734%
3	5.587	590	595	598	rBV	2117296	1994152	59.36%	10.199%
4	6.581	759	764	767	rBV	1764225	2009799	59.82%	10.279%
5	6.975	827	831	834	rBV	736344	599978	17.86%	3.069%
6	7.539	921	927	930	rBV	1798307	1899998	56.56%	9.717%
7	8.263	1045	1050	1053	rBV	929206	794670	23.65%	4.064%
8	9.345	1228	1234	1237	rBV	3644814	3347905	99.65%	17.123%
9	10.027	1345	1350	1353	rBV	1113813	919086	27.36%	4.701%
10	10.822	1480	1485	1488	rBV	1496377	1374536	40.91%	7.030%
11	11.527	1601	1605	1608	rBV	1082568	934678	27.82%	4.780%
12	13.127	1872	1877	1880	rBV	3622421	3359527	100.00%	17.182%
13	14.180	2052	2056	2060	rBV	848363	757083	22.54%	3.872%
14	15.727	2313	2319	2326	rBV	424863	545247	16.23%	2.789%




Sum of corrected areas: 19552404

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
Data File : BF131265.D
Acq On : 16 Nov 2022 15:04
Operator : CG\JU
Sample : PB149098BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149098BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

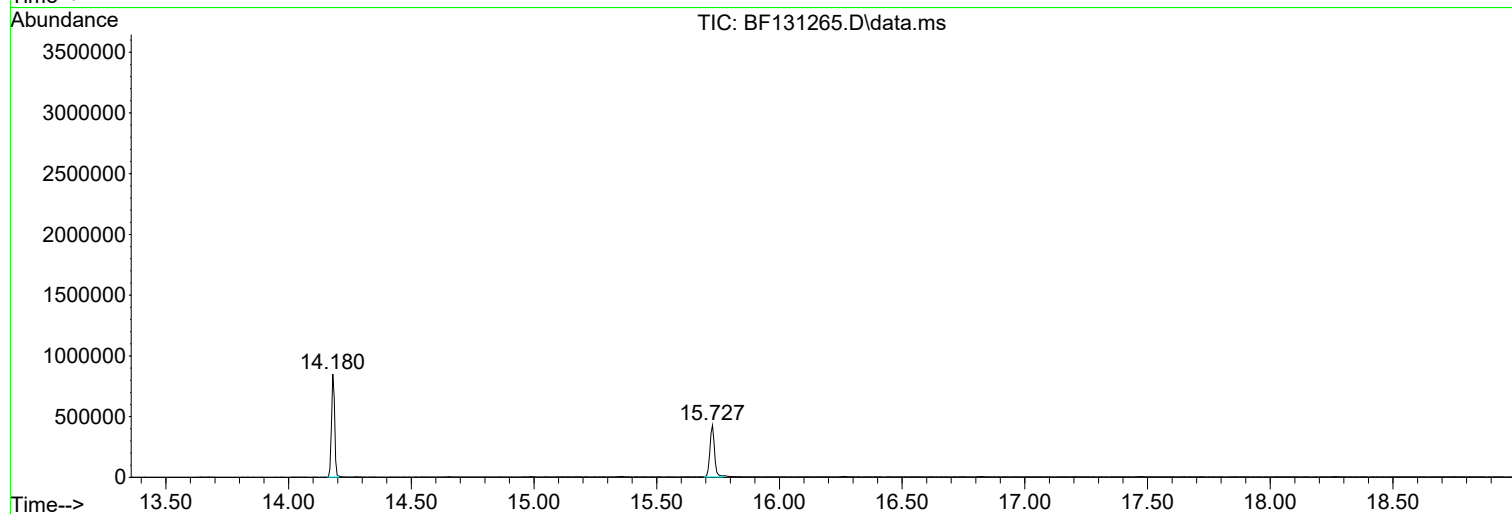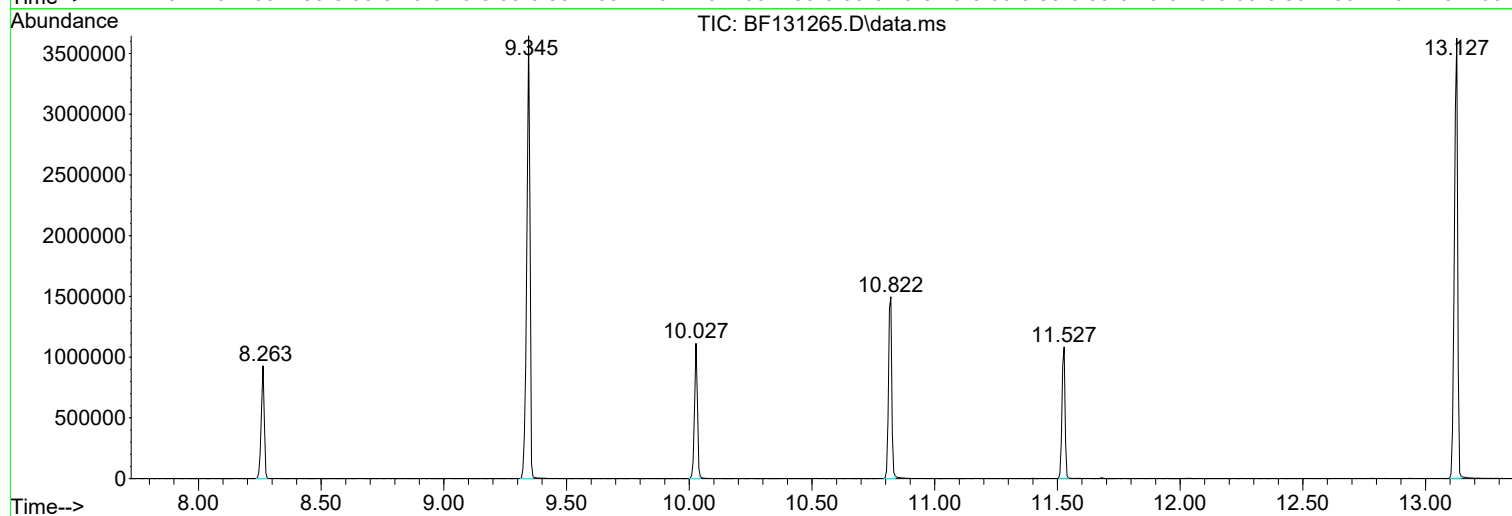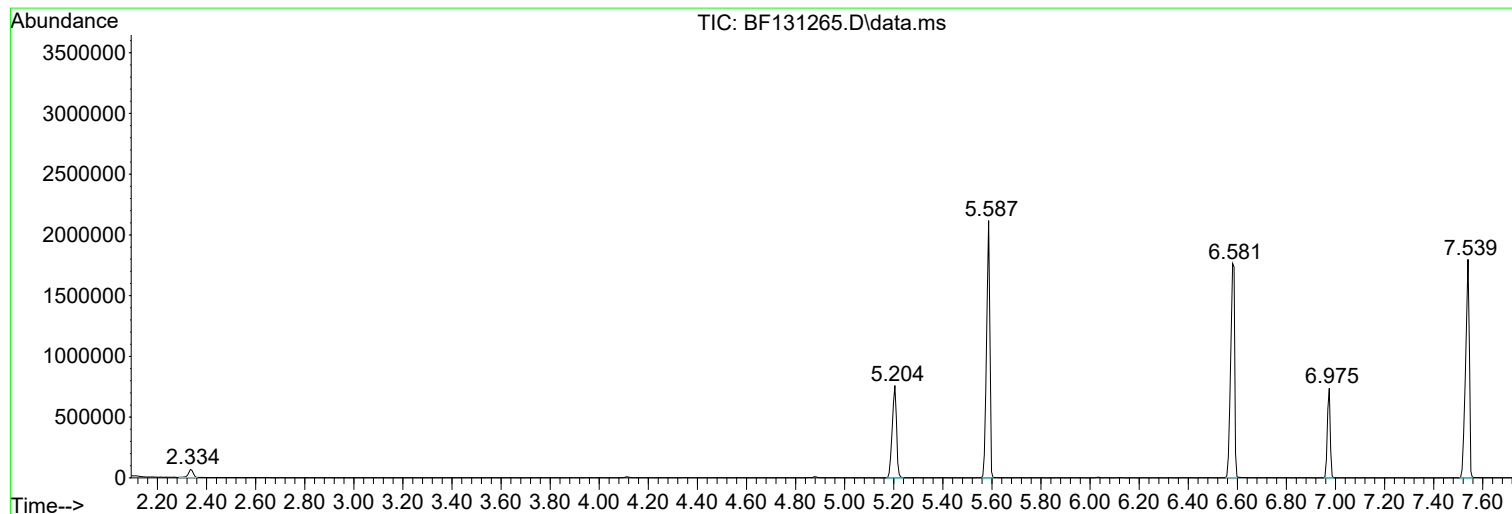

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
Data File : BF131265.D
Acq On : 16 Nov 2022 15:04
Operator : CG\JU
Sample : PB149098BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149098BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.334	3.01 ng	90230	1,4-Dichlorobenzene-d4	6.975

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	25
4			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	23
5			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	23

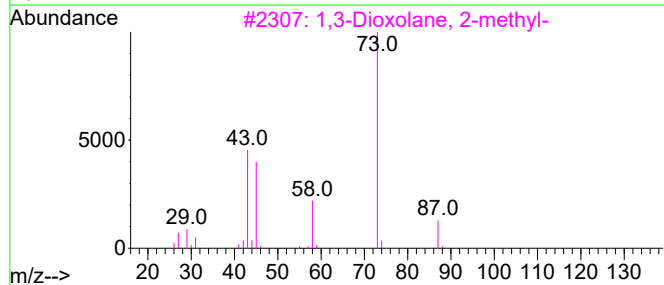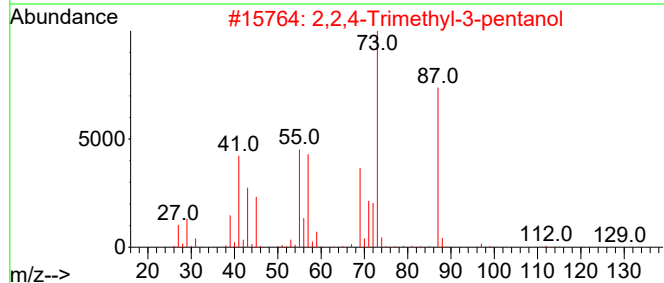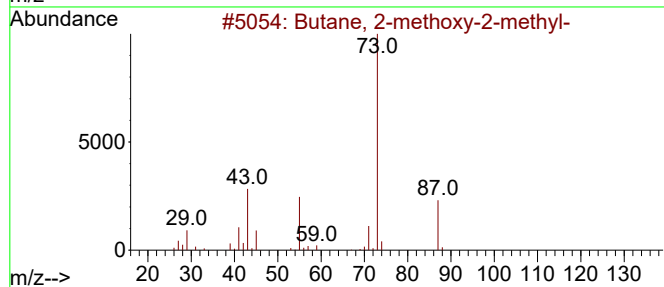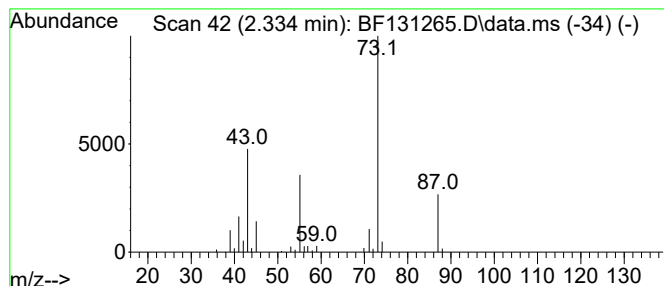

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
Data File : BF131265.D
Acq On : 16 Nov 2022 15:04
Operator : CG\JU
Sample : PB149098BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149098BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.204	30.85 ng	925515	1,4-Dichlorobenzene-d4	6.975

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	25
3			Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	23
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12
5			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	10

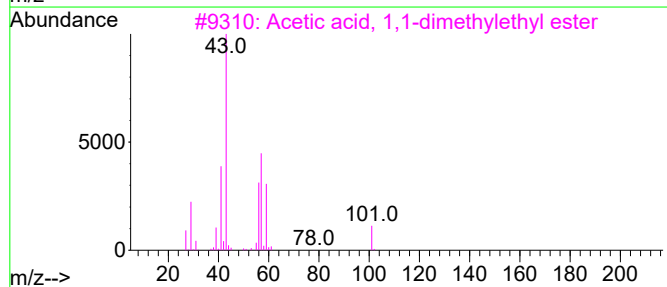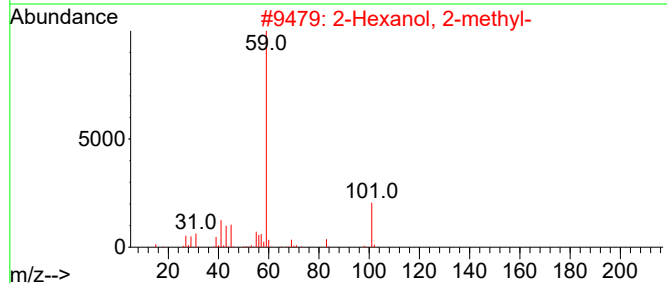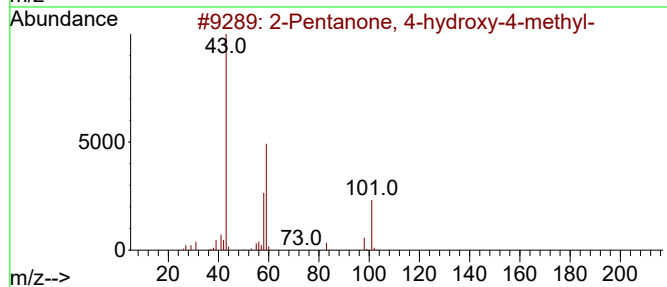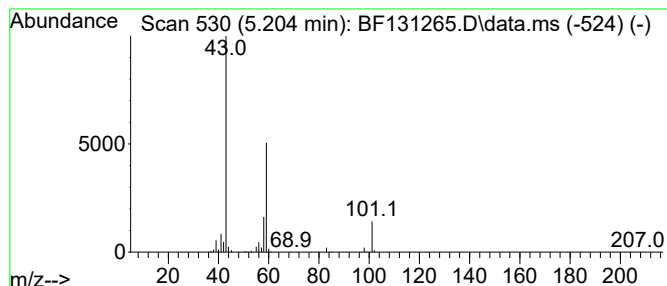

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
Data File : BF131265.D
Acq On : 16 Nov 2022 15:04
Operator : CG\JU
Sample : PB149098BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB149098BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.334	3.0	ng	90230	1	6.975	599978	20.0
2-Pentanone, 4-...	5.204	30.9	ng	925515	1	6.975	599978	20.0