
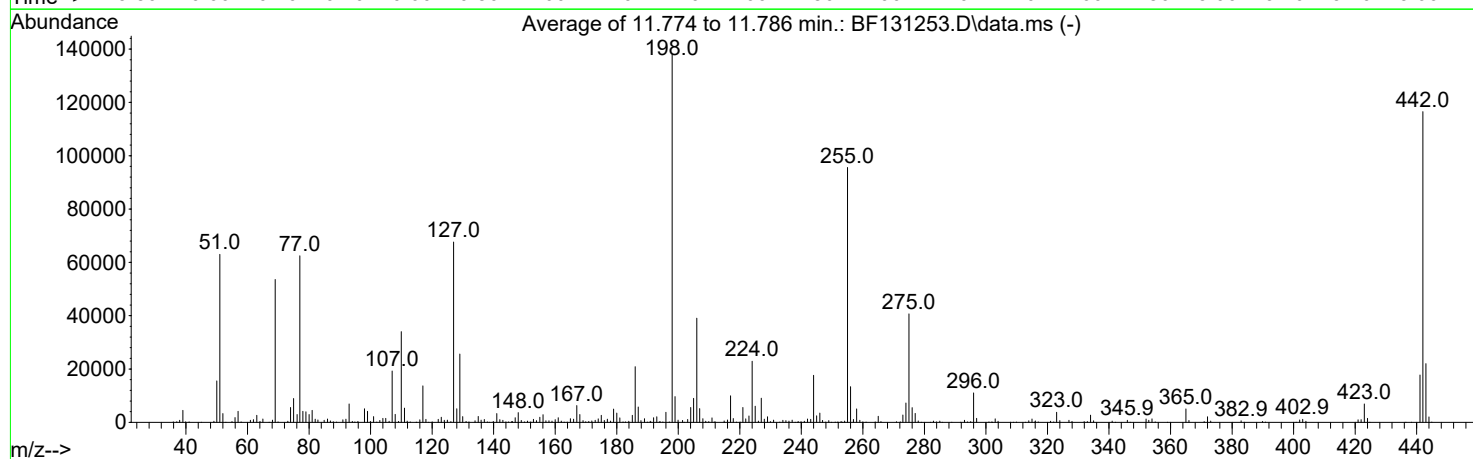


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
Data File : BF131253.D
Acq On : 16 Nov 2022 08:48
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 16 06:35:36 2022

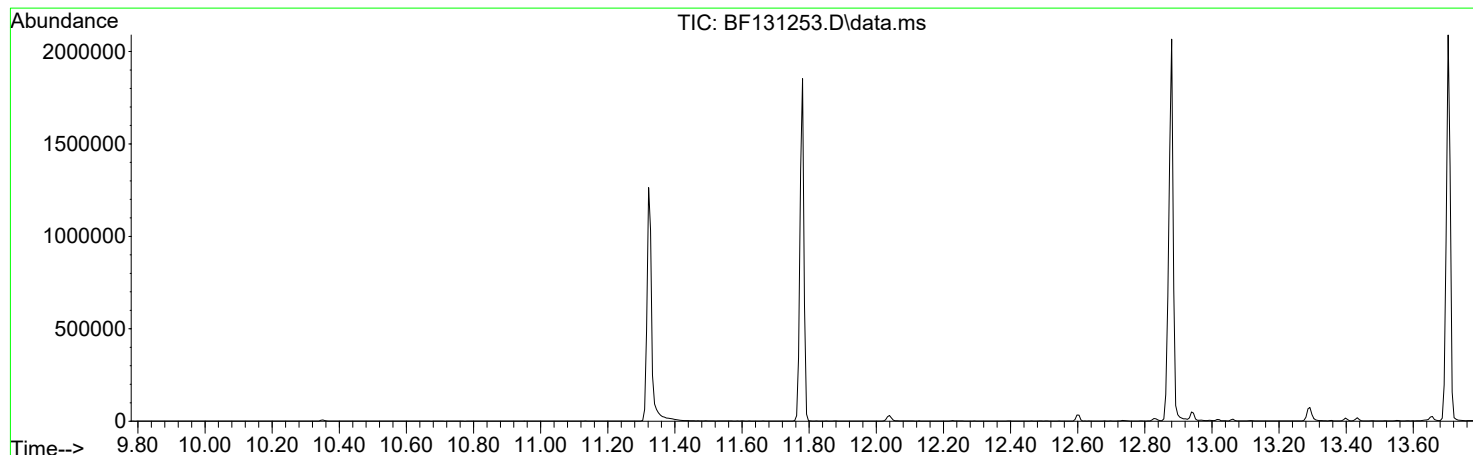

AutoFind: Scans 1647, 1648, 1649; Background Corrected with Scan 1641

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	45.7	63029	PASS
68	69	0.00	2	1.6	852	PASS
69	198	0.00	100	38.8	53591	PASS
70	69	0.00	2	0.4	202	PASS
127	198	10	80	49.0	67653	PASS
197	198	0.00	2	0.1	189	PASS
198	198	100	100	100.0	137968	PASS
199	198	5	9	7.0	9648	PASS
275	198	10	60	29.5	40680	PASS
365	198	1	100	3.7	5067	PASS
441	198	0.01	100	12.9	17788	PASS
442	442	50	100	100.0	116523	PASS
443	442	15	24	18.9	22043	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/16/2022	BNA_F	<u>BF131253.D</u>
Compound Name	Response	Retention Time
DDT	316796	13.704
DDD	5370	13.398
DDE	1319	13.057
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6689	323485	2.07

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
 Data File : BF131253.D
 Acq On : 16 Nov 2022 08:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 16 15:10:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 06:35:36 2022
 Response via : Initial Calibration

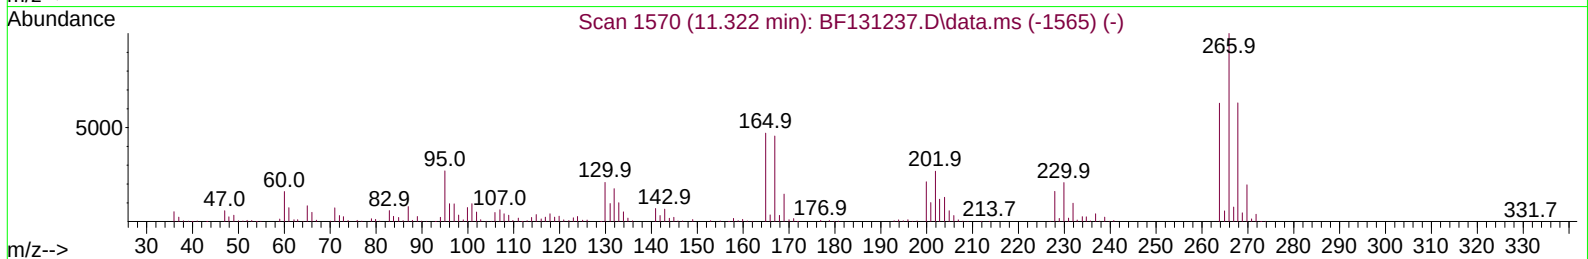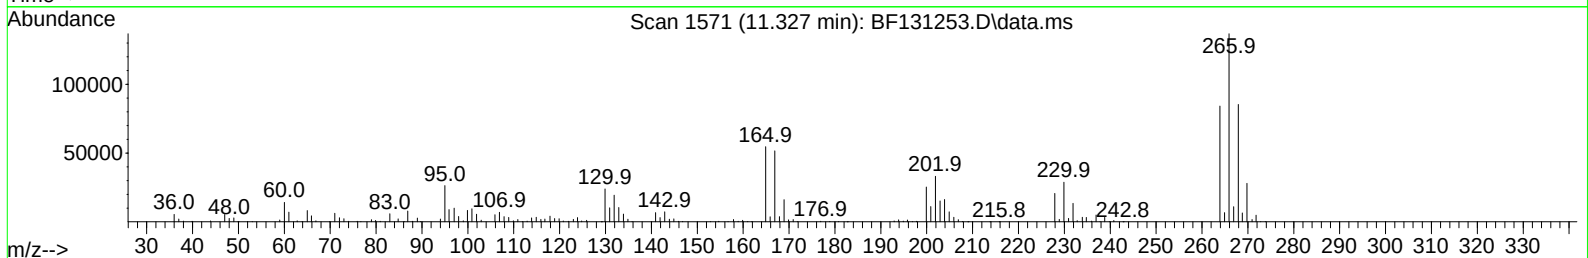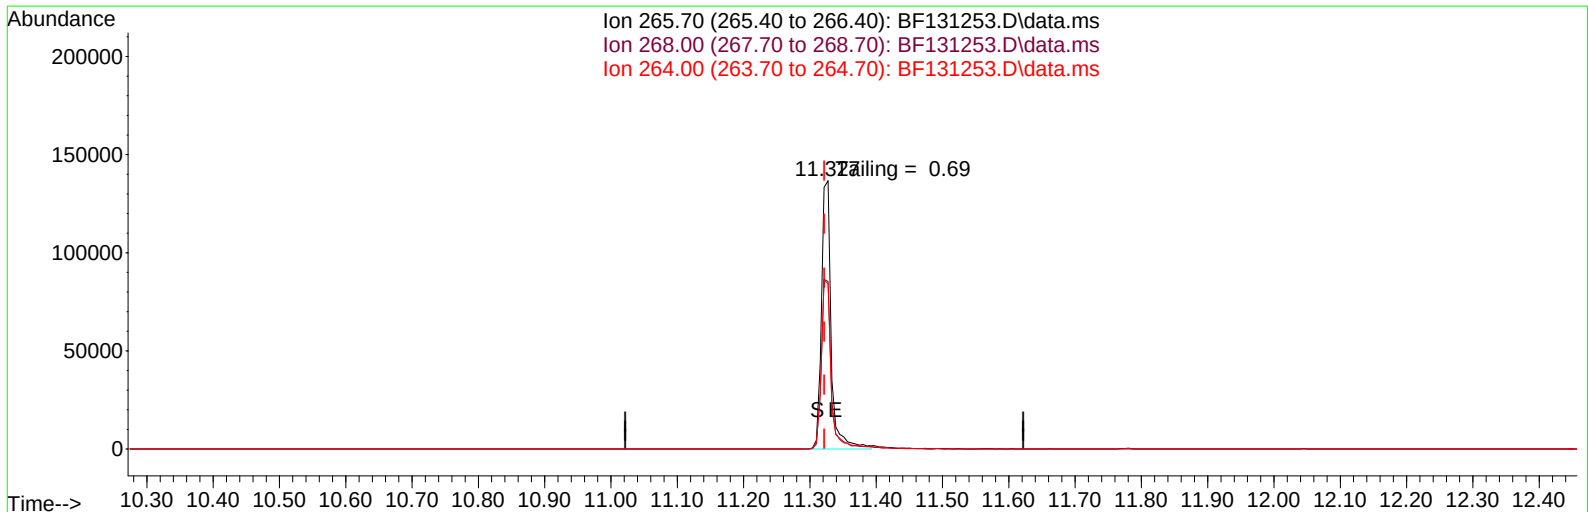

TIC: BF131253.D\data.ms

(70) Pentachlorophenol (C)

11.327min (+ 0.006) 325256.22 ng




response 142525

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.45
264.00	63.00	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111622\
 Data File : BF131253.D
 Acq On : 16 Nov 2022 08:48
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 16 15:10:07 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 16 06:35:36 2022
 Response via : Initial Calibration

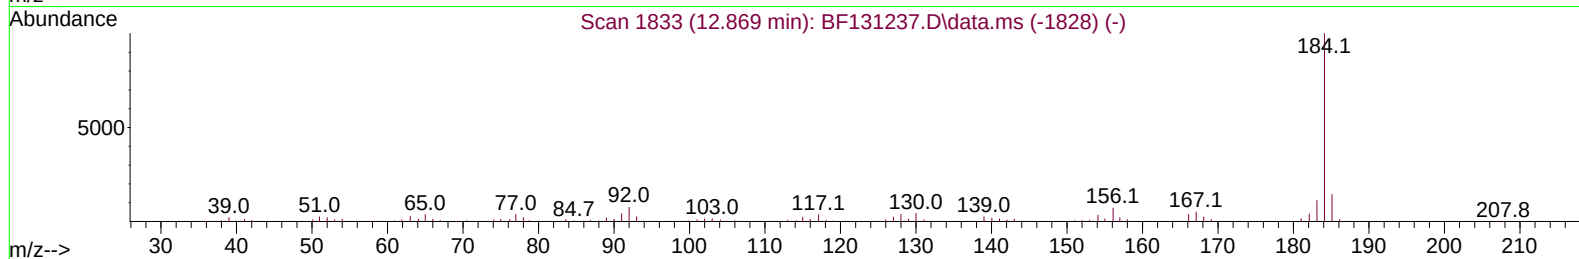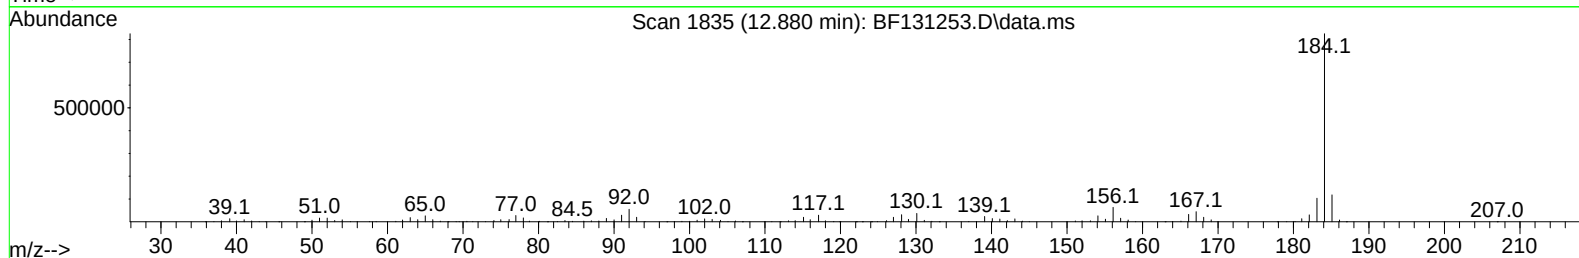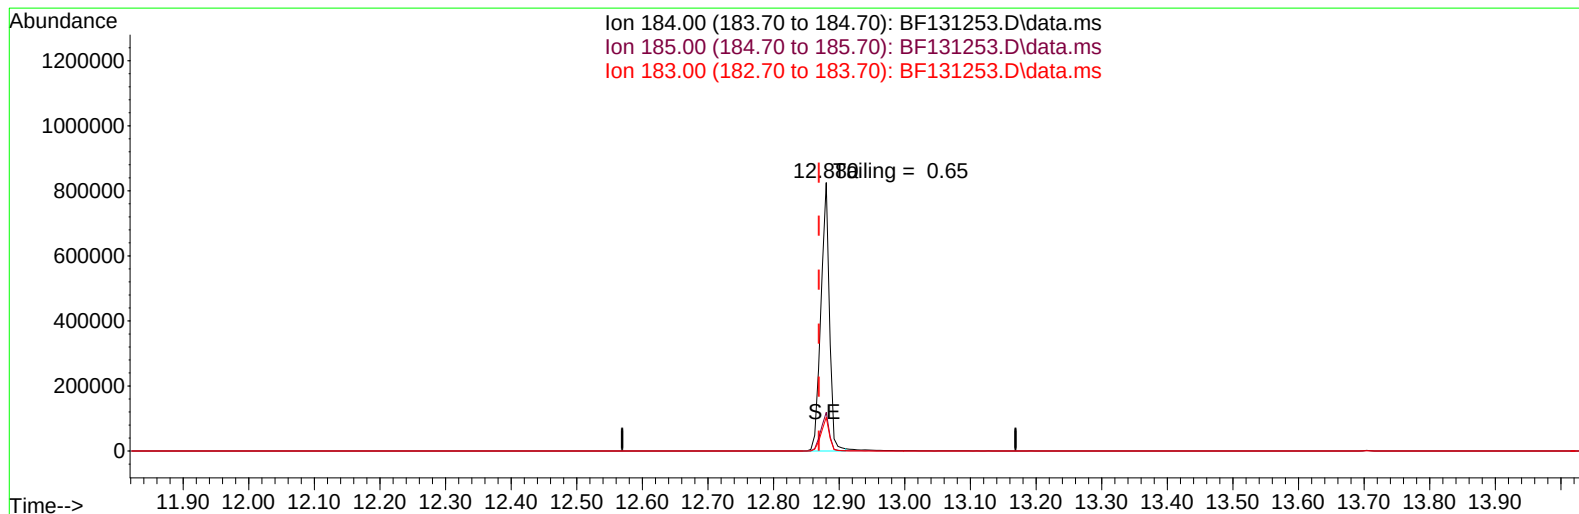

TIC: BF131253.D\data.ms

(77) Benzidine

12.880min (+ 0.011) 264531.36 ng

response 753953

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.36
183.00	11.20	12.53
0.00	0.00	0.00