

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111624\
 Data File : BF140418.D
 Acq On : 16 Nov 2024 10:02
 Operator : RC/JU
 Sample : PB164993BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB164993BL

Quant Time: Nov 18 00:04:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Nov 13 14:40:06 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	168054	20.000	ng	0.00
21) Naphthalene-d8	8.151	136	642488	20.000	ng	0.00
39) Acenaphthene-d10	9.910	164	365710	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188	717042	20.000	ng	0.00
76) Chrysene-d12	14.051	240	477442	20.000	ng	0.00
86) Perylene-d12	15.551	264	394046	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.522	112	1170263	118.896	ng	0.03
7) Phenol-d6	6.516	99	1523103	114.215	ng	0.01
23) Nitrobenzene-d5	7.434	82	1012557	82.114	ng	0.00
42) 2,4,6-Tribromophenol	10.704	330	458929	126.194	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	1866939	82.065	ng	0.00
79) Terphenyl-d14	12.992	244	2276360	82.760	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.434	70	136237	16.915	ng	# 77
25) Isophorone	7.434	82	1007044	46.079	ng	# 66
51) 2,6-Dinitrotoluene	9.910	165	47515	8.743	ng	# 22
57) 2,4-Dinitrotoluene	9.910	165	47515	6.643	ng	# 20
67) 4-Bromophenyl-phenylether	10.704	248	29681	4.141	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111624\
Data File : BF140418.D
Acq On : 16 Nov 2024 10:02
Operator : RC/JU
Sample : PB164993BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB164993BL


Quant Time: Nov 18 00:04:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

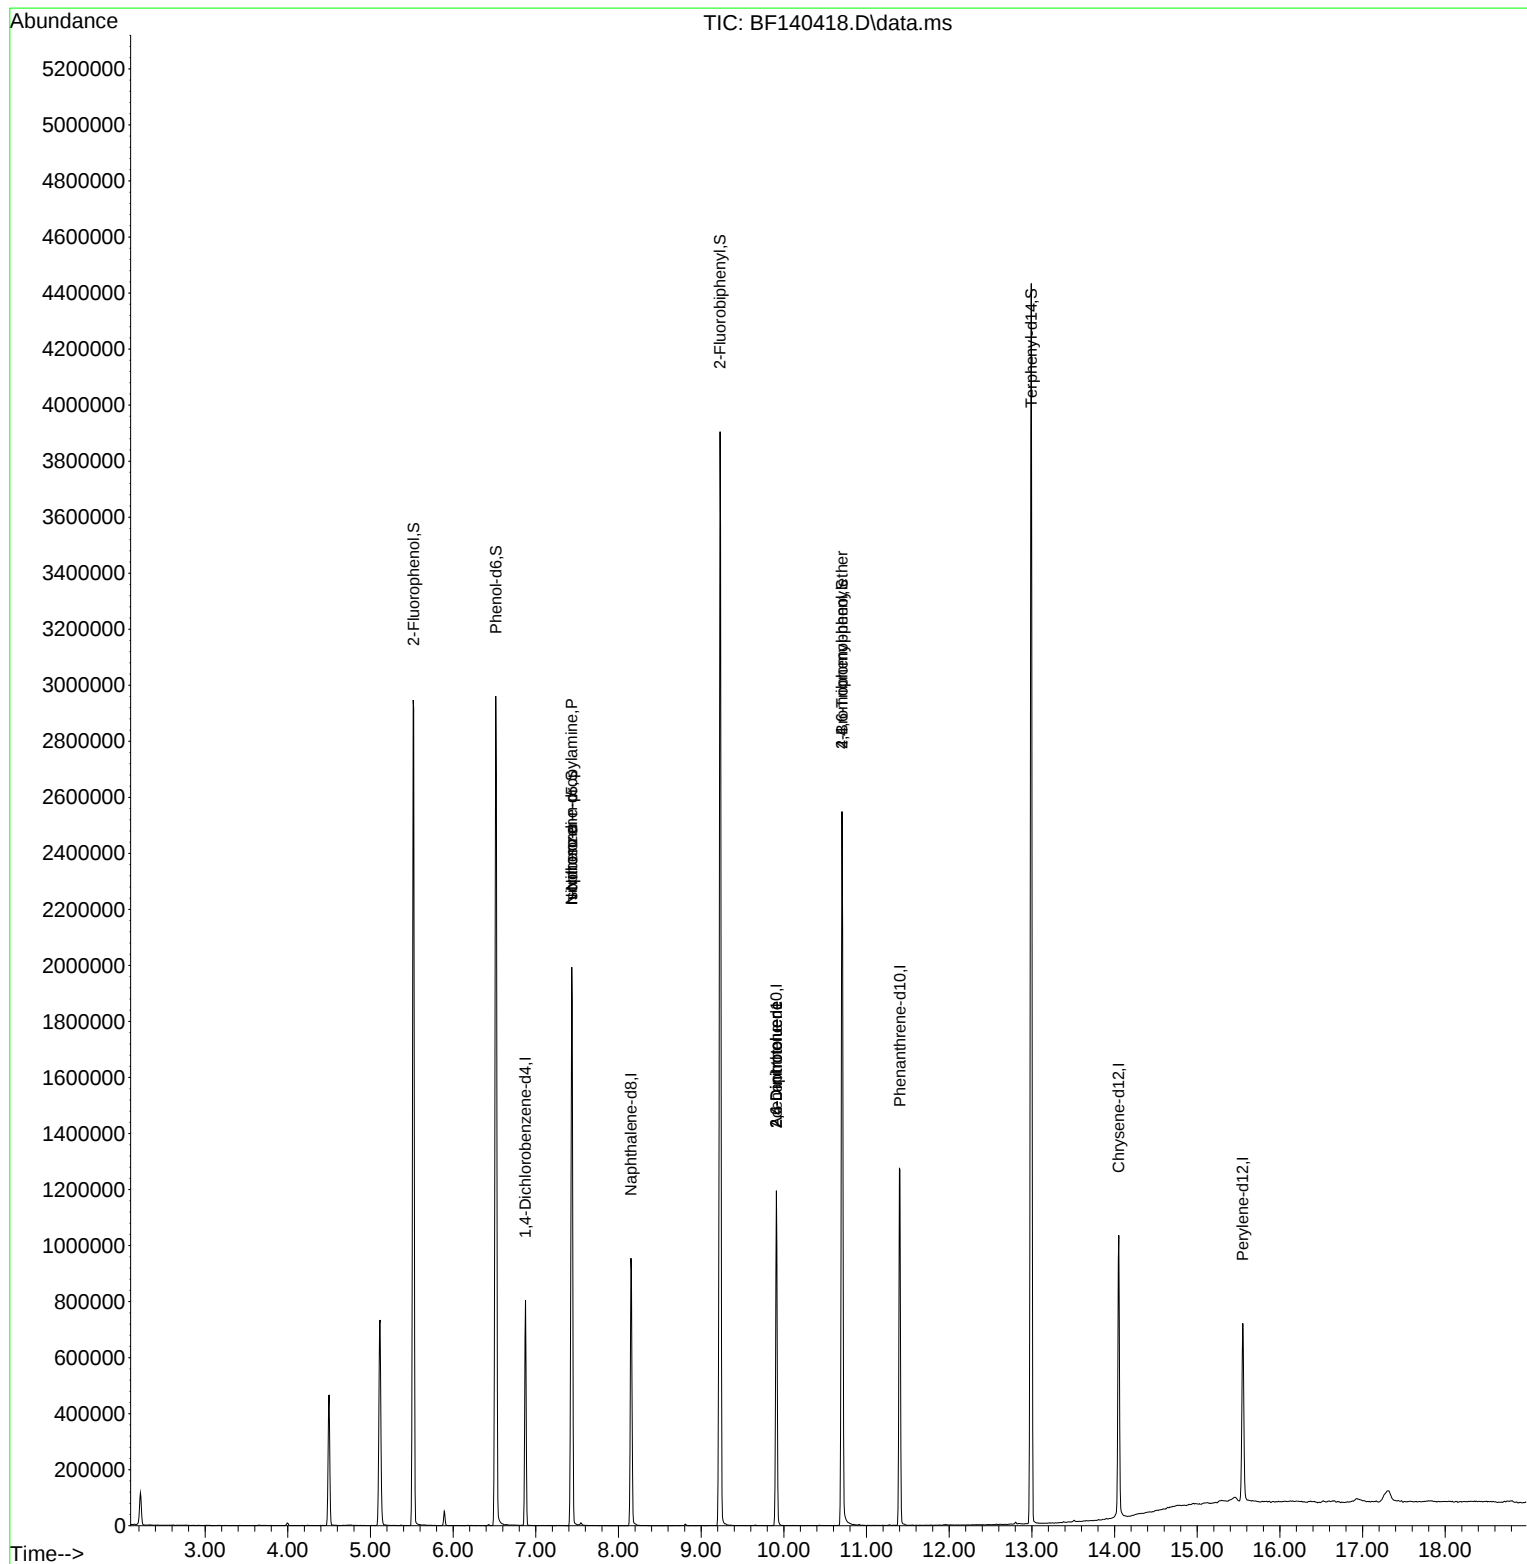






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 813
Delta R.T. -0.006 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02

Instrument :
BNA_F
ClientSampleId :
PB164993BL



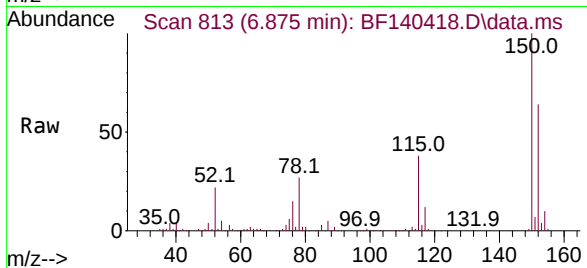



Tgt Ion:152 Resp: 168054
Ion Ratio Lower Upper
152 100
150 155.6 127.4 191.0
115 59.8 47.4 71.2

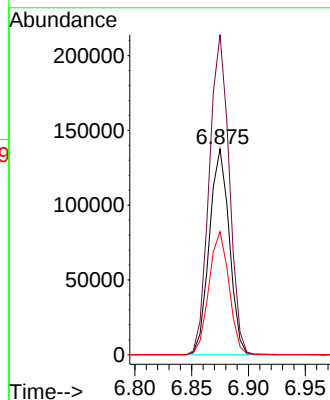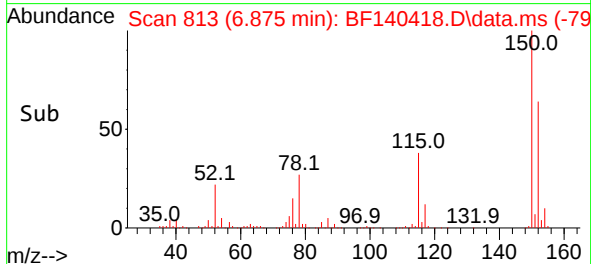

#5
2-Fluorophenol
Concen: 118.896 ng
RT: 5.522 min Scan# 583
Delta R.T. 0.029 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02

Tgt Ion:112 Resp: 1170263
Ion Ratio Lower Upper
112 100
64 60.9 49.2 73.8
63 31.7 25.6 38.4


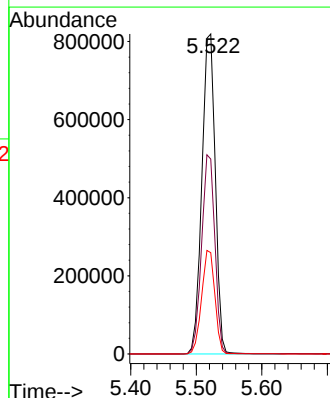
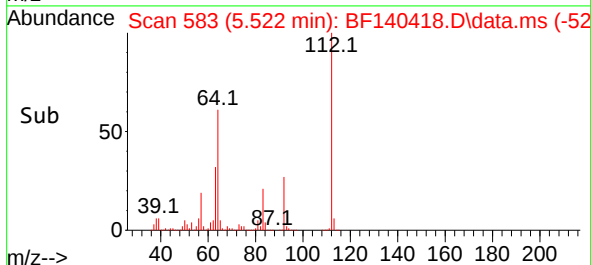
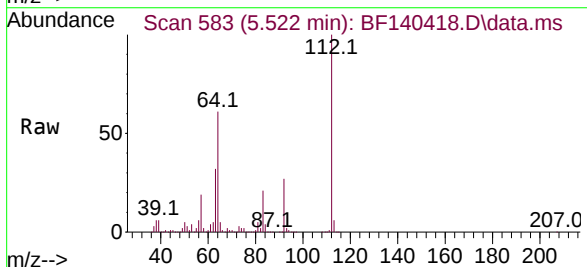




#7
Phenol-d6
Concen: 114.215 ng
RT: 6.516 min Scan# 71
Delta R.T. 0.012 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02




Instrument :
BNA_F
ClientSampleId :
PB164993BL


Tgt Ion: 99 Resp: 1523103
Ion Ratio Lower Upper
99 100
42 18.8 15.1 22.7
71 36.3 27.9 41.9

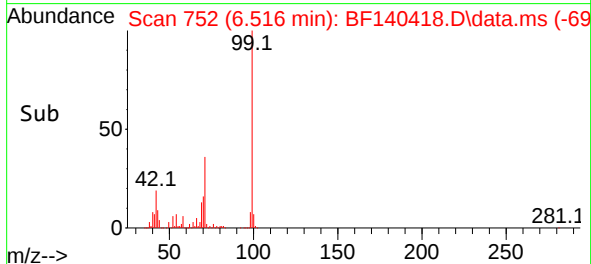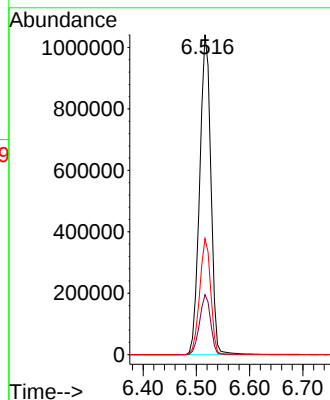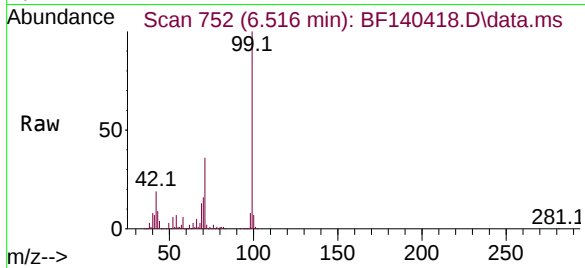

#19
n-Nitroso-di-n-propylamine
Concen: 16.915 ng
RT: 7.434 min Scan# 908
Delta R.T. 0.141 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02

Tgt Ion: 70 Resp: 136237
Ion Ratio Lower Upper
70 100
42 46.3 46.8 70.2#
101 0.0 7.5 11.3#
130 2.1 16.3 24.5#



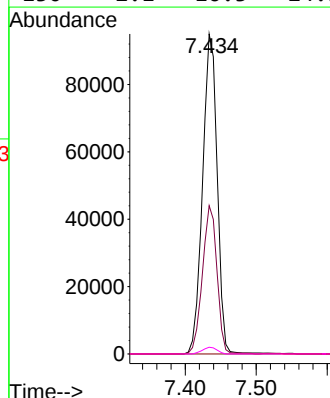
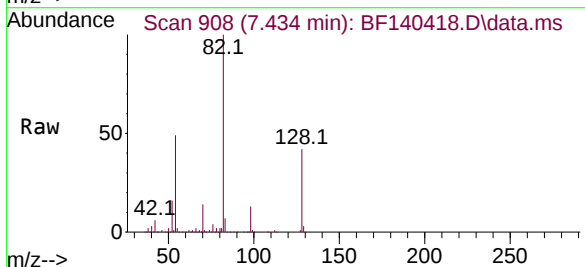




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.151 min Scan# 1031
Delta R.T. -0.006 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02




Instrument :
BNA_F
ClientSampleId :
PB164993BL


Tgt Ion:136 Resp: 642488
Ion Ratio Lower Upper
136 100
137 10.8 8.7 13.1
54 7.8 6.5 9.7
68 6.2 5.0 7.6

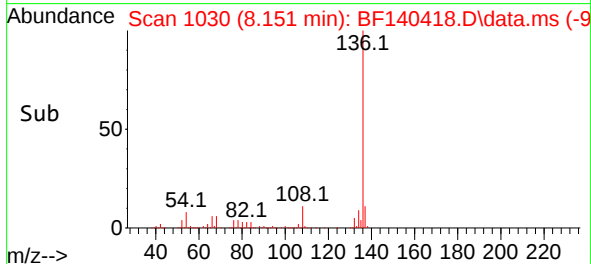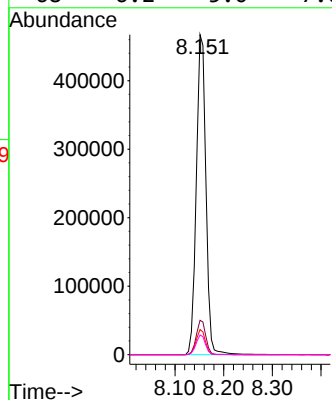

#23
Nitrobenzene-d5
Concen: 82.114 ng
RT: 7.434 min Scan# 908
Delta R.T. -0.006 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02

Tgt Ion: 82 Resp: 1012557
Ion Ratio Lower Upper
82 100
128 41.7 33.3 49.9
54 49.1 39.8 59.8


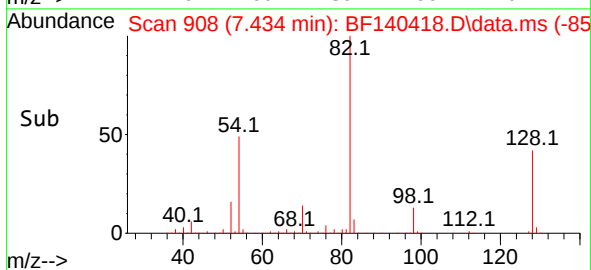
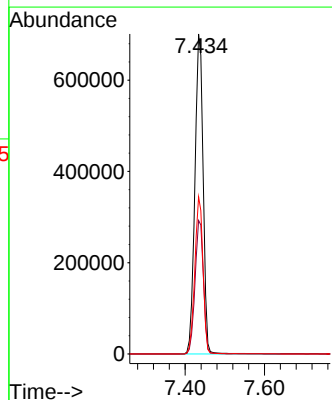
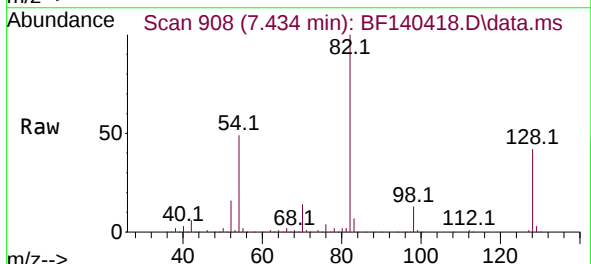




#25
Isophorone
Concen: 46.079 ng
RT: 7.434 min Scan# 90
Delta R.T. -0.265 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02




Instrument :
BNA_F
ClientSampleId :
PB164993BL


Tgt Ion: 82 Resp: 1007044
Ion Ratio Lower Upper
82 100
95 0.0 5.9 8.9#
138 0.0 13.4 20.2#

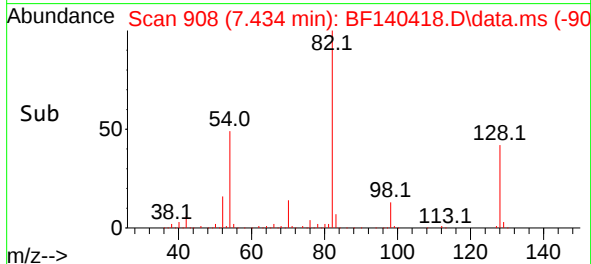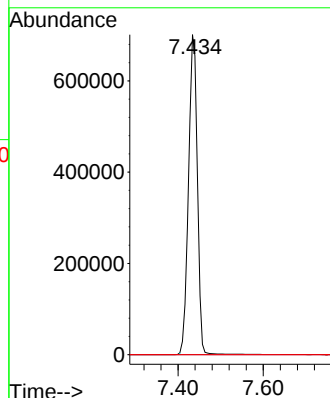

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02


Tgt Ion:164 Resp: 365710
Ion Ratio Lower Upper
164 100
162 100.0 79.8 119.8
160 44.6 35.4 53.0

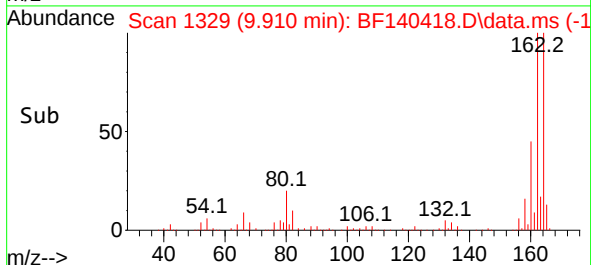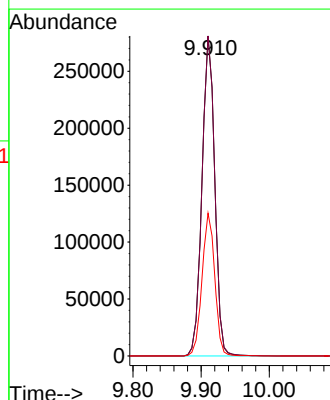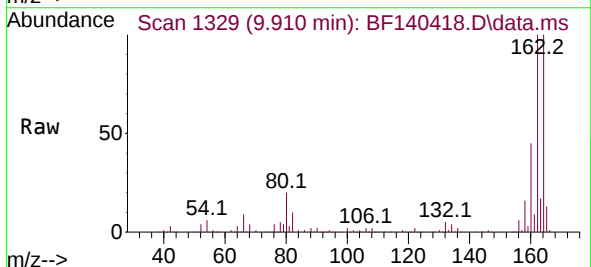






#42
2,4,6-Tribromophenol
Concen: 126.194 ng
RT: 10.704 min Scan# 1464
Delta R.T. 0.000 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02

Instrument :
BNA_F
ClientSampleId :
PB164993BL



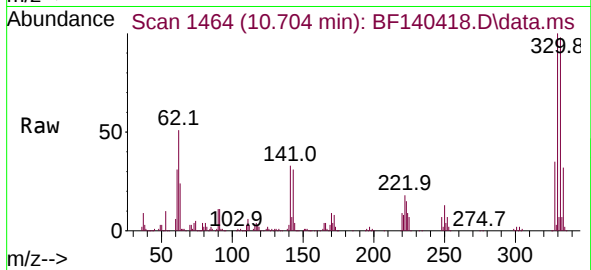



Tgt Ion: 330 Resp: 458929
Ion Ratio Lower Upper
330 100
332 97.3 75.9 113.9
141 32.3 26.9 40.3

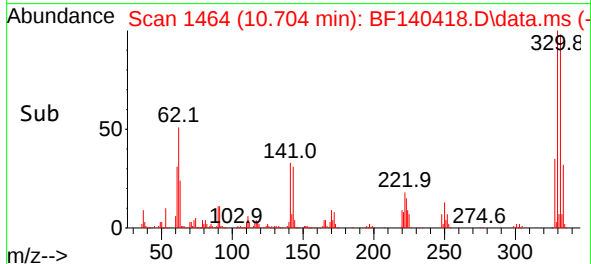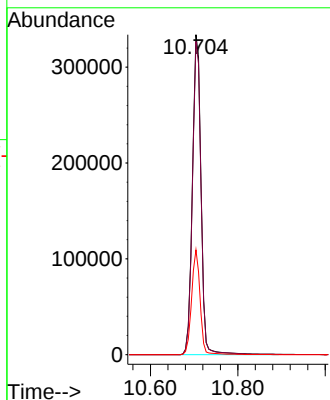

#45
2-Fluorobiphenyl
Concen: 82.065 ng
RT: 9.228 min Scan# 1213
Delta R.T. -0.006 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02

Tgt Ion: 172 Resp: 1866939
Ion Ratio Lower Upper
172 100
171 35.5 28.5 42.7
170 23.8 19.1 28.7


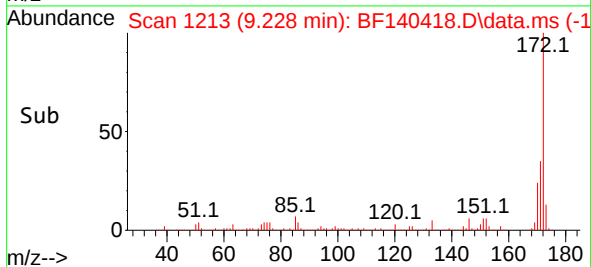
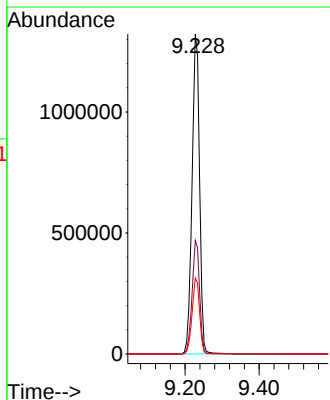
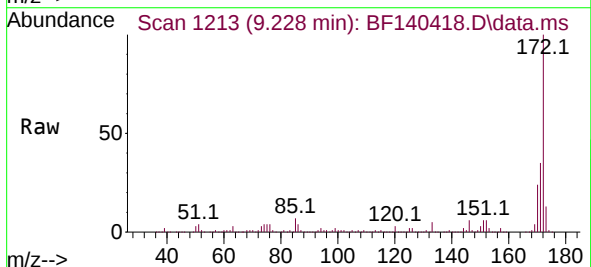




#51
2,6-Dinitrotoluene
Concen: 8.743 ng
RT: 9.910 min Scan# 11
Delta R.T. 0.212 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02




Instrument :
BNA_F
ClientSampleId :
PB164993BL


Tgt Ion:165 Resp: 47515
Ion Ratio Lower Upper
165 100
63 1.2 47.6 71.4#
89 1.2 48.1 72.1#

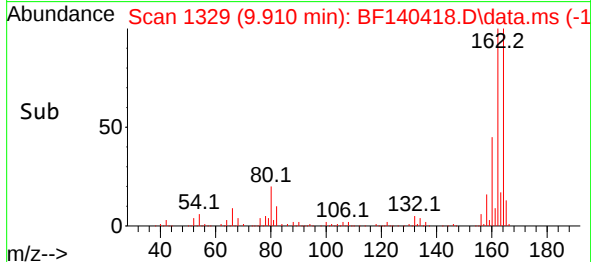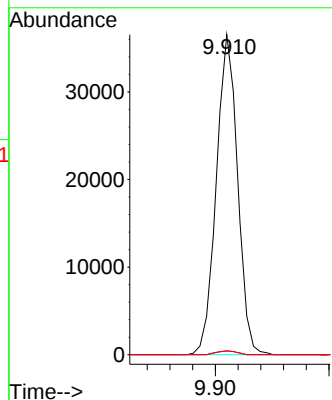

#57
2,4-Dinitrotoluene
Concen: 6.643 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.194 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02

Tgt Ion:165 Resp: 47515
Ion Ratio Lower Upper
165 100
63 1.2 39.4 59.0#
89 1.2 62.4 93.6#
182 0.0 2.1 3.1#


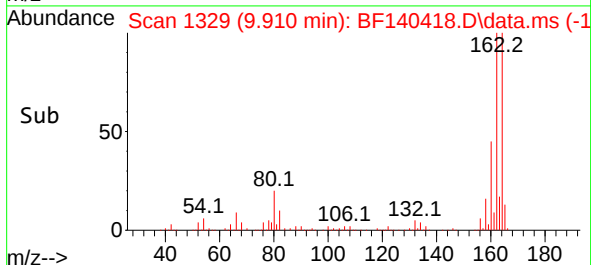
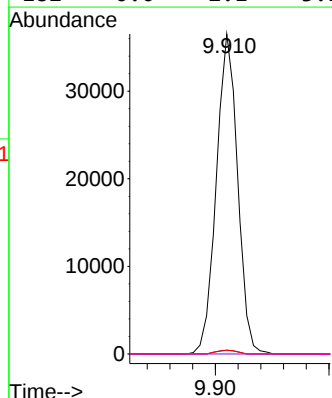
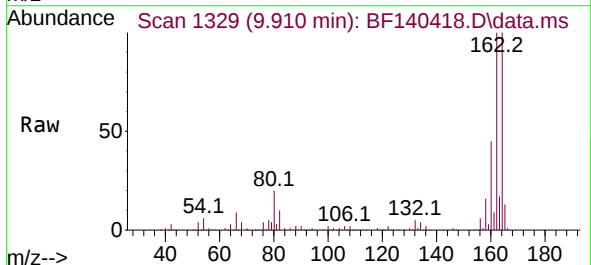




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.404 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02




Instrument :
BNA_F
ClientSampleId :
PB164993BL


Tgt Ion:188 Resp: 717042
Ion Ratio Lower Upper
188 100
94 8.9 7.6 11.4
80 9.6 8.0 12.0

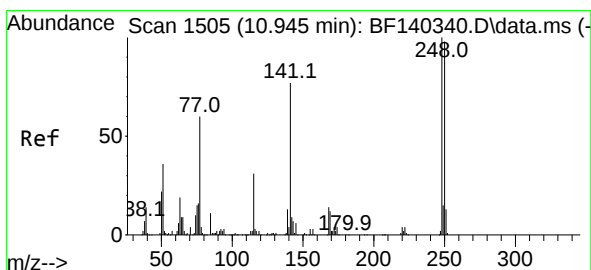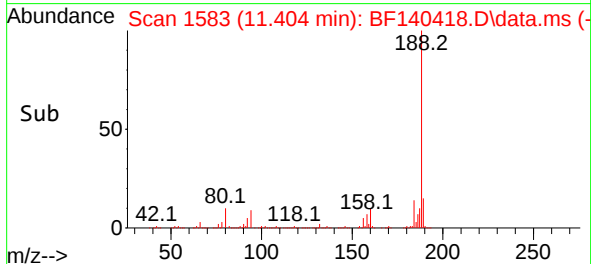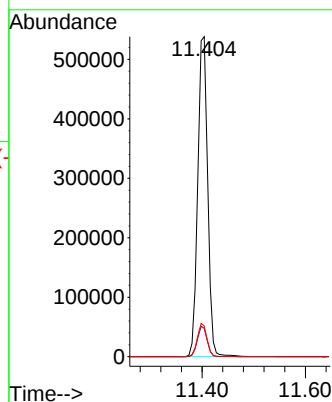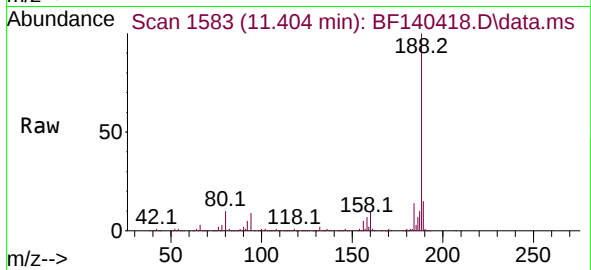

#67
4-Bromophenyl-phenylether
Concen: 4.141 ng
RT: 10.704 min Scan# 1464
Delta R.T. -0.241 min
Lab File: BF140418.D
Acq: 16 Nov 2024 10:02

Tgt Ion:248 Resp: 29681
Ion Ratio Lower Upper
248 100
250 199.5 77.9 116.9#
141 496.4 61.8 92.6#

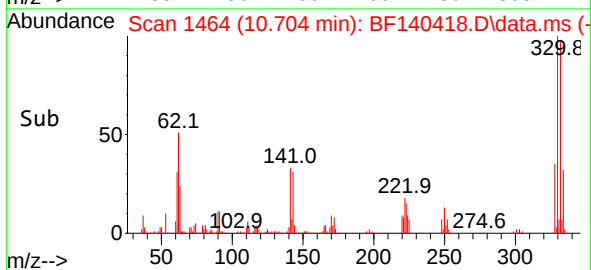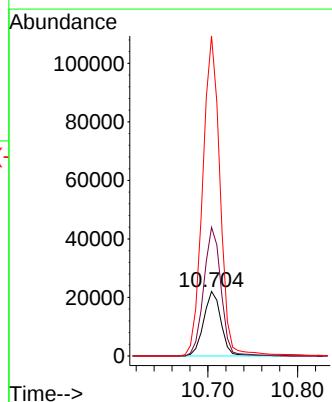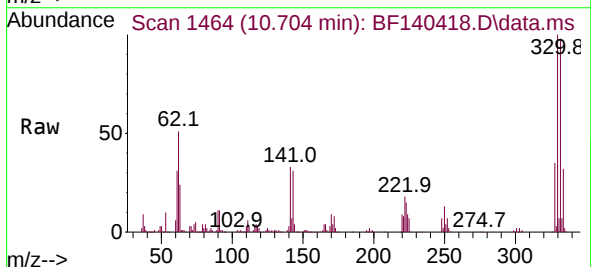



#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.051 min Scan# 2033

Delta R.T. 0.000 min

Lab File: BF140418.D

Acq: 16 Nov 2024 10:02

Instrument :

BNA_F

ClientSampleId :

PB164993BL





Tgt Ion:240 Resp: 477442

Ion Ratio Lower Upper

240 100

120 10.3 8.8 13.2

236 26.6 20.9 31.3

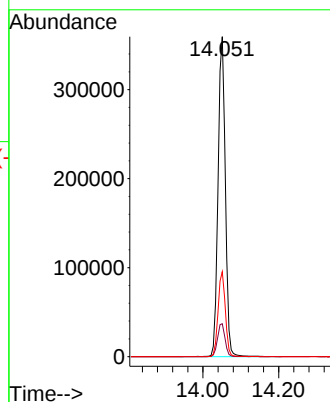

#79

Terphenyl-d14

Concen: 82.760 ng

RT: 12.992 min Scan# 1853

Delta R.T. 0.006 min

Lab File: BF140418.D

Acq: 16 Nov 2024 10:02




Tgt Ion:244 Resp: 2276360


Ion Ratio Lower Upper

244 100

212 7.2 5.8 8.8

122 10.5 8.8 13.2

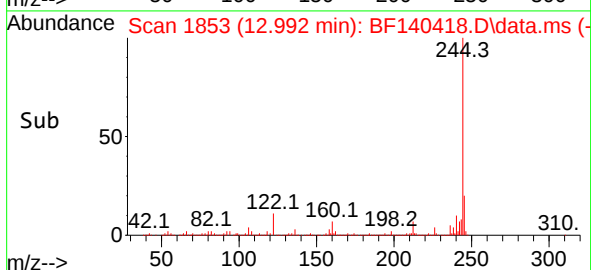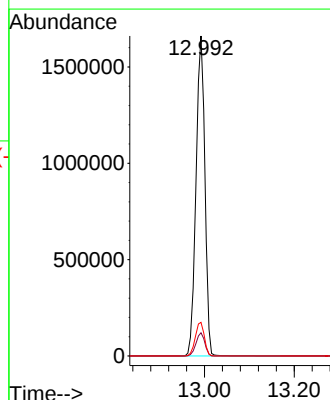



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.551 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BF140418.D
 Acq: 16 Nov 2024 10:02

Instrument :
 BNA_F
 ClientSampleId :
 PB164993BL

Tgt Ion:264 Resp: 394046
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.2 28.8
 265 21.6 17.1 25.7

