

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111624\
Data File : BF140424.D
Acq On : 16 Nov 2024 12:46
Operator : RC/JU
Sample : P4833-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Time: Nov 18 00:05:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.875	152	108709	20.000	ng	0.00
21) Naphthalene-d8	8.151	136	405539	20.000	ng	0.00
39) Acenaphthene-d10	9.910	164	218341	20.000	ng	0.00
64) Phenanthrene-d10	11.398	188	395523	20.000	ng	0.00
76) Chrysene-d12	14.045	240	229407	20.000	ng	0.00
86) Perylene-d12	15.533	264	248406	20.000	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	867579	136.262	ng	0.02
7) Phenol-d6	6.516	99	1099751	127.489	ng	0.01
23) Nitrobenzene-d5	7.434	82	746883	95.958	ng	0.00
42) 2,4,6-Tribromophenol	10.704	330	309978	142.766	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	1322684	97.383	ng	0.00
79) Terphenyl-d14	12.986	244	1347906	101.988	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111624\
Data File : BF140424.D
Acq On : 16 Nov 2024 12:46
Operator : RC/JU
Sample : P4833-08
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-2

Quant Time: Nov 18 00:05:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration




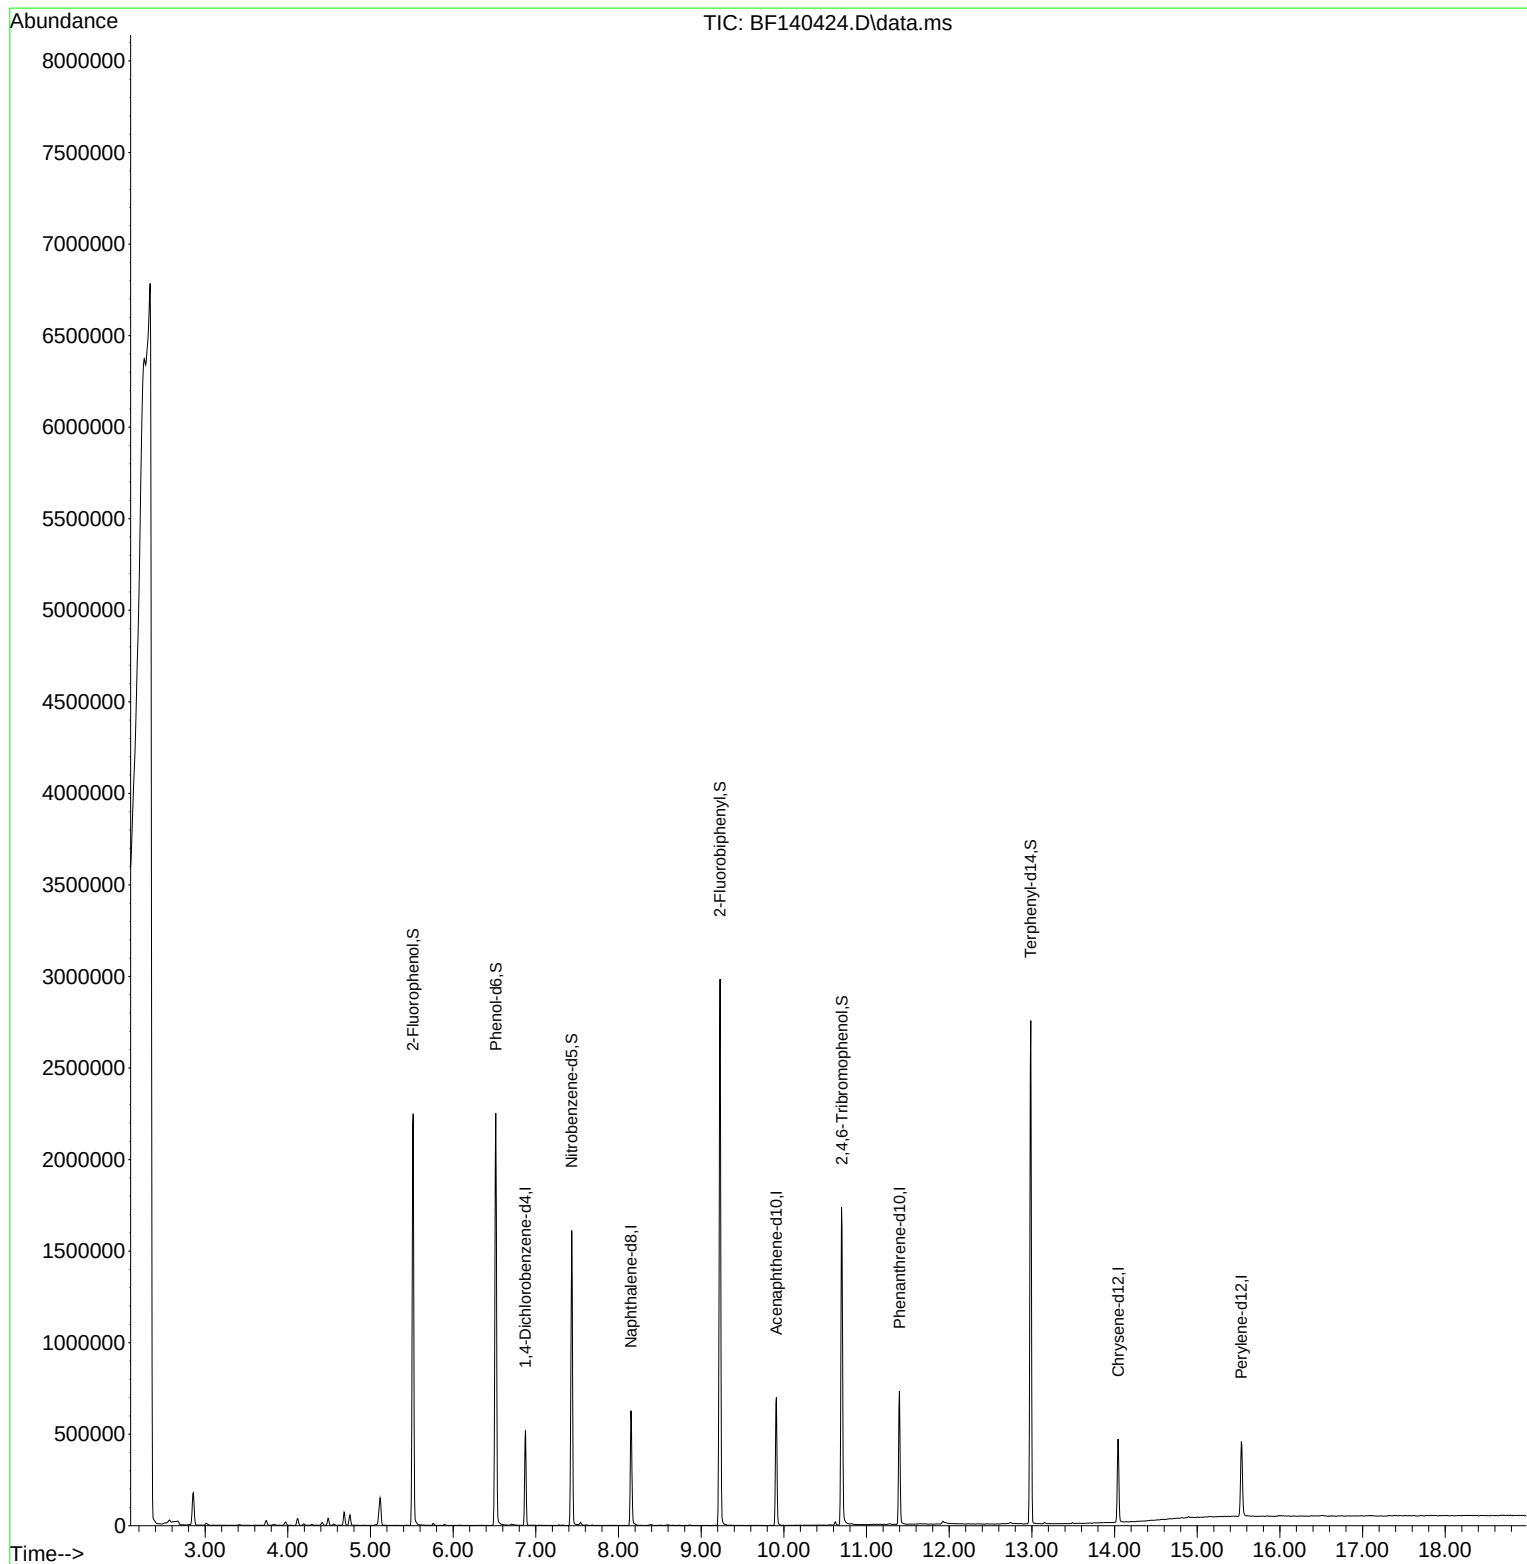


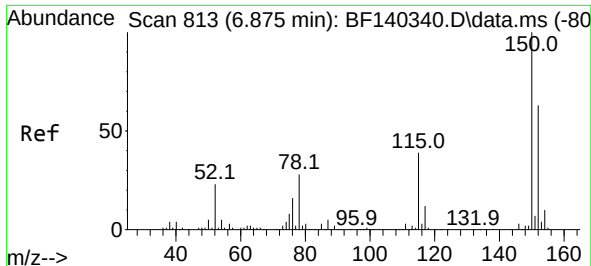

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.875 min Scan# 813
Delta R.T. -0.006 min
Lab File: BF140424.D
Acq: 16 Nov 2024 12:46




Instrument :
BNA_F
ClientSampleId :
TP-2


Tgt Ion:152 Resp: 108709
Ion Ratio Lower Upper
152 100
150 155.1 127.4 191.0
115 59.6 47.4 71.2

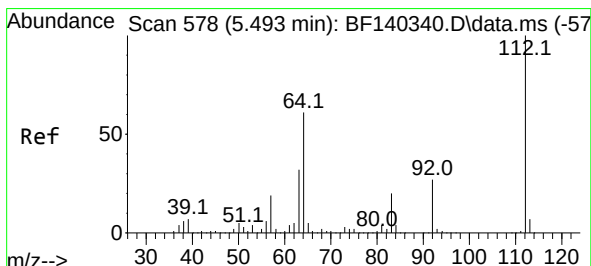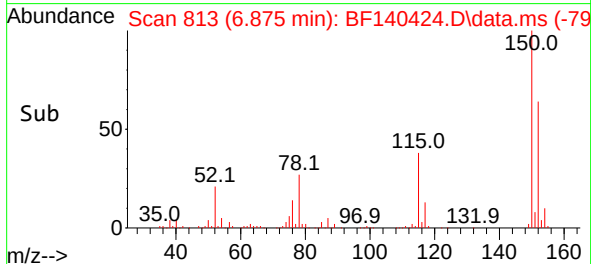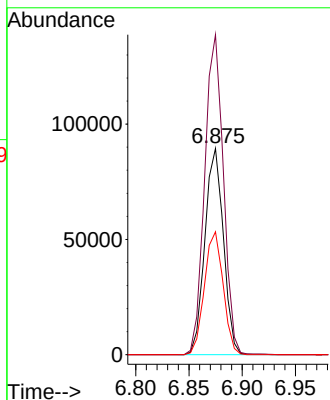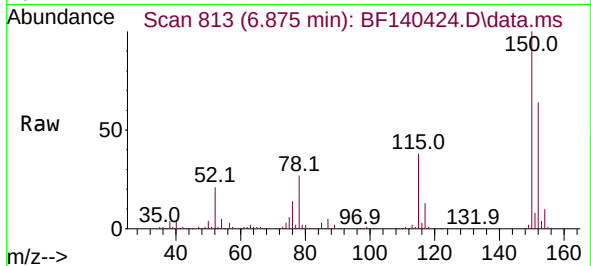

#5
2-Fluorophenol
Concen: 136.262 ng
RT: 5.516 min Scan# 582
Delta R.T. 0.024 min
Lab File: BF140424.D
Acq: 16 Nov 2024 12:46

Tgt Ion:112 Resp: 867579
Ion Ratio Lower Upper
112 100
64 59.7 49.2 73.8
63 31.2 25.6 38.4


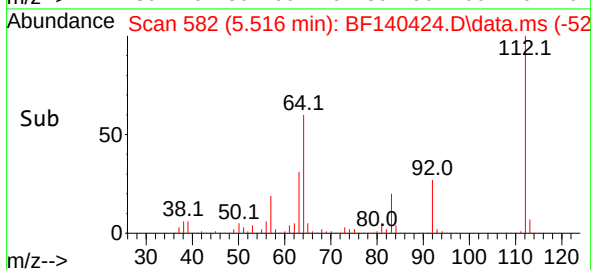
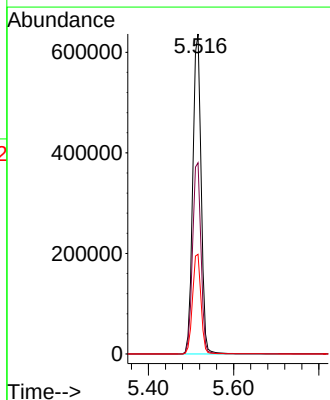
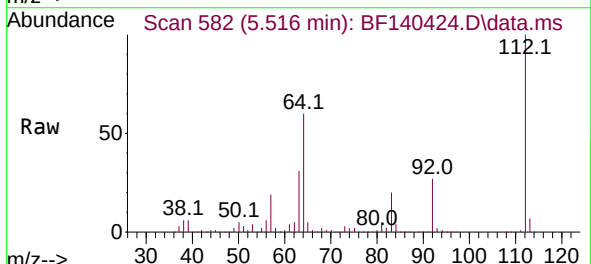


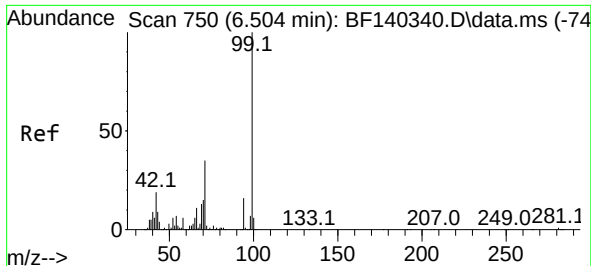

#7
Phenol-d6
Concen: 127.489 ng
RT: 6.516 min Scan# 71
Delta R.T. 0.012 min
Lab File: BF140424.D
Acq: 16 Nov 2024 12:46




Instrument :
BNA_F
ClientSampleId :
TP-2


Tgt Ion: 99 Resp: 1099751
Ion Ratio Lower Upper
99 100
42 18.1 15.1 22.7
71 34.8 27.9 41.9

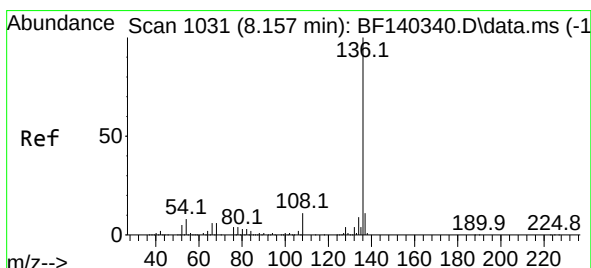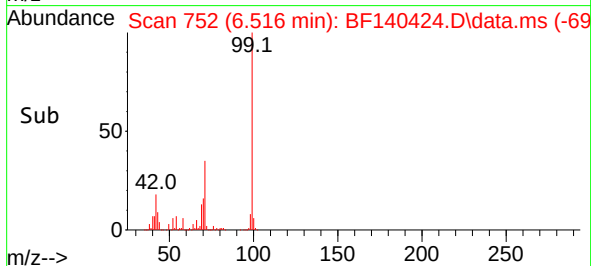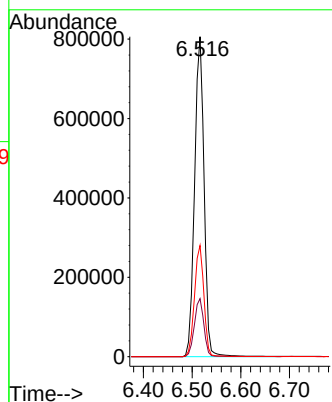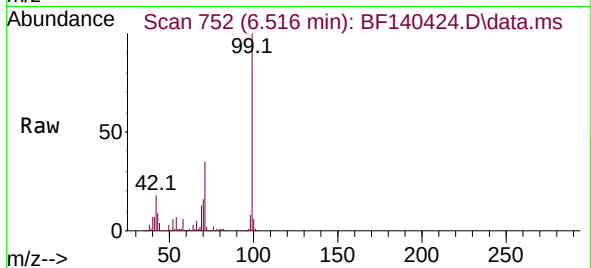

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.151 min Scan# 1030
Delta R.T. -0.006 min
Lab File: BF140424.D
Acq: 16 Nov 2024 12:46

Tgt Ion: 136 Resp: 405539
Ion Ratio Lower Upper
136 100
137 10.7 8.7 13.1
54 7.9 6.5 9.7
68 6.3 5.0 7.6


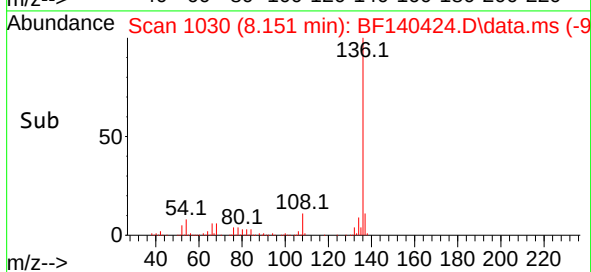
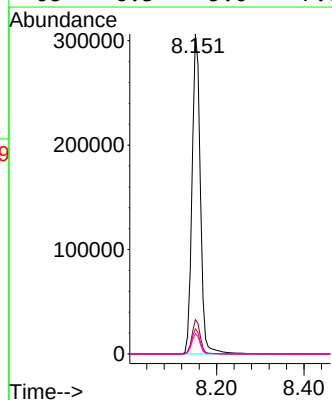
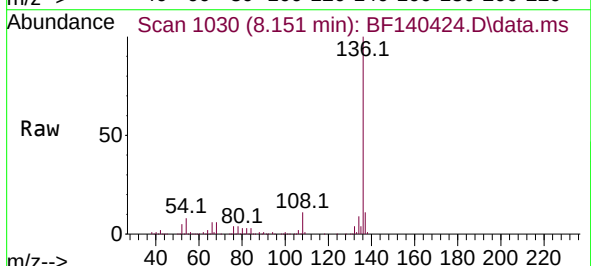


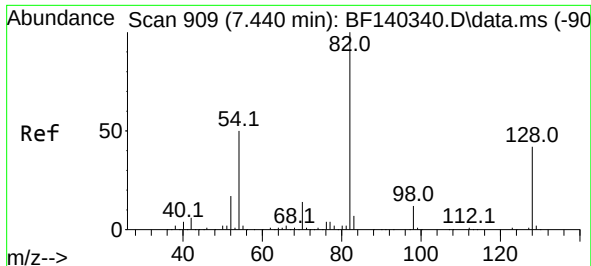

#23
Nitrobenzene-d5
Concen: 95.958 ng
RT: 7.434 min Scan# 909
Delta R.T. -0.006 min
Lab File: BF140424.D
Acq: 16 Nov 2024 12:46




Instrument :
BNA_F
ClientSampleId :
TP-2


Tgt Ion: 82 Resp: 746883
Ion Ratio Lower Upper
82 100
128 43.1 33.3 49.9
54 48.7 39.8 59.8

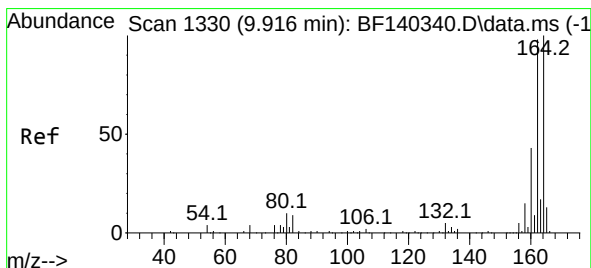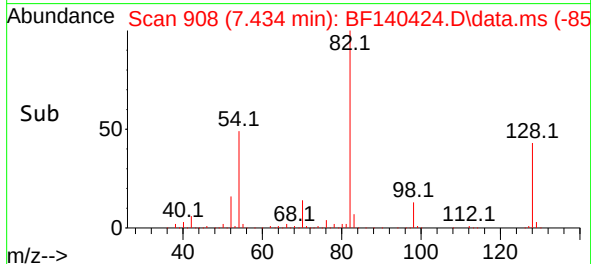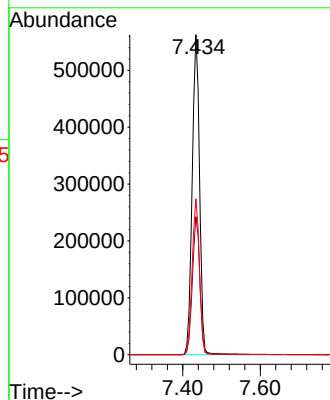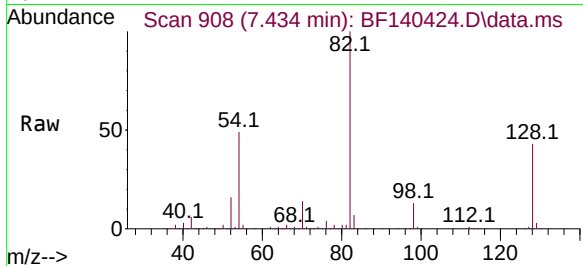

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.910 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BF140424.D
Acq: 16 Nov 2024 12:46

Tgt Ion:164 Resp: 218341
Ion Ratio Lower Upper
164 100
162 99.4 79.8 119.8
160 43.5 35.4 53.0


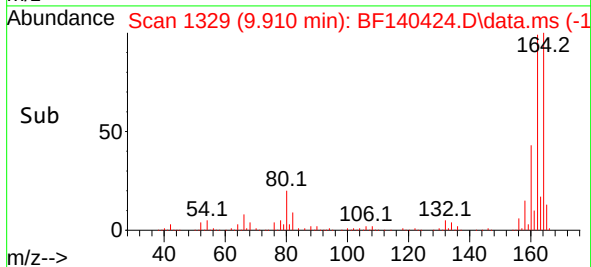
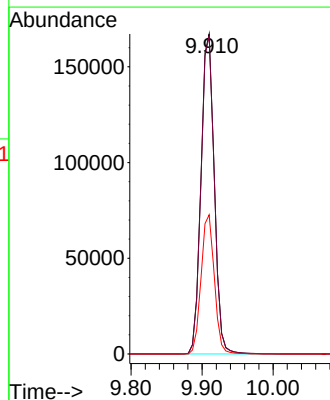
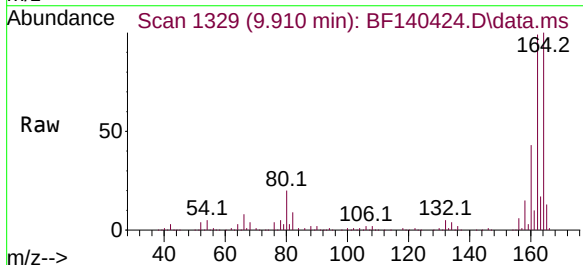


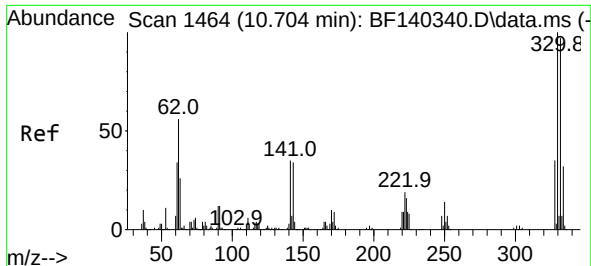

#42
2,4,6-Tribromophenol
Concen: 142.766 ng
RT: 10.704 min Scan# 1464
Delta R.T. -0.000 min
Lab File: BF140424.D
Acq: 16 Nov 2024 12:46




Instrument :
BNA_F
ClientSampleId :
TP-2


Tgt Ion: 330 Resp: 309978
Ion Ratio Lower Upper
330 100
332 96.7 75.9 113.9
141 33.7 26.9 40.3

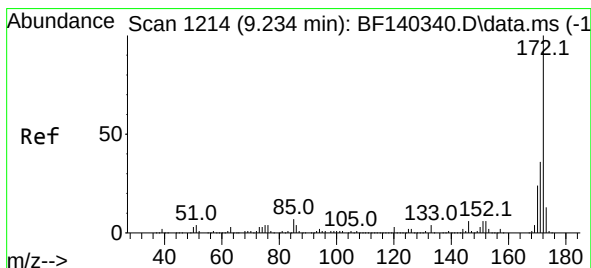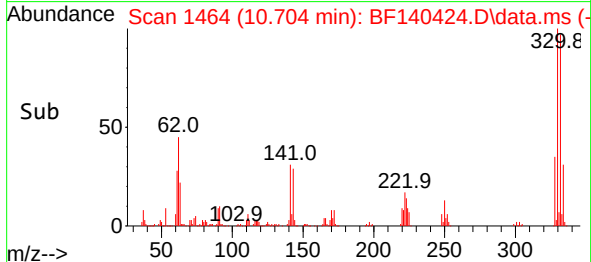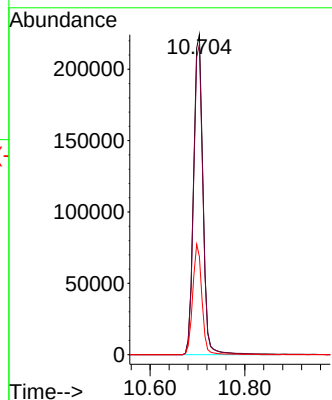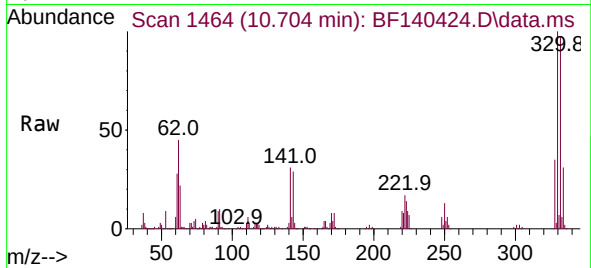

#45
2-Fluorobiphenyl
Concen: 97.383 ng
RT: 9.228 min Scan# 1213
Delta R.T. -0.006 min
Lab File: BF140424.D
Acq: 16 Nov 2024 12:46

Tgt Ion: 172 Resp: 1322684
Ion Ratio Lower Upper
172 100
171 35.6 28.5 42.7
170 23.5 19.1 28.7

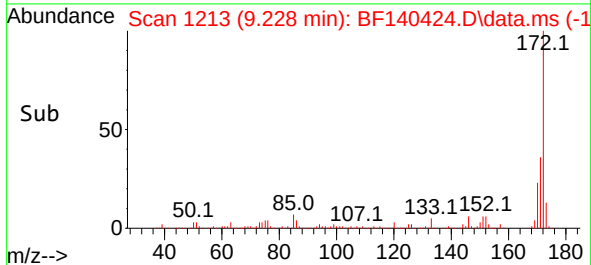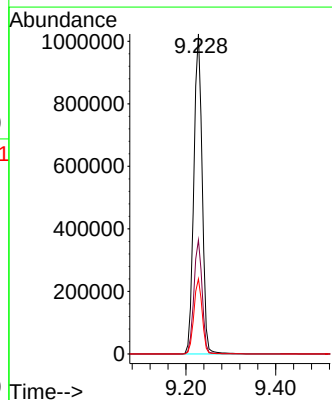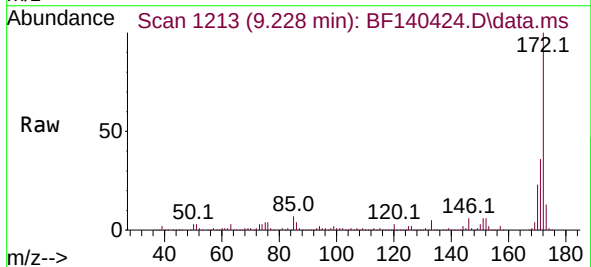

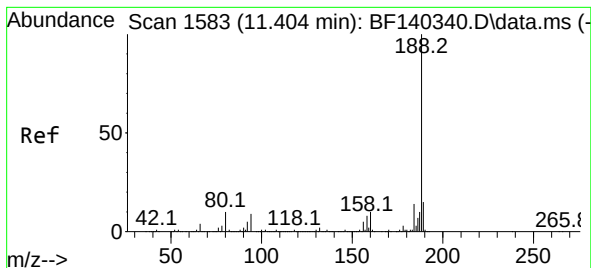

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.398 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF140424.D

Acq: 16 Nov 2024 12:46

Instrument :

BNA_F

ClientSampleId :

TP-2





Tgt Ion:188 Resp: 395523

Ion Ratio Lower Upper

188 100

94 9.1 7.6 11.4

80 9.9 8.0 12.0

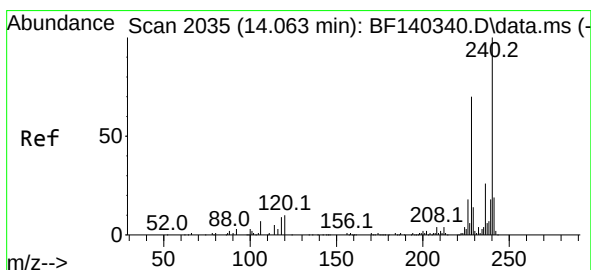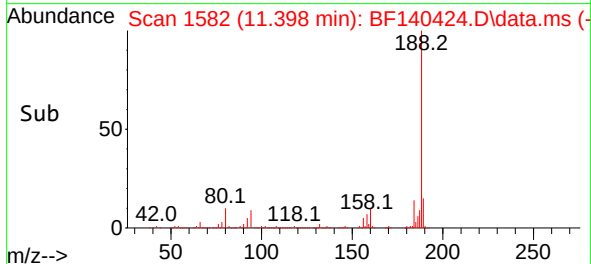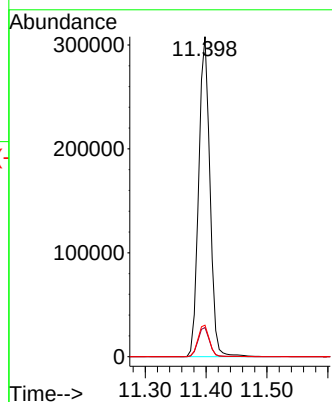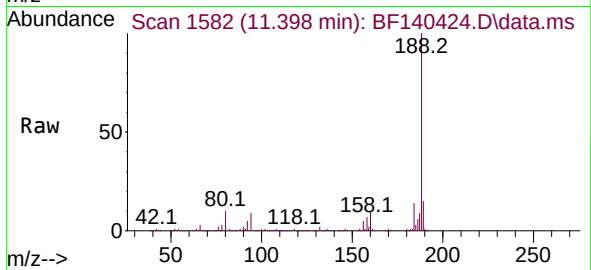

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.045 min Scan# 2032

Delta R.T. -0.006 min

Lab File: BF140424.D

Acq: 16 Nov 2024 12:46




Tgt Ion:240 Resp: 229407


Ion Ratio Lower Upper

240 100

120 10.1 8.8 13.2

236 26.0 20.9 31.3

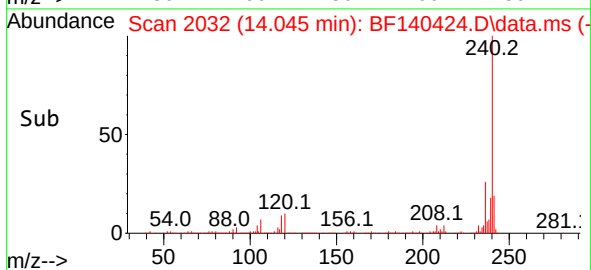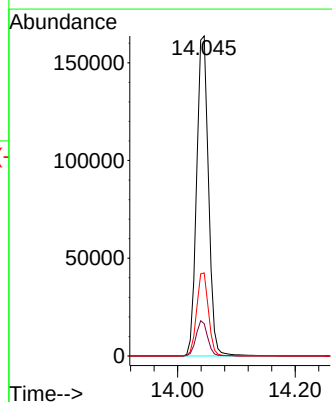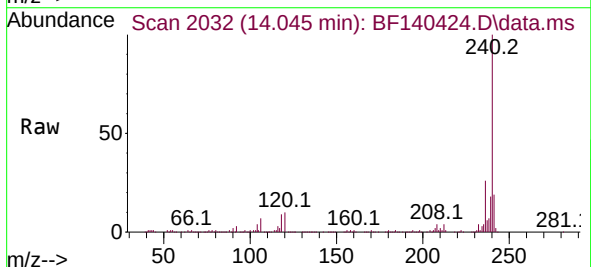

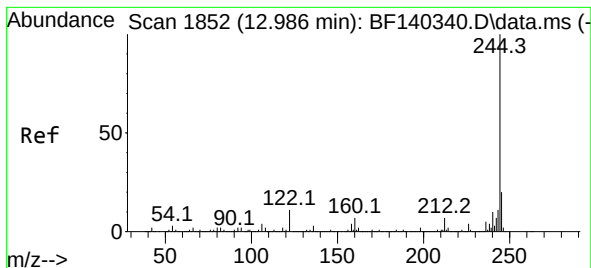

#79

Terphenyl-d14

Concen: 101.988 ng

RT: 12.986 min Scan# 1852

Delta R.T. -0.000 min

Lab File: BF140424.D

Acq: 16 Nov 2024 12:46

Instrument :

BNA_F

ClientSampleId :

TP-2





Tgt Ion:244 Resp: 1347906

Ion Ratio Lower Upper

244 100

212 6.9 5.8 8.8

122 10.6 8.8 13.2

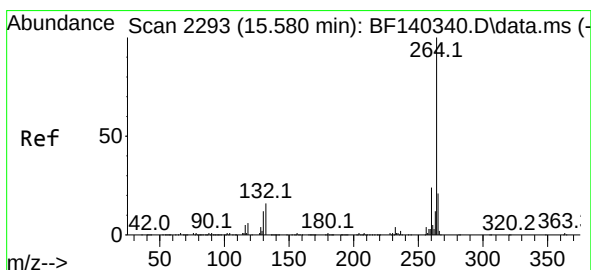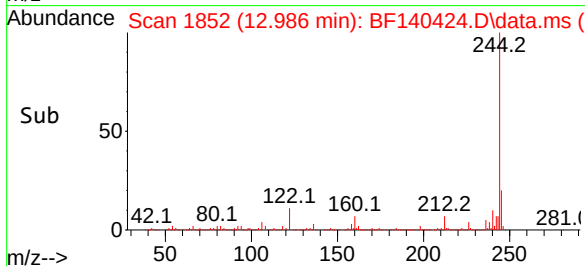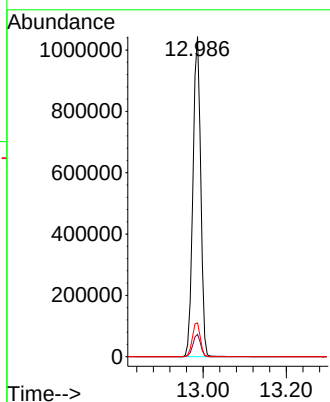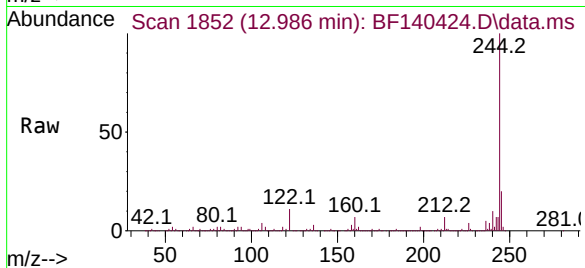

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.533 min Scan# 2285

Delta R.T. -0.024 min

Lab File: BF140424.D

Acq: 16 Nov 2024 12:46

Tgt Ion:264 Resp: 248406

Ion Ratio Lower Upper

264 100

260 24.0 19.2 28.8

265 21.7 17.1 25.7

