


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111624\
Data File : BF140416.D
Acq On : 16 Nov 2024 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

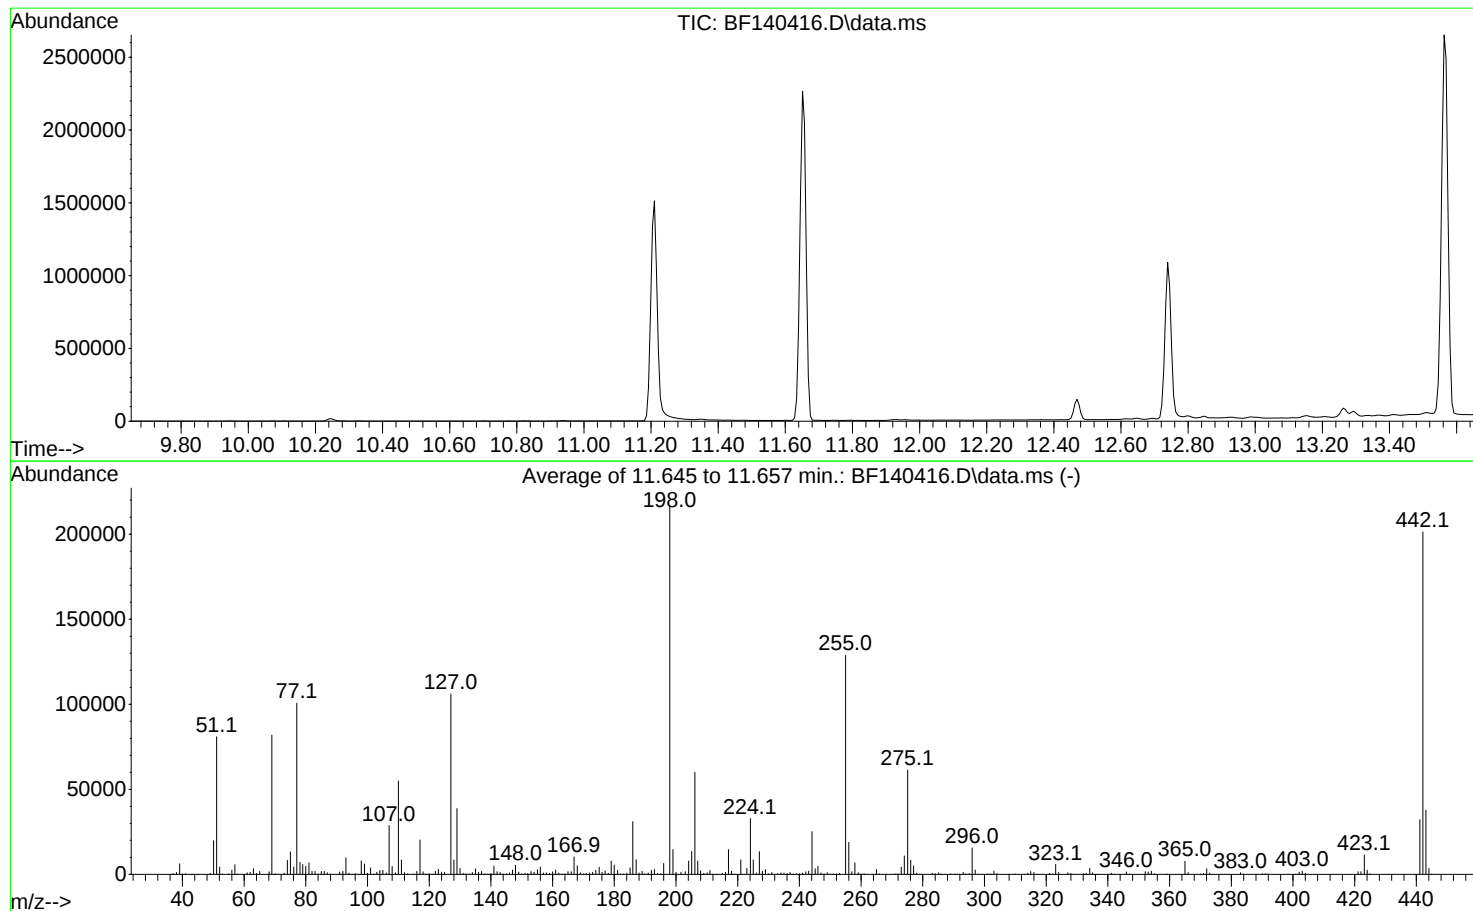

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	80915	PASS
68	69	0.00	2	1.8	1489	PASS
69	198	0.00	100	37.8	81809	PASS
70	69	0.00	2	0.6	505	PASS
127	198	10	80	49.0	106000	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	216277	PASS
199	198	5	9	6.8	14609	PASS
275	198	10	60	28.4	61384	PASS
365	198	1	100	3.6	7757	PASS
441	198	0.01	100	14.9	32184	PASS
442	442	50	100	100.0	201331	PASS
443	442	15	24	18.7	37749	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
11/16/2024	BNA_F	<u>BF140416.D</u>
Compound Name	Response	Retention Time
DDT	686763	13.563
DDD	22519	13.263
DDE	2035	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24554	711317	3.45

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111624\
Data File : BF140416.D
Acq On : 16 Nov 2024 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 18 00:20:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

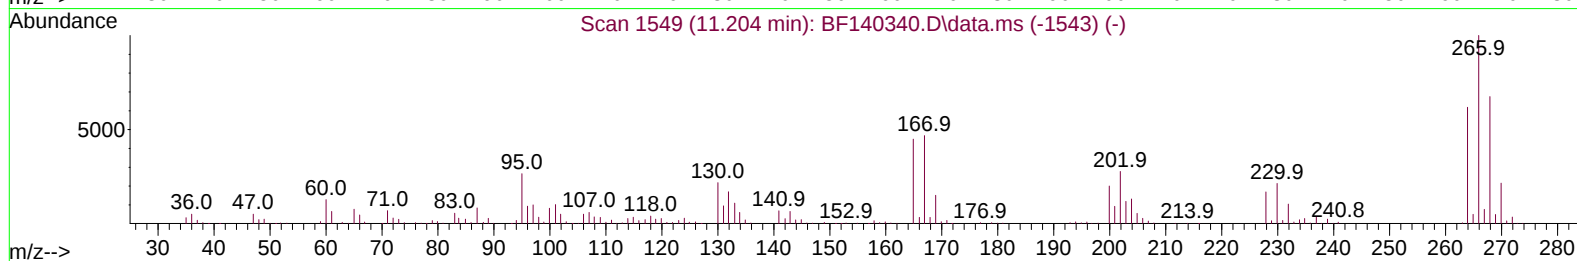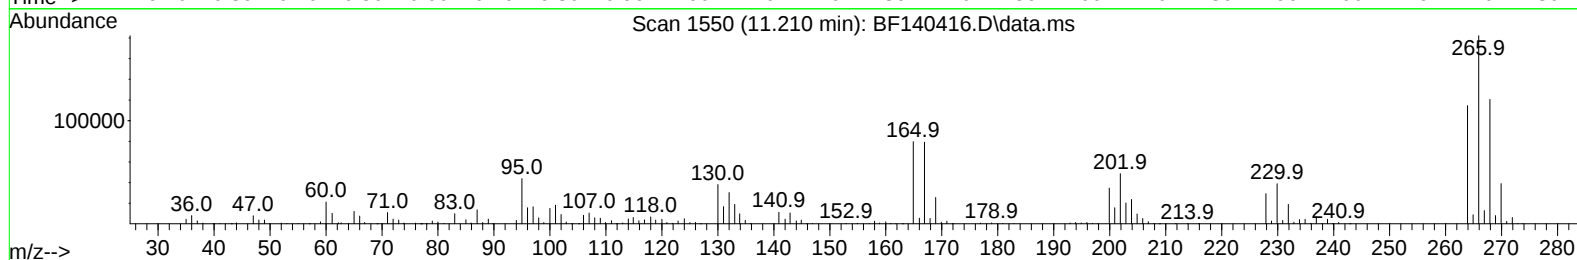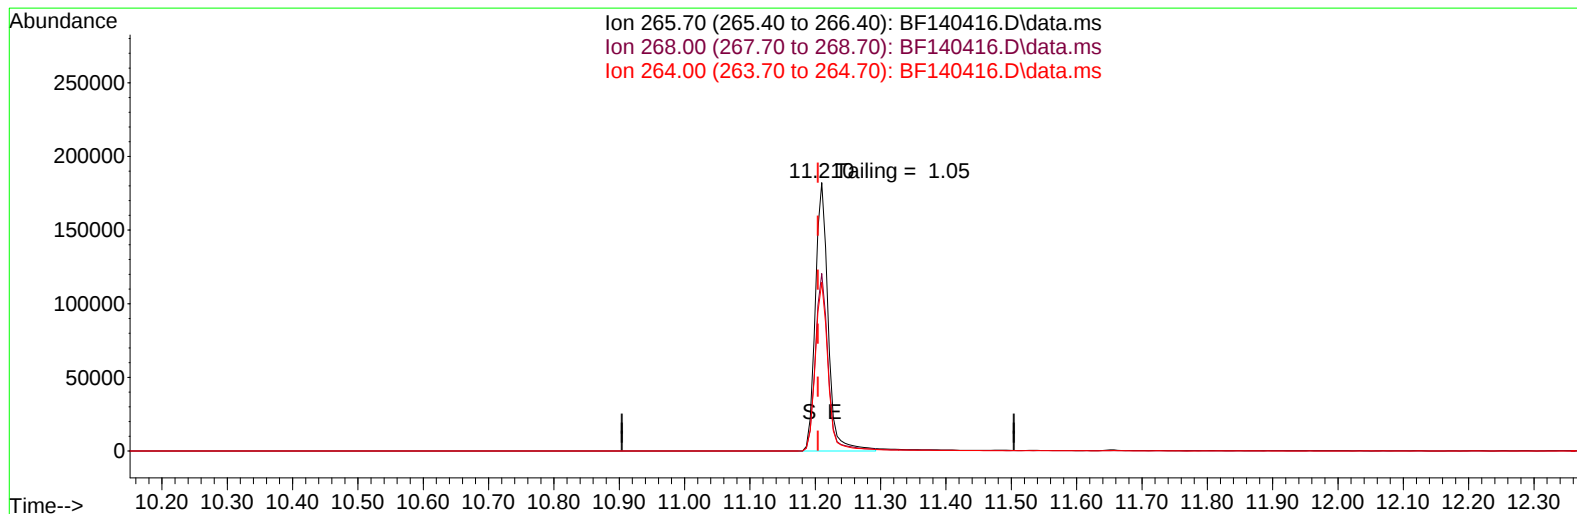

TIC: BF140416.D\data.ms

(70) Pentachlorophenol (C)

11.210min (+ 0.006) 65679.46 ng




response 253869

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	66.15
264.00	62.90	62.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111624\
Data File : BF140416.D
Acq On : 16 Nov 2024 09:08
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 18 00:20:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

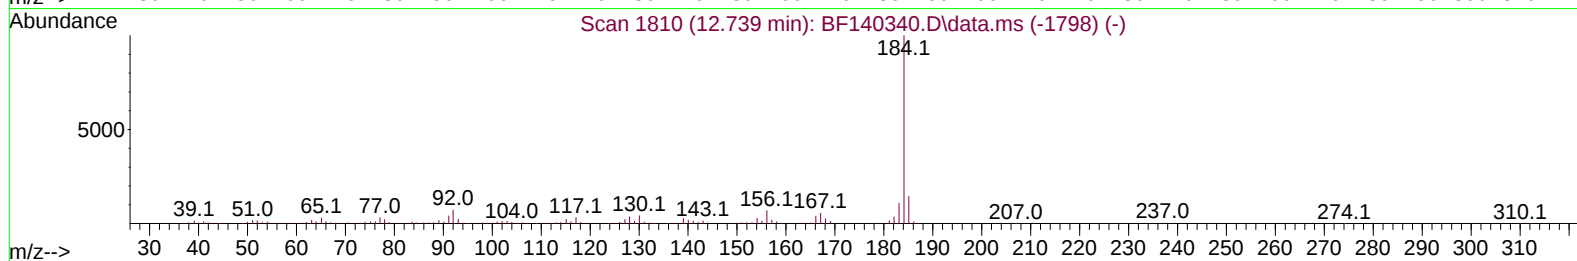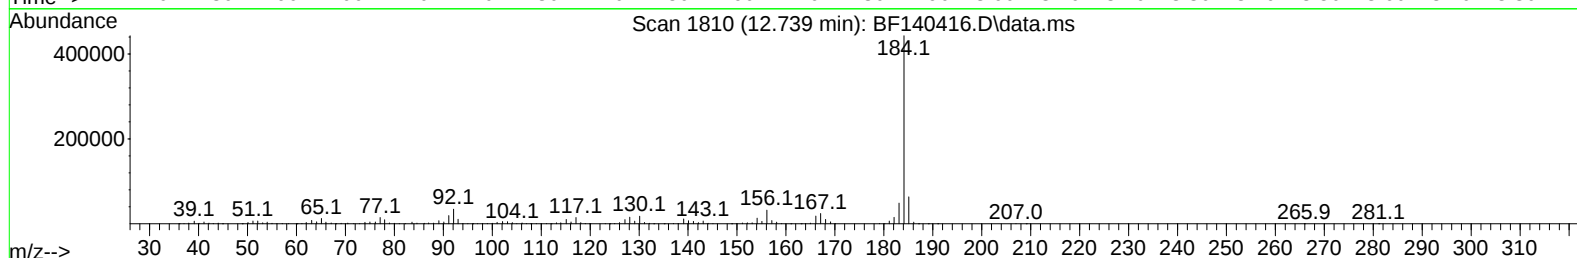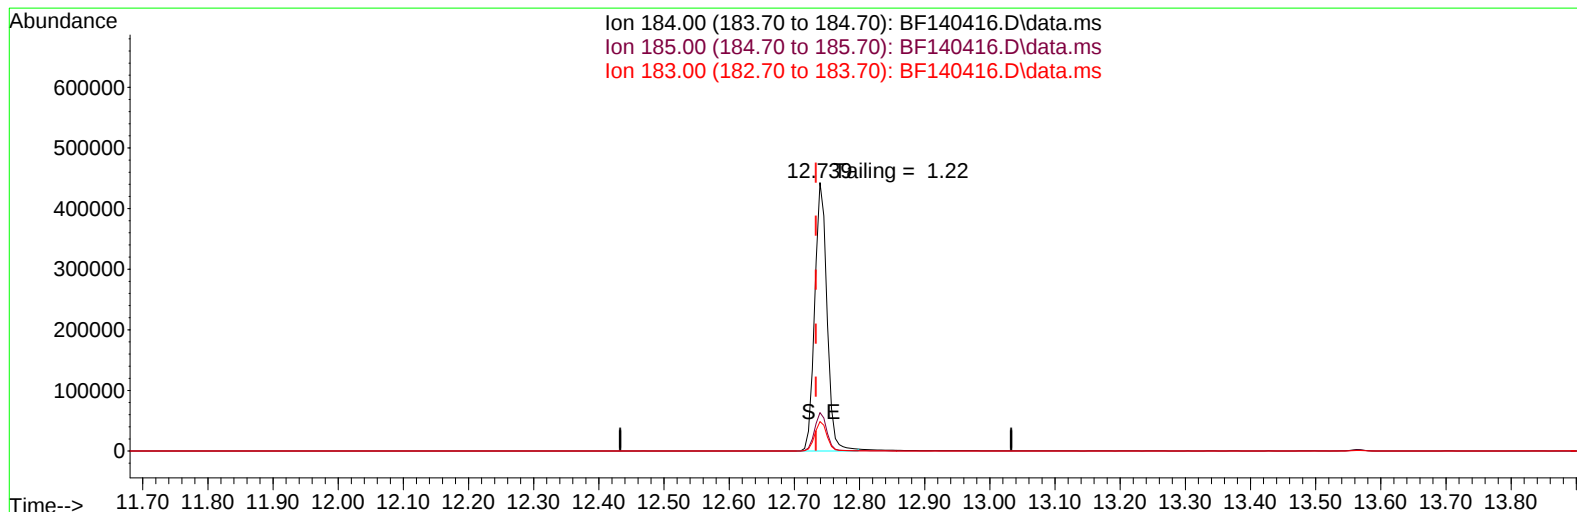

TIC: BF140416.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 10148.88 ng

response 590902

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.33
183.00	10.80	11.00
0.00	0.00	0.00