


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111715\
 Data File : BF082970.D
 Acq On : 17 Nov 2015 16:40
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Nov 18 13:32:32 2015

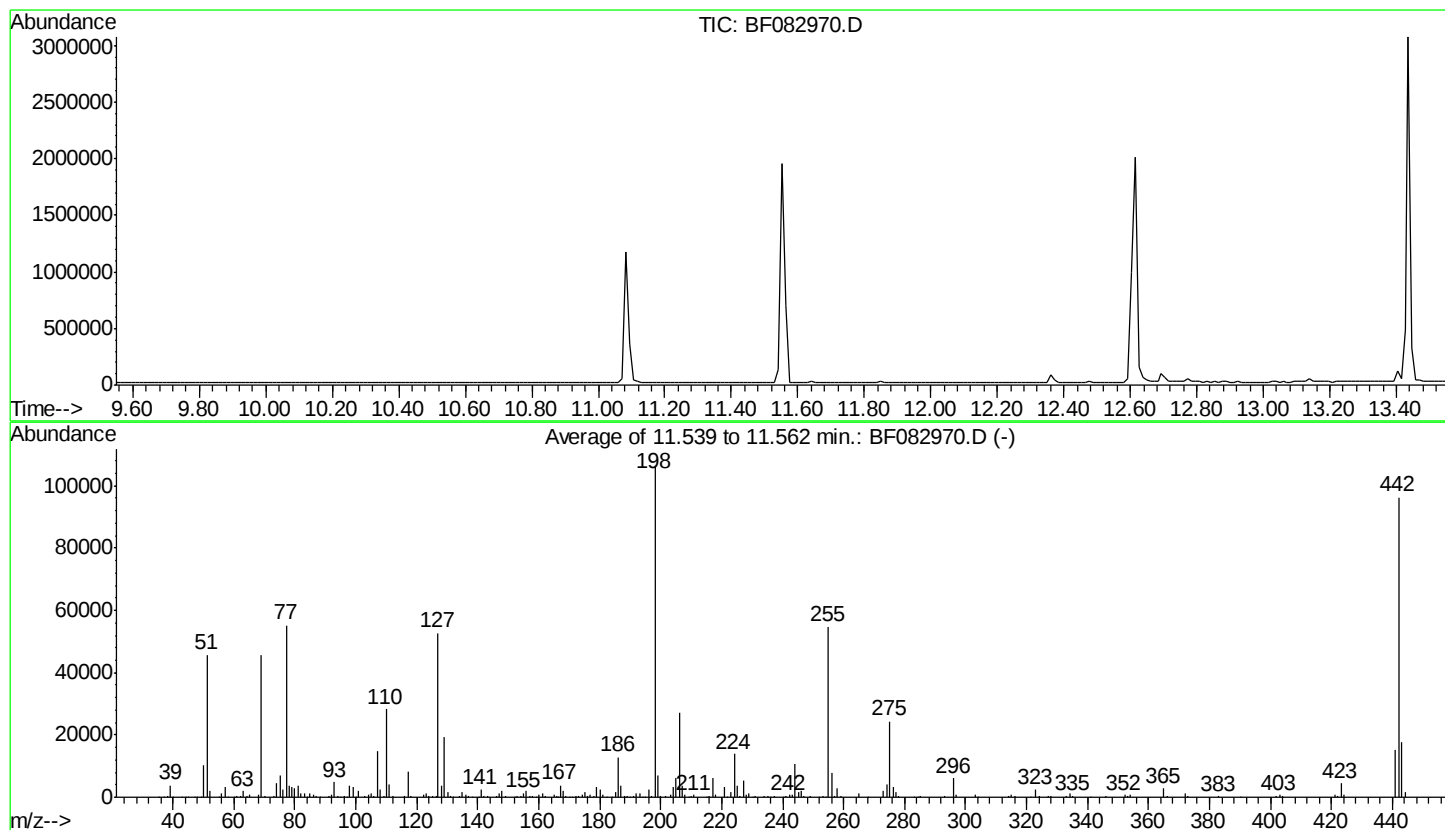

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.0	45784	PASS
68	69	0.00	2	1.7	762	PASS
69	198	0.00	100	43.0	45738	PASS
70	69	0.00	2	0.5	225	PASS
127	198	10	80	49.4	52622	PASS
197	198	0.00	2	0.5	536	PASS
198	198	100	100	100.0	106478	PASS
199	198	5	9	6.7	7159	PASS
275	198	10	60	22.8	24319	PASS
365	198	1	100	2.6	2729	PASS
441	442	0.01	24	15.9	15304	PASS
442	198	50	100	90.4	96260	PASS
443	442	15	24	18.6	17875	PASS