


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111715\
Data File : BF082994.D
Acq On : 18 Nov 2015 4:51
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 18 13:32:32 2015

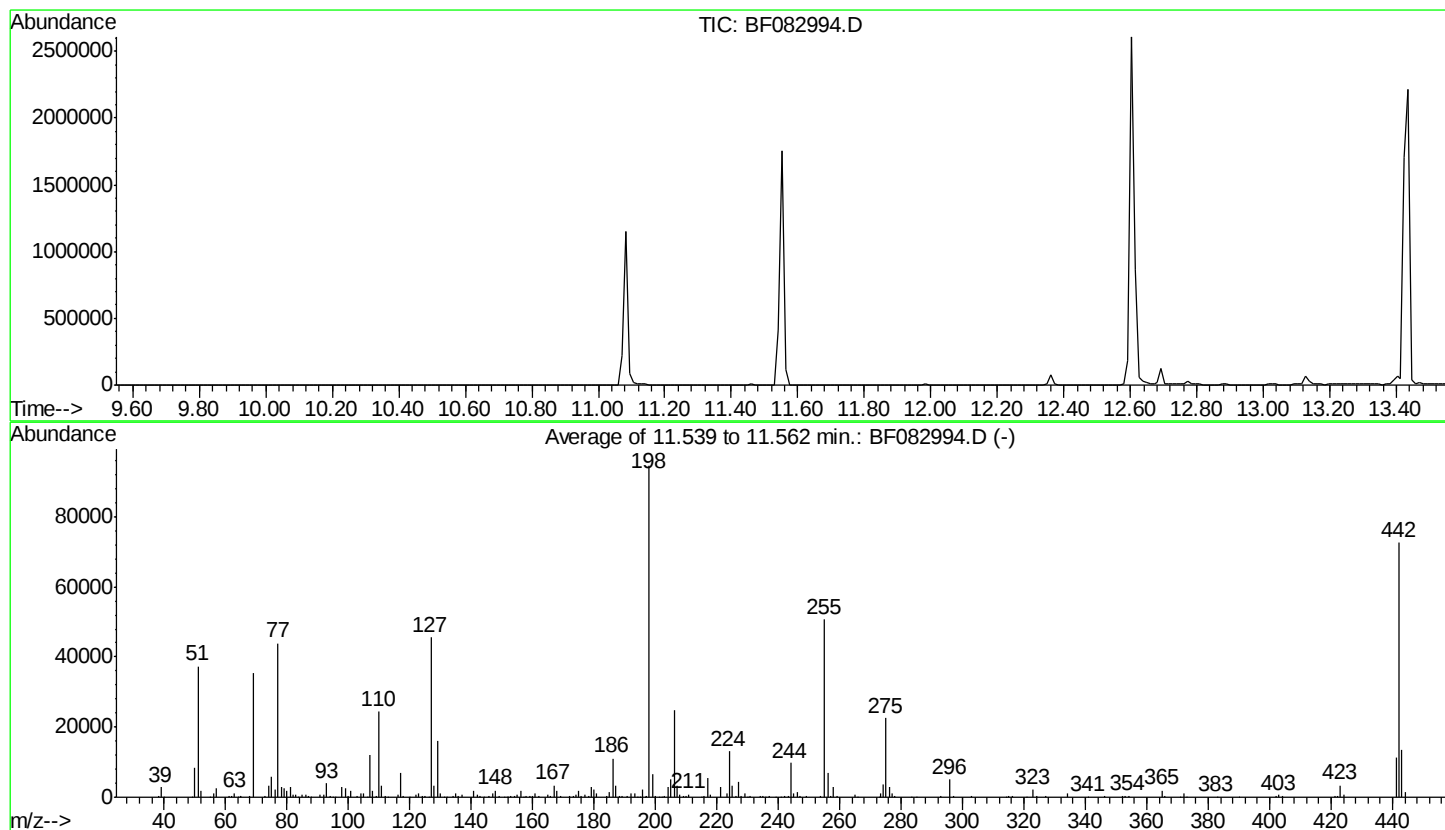

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	37264	PASS
68	69	0.00	2	1.6	558	PASS
69	198	0.00	100	37.3	35301	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.2	45545	PASS
197	198	0.00	2	0.5	426	PASS
198	198	100	100	100.0	94544	PASS
199	198	5	9	6.8	6428	PASS
275	198	10	60	23.9	22596	PASS
365	198	1	100	2.1	1974	PASS
441	442	0.01	24	15.5	11225	PASS
442	198	50	100	76.7	72475	PASS
443	442	15	24	18.8	13595	PASS