
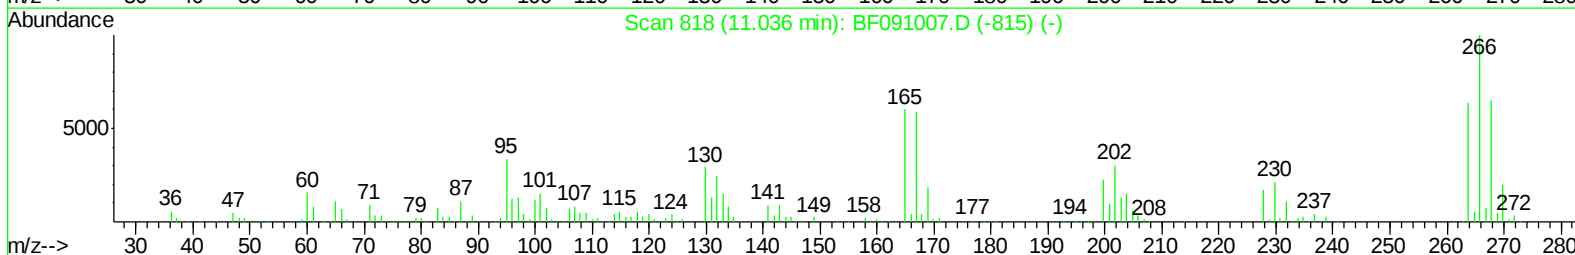
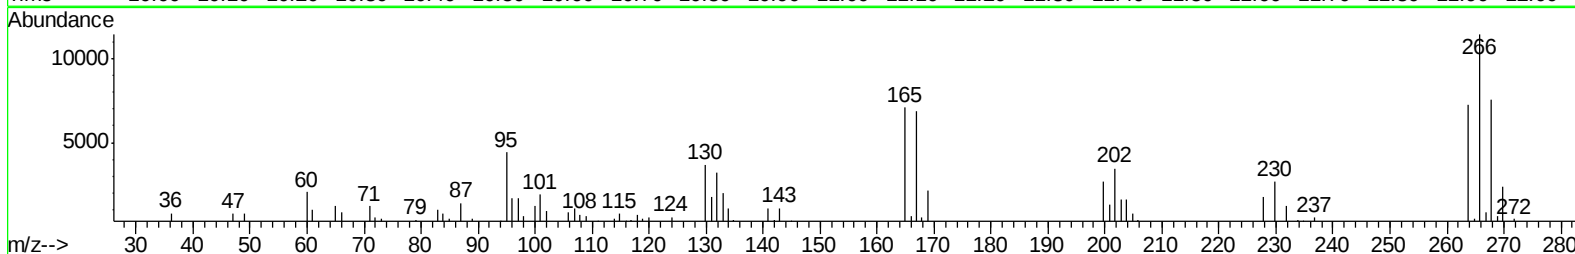


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111716\
Data File : BF091209.D
Acq On : 17 Nov 2016 11:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 07:54:44 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

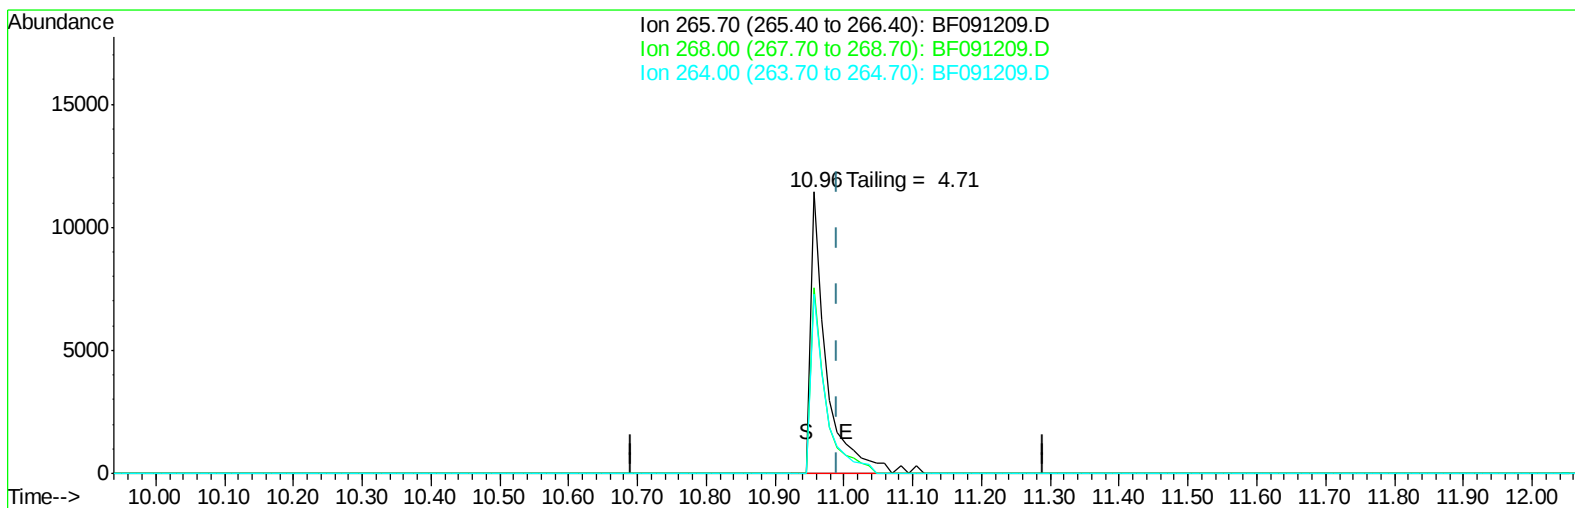

TIC: BF091209.D

(69) Pentachlorophenol (C)




10.956min (-0.034) 0.00ng

response 18149

Ion	Exp%	Act%
265.70	100	100
268.00	65.10	66.06
264.00	63.90	63.58
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111716\
Data File : BF091209.D
Acq On : 17 Nov 2016 11:11
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 07:54:44 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

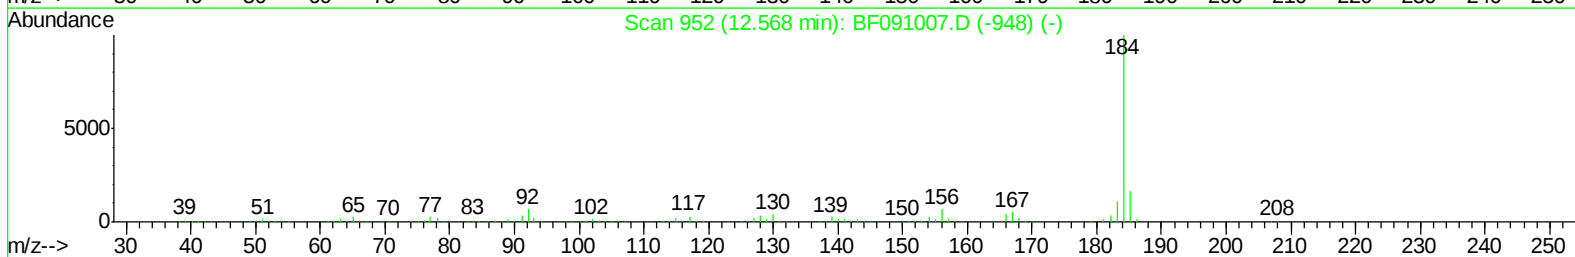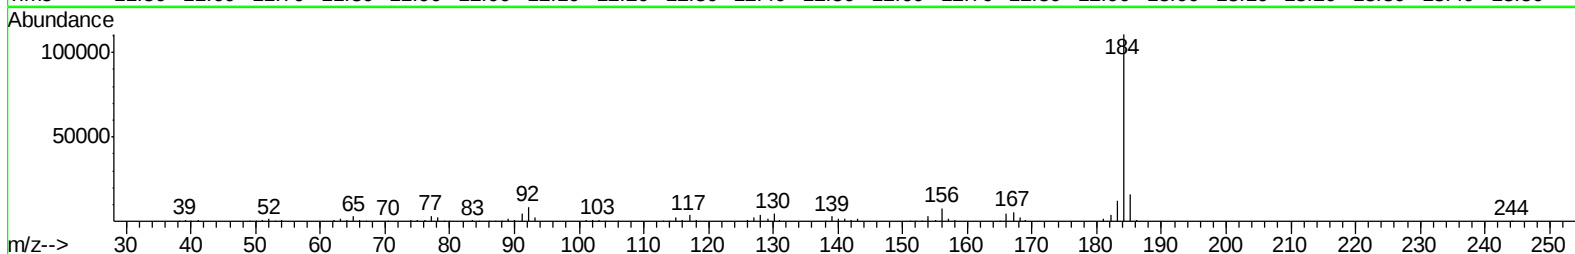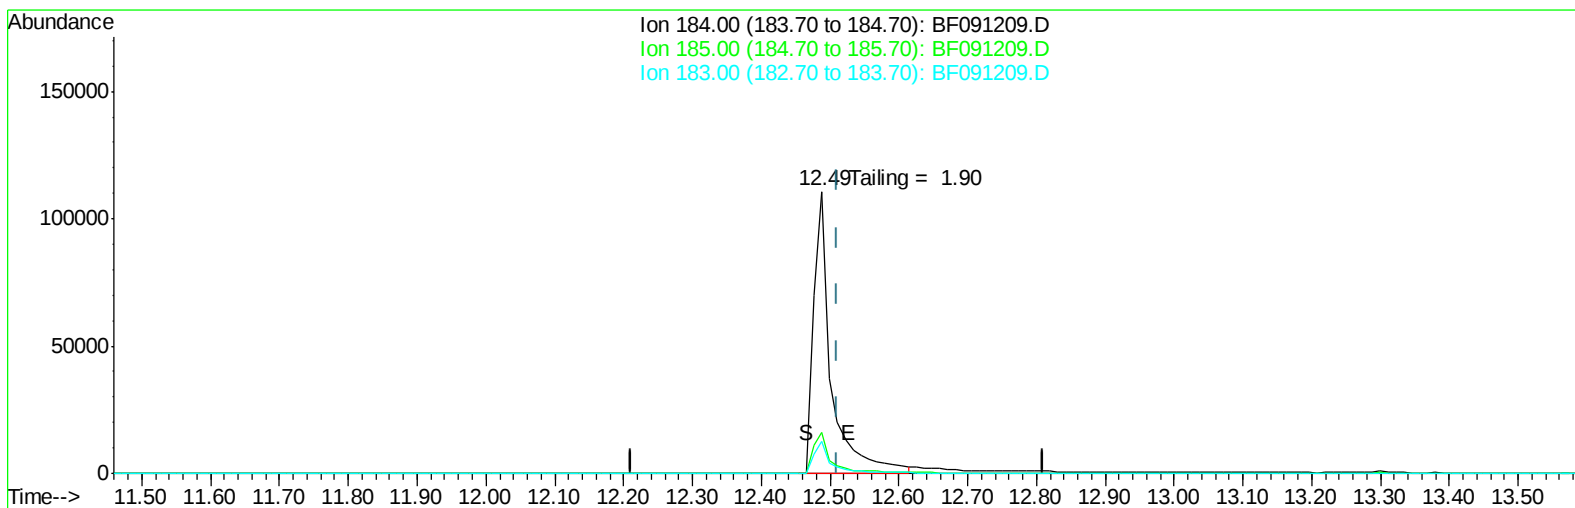

TIC: BF091209.D

(76) Benzidine

12.488min (-0.023) 923.05ng

response 195348

Ion	Exp%	Act%
184.00	100	100
185.00	16.20	14.71
183.00	10.90	11.28
0.00	0.00	0.00