

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111716\
 Data File : BF091226.D
 Acq On : 17 Nov 2016 21:37
 Operator : UM/SJ
 Sample : H5681-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WQ-2W

Quant Time: Nov 18 04:03:07 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 08 12:59:29 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.61	152	185393	20.00	ng	-0.05
21) Naphthalene-d8	7.90	136	762945	20.00	ng	-0.05
38) Acenaphthene-d10	9.65	164	403145	20.00	ng	-0.05
63) Phenanthrene-d10	11.14	188	731354	20.00	ng	-0.03
75) Chrysene-d12	13.77	240	471874	20.00	ng	-0.05
86) Perylene-d12	15.14	264	343489	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.21	112	815371	72.64	ng	-0.03
7) Phenol-d6	6.27	99	705380	46.30	ng	-0.05
23) Nitrobenzene-d5	7.20	82	1231222	88.03	ng	-0.05
41) 2,4,6-Tribromophenol	10.45	330	556296	152.63	ng	-0.03
44) 2-Fluorobiphenyl	8.99	172	2035026	86.91	ng	-0.05
78) Terphenyl-d14	12.73	244	1844460	97.54	ng	-0.03


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111716\
Data File : BF091226.D
Acq On : 17 Nov 2016 21:37
Operator : UM/SJ
Sample : H5681-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WQ-2W

Quant Time: Nov 18 04:03:07 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 08 12:59:29 2016
Response via : Initial Calibration

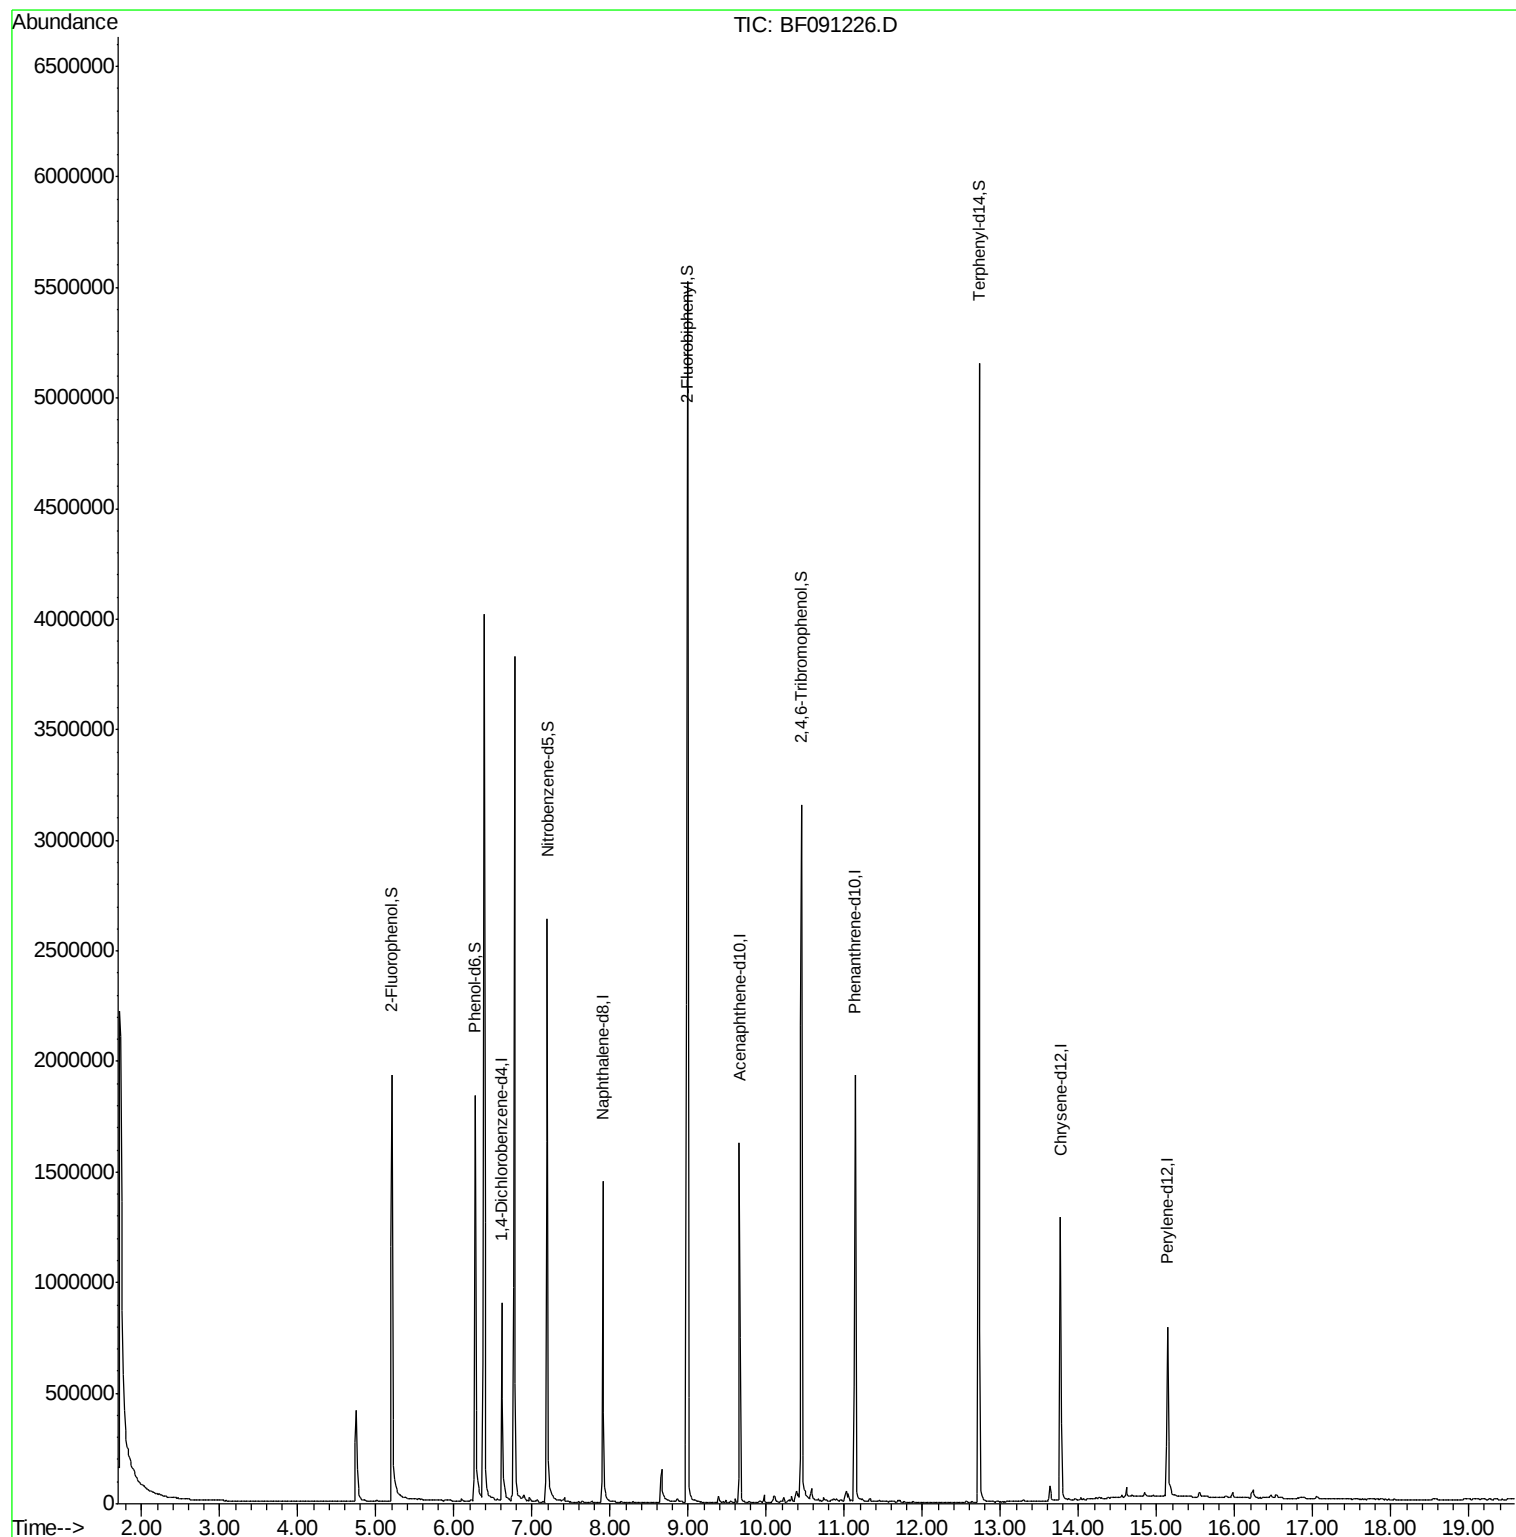

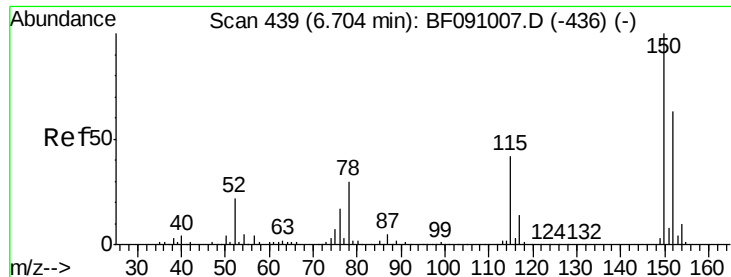

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.61 min Scan# 431

Delta R.T. -0.05 min

Lab File: BF091226.D

Acq: 17 Nov 2016 21:37

Instrument :

BNA_F

ClientSampleId :

WQ-2W


Tot Ion:152 Resp: 185393

Ion Ratio Lower Upper

152 100

150 160.6 126.8 190.2




115 73.2 53.3 79.9

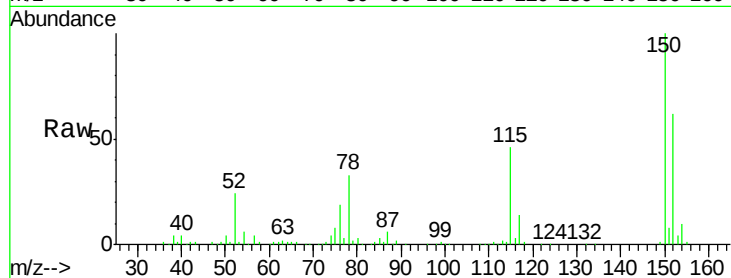

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

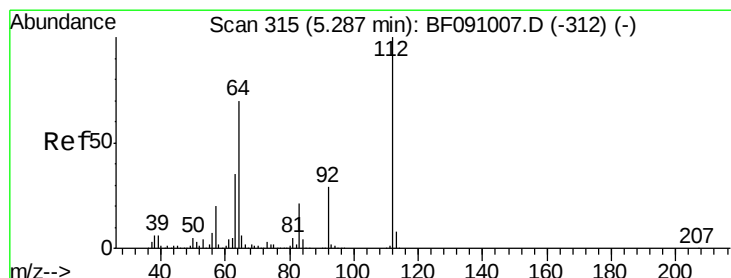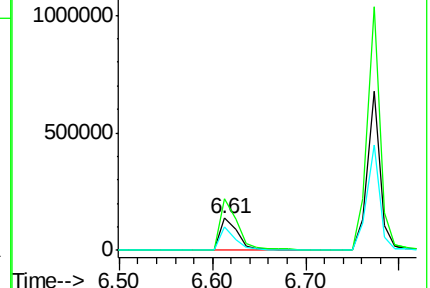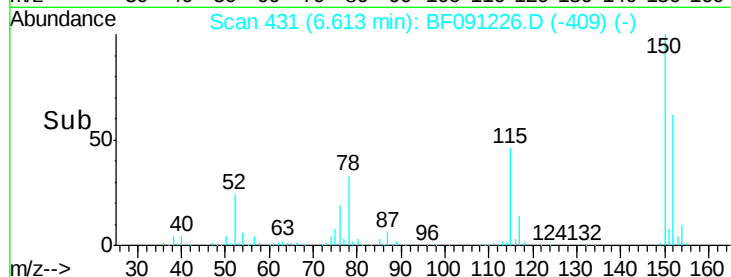

#5

2-Fluorophenol

Concen: 72.64 ng

RT: 5.21 min Scan# 308

Delta R.T. -0.03 min

Lab File: BF091226.D

Acq: 17 Nov 2016 21:37


Tgt Ion:112 Resp: 815371

Ion Ratio Lower Upper

112 100

64 54.3 55.8 83.6#



63 27.4 28.0 42.0#

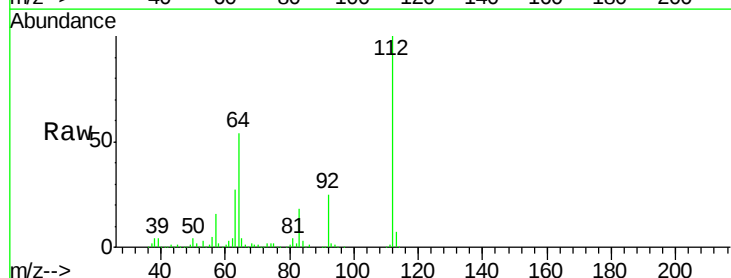


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

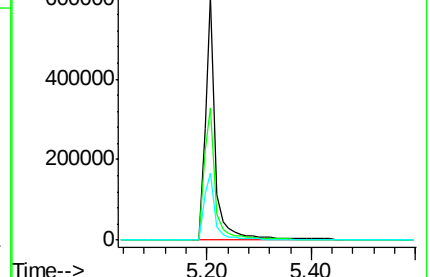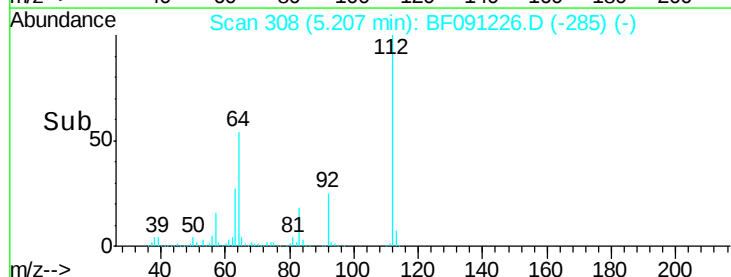

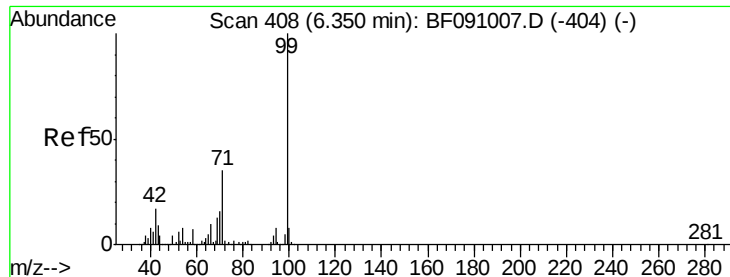

#7

Phenol-d6

Concen: 46.30 ng

RT: 6.27 min Scan# 401

Delta R.T. -0.05 min

Lab File: BF091226.D

Acq: 17 Nov 2016 21:37

Instrument :

BNA_F

ClientSampleId :

WQ-2W


Tot Ion: 99 Resp: 705380

Ion Ratio Lower Upper

99 100

42 15.7 13.9 20.9




71 33.2 27.8 41.8

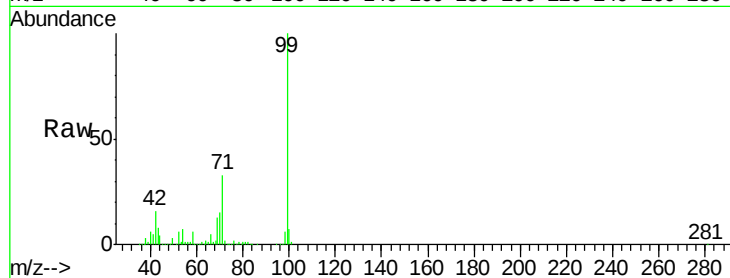

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

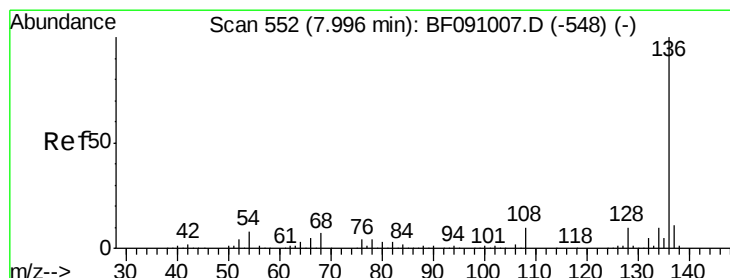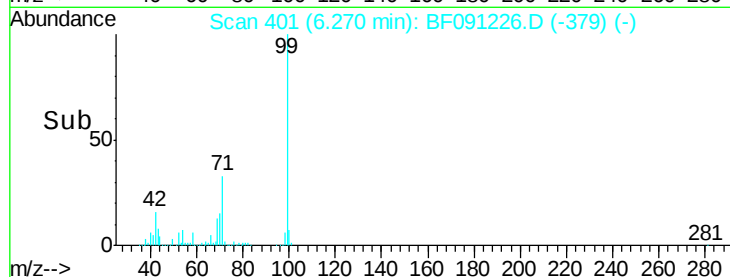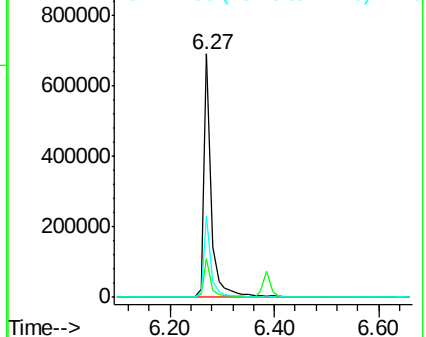

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.90 min Scan# 544

Delta R.T. -0.05 min

Lab File: BF091226.D

Acq: 17 Nov 2016 21:37

Tgt Ion: 136 Resp: 762945


Ion Ratio Lower Upper

136 100

137 11.5 8.9 13.3

54 7.9 6.2 9.2

68 7.0 5.5 8.3


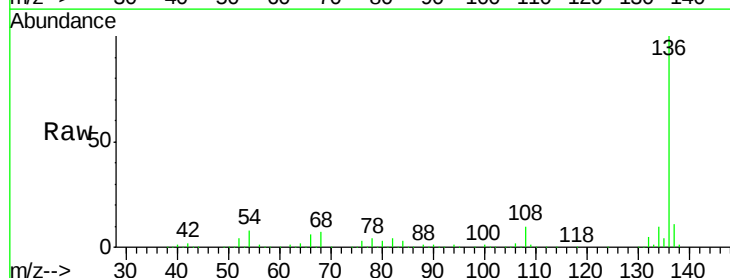



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0



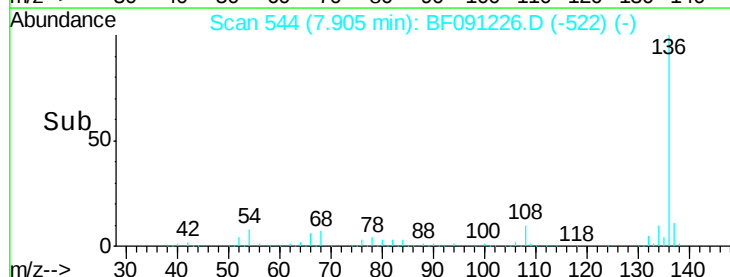
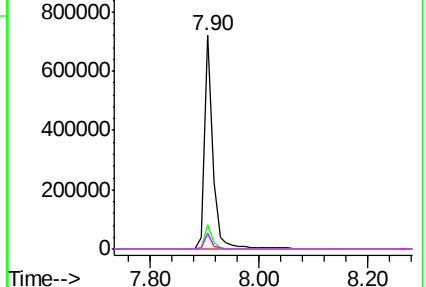


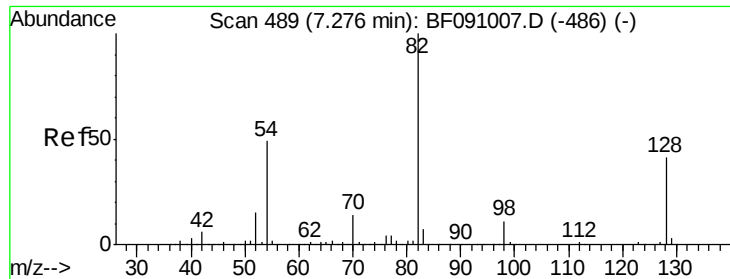

#23
 Nitrobenzene-d5
 Concen: 88.03 ng
 RT: 7.20 min Scan# 482
 Delta R.T. -0.05 min
 Lab File: BF091226.D
 Acq: 17 Nov 2016 21:37




Instrument :
 BNA_F
 ClientSampleId :
 WQ-2W


Tot Ion: 82 Resp: 1231222
 Ion Ratio Lower Upper
 82 100
 128 51.0 32.4 48.6#
 54 42.6 39.2 58.8

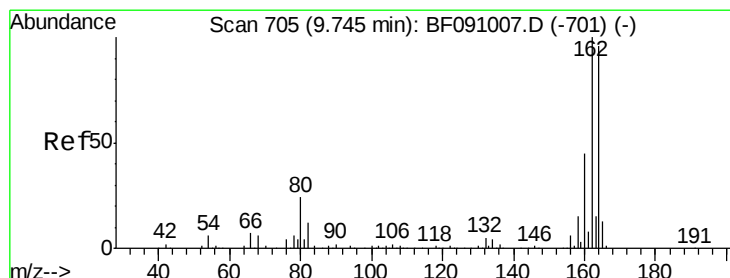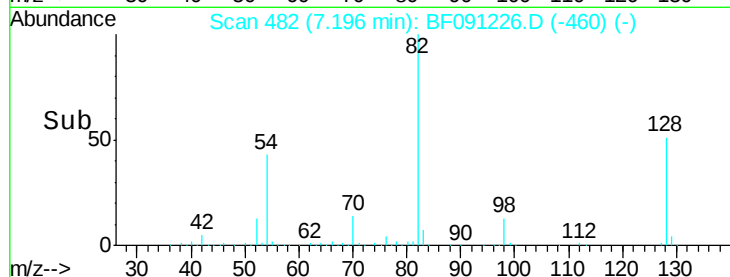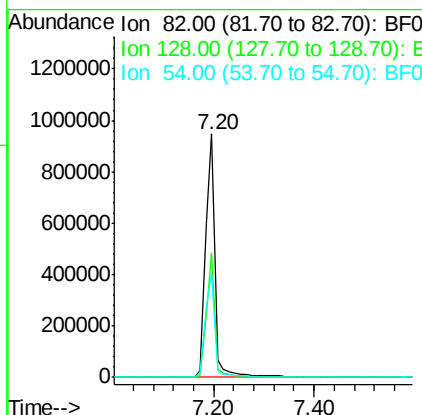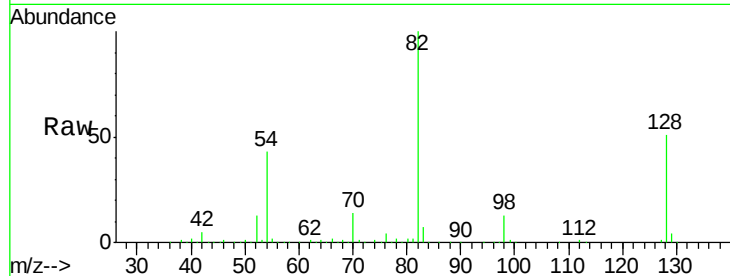

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.65 min Scan# 697
 Delta R.T. -0.05 min
 Lab File: BF091226.D
 Acq: 17 Nov 2016 21:37

Tgt Ion:164 Resp: 403145
 Ion Ratio Lower Upper
 164 100
 162 105.2 83.6 125.4
 160 47.5 37.9 56.9

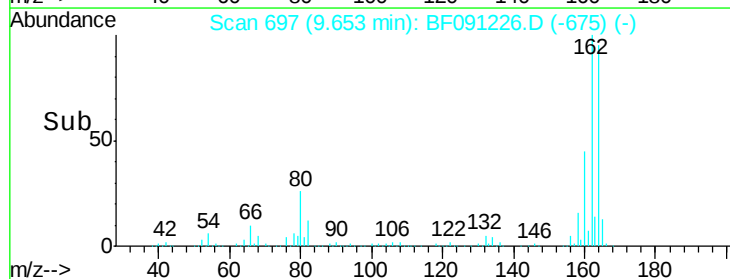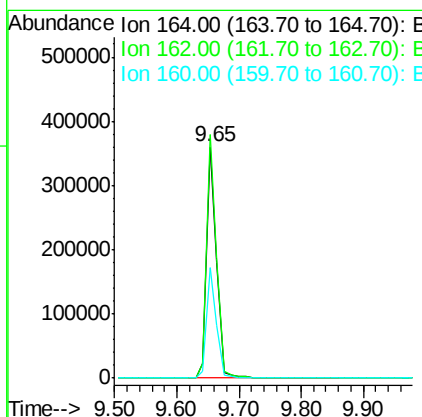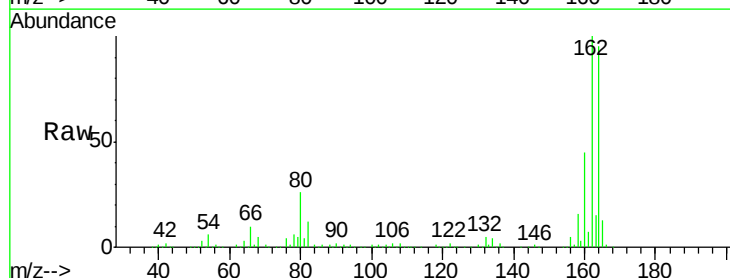


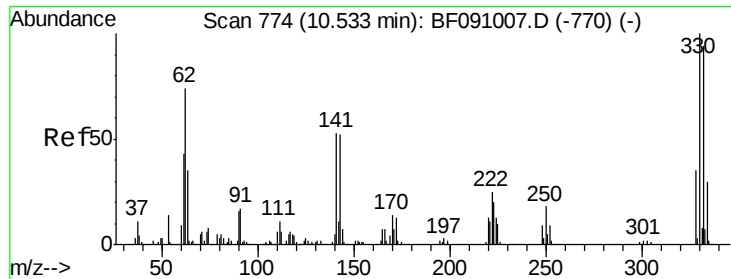




#41
 2,4,6-Tribromophenol
 Concen: 152.63 ng
 RT: 10.45 min Scan# 767
 Delta R.T. -0.03 min
 Lab File: BF091226.D
 Acq: 17 Nov 2016 21:37

Instrument :
 BNA_F
 ClientSampleId :
 WQ-2W

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.0	75.9	113.9
141	33.6	36.1	54.1#

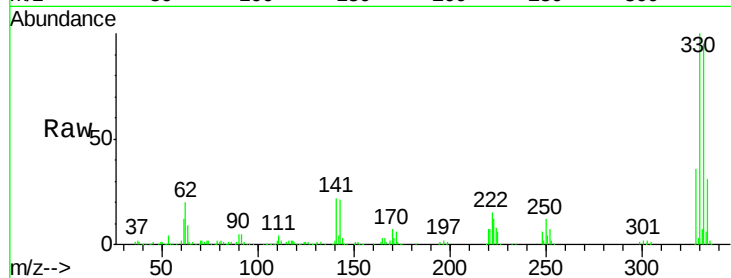


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

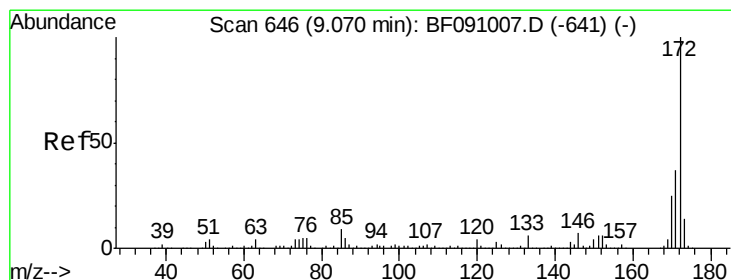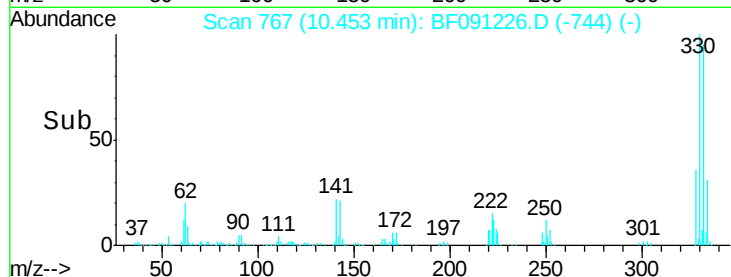
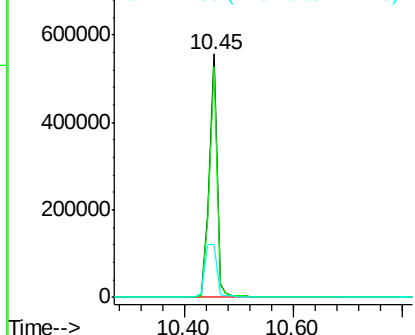



#44
 2-Fluorobiphenyl
 Concen: 86.91 ng
 RT: 8.99 min Scan# 639
 Delta R.T. -0.05 min
 Lab File: BF091226.D
 Acq: 17 Nov 2016 21:37

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.6	29.8	44.6
170	25.9	20.3	30.5

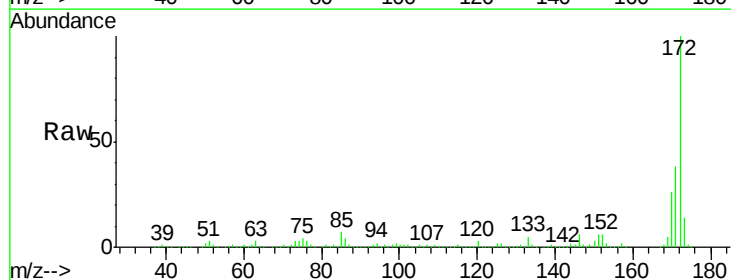

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



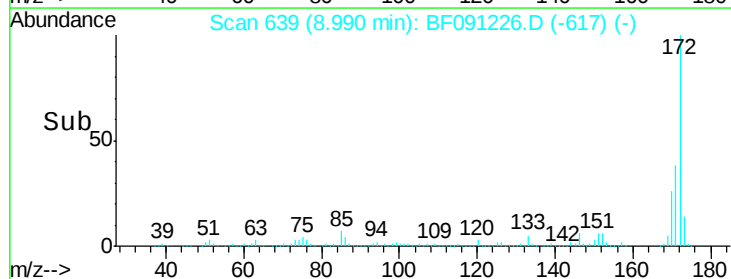
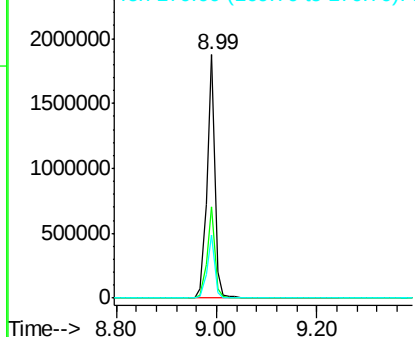


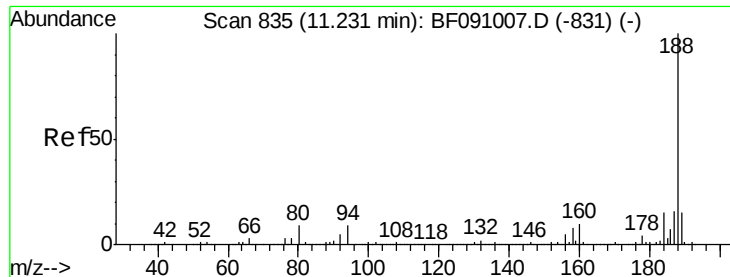

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.14 min Scan# 827
Delta R.T. -0.03 min
Lab File: BF091226.D
Acq: 17 Nov 2016 21:37




Instrument :
BNA_F
ClientSampled :
WQ-2W


Tot Ion:188 Resp: 731354
Ion Ratio Lower Upper
188 100
94 9.8 7.0 10.4
80 10.4 7.5 11.3

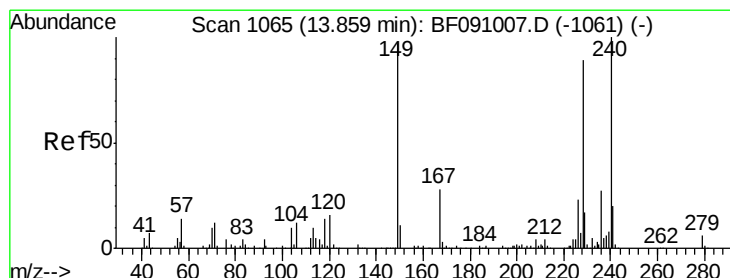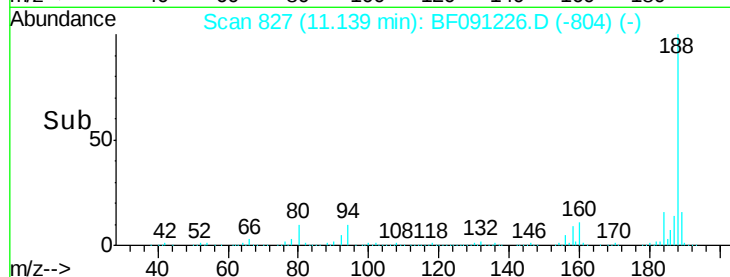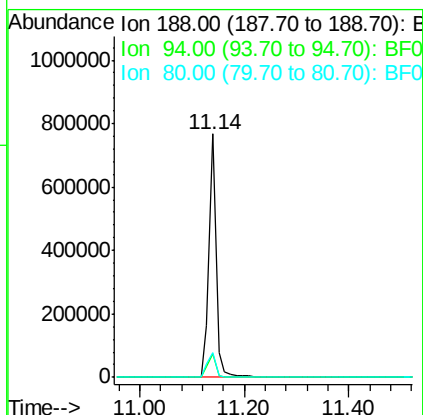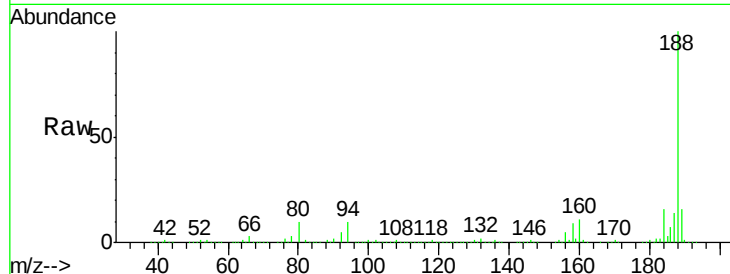

#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.77 min Scan# 1057
Delta R.T. -0.05 min
Lab File: BF091226.D
Acq: 17 Nov 2016 21:37

Tgt Ion:240 Resp: 471874
Ion Ratio Lower Upper
240 100
120 13.9 12.9 19.3
236 27.3 21.9 32.9


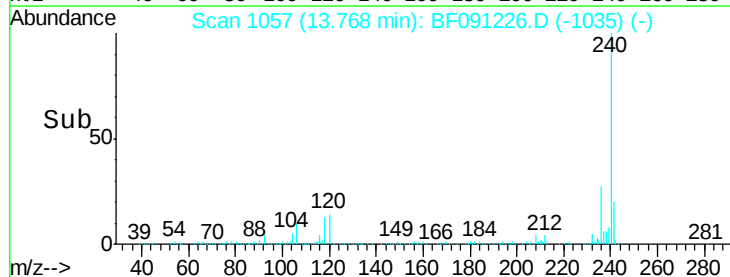
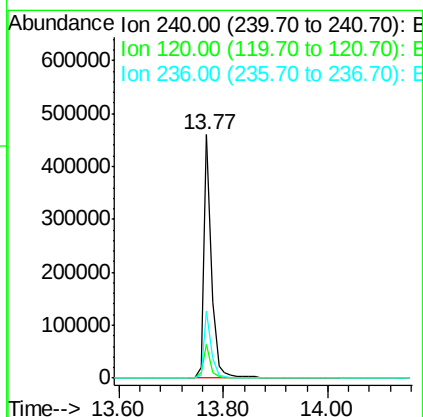
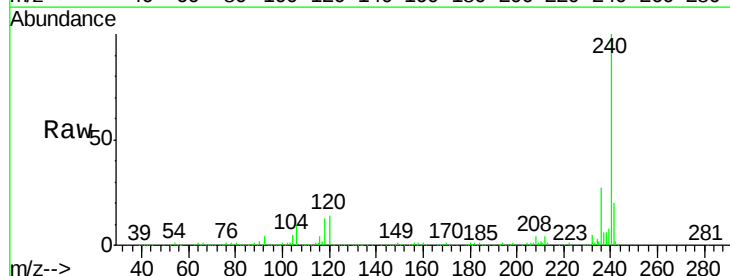


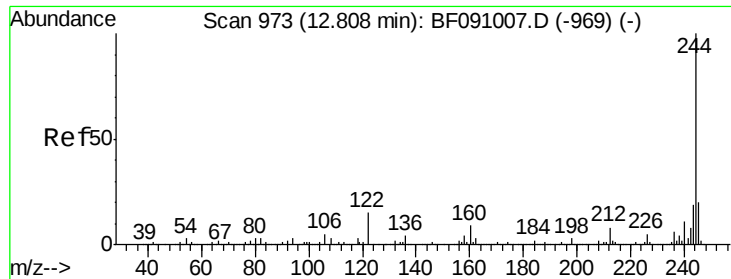

#78
 Terphenyl-d14
 Concen: 97.54 ng
 RT: 12.73 min Scan# 966
 Delta R.T. -0.03 min
 Lab File: BF091226.D
 Acq: 17 Nov 2016 21:37

Instrument :
 BNA_F
 ClientSampleId :
 WQ-2W

Tot Ion:244 Resp: 1844460
 Ion Ratio Lower Upper
 244 100
 212 7.4 6.4 9.6
 122 11.7 12.3 18.5#

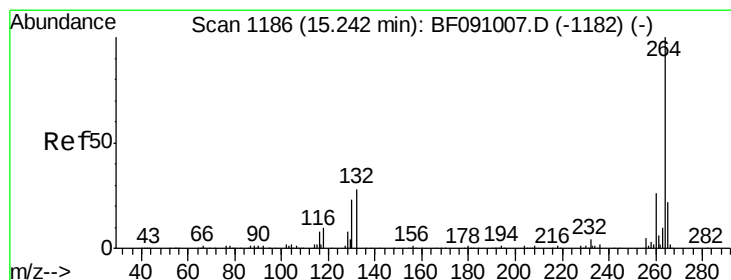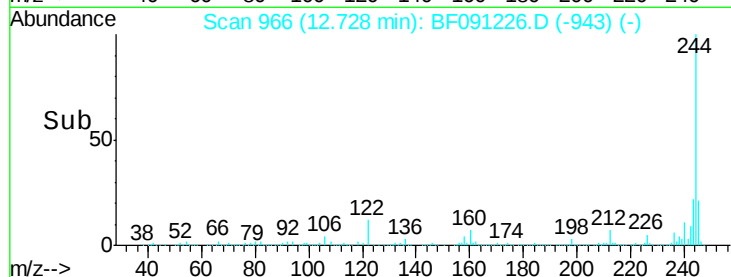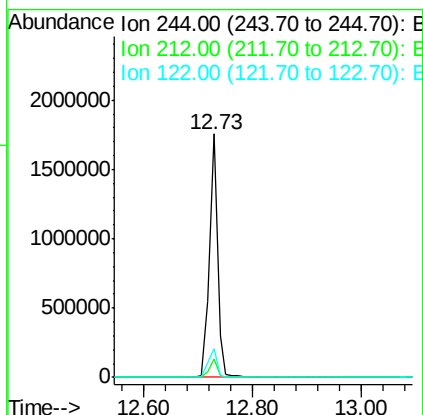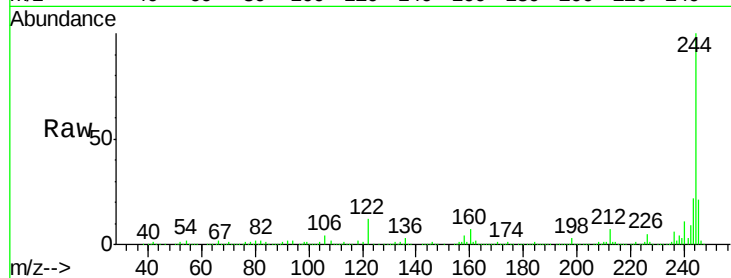

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.14 min Scan# 1177
 Delta R.T. -0.05 min
 Lab File: BF091226.D
 Acq: 17 Nov 2016 21:37

Tgt Ion:264 Resp: 343489
 Ion Ratio Lower Upper
 264 100
 260 24.8 20.6 30.8
 265 21.3 17.8 26.8

