

Data File : BF100723.D
Acq On : 18 Nov 2017 15:18
Operator : SJ/JU
Sample : I6517-03
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HP-WC(COMP)

Quant Time: Nov 20 00:14:11 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	93214	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	363893	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	159104	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	278643	20.00	ng	0.00
75) Chrysene-d12	14.04	240	198667	20.00	ng	0.00
86) Perylene-d12	15.52	264	179104	20.00	ng	0.00

System Monitoring Compounds						
5) 2-Fluorophenol	5.52	112	628607	108.10	ng	0.02
7) Phenol-d6	6.51	99	689143	96.11	ng	0.00
23) Nitrobenzene-d5	7.45	82	551610	100.22	ng	0.00
41) 2,4,6-Tribromophenol	10.71	330	212939	131.34	ng	0.00
44) 2-Fluorobiphenyl	9.24	172	1054153	100.89	ng	0.00
78) Terphenyl-d14	12.99	244	860465	99.52	ng	0.00

Target Compounds						Qvalue
9) Benzaldehyde	6.66	77	14626	2.86	ng	82
19) n-Nitroso-di-n-propylamine	7.45	70	72982	14.68	ng	# 78
25) Isophorone	7.45	82	551606	47.69	ng	# 64
47) 2-Nitroaniline	9.24	65	1564	3.28	ng	# 7
50) 2,6-Dinitrotoluene	9.92	165	20405	8.49	ng	# 24
56) 2,4-Dinitrotoluene	9.92	165	20405	6.73	ng	# 21
64) 4,6-Dinitro-2-methylphenol	10.70	198	261	8.72	ng	# 1
66) 4-Bromophenyl-phenylether	10.71	248	13043	4.37	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BF100723.D

Acq On : 18 Nov 2017 15:18

Operator : SJ/JU

Sample : I6517-03

Misc :

ALS Vial : 43 Sample Multiplier: 1

Instrument :

BNA_F

ClientSampleId :

HP-WC(COMP)


Quant Time: Nov 20 00:14:11 2017


Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Nov 17 15:22:08 2017

Response via : Initial Calibration

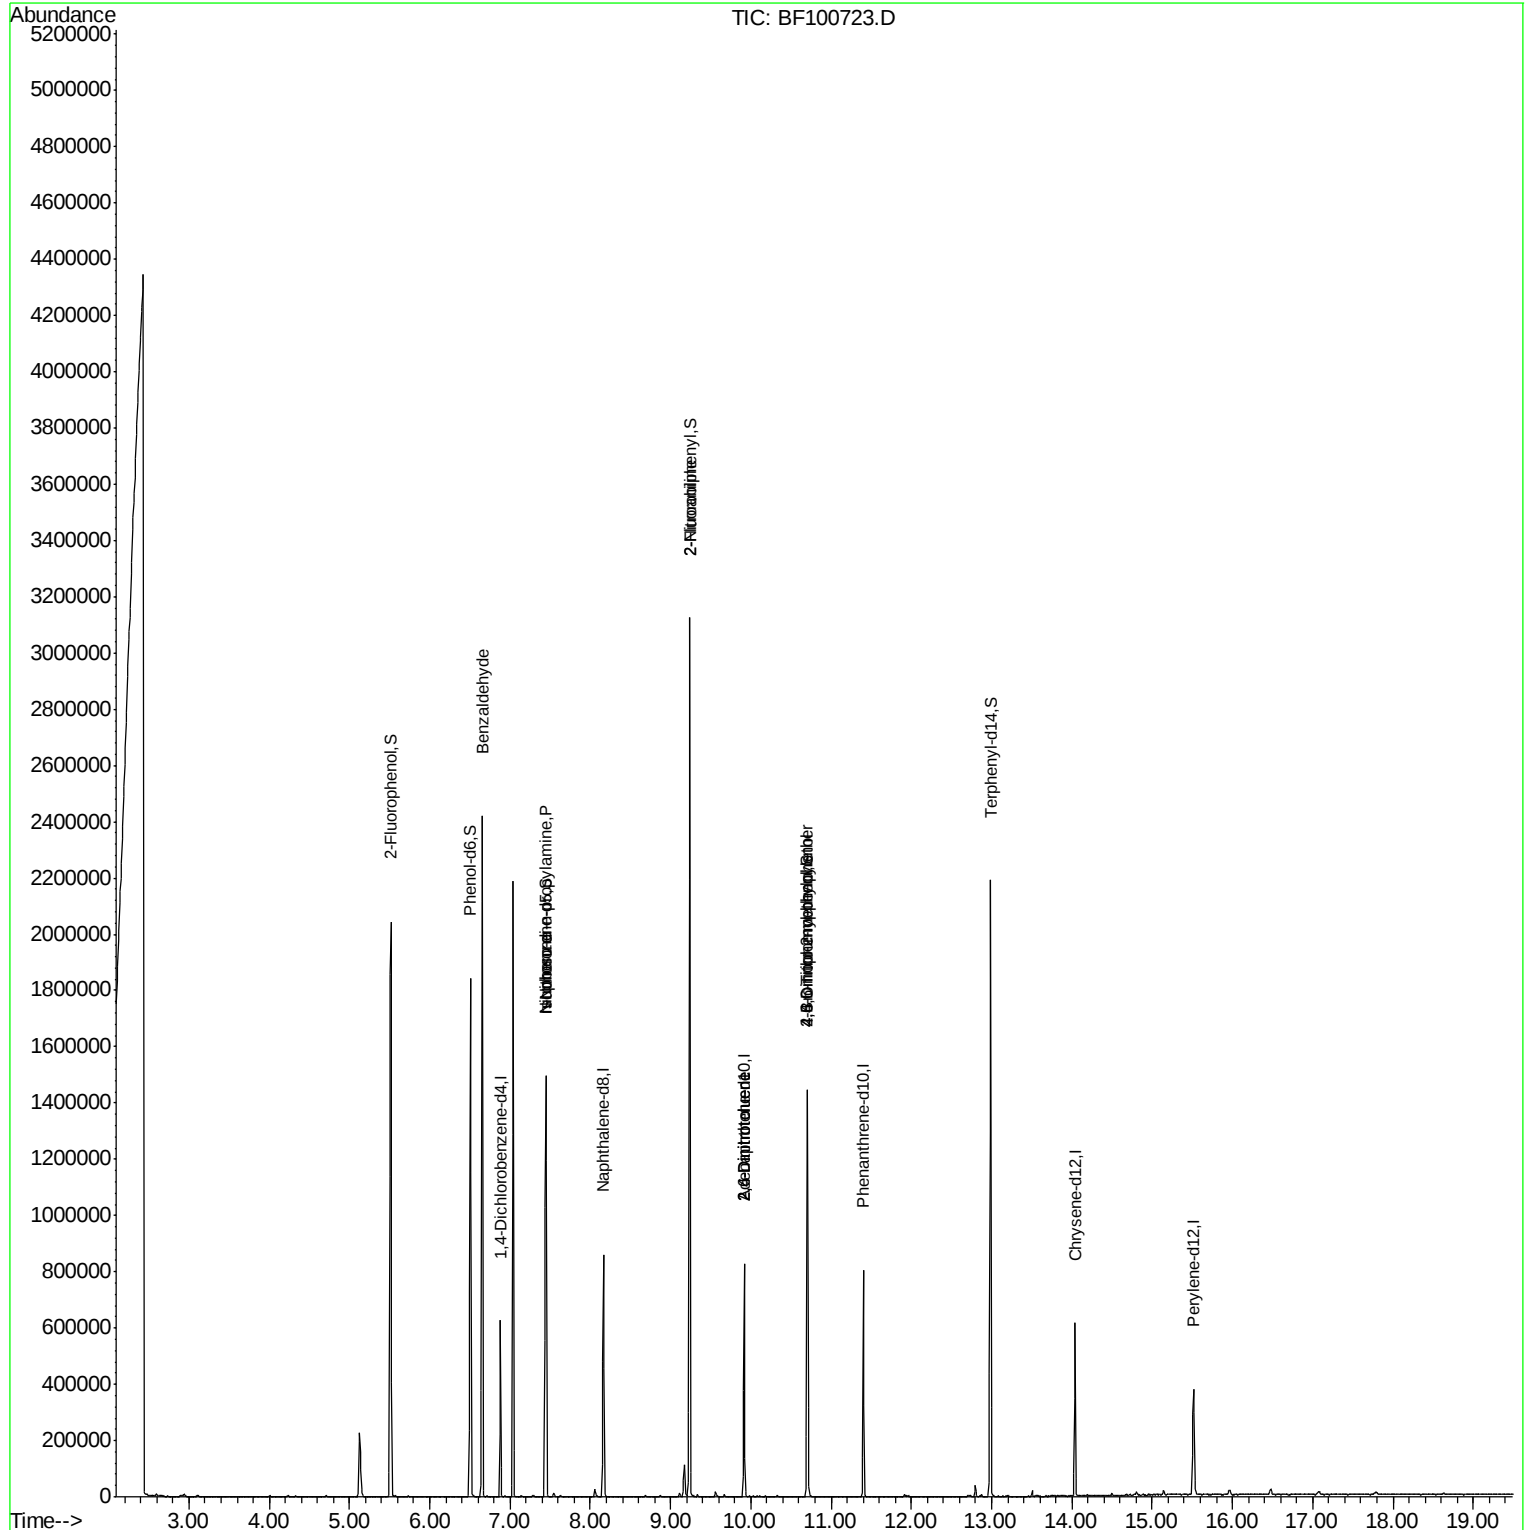

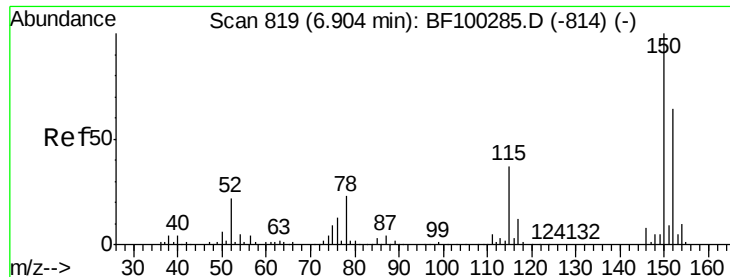


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.88 min Scan# 815
Delta R.T. -0.00 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18

Instrument :
BNA_F
ClientSampleId :
HP-WC(COMP)

Tgt Ion:152 Resp: 93214
Ion Ratio Lower Upper
152 100
150 160.3 124.6 186.8
115 61.1 50.1 75.1

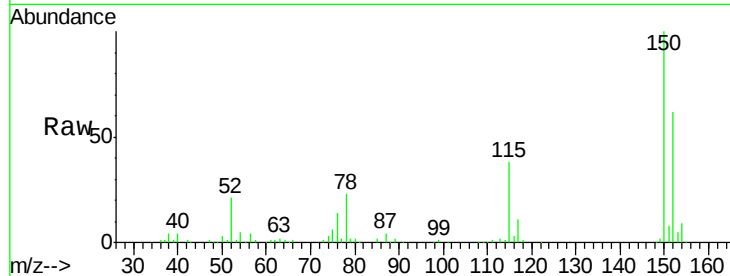


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

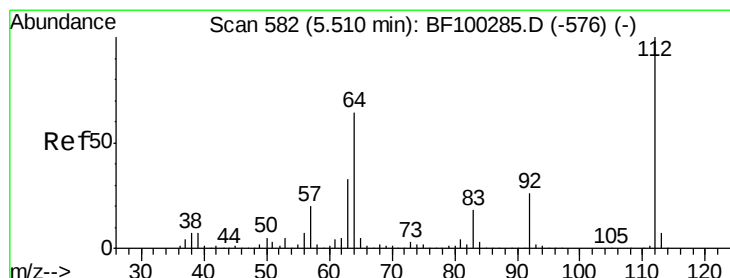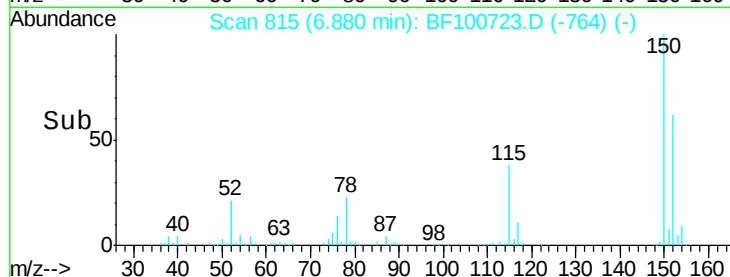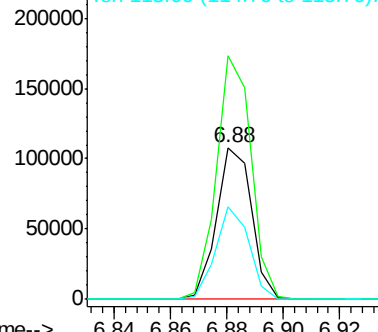



#5

2-Fluorophenol
Concen: 108.10 ng
RT: 5.52 min Scan# 583
Delta R.T. 0.02 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18

Tgt Ion:112 Resp: 628607
Ion Ratio Lower Upper
112 100
64 59.3 47.9 71.9
63 29.4 23.7 35.5

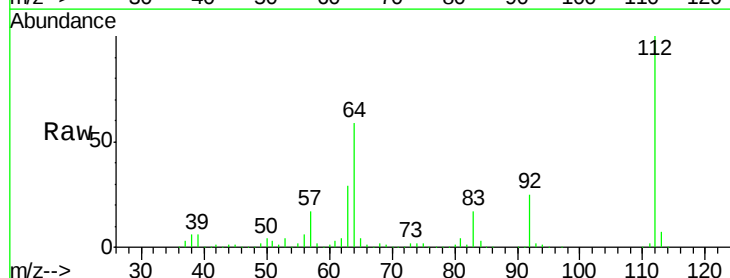

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

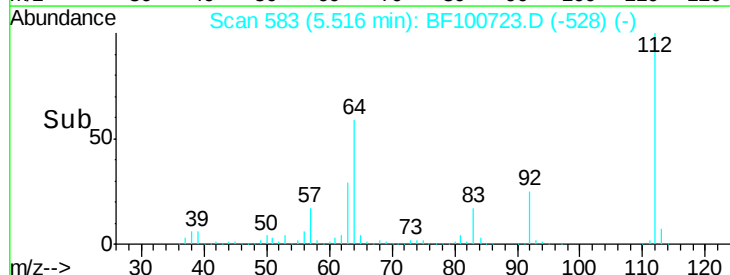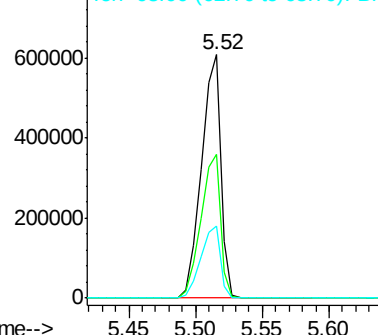



#7

Phenol-d6

Concen: 96.11 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.00 min

Lab File: BF100723.D

Acq: 18 Nov 2017 15:18

Instrument :

BNA_F

ClientSampleId :

HP-WC(COMP)


Tgt Ion: 99 Resp: 689143

Ion Ratio Lower Upper

99 100

42 19.4 14.5 21.7




71 32.5 25.4 38.0

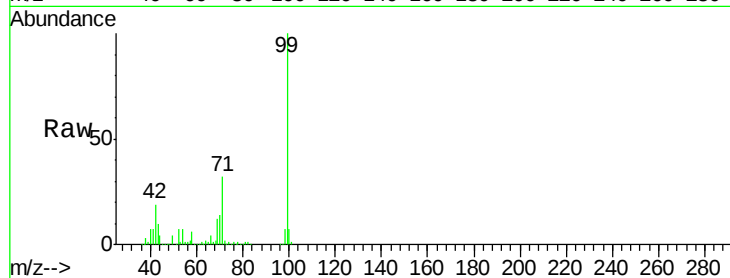

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

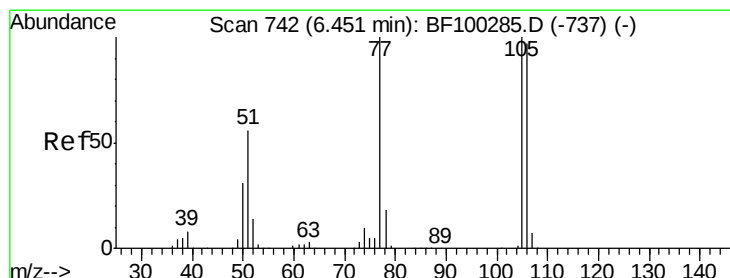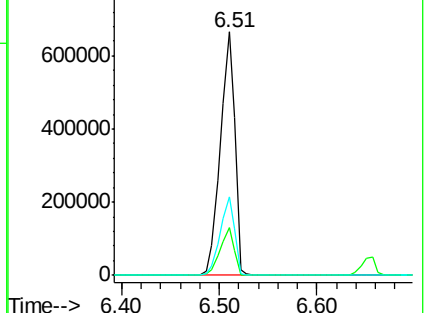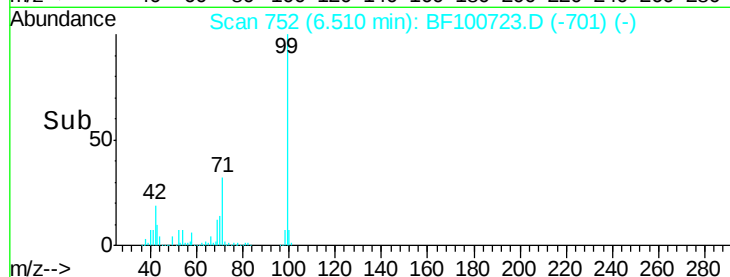

#9

Benzaldehyde

Concen: 2.86 ng

RT: 6.66 min Scan# 777

Delta R.T. 0.22 min

Lab File: BF100723.D

Acq: 18 Nov 2017 15:18


Tgt Ion: 77 Resp: 14626

Ion Ratio Lower Upper

77 100

105 82.6 81.1 121.1



106 77.1 74.5 114.5

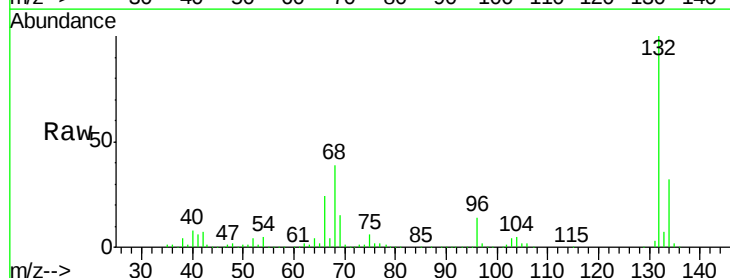

Abundance Ion 77.00 (76.70 to 77.70): BF1

Ion 105.00 (104.70 to 105.70): B

Ion 106.00 (105.70 to 106.70): B

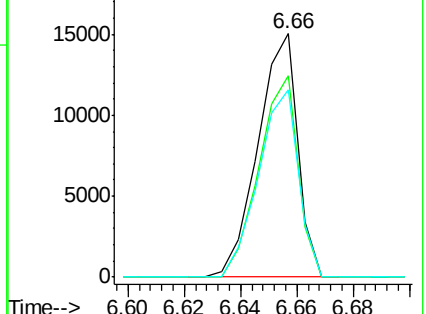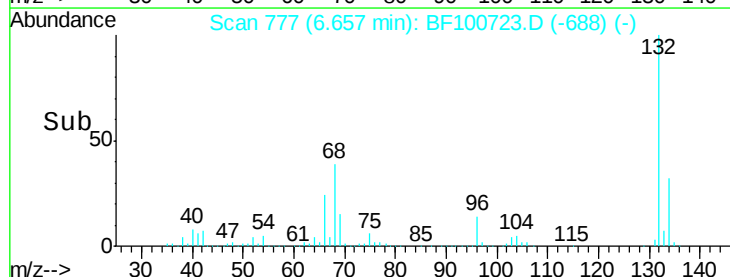



#19

n-Nitroso-di-n-propylamine

Concen: 14.68 ng

RT: 7.45 min Scan# 911

Delta R.T. 0.15 min

Lab File: BF100723.D

Acq: 18 Nov 2017 15:18

Instrument :

BNA_F

ClientSampleId :

HP-WC(COMP)

Tgt Ion: 70 Resp: 72982



Ion Ratio Lower Upper

70 100

42 48.0 47.5 71.3

101 0.0 7.4 11.2#

130 2.2 16.6 25.0#





Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

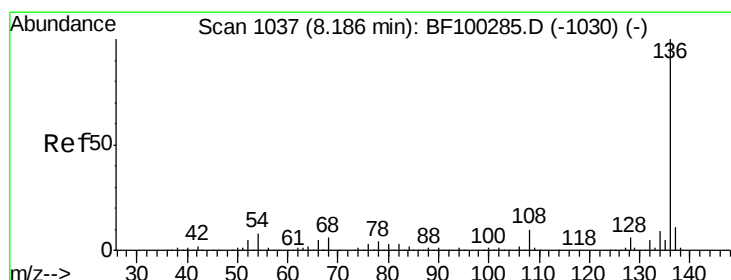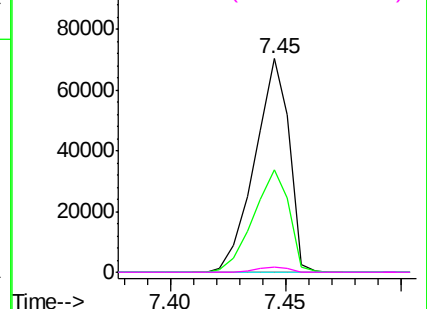

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.16 min Scan# 1033

Delta R.T. -0.01 min

Lab File: BF100723.D

Acq: 18 Nov 2017 15:18

Tgt Ion: 136 Resp: 363893



Ion Ratio Lower Upper

136 100

137 11.1 8.9 13.3

54 8.3 6.6 9.8

68 5.6 5.0 7.4




Abundance Ion 136.00 (135.70 to 136.70): BF1

Ion 137.00 (136.70 to 137.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1




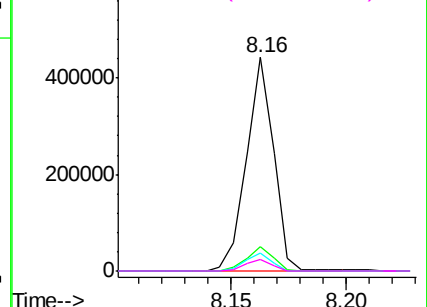




#23
Nitrobenzene-d5
Concen: 100.22 ng
RT: 7.45 min Scan# 911
Delta R.T. -0.01 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18




Instrument :
BNA_F
ClientSampleId :
HP-WC(COMP)

Tgt Ion: 82 Resp: 551610
Ion Ratio Lower Upper
82 100
128 46.7 36.1 54.1
54 53.9 41.4 62.2

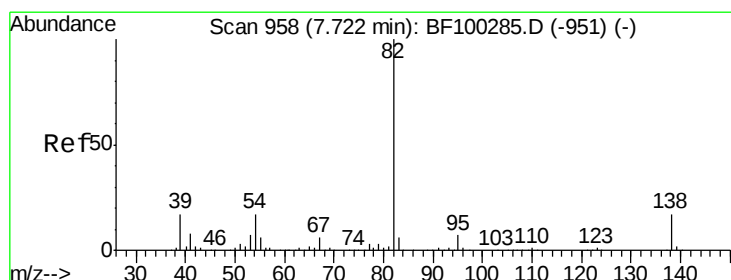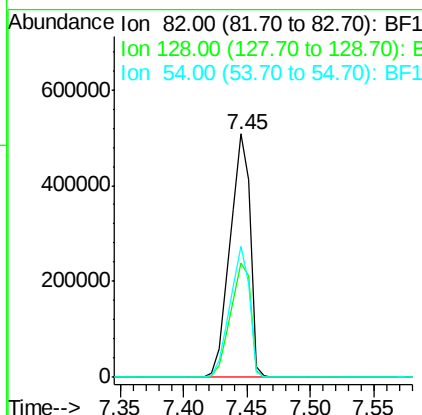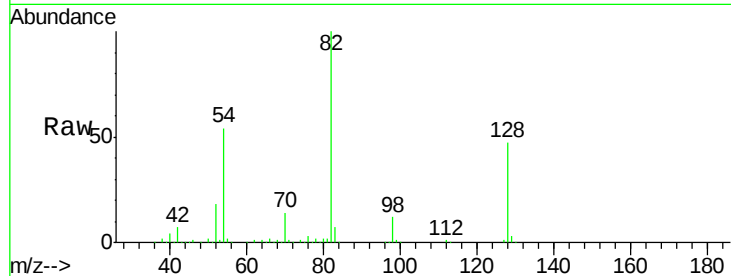

#25
Isophorone
Concen: 47.69 ng
RT: 7.45 min Scan# 911
Delta R.T. -0.26 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18

Tgt Ion: 82 Resp: 551606
Ion Ratio Lower Upper
82 100
95 0.0 5.2 7.8#
138 0.0 14.9 22.3#


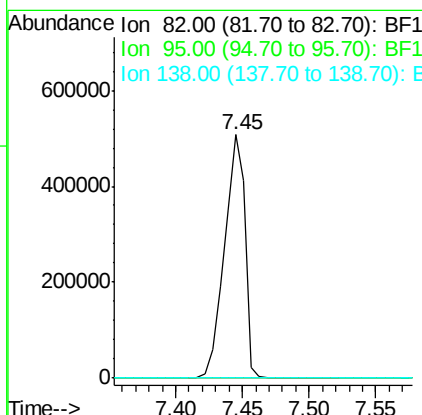






#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.01 min
 Lab File: BF100723.D
 Acq: 18 Nov 2017 15:18




Instrument :
 BNA_F
 ClientSampleId :
 HP-WC(COMP)


Tgt Ion:164 Resp: 159104
 Ion Ratio Lower Upper
 164 100
 162 107.1 86.1 129.1
 160 46.7 38.3 57.5

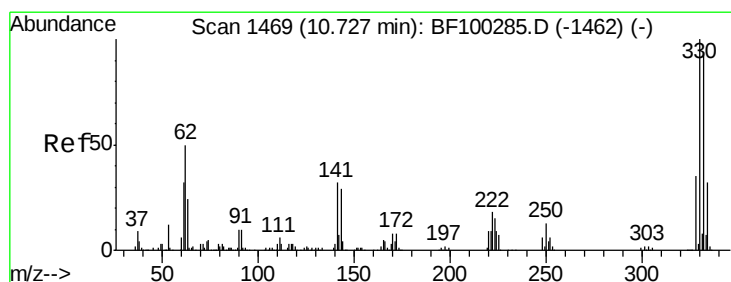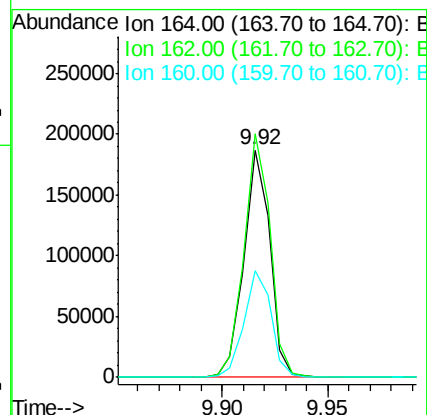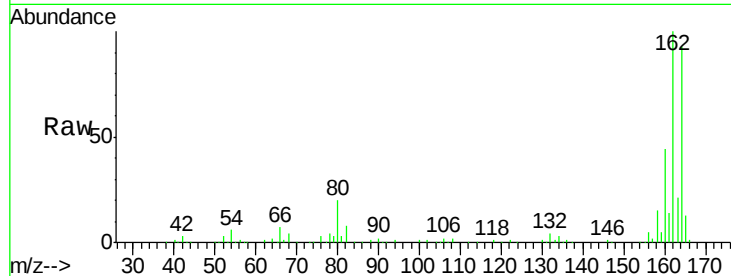

#41
 2,4,6-Tribromophenol
 Concen: 131.34 ng
 RT: 10.71 min Scan# 1466
 Delta R.T. -0.00 min
 Lab File: BF100723.D
 Acq: 18 Nov 2017 15:18

Tgt Ion:330 Resp: 212939
 Ion Ratio Lower Upper
 330 100
 332 95.5 77.0 115.6
 141 28.5 29.9 44.9#

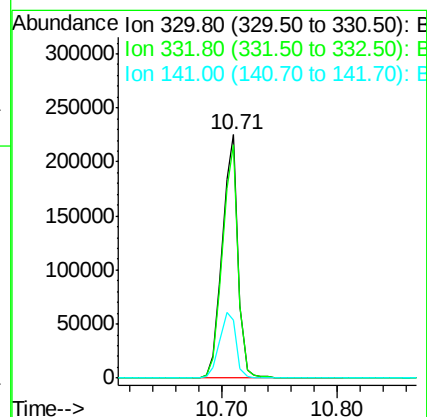


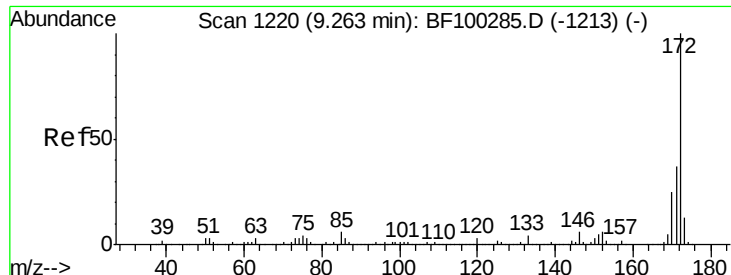



#44
 2-Fluorobiphenyl
 Concen: 100.89 ng
 RT: 9.24 min Scan# 1216
 Delta R.T. -0.00 min
 Lab File: BF100723.D
 Acq: 18 Nov 2017 15:18

Instrument :
 BNA_F
 ClientSampleId :
 HP-WC(COMP)

Tgt Ion: 172 Resp: 1054153
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.7 44.5
 170 24.1 19.6 29.4

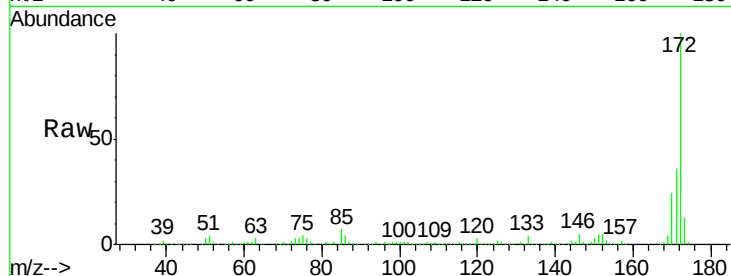


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


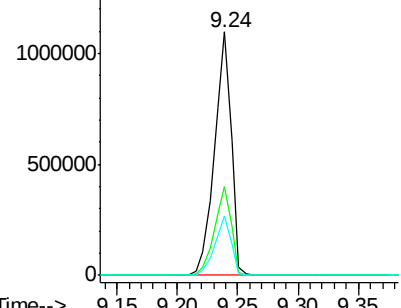



#47
 2-Nitroaniline
 Concen: 3.28 ng
 RT: 9.24 min Scan# 1216
 Delta R.T. -0.22 min
 Lab File: BF100723.D
 Acq: 18 Nov 2017 15:18

Tgt Ion: 65 Resp: 1564
 Ion Ratio Lower Upper
 65 100
 92 178.6 55.8 83.6#
 138 40.6 91.2 136.8#



Abundance Ion 65.00 (64.70 to 65.70): BF1
 Ion 92.00 (91.70 to 92.70): BF1
 Ion 138.00 (137.70 to 138.70): E




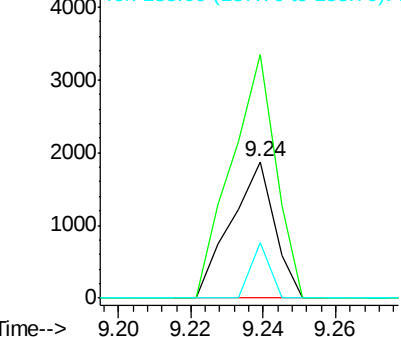


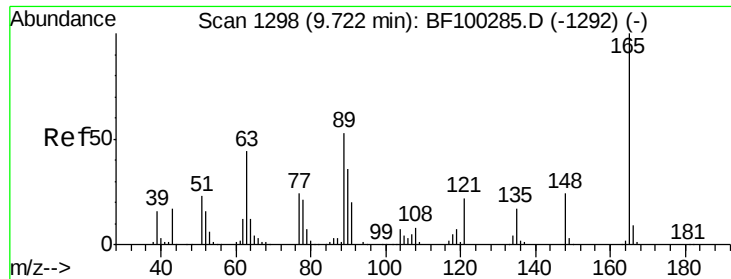

#50
2,6-Dinitrotoluene
Concen: 8.49 ng
RT: 9.92 min Scan# 1331
Delta R.T. 0.21 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18




Instrument :
BNA_F
ClientSampleId :
HP-WC(COMP)


Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	44.7	67.1#
89	0.0	44.0	66.0#

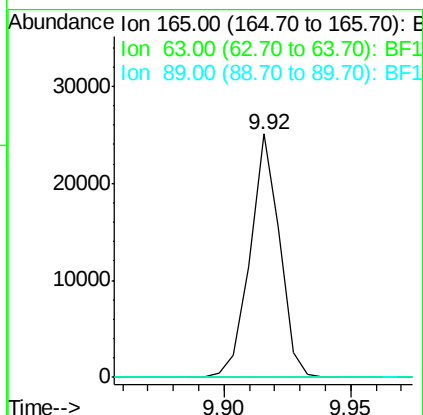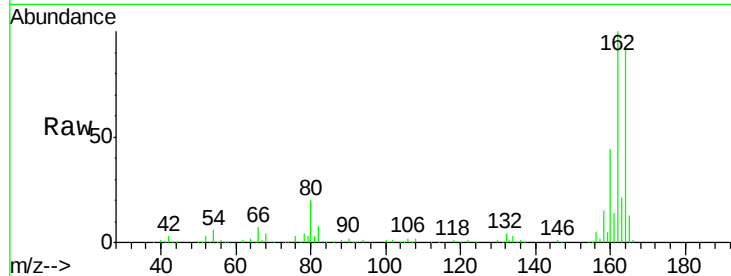

#56
2,4-Dinitrotoluene
Concen: 6.73 ng
RT: 9.92 min Scan# 1331
Delta R.T. -0.19 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18

Tgt Ion	Ratio	Lower	Upper
165	100		
63	0.0	36.4	54.6#
89	0.0	57.8	86.6#
182	0.0	1.6	2.4#


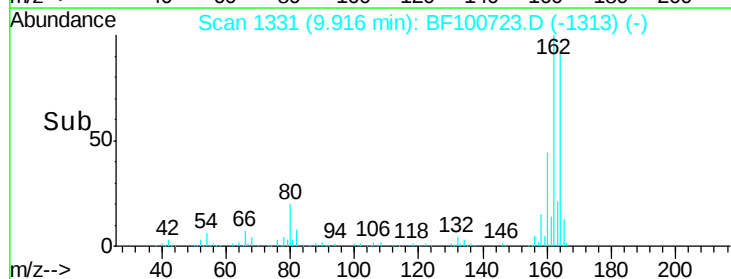
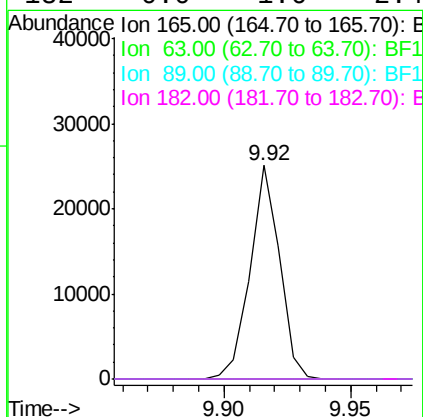



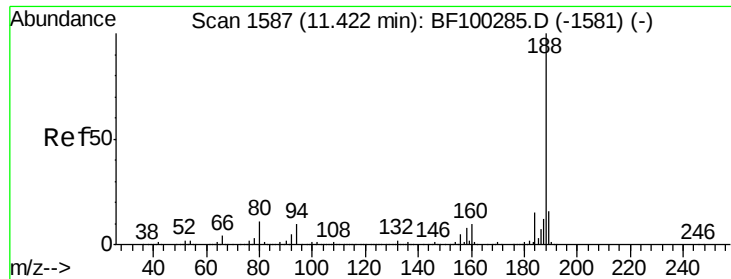

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.40 min Scan# 1584
Delta R.T. -0.00 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18




Instrument :
BNA_F
ClientSampleId :
HP-WC(COMP)


Tgt Ion:188 Resp: 278643
Ion Ratio Lower Upper
188 100
94 8.9 8.5 12.7
80 9.0 9.2 13.8#

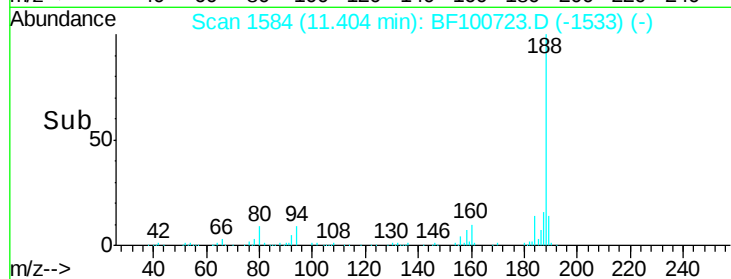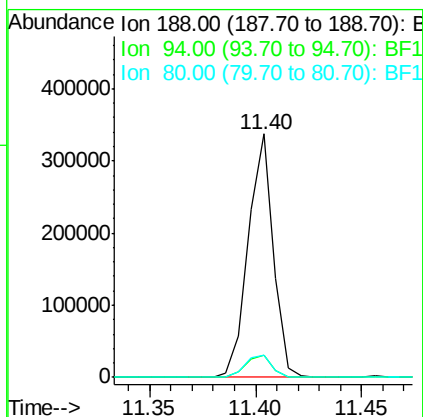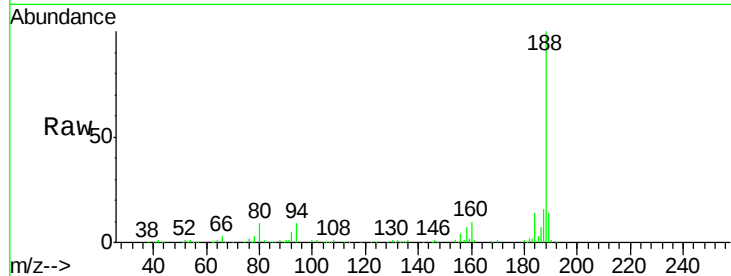

#64
4,6-Dinitro-2-methylphenol
Concen: 8.72 ng
RT: 10.70 min Scan# 1465
Delta R.T. 0.19 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18

Tgt Ion:198 Resp: 261
Ion Ratio Lower Upper
198 100
51 232.8 37.7 77.7#
105 261.3 36.3 76.3#

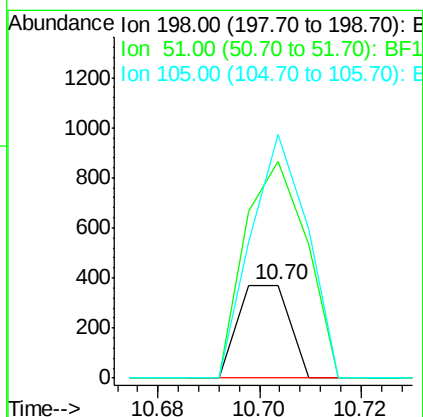


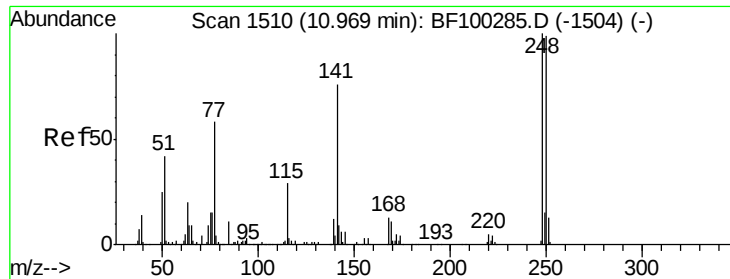




#66
4-Bromophenyl-phenylether
Concen: 4.37 ng
RT: 10.71 min Scan# 1466
Delta R.T. -0.24 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18

Instrument :
BNA_F
ClientSampleId :
HP-WC(COMP)

Tgt Ion:248 Resp: 13043
Ion Ratio Lower Upper
248 100
250 194.1 76.9 115.3#
141 411.5 74.4 111.6#

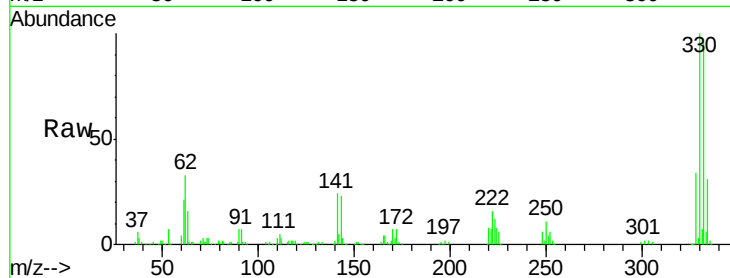


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

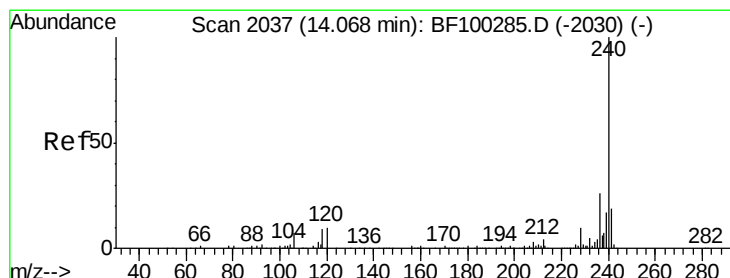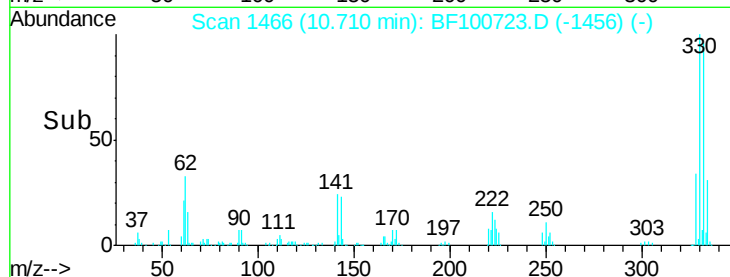
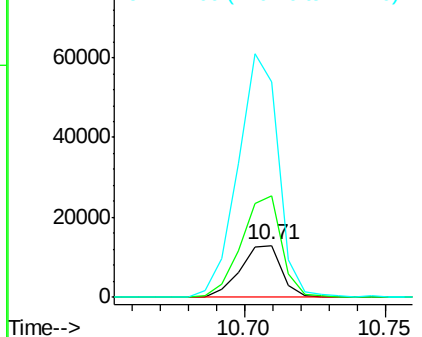



#75
Chrysene-d12
Concen: 20.00 ng
RT: 14.04 min Scan# 2032
Delta R.T. -0.01 min
Lab File: BF100723.D
Acq: 18 Nov 2017 15:18

Tgt Ion:240 Resp: 198667
Ion Ratio Lower Upper
240 100
120 11.6 9.5 14.3
236 26.0 20.7 31.1

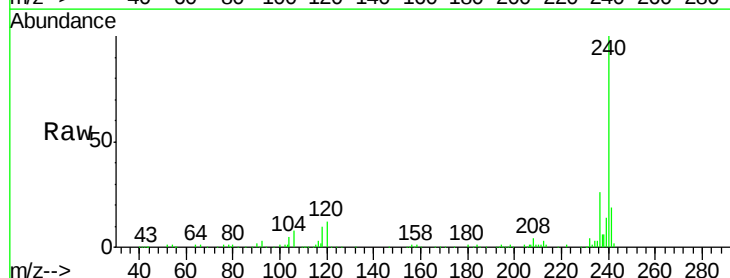

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



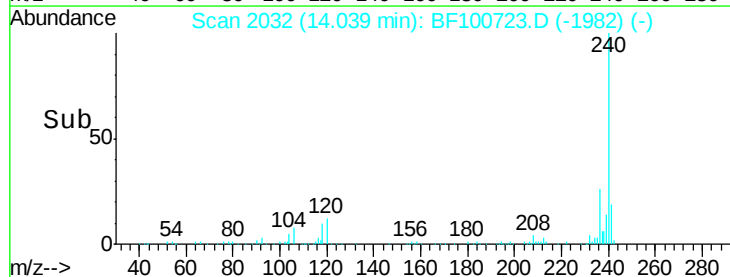
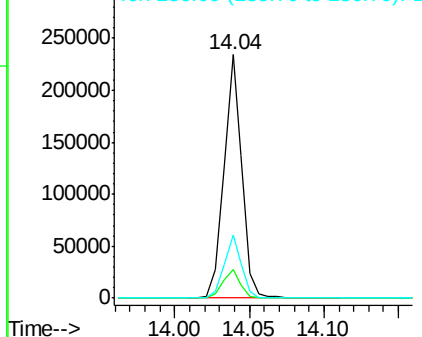


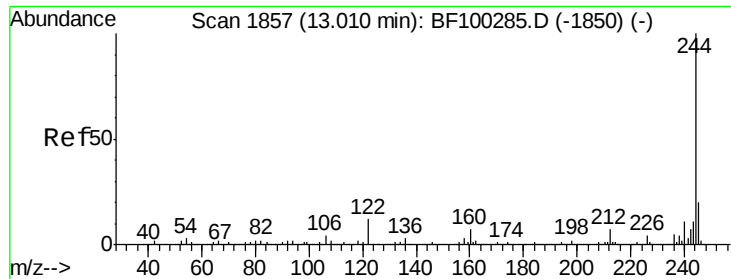

#78
 Terphenyl-d14
 Concen: 99.52 ng
 RT: 12.99 min Scan# 1854
 Delta R.T. 0.01 min
 Lab File: BF100723.D
 Acq: 18 Nov 2017 15:18

Instrument :
 BNA_F
 ClientSampleId :
 HP-WC(COMP)

Tgt Ion:244 Resp: 860465
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.4 8.0
 122 10.0 11.0 16.4#

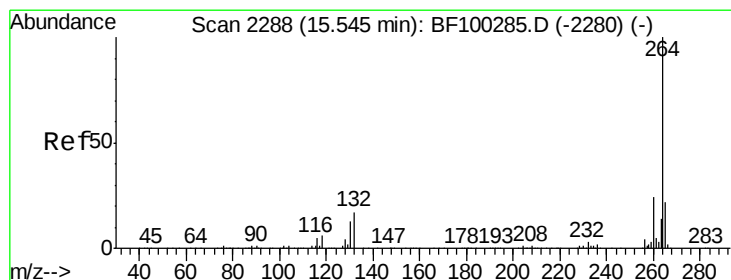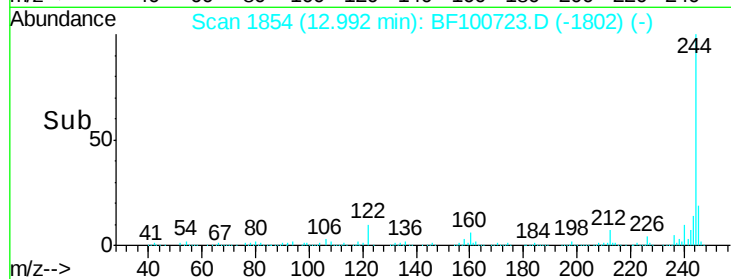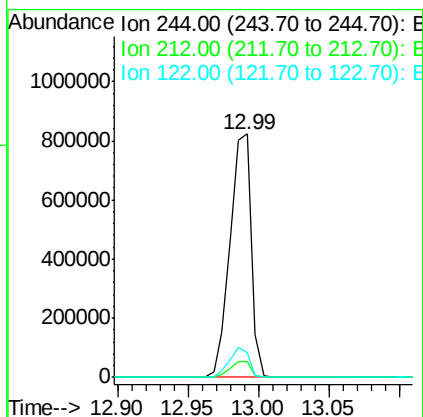

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.52 min Scan# 2283
 Delta R.T. -0.00 min
 Lab File: BF100723.D
 Acq: 18 Nov 2017 15:18

Tgt Ion:264 Resp: 179104
 Ion Ratio Lower Upper
 264 100
 260 23.4 19.2 28.8
 265 21.1 17.5 26.3

