

Data File : BF100664.D

Acq On : 17 Nov 2017 9:20

Operator : SJ/JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Nov 18 03:19:22 2017

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Nov 17 15:22:08 2017

Response via : Initial Calibration

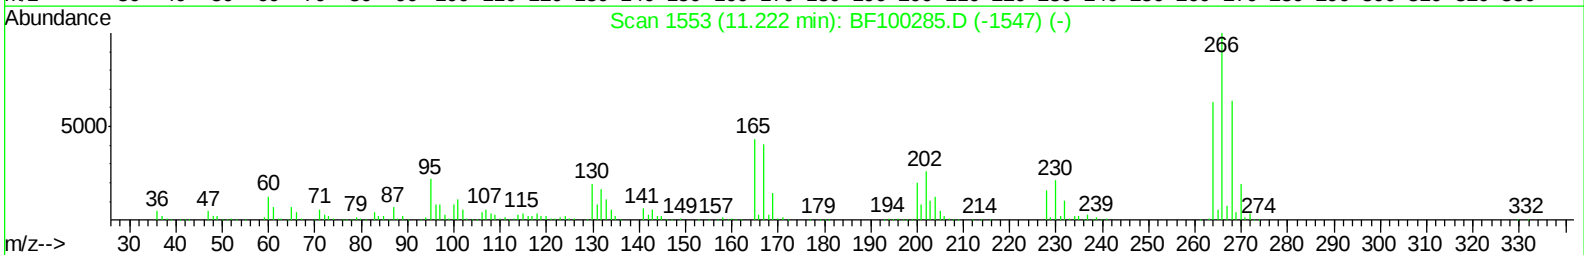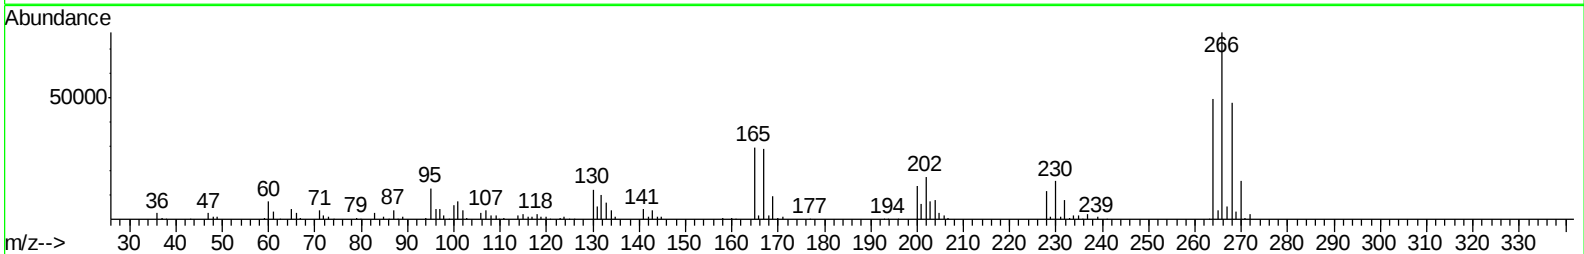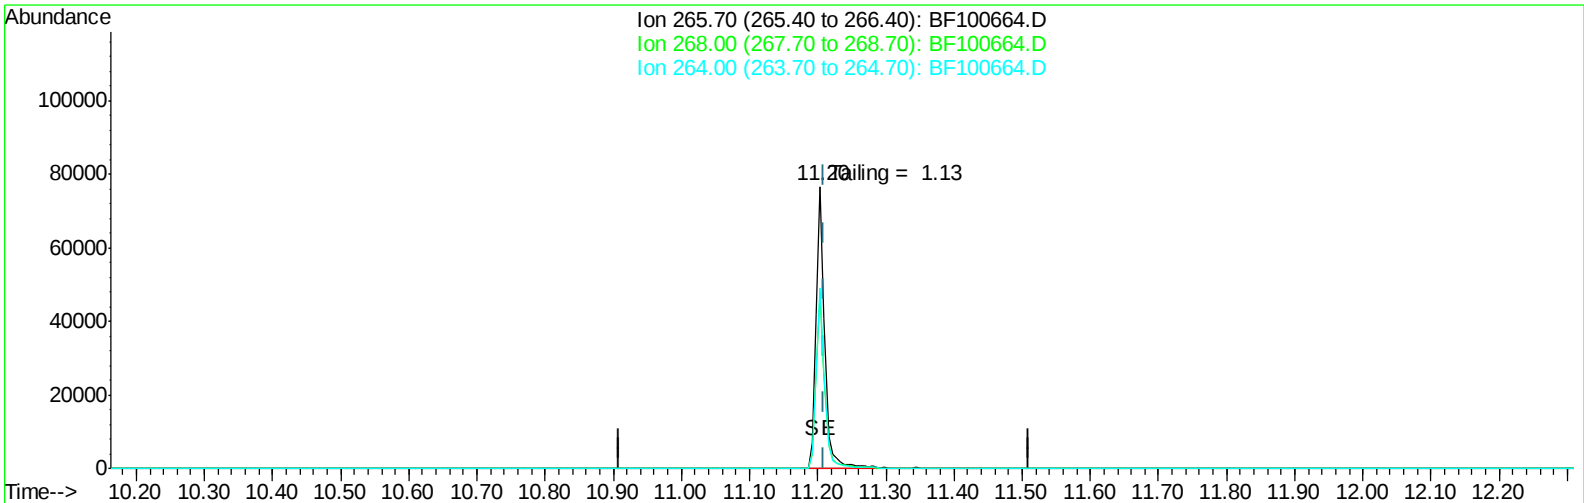

TIC: BF100664.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 0.00ng

response 67176

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.41
264.00	61.90	64.29
0.00	0.00	0.00

Data File : BF100664.D
Acq On : 17 Nov 2017 9:20
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 03:19:22 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

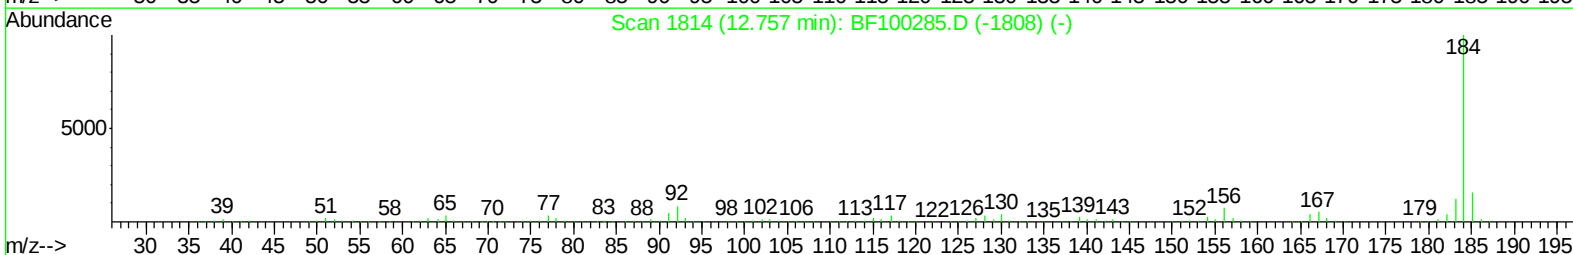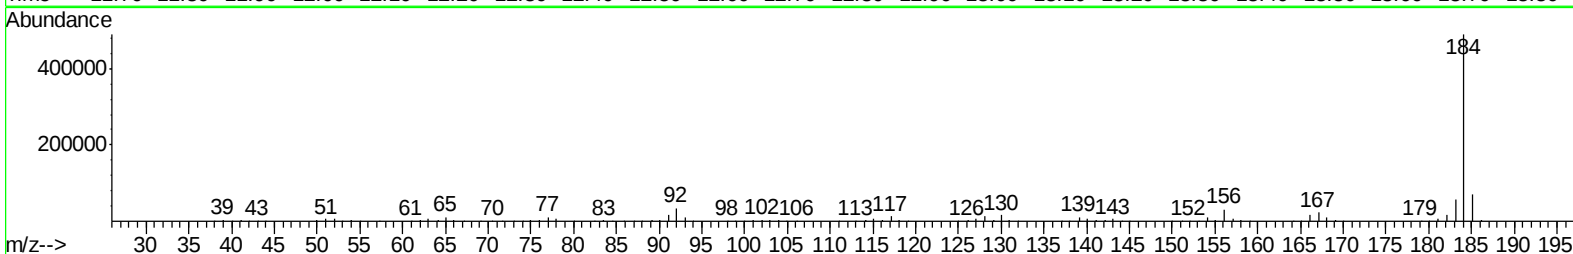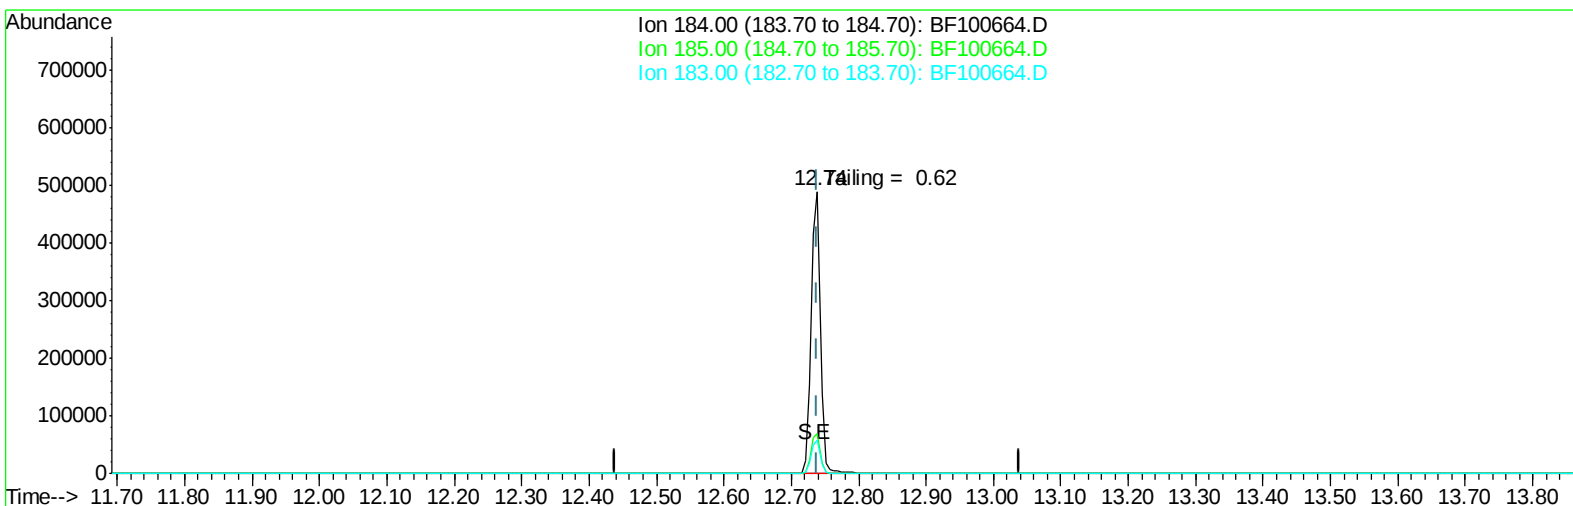

TIC: BF100664.D

(76) Benzidine

12.739min (-0.000) 0.00ng

response 446898

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.15
183.00	11.60	11.65
0.00	0.00	0.00