
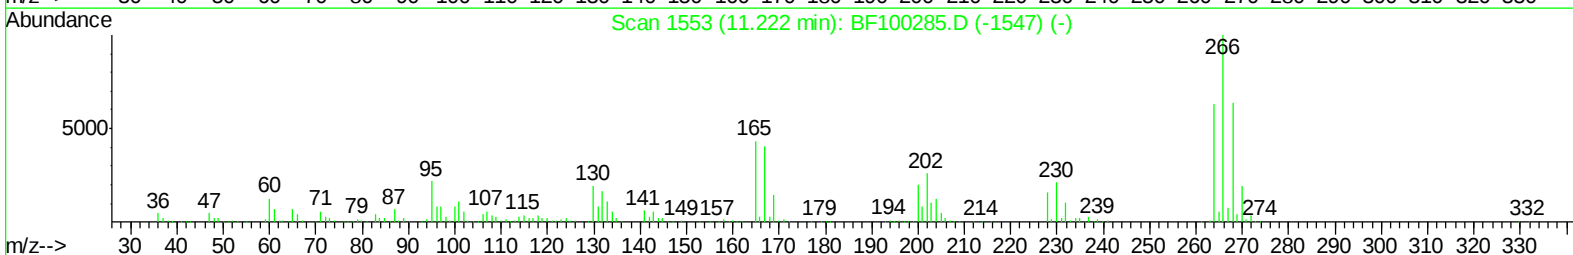
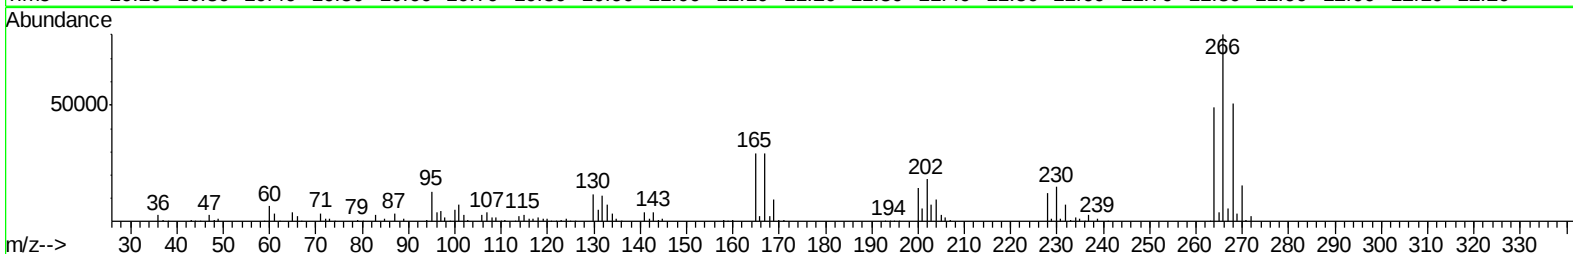


Data File : BF100679.D  
Acq On : 17 Nov 2017 17:50  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 03:18:00 2017  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Nov 17 15:22:08 2017  
Response via : Initial Calibration

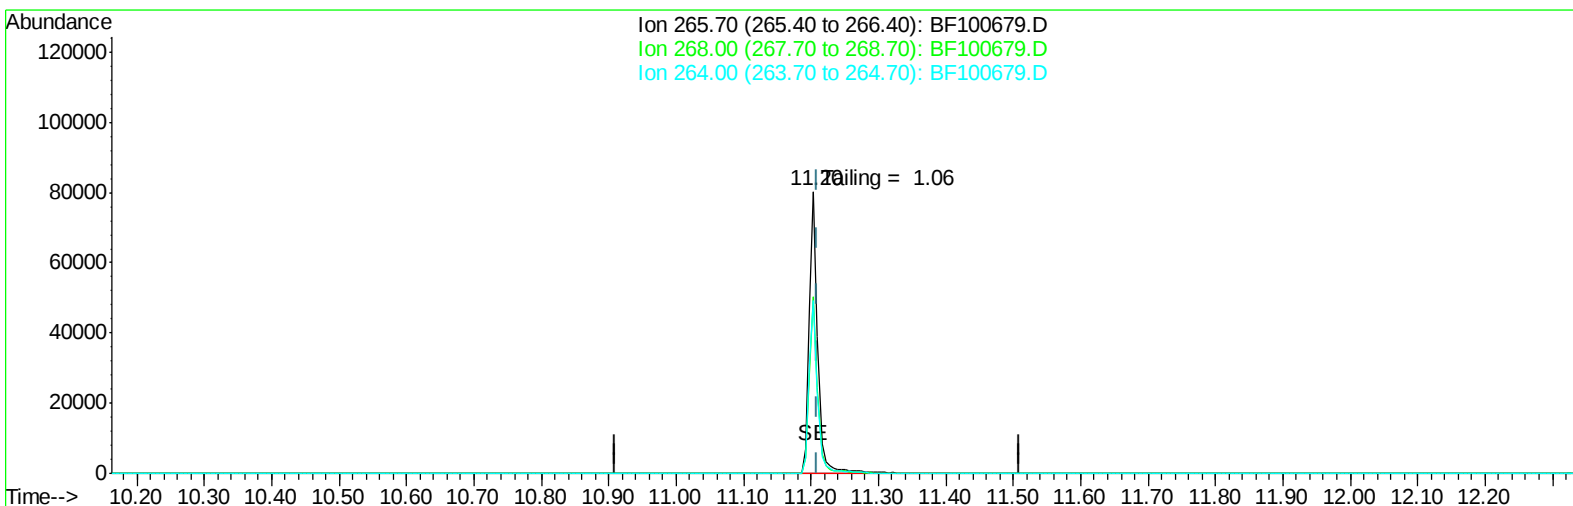

TIC: BF100679.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 0.00ng

response 69959

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 62.95 |
| 264.00 | 61.90 | 61.45 |
| 0.00   | 0.00  | 0.00  |

Data File : BF100679.D  
Acq On : 17 Nov 2017 17:50  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 03:18:00 2017  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF110817.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Nov 17 15:22:08 2017  
Response via : Initial Calibration

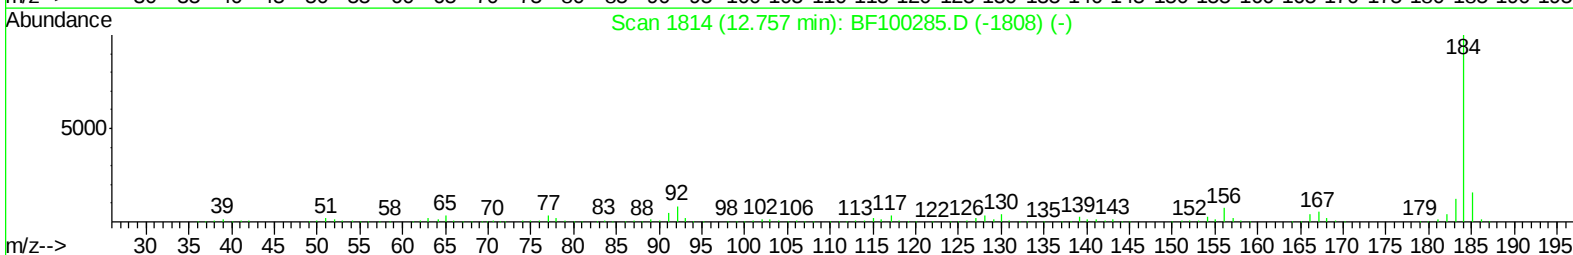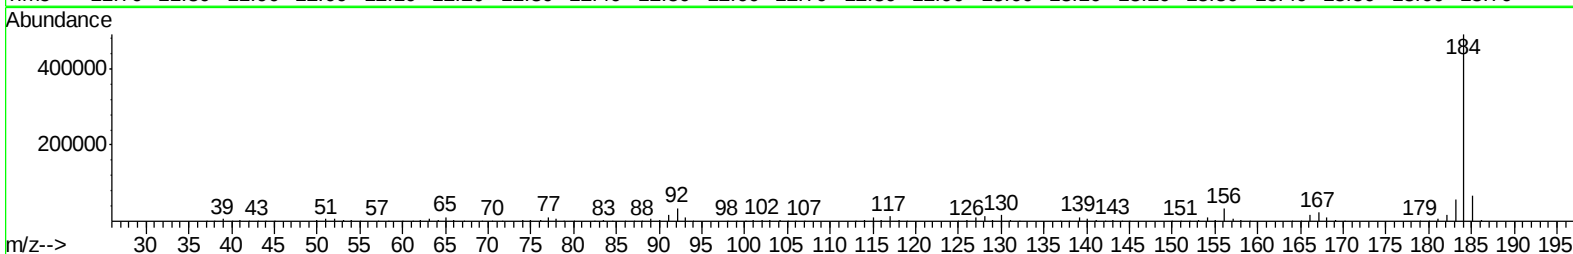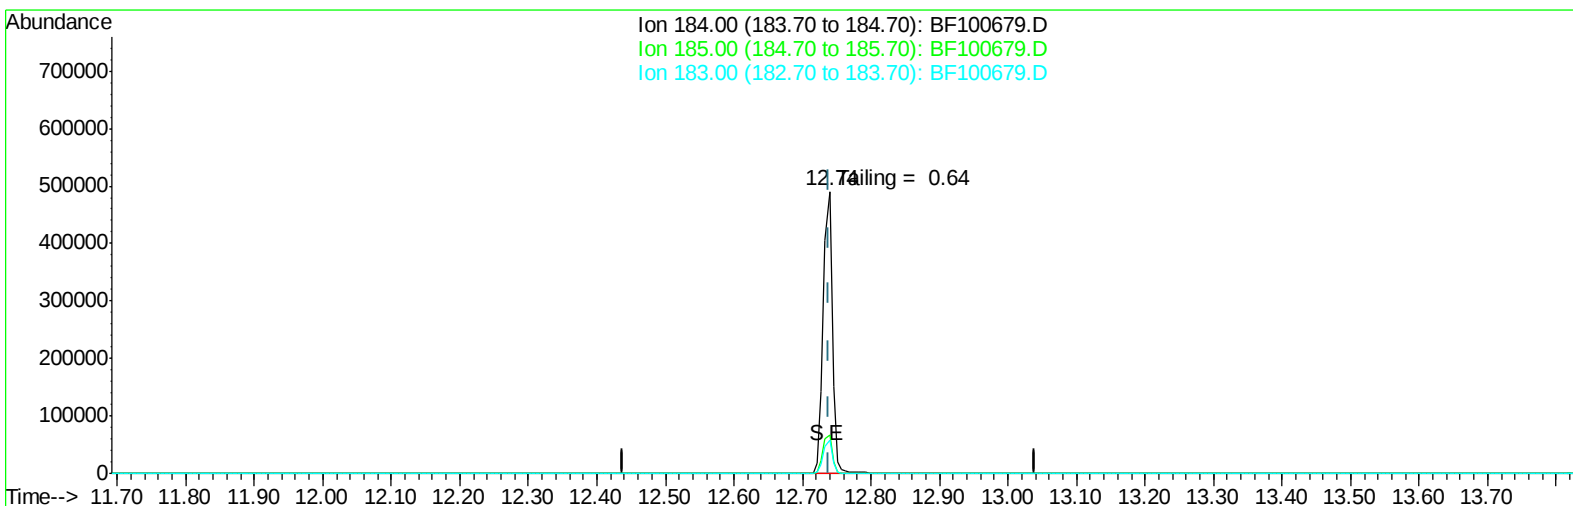

TIC: BF100679.D

(76) Benzidine

12.739min (-0.000) 0.00ng

response 442885

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 13.72 |
| 183.00 | 11.60 | 11.81 |
| 0.00   | 0.00  | 0.00  |