
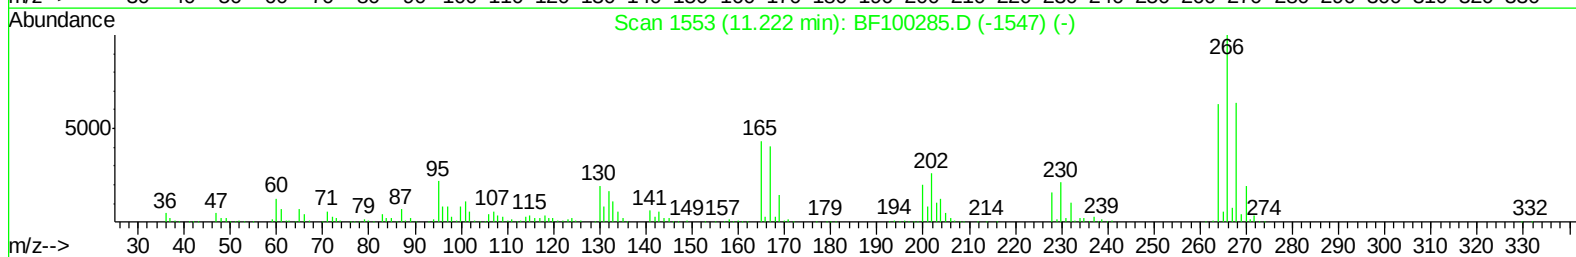
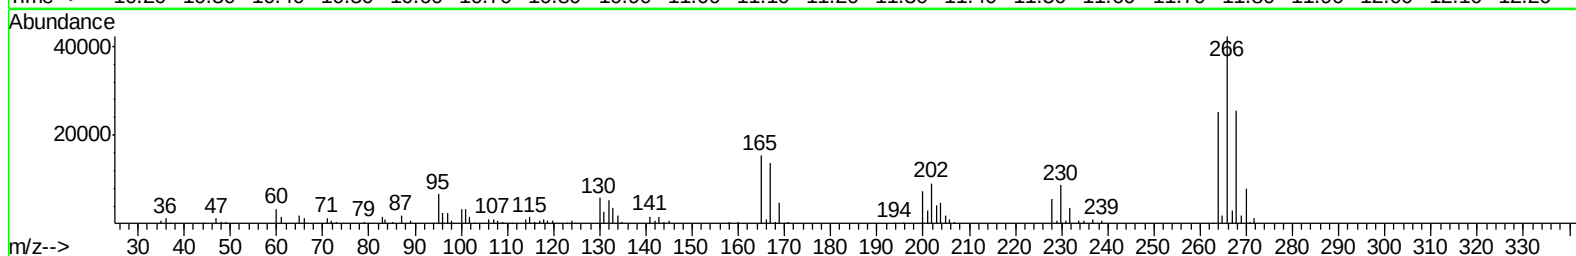


Data File : BF100705.D
Acq On : 18 Nov 2017 6:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 04:55:13 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

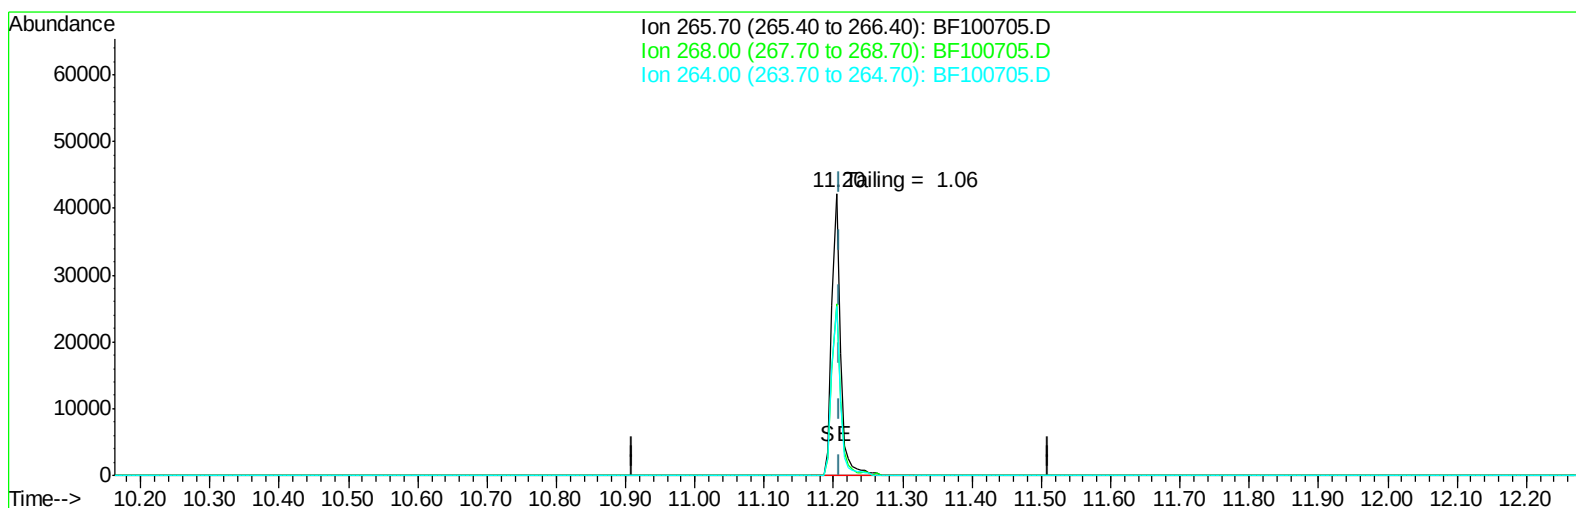

TIC: BF100705.D

(69) Pentachlorophenol (C)




11.204min (-0.006) 0.00ng

response 35781

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.79
264.00	61.90	60.00
0.00	0.00	0.00

Data File : BF100705.D
Acq On : 18 Nov 2017 6:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 20 04:55:13 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

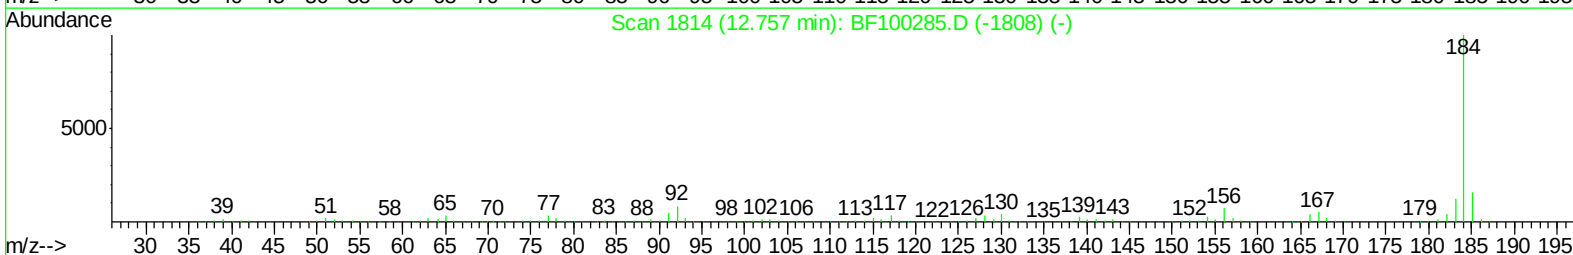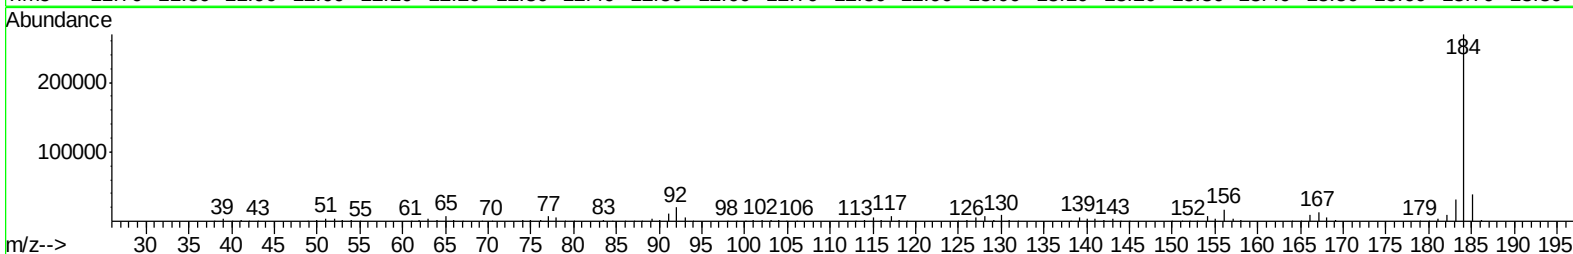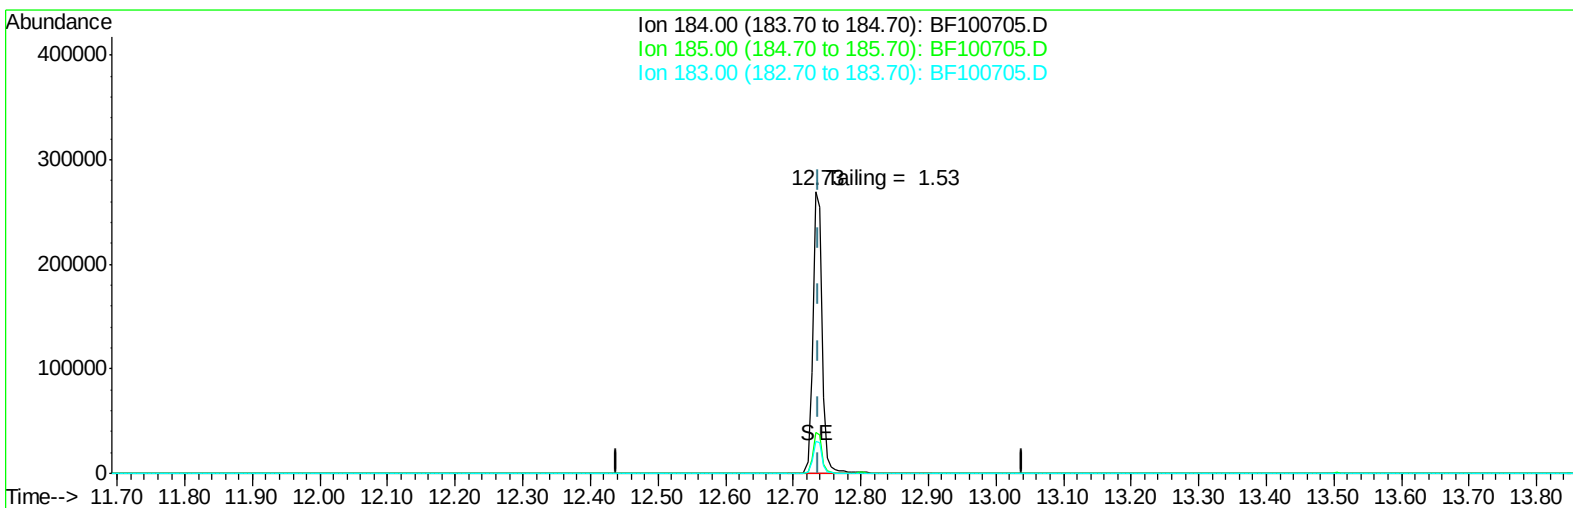

TIC: BF100705.D

(76) Benzidine

12.733min (-0.006) 0.00ng

response 262687

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.43
183.00	11.60	11.44
0.00	0.00	0.00