

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111717\
 Data File : BF100708.D
 Acq On : 18 Nov 2017 8:37
 Operator : SJ/JU
 Sample : I6460-01 10X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-28-2-0-1.5

Quant Time: Nov 20 00:42:06 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Nov 17 15:22:08 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.88	152	89388	20.00	ng	0.00
21) Naphthalene-d8	8.16	136	344565	20.00	ng	0.00
38) Acenaphthene-d10	9.92	164	143003	20.00	ng	0.00
63) Phenanthrene-d10	11.40	188	221015	20.00	ng	0.00
75) Chrysene-d12	14.04	240	194998	20.00	ng	0.00
86) Perylene-d12	15.52	264	158264	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	53903	9.67	ng	0.00
7) Phenol-d6	6.49	99	66409	9.66	ng	-0.02
23) Nitrobenzene-d5	7.44	82	37069	7.11	ng	-0.01
41) 2,4,6-Tribromophenol	10.70	330	11282	7.74	ng	0.00
44) 2-Fluorobiphenyl	9.23	172	76470	8.14	ng	0.00
78) Terphenyl-d14	12.98	244	48075	5.66	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111717\
Data File : BF100708.D
Acq On : 18 Nov 2017 8:37
Operator : SJ/JU
Sample : I6460-01 10X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-28-2-0-1.5

Quant Time: Nov 20 00:42:06 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Nov 17 15:22:08 2017
Response via : Initial Calibration

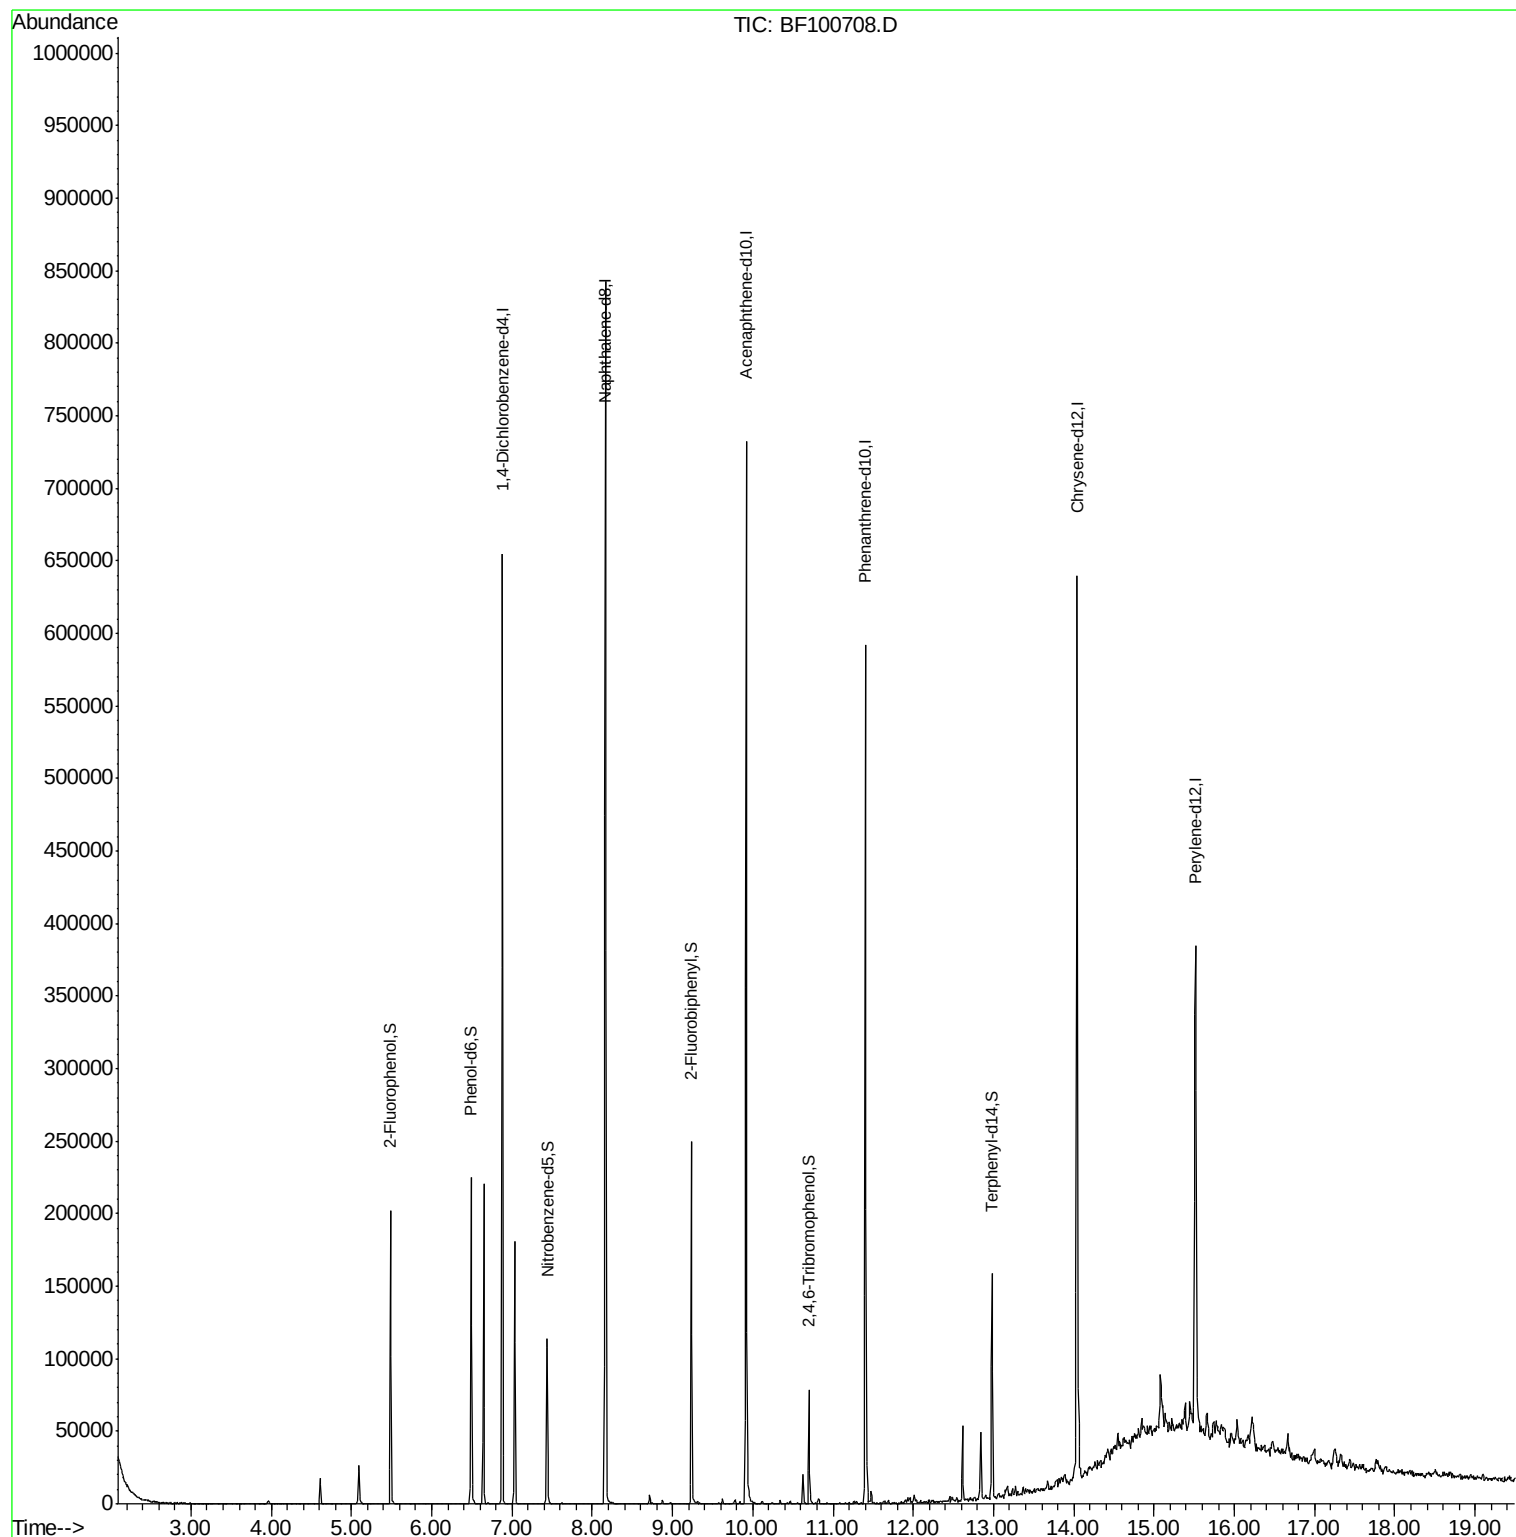

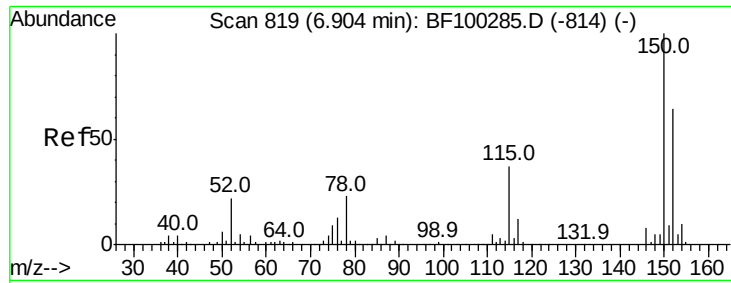


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.88 min Scan# 815
Delta R.T. 0.00 min
Lab File: BF100708.D
Acq: 18 Nov 2017 8:37

Instrument :
BNA_F
ClientSampleId :
G-28-2-0-1.5

Tot Ion	Ratio	Lower	Upper
152	100		
150	160.1	124.6	186.8
115	58.0	50.1	75.1

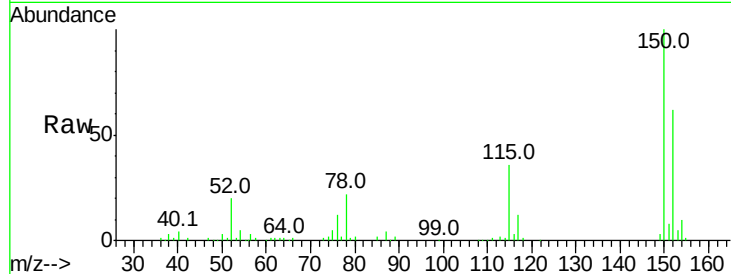


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

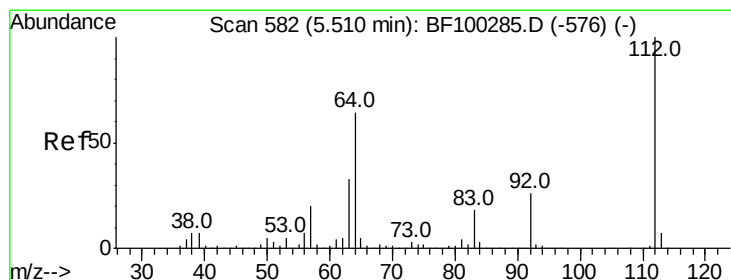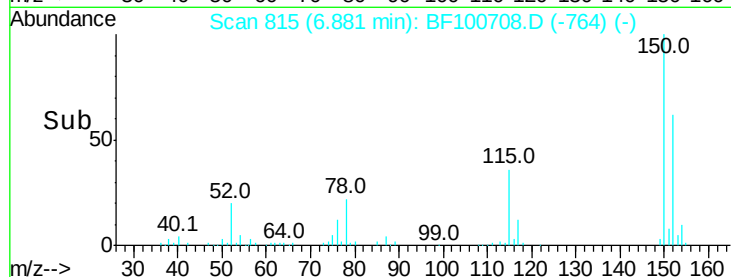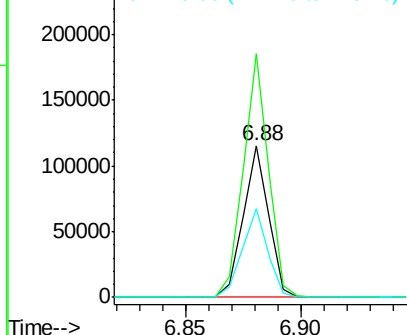



#5


2-Fluorophenol
Concen: 9.666 ng
RT: 5.49 min Scan# 578
Delta R.T. -0.01 min
Lab File: BF100708.D
Acq: 18 Nov 2017 8:37

Tgt Ion	Ratio	Lower	Upper
112	100		
64	53.8	47.9	71.9
63	26.8	23.7	35.5

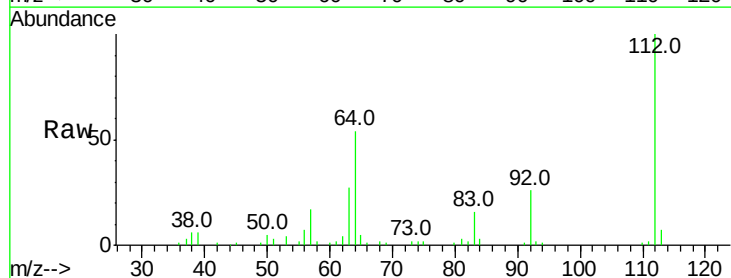

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

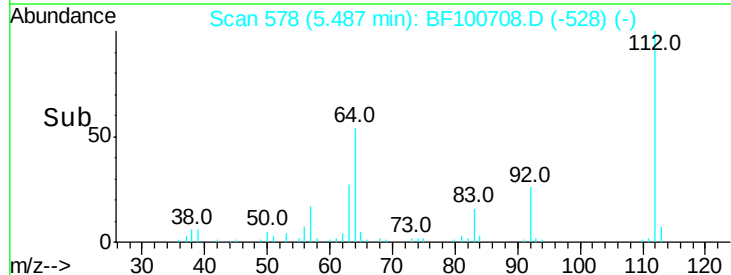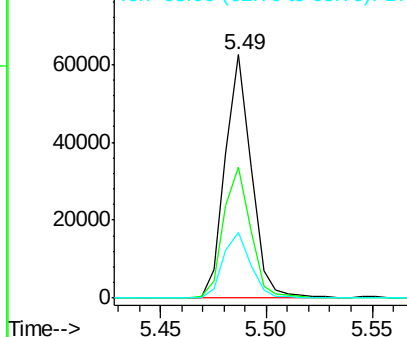

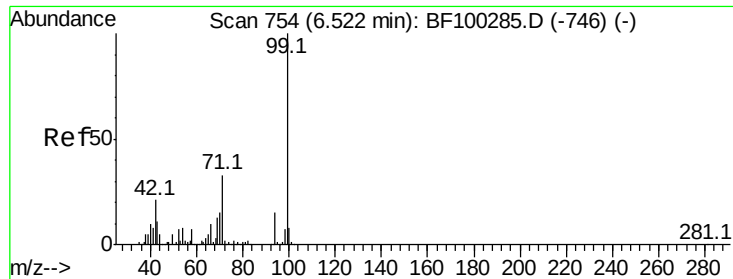

#7

Phenol-d6

Concen: 9.658 ng

RT: 6.49 min Scan# 749

Delta R.T. -0.02 min

Lab File: BF100708.D

Acq: 18 Nov 2017 8:37

Instrument :

BNA_F

ClientSampleId :

G-28-2-0-1.5





Tot Ion: 99 Resp: 66409

Ion Ratio Lower Upper

99 100

42 17.8 14.5 21.7

71 30.3 25.4 38.0

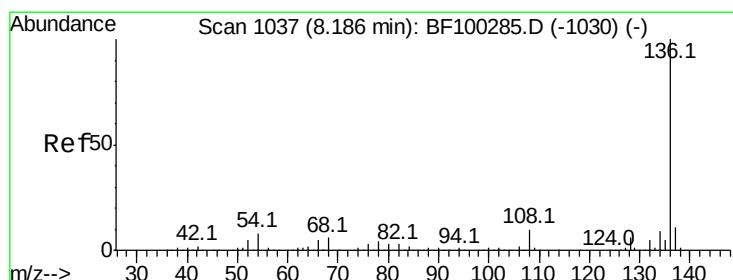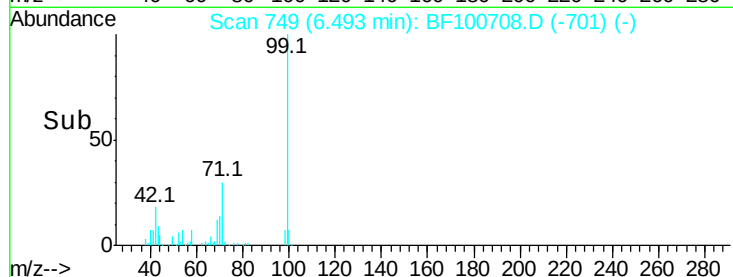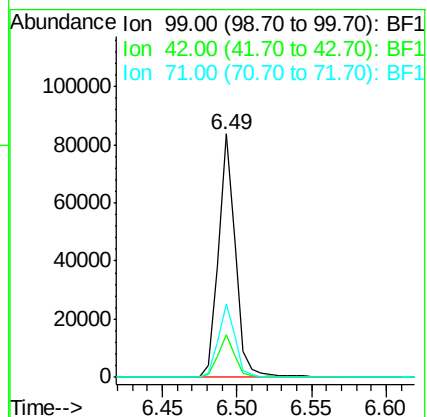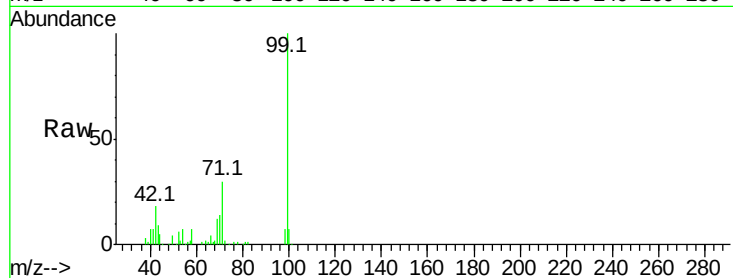

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.16 min Scan# 1033

Delta R.T. -0.01 min

Lab File: BF100708.D

Acq: 18 Nov 2017 8:37

Tgt Ion: 136 Resp: 344565




Ion Ratio Lower Upper


136 100

137 11.0 8.9 13.3

54 8.0 6.6 9.8

68 5.6 5.0 7.4

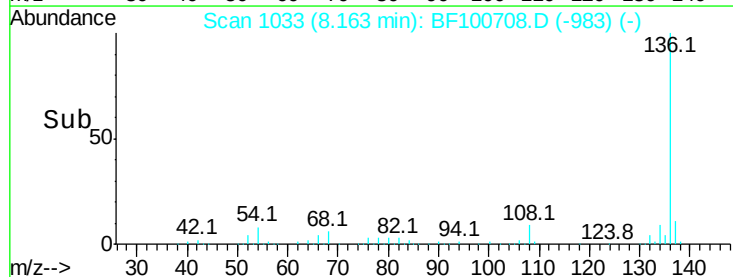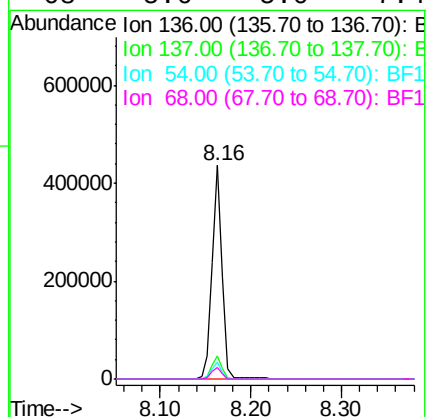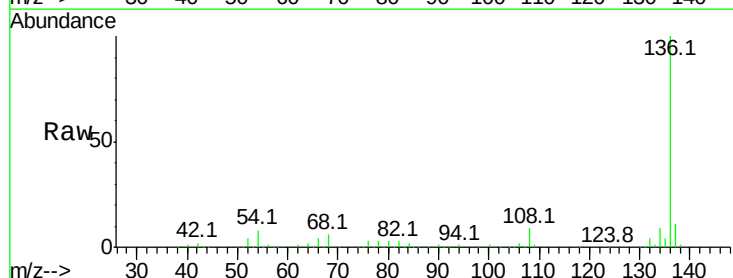


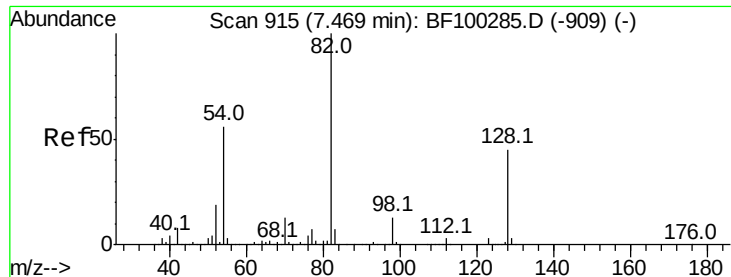




#23
 Nitrobenzene-d5
 Concen: 7.113 ng
 RT: 7.44 min Scan# 910
 Delta R.T. -0.01 min
 Lab File: BF100708.D
 Acq: 18 Nov 2017 8:37

Instrument :
 BNA_F
 ClientSampleId :
 G-28-2-0-1.5

Tot Ion: 82 Resp: 37069
 Ion Ratio Lower Upper
 82 100
 128 47.8 36.1 54.1
 54 53.4 41.4 62.2

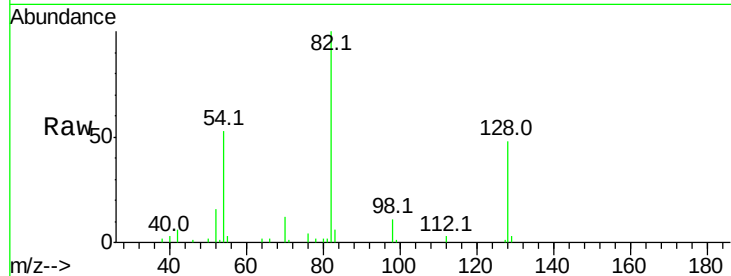


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

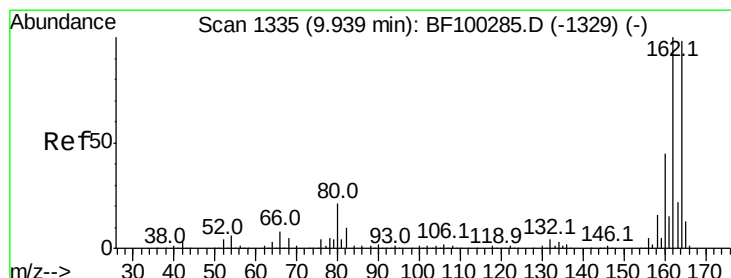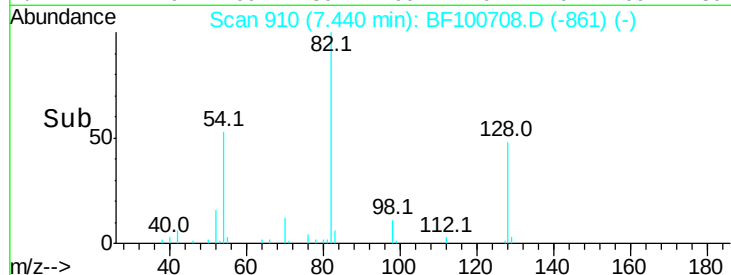
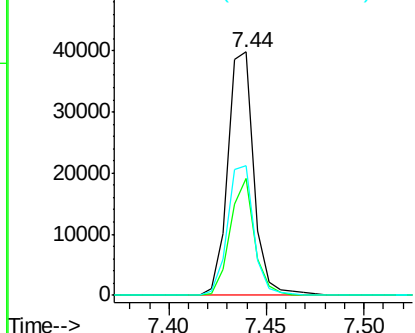



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.92 min Scan# 1331
 Delta R.T. -0.01 min
 Lab File: BF100708.D
 Acq: 18 Nov 2017 8:37

Tgt Ion: 164 Resp: 143003
 Ion Ratio Lower Upper
 164 100
 162 107.8 86.1 129.1
 160 47.5 38.3 57.5

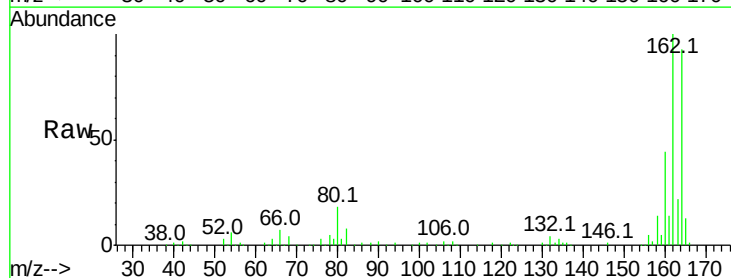

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

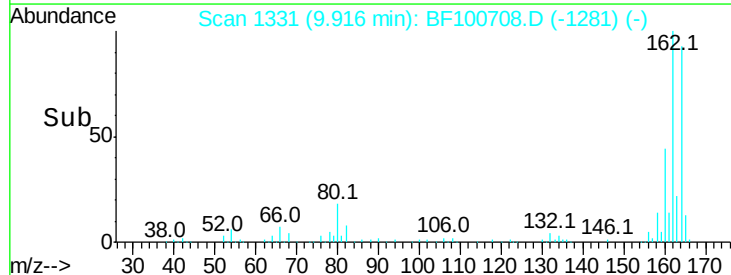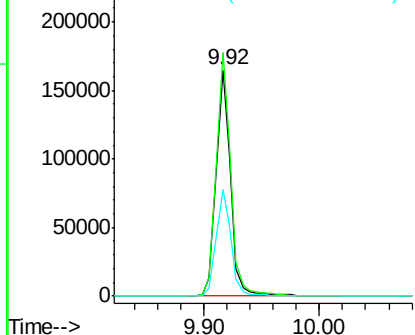


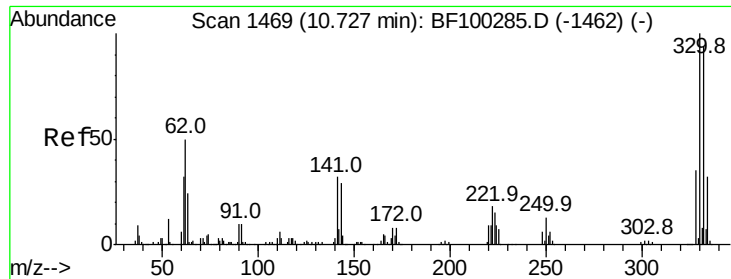




#41
 2,4,6-Tribromophenol
 Concen: 7.742 ng
 RT: 10.70 min Scan# 1465
 Delta R.T. -0.01 min
 Lab File: BF100708.D
 Acq: 18 Nov 2017 8:37

Instrument :
 BNA_F
 ClientSampleId :
 G-28-2-0-1.5

Tot Ion	Ratio	Lower	Upper
330	100		
332	99.1	77.0	115.6
141	29.7	29.9	44.9#

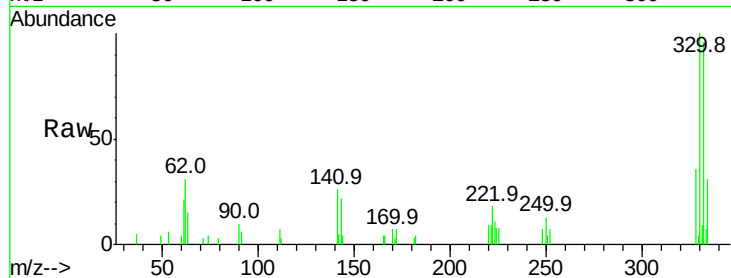


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

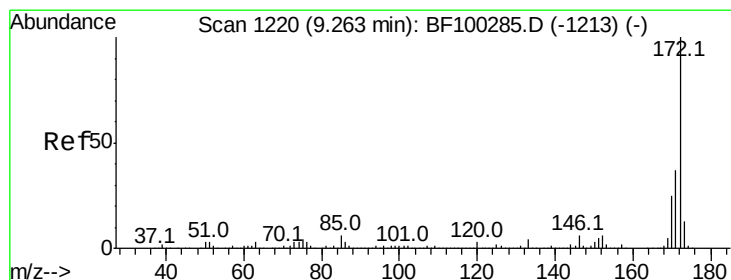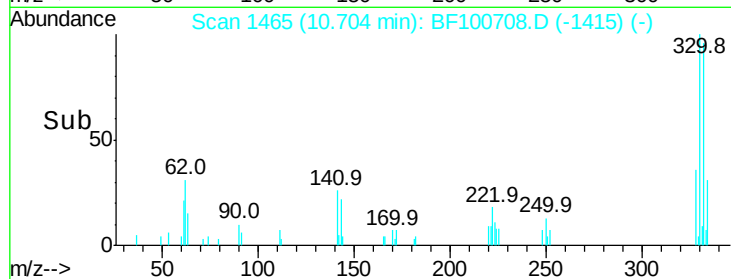
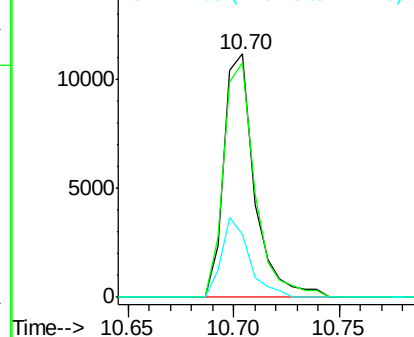



#44
 2-Fluorobiphenyl
 Concen: 8.143 ng
 RT: 9.23 min Scan# 1215
 Delta R.T. -0.01 min
 Lab File: BF100708.D
 Acq: 18 Nov 2017 8:37

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.2	29.7	44.5
170	23.5	19.6	29.4

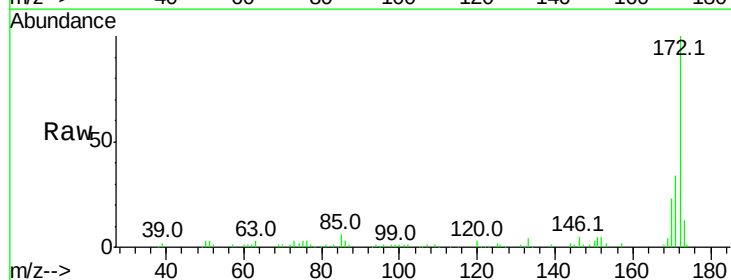

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



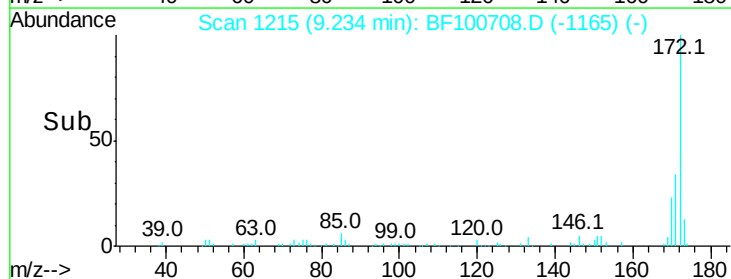
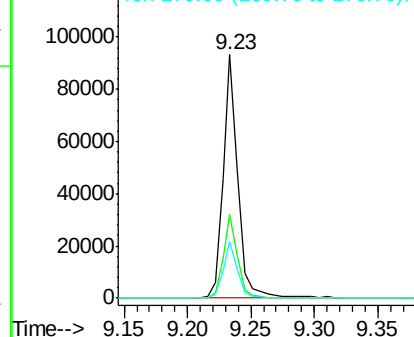


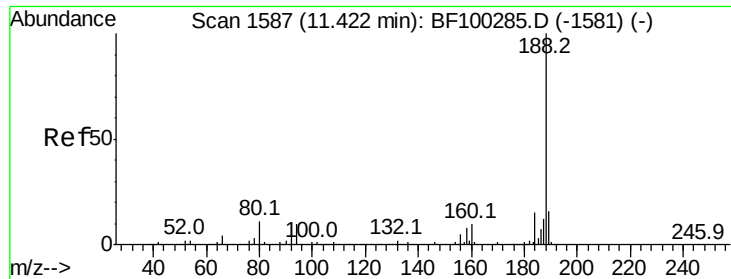

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.40 min Scan# 1584
 Delta R.T. 0.00 min
 Lab File: BF100708.D
 Acq: 18 Nov 2017 8:37




Instrument :
 BNA_F
 ClientSampleId :
 G-28-2-0-1.5


Tot Ion	Ratio	Lower	Upper
188	100		
94	8.6	8.5	12.7
80	8.7	9.2	13.8#

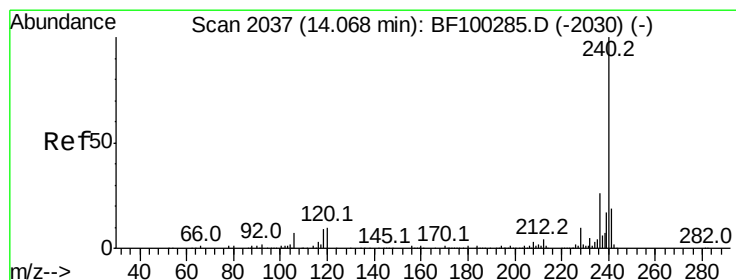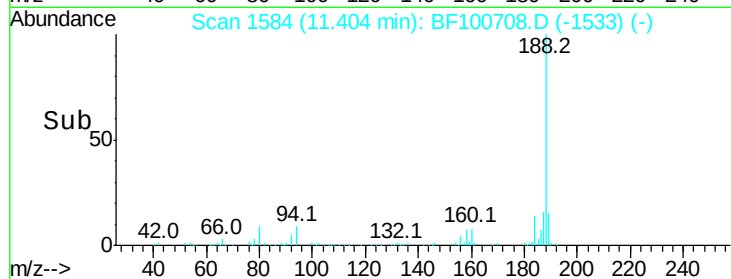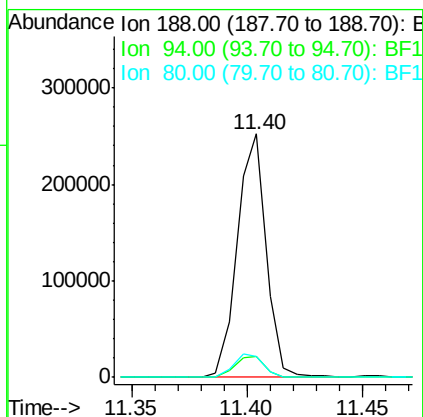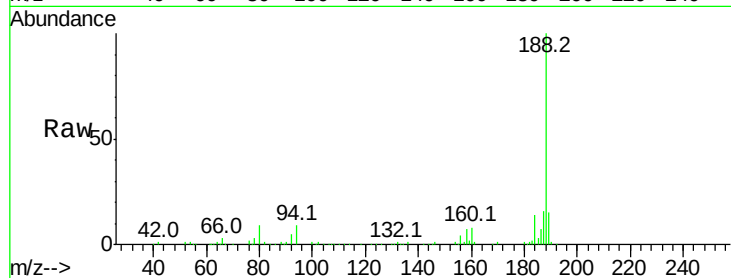

#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 14.04 min Scan# 2032
 Delta R.T. -0.01 min
 Lab File: BF100708.D
 Acq: 18 Nov 2017 8:37

Tgt Ion	Ratio	Lower	Upper
240	100		
120	10.6	9.5	14.3
236	25.6	20.7	31.1

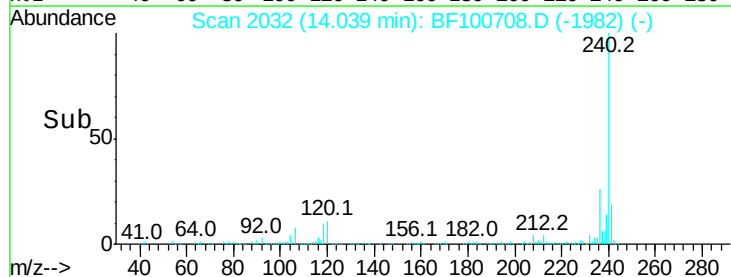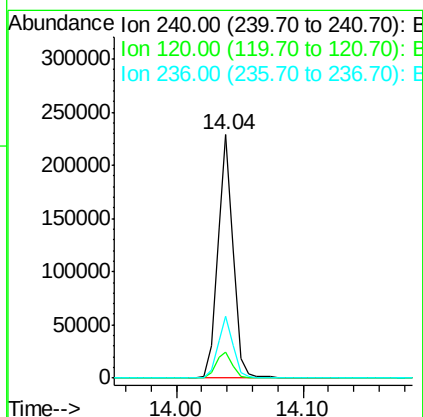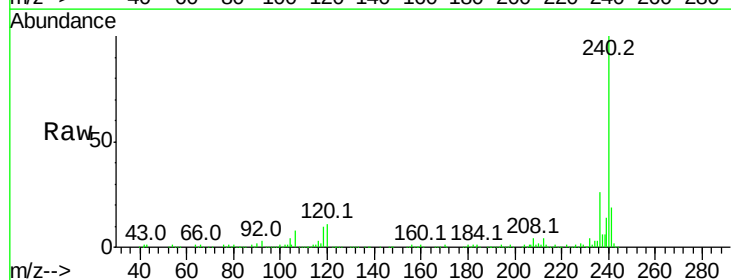

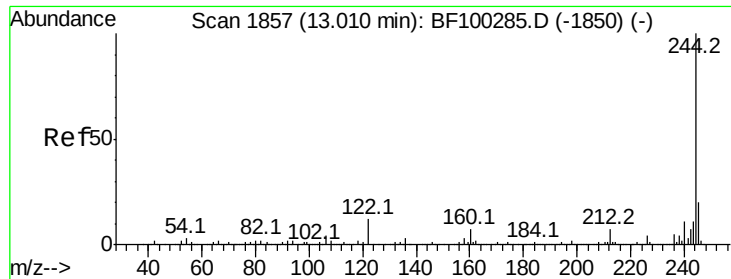

#78

Terphenyl-d14

Concen: 5.665 ng

RT: 12.98 min Scan# 1852

Delta R.T. -0.01 min

Lab File: BF100708.D

Acq: 18 Nov 2017 8:37

Instrument :

BNA_F

ClientSampleId :

G-28-2-0-1.5


Tot Ion:244 Resp: 48075

Ion Ratio Lower Upper

244 100

212 6.6 5.4 8.0




122 11.5 11.0 16.4

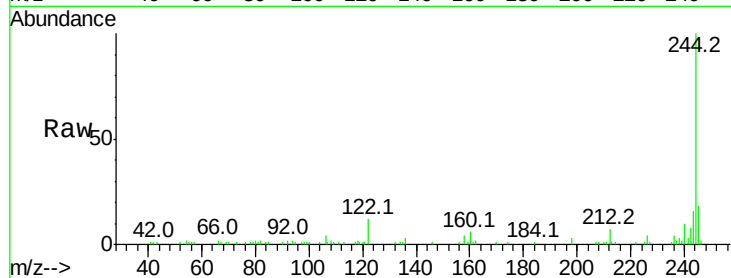

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

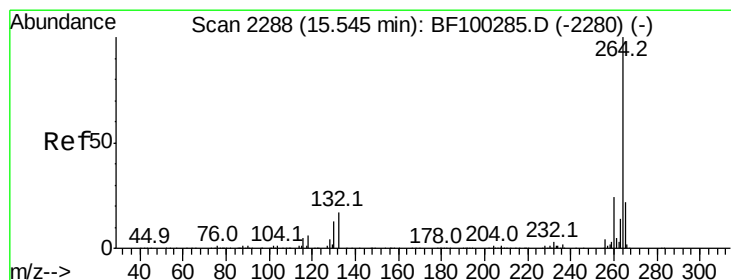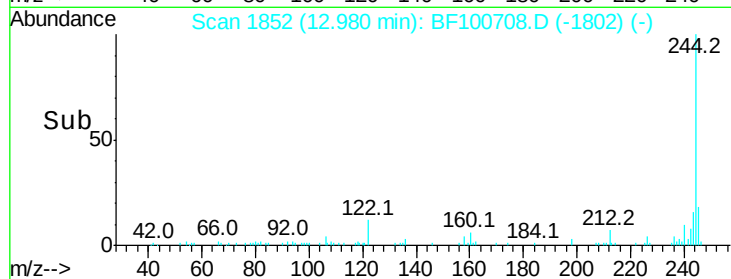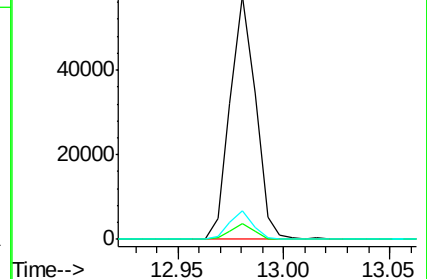

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.52 min Scan# 2283

Delta R.T. 0.00 min

Lab File: BF100708.D

Acq: 18 Nov 2017 8:37


Tgt Ion:264 Resp: 158264

Ion Ratio Lower Upper

264 100

260 24.5 19.2 28.8

265 21.1 17.5 26.3

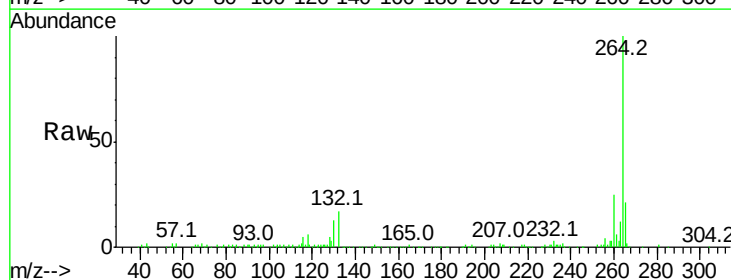

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

