

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111717\
 Data File : BF100666.D
 Acq On : 17 Nov 2017 10:21
 Operator : SJ/JU
 Sample : I6477-01 100X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TOTE-1-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.963	314	319	323	rBV	17564	22247	2.34%	0.378%
2	6.645	770	775	778	rBV	24052	19675	2.07%	0.334%
3	6.881	811	815	818	rBV	687801	552511	58.21%	9.393%
4	7.034	838	841	844	rVB	28032	20493	2.16%	0.348%
5	7.434	906	909	913	rBV	20179	16379	1.73%	0.278%
6	7.951	992	997	1003	rVB	16492	16448	1.73%	0.280%
7	8.163	1028	1033	1036	rBV	908008	749552	78.97%	12.743%
8	9.234	1211	1215	1218	rBV	45558	36488	3.84%	0.620%
9	9.381	1236	1240	1244	rBV	21283	22976	2.42%	0.391%
10	9.916	1326	1331	1335	rBV	970271	866819	91.33%	14.736%
11	10.110	1359	1364	1370	rBV2	30311	38132	4.02%	0.648%
12	10.539	1434	1437	1446	rVB	17635	28329	2.98%	0.482%
13	10.698	1461	1464	1468	rBV2	24230	22321	2.35%	0.379%
14	10.769	1473	1476	1480	rBV	68476	68128	7.18%	1.158%
15	11.051	1521	1524	1530	rVB6	14929	18871	1.99%	0.321%
16	11.404	1580	1584	1587	rBV	1079074	949151	100.00%	16.136%
17	11.680	1627	1631	1634	rBV5	12029	14712	1.55%	0.250%
18	11.916	1666	1671	1676	rBV	77970	93578	9.86%	1.591%
19	11.963	1676	1679	1690	rVB	122507	115898	12.21%	1.970%
20	12.698	1800	1804	1809	rBV3	37755	39627	4.17%	0.674%
21	12.980	1848	1852	1854	rBV	66666	55233	5.82%	0.939%
22	13.010	1854	1857	1863	rVB	91043	88057	9.28%	1.497%
23	13.227	1889	1894	1902	rVV3	22404	46636	4.91%	0.793%
24	13.316	1906	1909	1915	rVB6	8246	13945	1.47%	0.237%
25	13.457	1925	1933	1938	rBV3	21335	48242	5.08%	0.820%
26	13.527	1942	1945	1949	rVB	13463	16845	1.77%	0.286%
27	13.939	2010	2015	2023	rVB	47499	65221	6.87%	1.109%
28	14.010	2023	2027	2028	rBV	31091	28025	2.95%	0.476%
29	14.039	2028	2032	2035	rVB	1059707	919040	96.83%	15.624%
30	14.468	2102	2105	2107	rBV4	10019	12700	1.34%	0.216%
31	14.786	2155	2159	2161	rBV6	13188	22442	2.36%	0.382%
32	14.957	2185	2188	2192	rBV5	10575	14605	1.54%	0.248%
33	15.145	2215	2220	2223	rBV4	13529	16956	1.79%	0.288%
34	15.327	2245	2251	2259	rBV8	15648	36594	3.86%	0.622%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100666.D
Acq On : 17 Nov 2017 10:21
Operator : SJ/JU
Sample : I6477-01 100X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TOTE-1-2

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.515	2277	2283	2291	rVB	584188	734157	77.35%	12.481%
36	15.963	2356	2359	2364	rVB4	10996	15289	1.61%	0.260%
37	16.474	2440	2446	2451	rBV6	10925	21362	2.25%	0.363%
38	17.774	2663	2667	2673	rBV7	7779	14565	1.53%	0.248%


Sum of corrected areas: 5882249

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100666.D
Acq On : 17 Nov 2017 10:21
Operator : SJ/JU
Sample : I6477-01 100X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TOTE-1-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

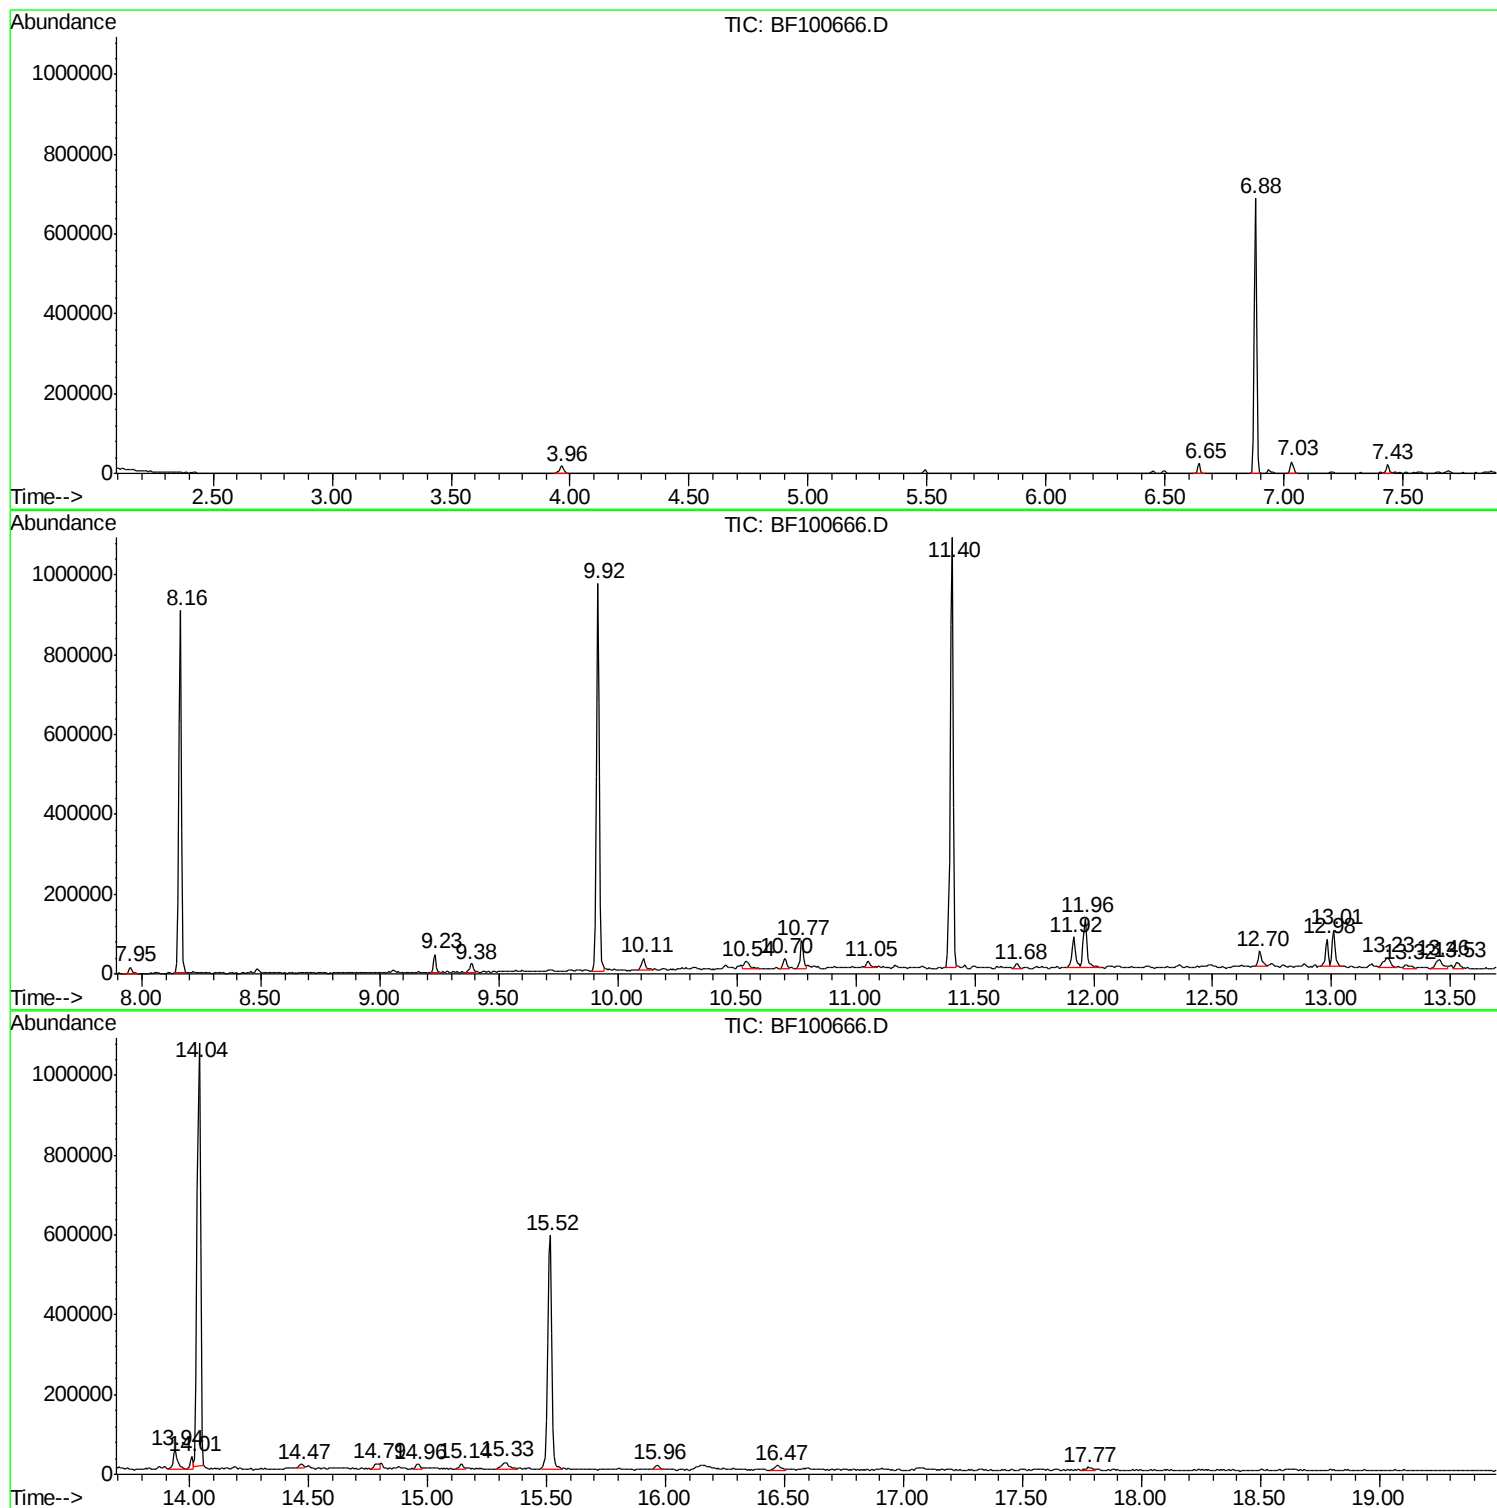

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111717\
Data File : BF100666.D
Acq On : 17 Nov 2017 10:21
Operator : SJ/JU
Sample : I6477-01 100X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TOTE-1-2










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triethylene glycol monododecyl... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.96	2.44 ng	115898	Phenanthrene-d10	11.40

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triethylene glycol monododecyl e...	318	C18H38O4	003055-94-5	64
2			Heptaethylene glycol	326	C14H30O8	005617-32-3	49
3			Hexaethylene glycol	282	C12H26O7	002615-15-8	49
4			2-[2-[2-[2-[2-[2-(2-Hydroxyet...	370	C16H34O9	005117-19-1	47
5			3,6,9,12-Tetraoxatetradecan-1-ol	222	C10H22O5	005650-20-4	43

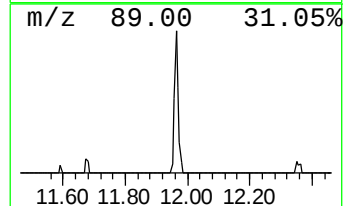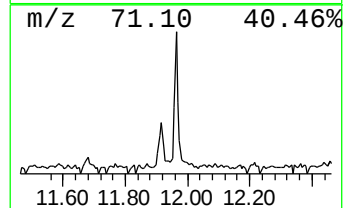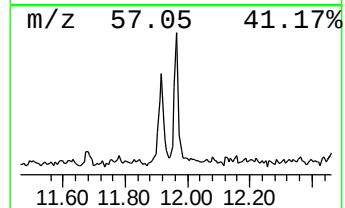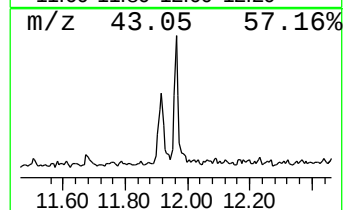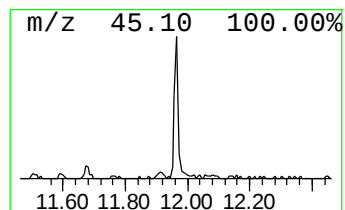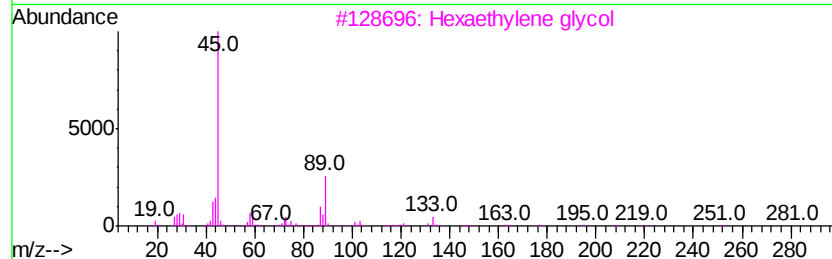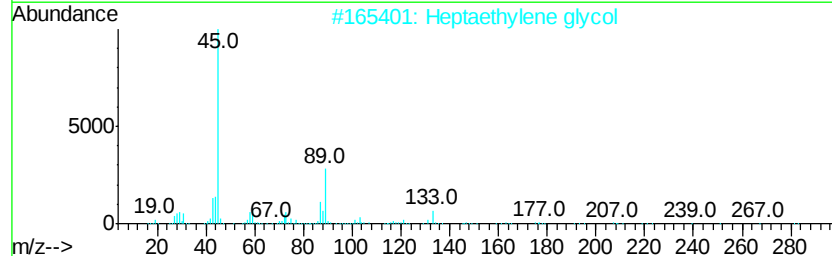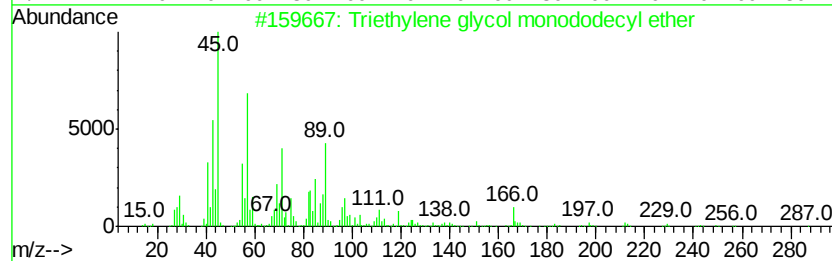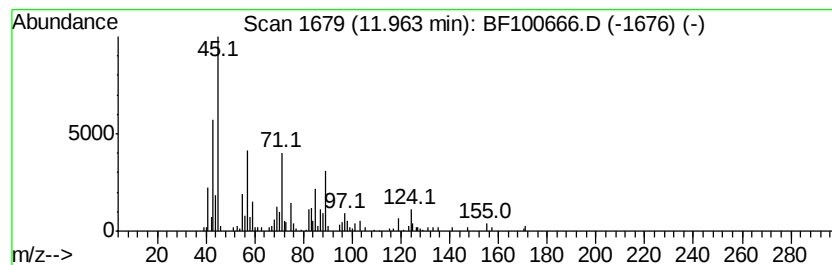

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100666.D
Acq On : 17 Nov 2017 10:21
Operator : SJ/JU
Sample : I6477-01 100X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TOTE-1-2

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triethylene glyco...	11.96	2.4	ng	115898	4	11.40	949151	20.0