

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111717\
 Data File : BF100709.D
 Acq On : 18 Nov 2017 9:04
 Operator : SJ/JU
 Sample : I6460-02 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-28-2-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.092	508	511	517	rBV	26703	26214	4.14%	0.510%
2	5.487	574	578	587	rBB	200521	170330	26.91%	3.314%
3	6.492	746	749	756	rBV	208305	172223	27.21%	3.351%
4	6.645	771	775	778	rBV	216177	178797	28.25%	3.479%
5	6.881	811	815	819	rBV	651152	505889	79.93%	9.843%
6	7.033	838	841	845	rBV	173768	139073	21.97%	2.706%
7	7.439	906	910	914	rBV	108483	98191	15.51%	1.910%
8	8.163	1029	1033	1036	rBV	797262	617684	97.59%	12.018%
9	9.233	1212	1215	1226	rVB	214925	167145	26.41%	3.252%
10	9.916	1327	1331	1343	rBV	673847	580158	91.66%	11.288%
11	10.621	1449	1451	1457	rBB	17315	16780	2.65%	0.326%
12	10.704	1461	1465	1472	rBB	66332	65761	10.39%	1.279%
13	11.404	1580	1584	1586	rBV	559545	502739	79.43%	9.781%
14	11.421	1586	1587	1591	rVV	38663	30123	4.76%	0.586%
15	11.474	1594	1596	1600	rVB	11561	9497	1.50%	0.185%
16	12.615	1786	1790	1793	rBV	65702	58034	9.17%	1.129%
17	12.839	1822	1828	1835	rBV	64640	72044	11.38%	1.402%
18	12.980	1849	1852	1855	rBV	178706	133183	21.04%	2.591%
19	13.168	1876	1884	1887	rBV4	12325	20103	3.18%	0.391%
20	13.274	1899	1902	1904	rVB2	9410	8833	1.40%	0.172%
21	13.674	1967	1970	1974	rVB	8108	8448	1.33%	0.164%
22	13.786	1985	1989	1992	rBV4	10348	13922	2.20%	0.271%
23	13.839	1996	1998	2003	rBV4	7532	16877	2.67%	0.328%
24	13.968	2016	2020	2021	rBV3	6819	9688	1.53%	0.188%
25	14.009	2024	2027	2028	rVV2	22514	21002	3.32%	0.409%
26	14.039	2028	2032	2035	rVV	684827	632949	100.00%	12.315%
27	14.062	2035	2036	2039	rVB	45180	26603	4.20%	0.518%
28	14.145	2047	2050	2053	rBV5	7582	8651	1.37%	0.168%
29	14.192	2055	2058	2061	rBV5	10660	13982	2.21%	0.272%
30	14.451	2101	2102	2106	rBV4	8059	10495	1.66%	0.204%
31	14.545	2116	2118	2121	rBV4	9547	10830	1.71%	0.211%
32	15.080	2205	2209	2212	rBV	47260	75473	11.92%	1.468%
33	15.139	2217	2219	2225	rVB6	13661	17206	2.72%	0.335%
34	15.386	2259	2261	2265	rVB	25700	31951	5.05%	0.622%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111717\
Data File : BF100709.D
Acq On : 18 Nov 2017 9:04
Operator : SJ/JU
Sample : I6460-02 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-28-2-1.5-3

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.451	2268	2272	2278	rBV	31551	51568	8.15%	1.003%
36	15.515	2278	2283	2291	rVV	379206	508207	80.29%	9.888%
37	15.839	2336	2338	2341	rBV4	9383	14335	2.26%	0.279%
38	16.221	2399	2403	2412	rVB4	21216	43725	6.91%	0.851%
39	16.662	2475	2478	2485	rVB7	14877	25569	4.04%	0.497%
40	17.245	2573	2577	2586	rVB9	12303	25440	4.02%	0.495%


Sum of corrected areas: 5139722

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100709.D
Acq On : 18 Nov 2017 9:04
Operator : SJ/JU
Sample : I6460-02 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-28-2-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

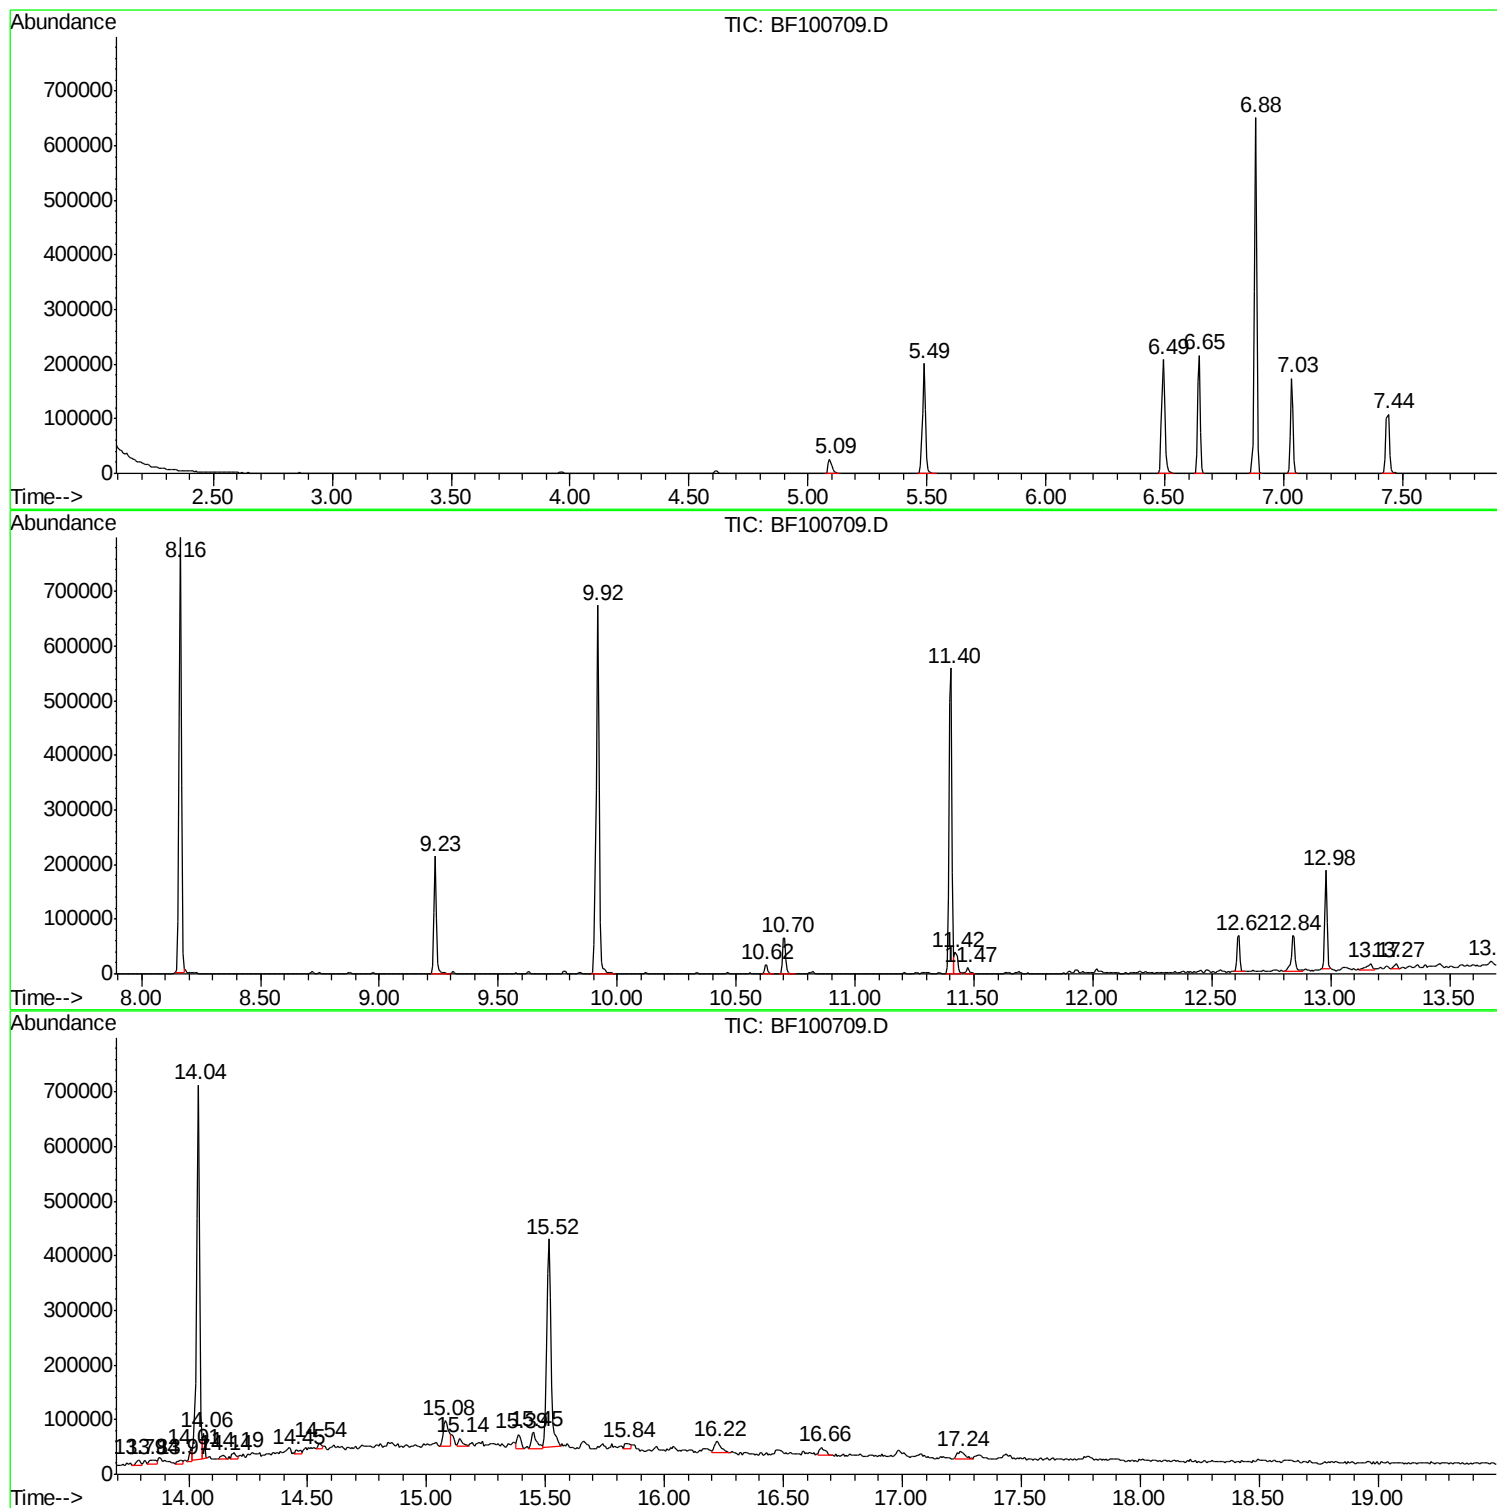

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100709.D
Acq On : 18 Nov 2017 9:04
Operator : SJ/JU
Sample : I6460-02 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-28-2-1.5-3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	7.07 ng	178797	1,4-Dichlorobenzene-d4	6.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

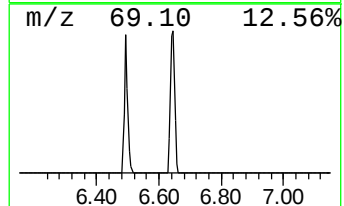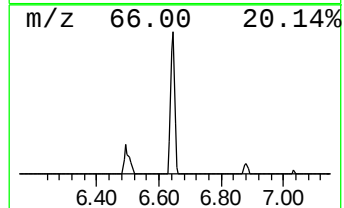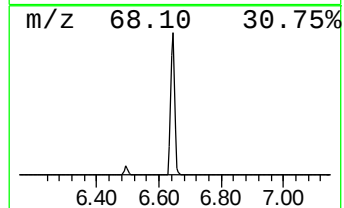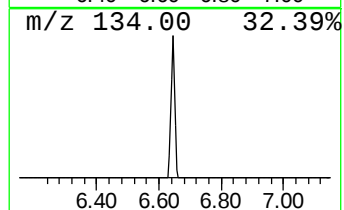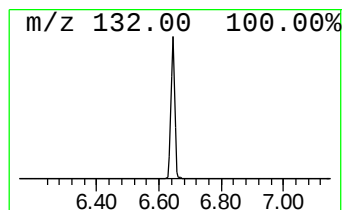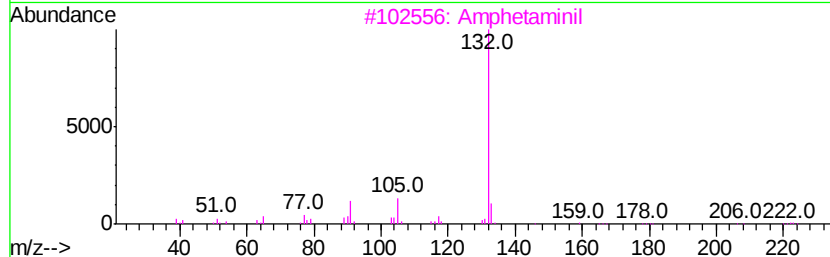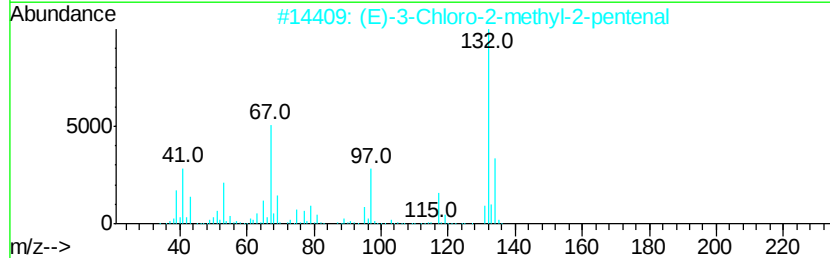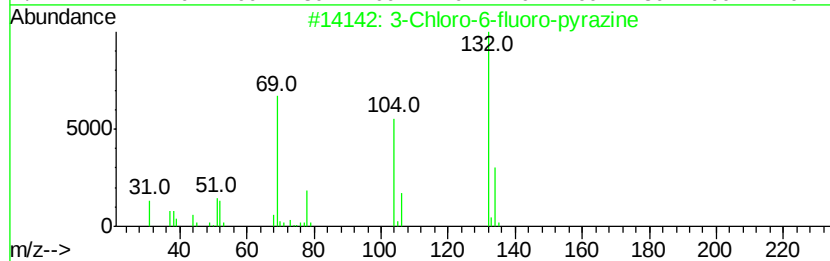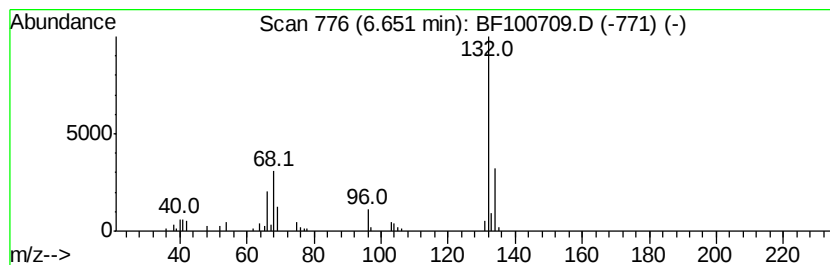

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100709.D
Acq On : 18 Nov 2017 9:04
Operator : SJ/JU
Sample : I6460-02 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-28-2-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.65	6.65	7.1	ng	178797	1	6.88	505889	20.0