

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
 Data File : BF100710.D
 Acq On : 18 Nov 2017 9:30
 Operator : SJ/JU
 Sample : I6460-03 10X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-31-2-0-1.5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.093	508	511	517	rBV	19532	20062	2.47%	0.361%
2	5.487	574	578	584	rBV	139441	124431	15.35%	2.237%
3	6.493	746	749	759	rBB	156187	128294	15.83%	2.306%
4	6.645	771	775	778	rBV	160565	135502	16.71%	2.436%
5	6.881	811	815	818	rBV	820360	646632	79.76%	11.623%
6	7.034	838	841	845	rBV	136685	107030	13.20%	1.924%
7	7.434	906	909	914	rBV	82566	74239	9.16%	1.334%
8	8.163	1029	1033	1036	rBV	1032551	810696	100.00%	14.572%
9	9.234	1212	1215	1223	rBV	203844	154333	19.04%	2.774%
10	9.628	1278	1282	1285	rBV3	13720	14158	1.75%	0.254%
11	9.916	1327	1331	1335	rBV2	877709	782228	96.49%	14.060%
12	10.557	1437	1440	1446	rVB3	7770	9979	1.23%	0.179%
13	10.628	1449	1452	1456	rBV	16086	16117	1.99%	0.290%
14	10.698	1462	1464	1469	rBV	56363	52887	6.52%	0.951%
15	10.822	1481	1485	1488	rBV	19706	21740	2.68%	0.391%
16	11.292	1561	1565	1570	rBV2	15674	20123	2.48%	0.362%
17	11.404	1580	1584	1587	rBV	801349	681068	84.01%	12.242%
18	12.616	1787	1790	1792	rBV	20032	14518	1.79%	0.261%
19	12.710	1802	1806	1808	rBV4	12671	15494	1.91%	0.278%
20	12.769	1813	1816	1817	rBV2	11527	10003	1.23%	0.180%
21	12.845	1826	1829	1831	rBV2	21809	25077	3.09%	0.451%
22	12.980	1847	1852	1859	rBV	158517	155437	19.17%	2.794%
23	13.169	1882	1884	1887	rVB4	15512	10900	1.34%	0.196%
24	13.427	1926	1928	1932	rVB4	22901	18083	2.23%	0.325%
25	14.010	2024	2027	2029	rBV	363989	321288	39.63%	5.775%
26	14.039	2029	2032	2036	rVB	736427	655348	80.84%	11.780%
27	15.521	2279	2284	2289	rVB	400460	537719	66.33%	9.665%


Sum of corrected areas: 5563386

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100710.D
Acq On : 18 Nov 2017 9:30
Operator : SJ/JU
Sample : I6460-03 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-2-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

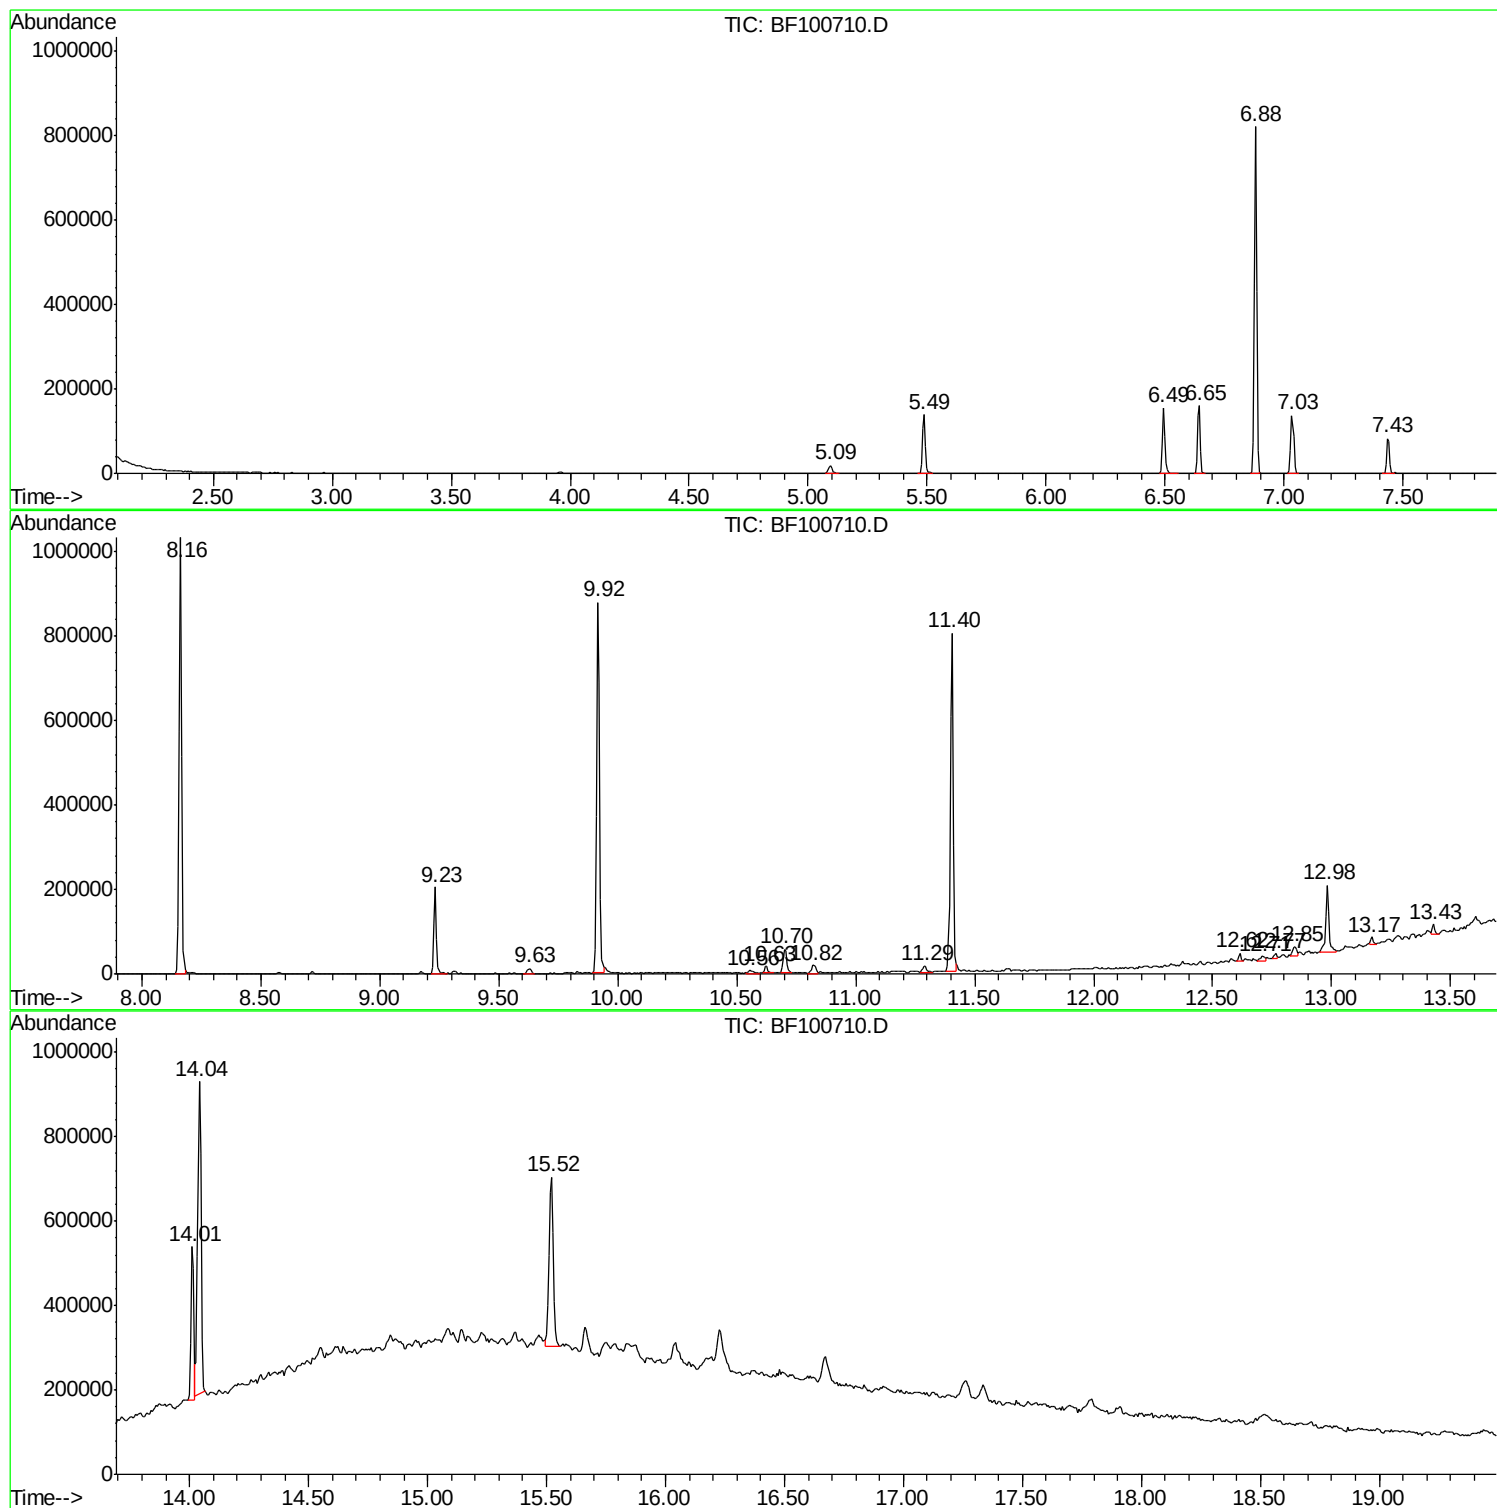

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100710.D
Acq On : 18 Nov 2017 9:30
Operator : SJ/JU
Sample : I6460-03 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-2-0-1.5










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	4.19 ng	135502	1,4-Dichlorobenzene-d4	6.88

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	38
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	35
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	10
5		4-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-60-2	9

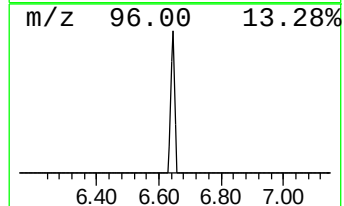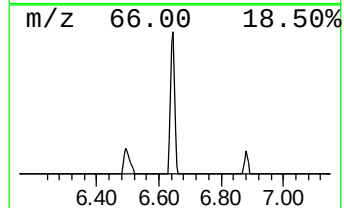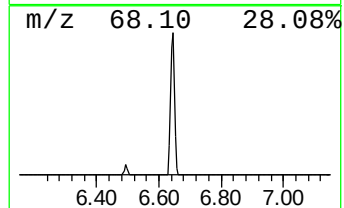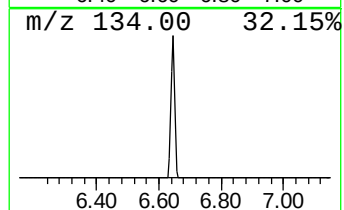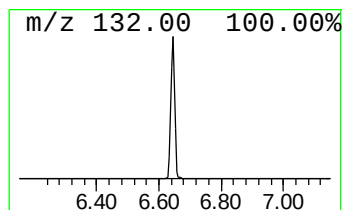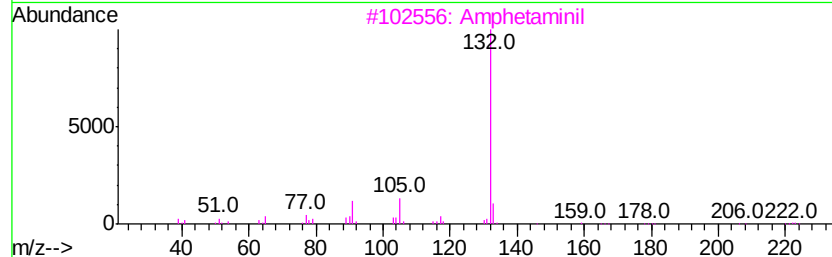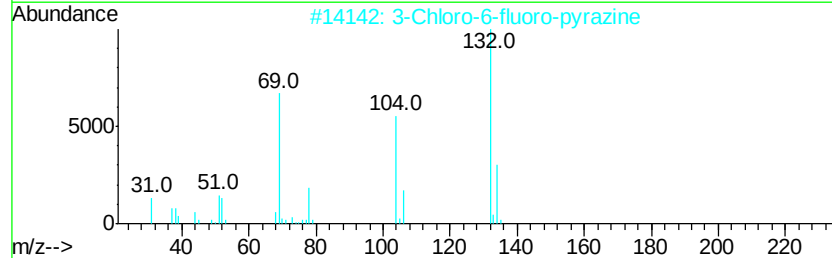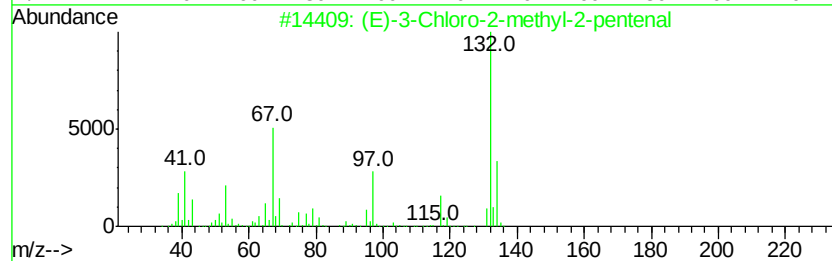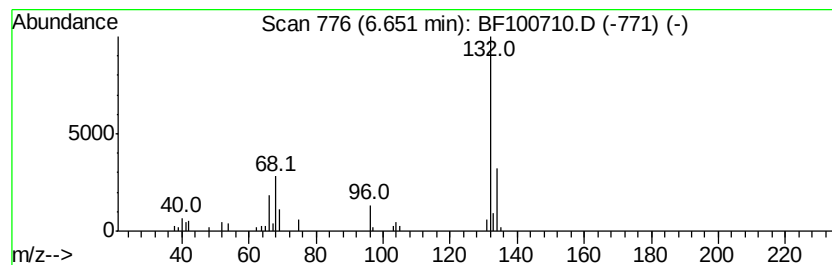

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100710.D
Acq On : 18 Nov 2017 9:30
Operator : SJ/JU
Sample : I6460-03 10X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-2-0-1.5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.65	6.65	4.2	ng	135502	1	6.88	646632	20.0