

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111717\
 Data File : BF100711.D
 Acq On : 18 Nov 2017 9:57
 Operator : SJ/JU
 Sample : I6460-04 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-31-2-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.092	508	511	520	rBV	37533	37630	4.38%	0.528%
2	5.487	574	578	585	rBV	236264	210694	24.54%	2.957%
3	6.492	746	749	759	rBV	245138	220068	25.64%	3.088%
4	6.645	771	775	778	rBV	282302	223178	26.00%	3.132%
5	6.881	811	815	819	rBV	591840	479576	55.87%	6.730%
6	7.034	838	841	845	rBV	198121	167543	19.52%	2.351%
7	7.439	906	910	914	rBV	146109	122674	14.29%	1.722%
8	8.163	1029	1033	1036	rBV	745276	585577	68.21%	8.218%
9	8.186	1036	1037	1040	rVB	24926	10883	1.27%	0.153%
10	9.233	1211	1215	1226	rBV	267480	209013	24.35%	2.933%
11	9.780	1305	1308	1311	rBB	15349	13300	1.55%	0.187%
12	9.916	1327	1331	1335	rBV	590151	529393	61.67%	7.429%
13	9.951	1335	1337	1342	rVB	19130	16177	1.88%	0.227%
14	10.122	1363	1366	1370	rVB	10836	8982	1.05%	0.126%
15	10.627	1448	1452	1458	rVB	25172	23135	2.69%	0.325%
16	10.704	1462	1465	1472	rVV	97890	91775	10.69%	1.288%
17	11.404	1580	1584	1587	rBV	578654	492148	57.33%	6.907%
18	11.427	1587	1588	1592	rVV	56451	29784	3.47%	0.418%
19	11.480	1594	1597	1600	rVB	35659	33112	3.86%	0.465%
20	11.633	1616	1623	1629	rBV	10357	13692	1.59%	0.192%
21	11.933	1671	1674	1676	rVB	11801	10602	1.24%	0.149%
22	12.016	1685	1688	1691	rBV	18767	20366	2.37%	0.286%
23	12.221	1721	1723	1726	rVB2	11455	8908	1.04%	0.125%
24	12.451	1759	1762	1765	rBV2	9662	10321	1.20%	0.145%
25	12.539	1774	1777	1781	rBV2	21481	20295	2.36%	0.285%
26	12.616	1786	1790	1793	rVV	255915	211168	24.60%	2.963%
27	12.674	1798	1800	1804	rVB3	12286	10270	1.20%	0.144%
28	12.751	1808	1813	1814	rBV4	8937	10925	1.27%	0.153%
29	12.845	1822	1829	1835	rBV	268463	257543	30.00%	3.614%
30	12.898	1835	1838	1842	rVB4	12055	12647	1.47%	0.177%
31	12.980	1849	1852	1855	rBV	210037	170025	19.81%	2.386%
32	13.063	1861	1866	1870	rBV5	23257	37381	4.35%	0.525%
33	13.168	1877	1884	1888	rBV3	44487	70272	8.19%	0.986%
34	13.239	1893	1896	1898	rVV	34015	30022	3.50%	0.421%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF111717\
 Data File : BF100711.D
 Acq On : 18 Nov 2017 9:57
 Operator : SJ/JU
 Sample : I6460-04 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-31-2-1.5-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	13.274	1898	1902	1904	rVV2	31321	34909	4.07%	0.490%
36	13.298	1904	1906	1908	rVB2	13358	9811	1.14%	0.138%
37	13.368	1915	1918	1920	rBV	19814	19459	2.27%	0.273%
38	13.398	1920	1923	1926	rVB2	15544	16433	1.91%	0.231%
39	13.427	1926	1928	1930	rBV3	9188	8793	1.02%	0.123%
40	13.551	1945	1949	1950	rBV4	11924	14070	1.64%	0.197%
41	13.651	1963	1966	1968	rBV3	11730	14521	1.69%	0.204%
42	13.680	1968	1971	1974	rVV2	24786	29873	3.48%	0.419%
43	13.792	1986	1990	1992	rBV2	25844	29514	3.44%	0.414%
44	13.815	1992	1994	1996	rBV	22257	19307	2.25%	0.271%
45	13.839	1996	1998	2003	rVV2	39571	47161	5.49%	0.662%
46	13.886	2003	2006	2007	rVV2	21315	19532	2.28%	0.274%
47	14.039	2024	2032	2035	rBV2	662342	858442	100.00%	12.047%
48	14.068	2035	2037	2042	rVB	180196	180001	20.97%	2.526%
49	14.145	2048	2050	2052	rBV	52983	40134	4.68%	0.563%
50	14.257	2067	2069	2074	rVB3	21996	22135	2.58%	0.311%
51	14.462	2101	2104	2107	rVB2	20919	22037	2.57%	0.309%
52	14.551	2116	2119	2121	rBV	35664	37030	4.31%	0.520%
53	15.080	2205	2209	2213	rBV	204610	310025	36.11%	4.351%
54	15.192	2225	2228	2231	rVB	37139	33667	3.92%	0.472%
55	15.386	2258	2261	2268	rVB	108706	151114	17.60%	2.121%
56	15.451	2268	2272	2278	rBV	122577	159956	18.63%	2.245%
57	15.515	2278	2283	2287	rBV	338395	458330	53.39%	6.432%
58	16.998	2530	2535	2539	rVB3	37515	68513	7.98%	0.961%
59	17.445	2606	2611	2626	rVB	40327	121822	14.19%	1.710%


Sum of corrected areas: 7125668

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100711.D
Acq On : 18 Nov 2017 9:57
Operator : SJ/JU
Sample : I6460-04 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-2-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

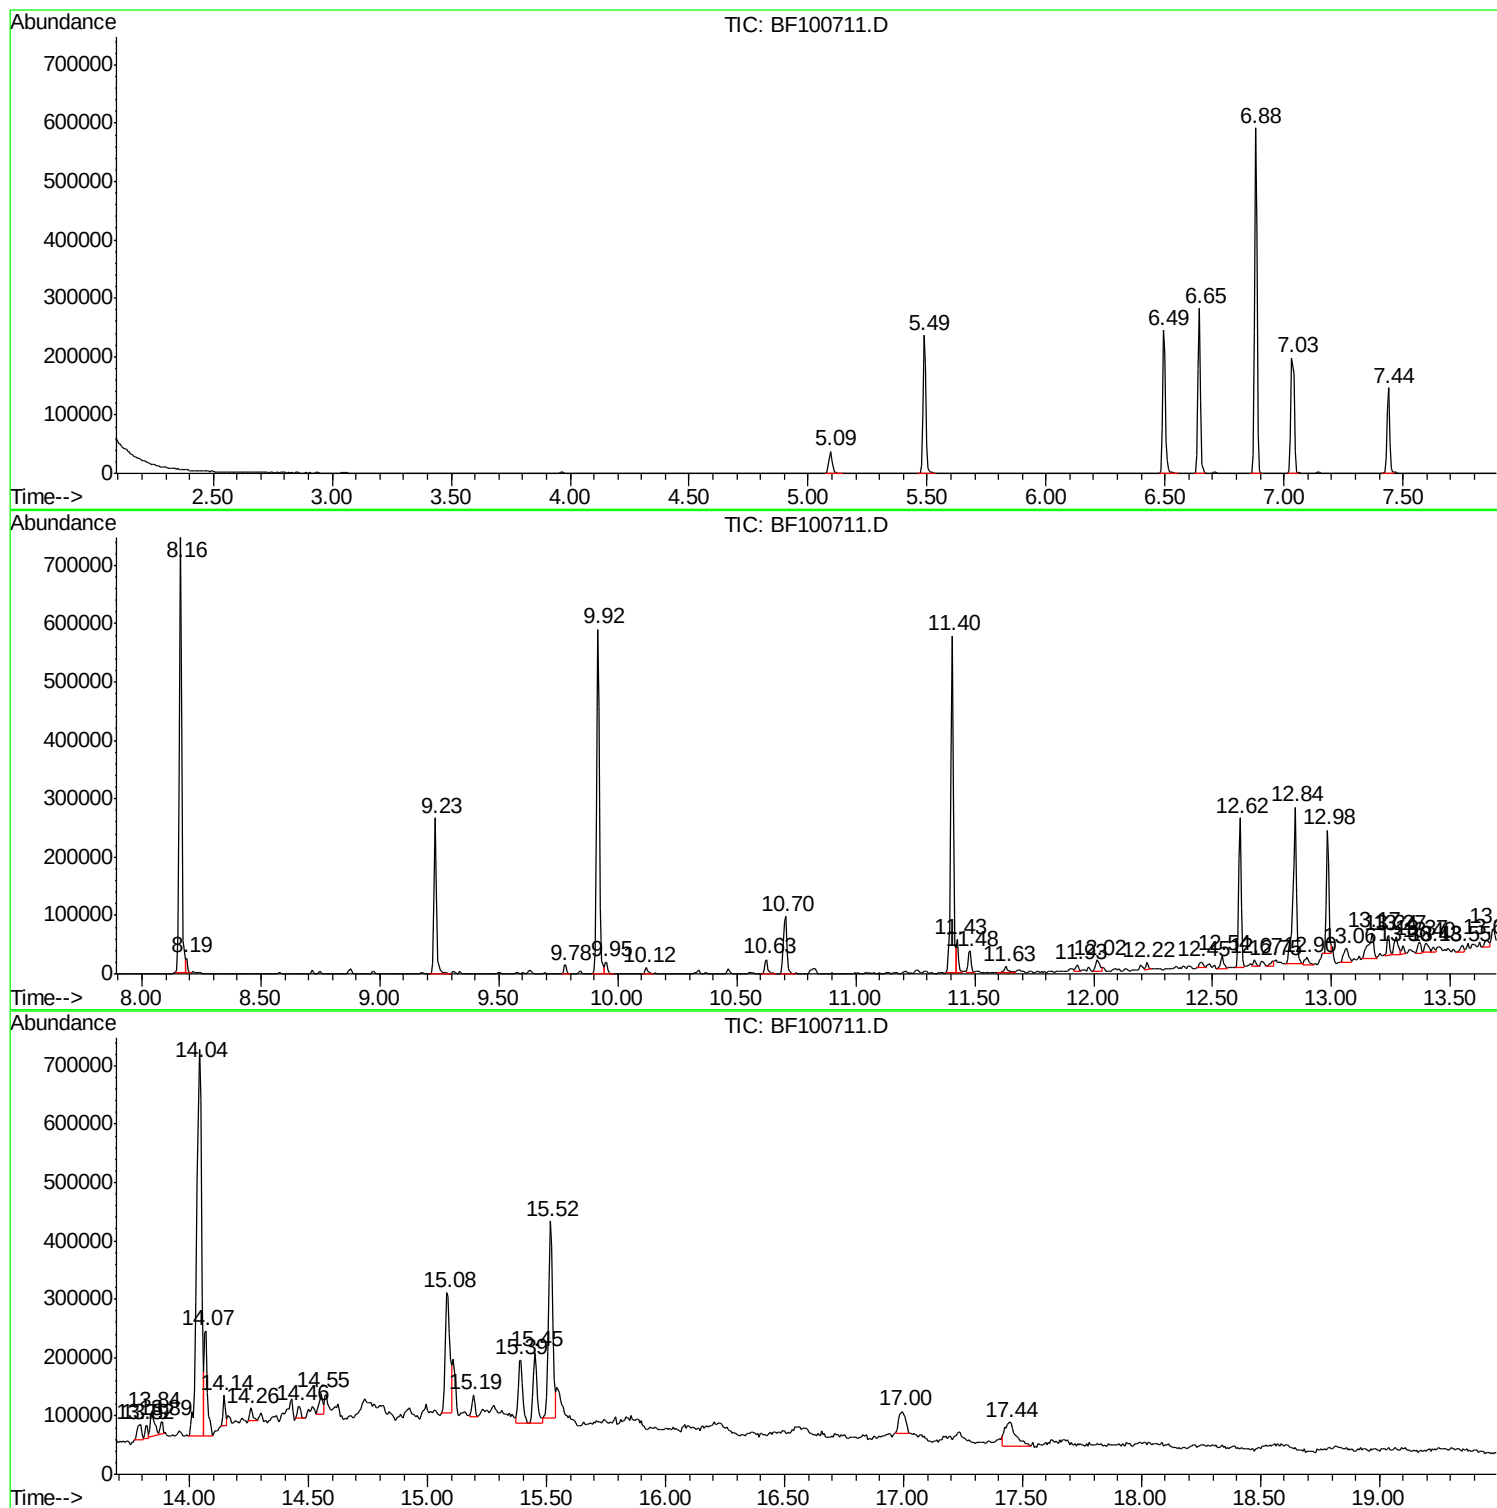

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100711.D
Acq On : 18 Nov 2017 9:57
Operator : SJ/JU
Sample : I6460-04 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-2-1.5-3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.65 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.65	9.31 ng	223178	1,4-Dichlorobenzene-d4	6.88

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4			Amphetaminil	250	C17H18N2	017590-01-1	10
5			N-(-phenylisopropyl)benzalimine	223	C16H17N	1000379-01-3	10

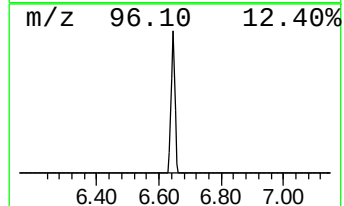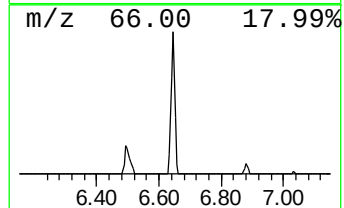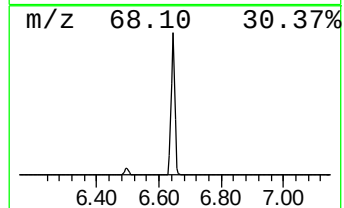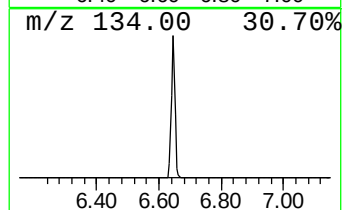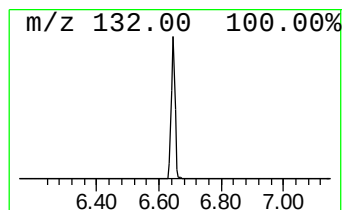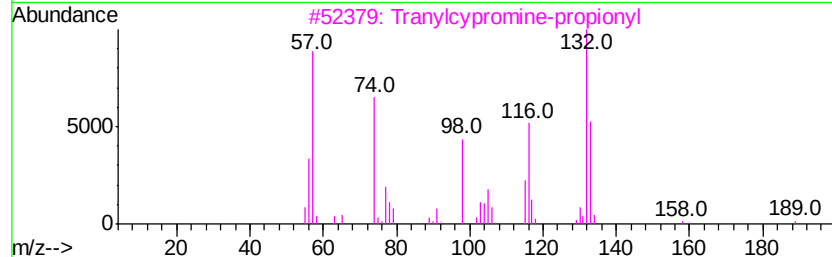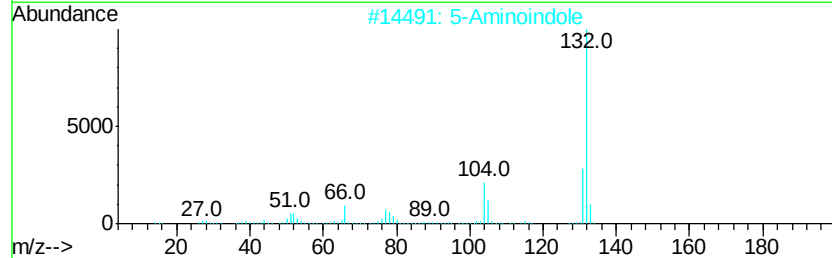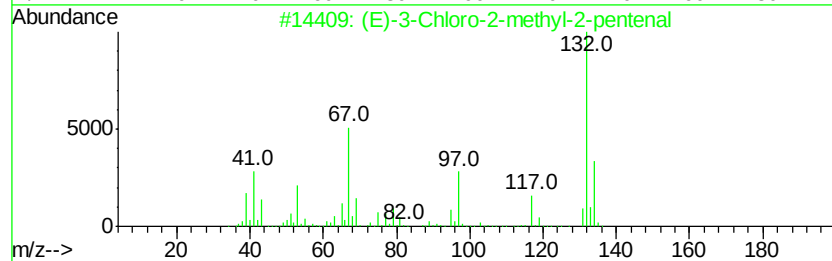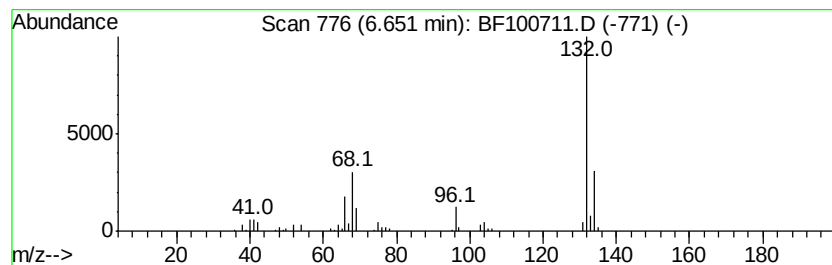

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF111717\
Data File : BF100711.D
Acq On : 18 Nov 2017 9:57
Operator : SJ/JU
Sample : I6460-04 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-31-2-1.5-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.65	6.65	9.3	ng	223178	1	6.88	479576	20.0