


Data Path : Z:\HPCHEM1\BNA_F\Data\BF111717\
 Data File : BF100664.D
 Acq On : 17 Nov 2017 9:20
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 15:22:08 2017

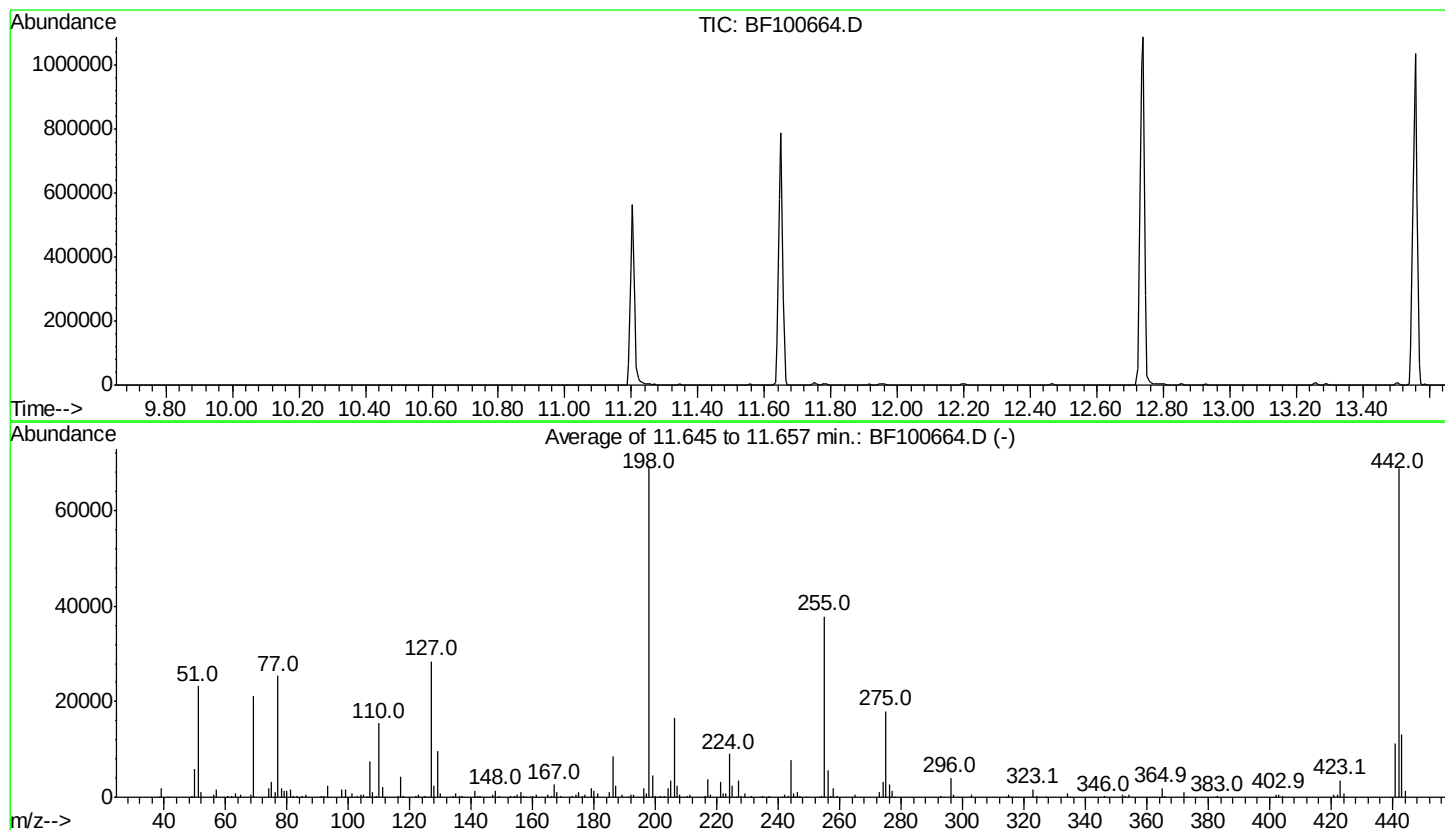

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	23268	PASS
68	69	0.00	2	2.0	419	PASS
69	198	0.00	100	30.6	21251	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	28483	PASS
197	198	0.00	2	1.1	733	PASS
198	198	100	100	100.0	69434	PASS
199	198	5	9	6.7	4636	PASS
275	198	10	60	26.0	18048	PASS
365	198	1	100	2.9	2006	PASS
441	443	0.01	100	85.3	11287	PASS
442	198	50	100	99.3	68925	PASS
443	442	15	24	19.2	13231	PASS