


Data Path : Z:\HPCHEM1\BNA F\Data\BF111717\
 Data File : BF100679.D
 Acq On : 17 Nov 2017 17:50
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF110817.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Nov 17 15:22:08 2017

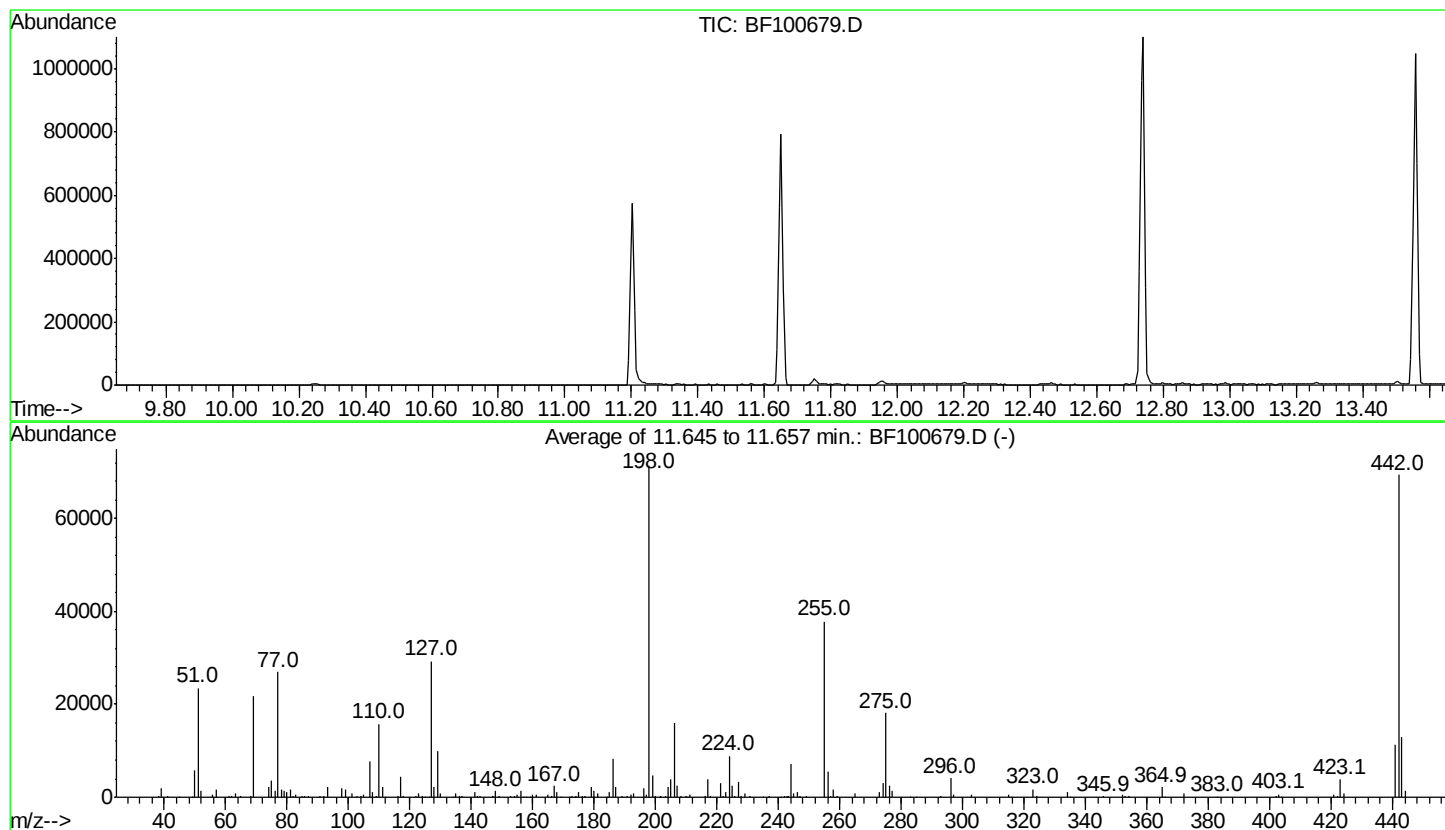

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	23463	PASS
68	69	0.00	2	1.7	376	PASS
69	198	0.00	100	30.4	21710	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	41.0	29300	PASS
197	198	0.00	2	0.7	467	PASS
198	198	100	100	100.0	71410	PASS
199	198	5	9	6.6	4711	PASS
275	198	10	60	25.5	18184	PASS
365	198	1	100	3.0	2116	PASS
441	443	0.01	100	86.1	11214	PASS
442	198	50	100	97.1	69370	PASS
443	442	15	24	18.8	13030	PASS