
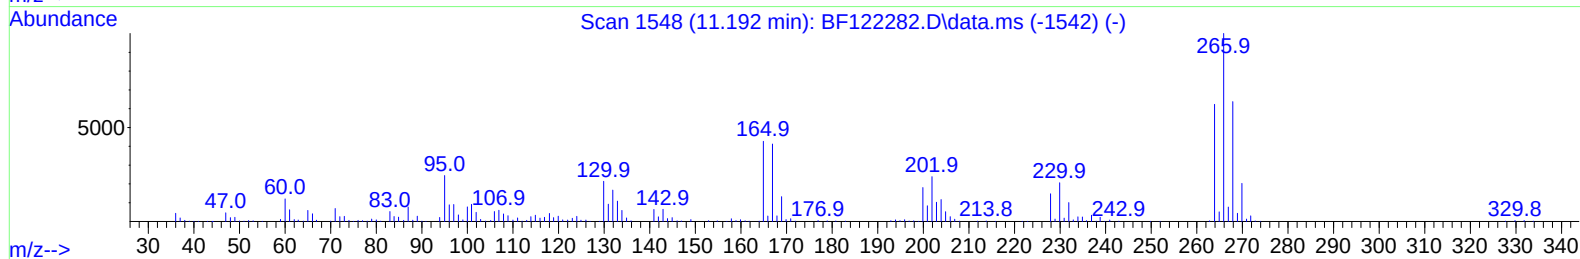
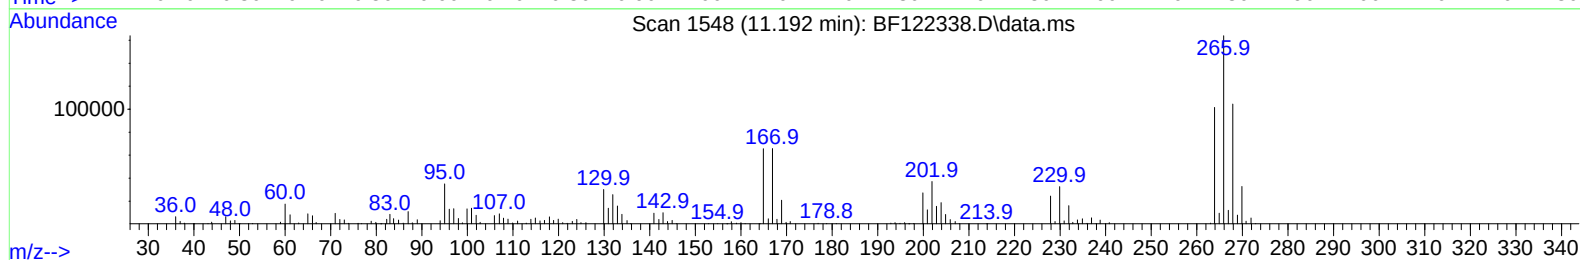


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111720\  
Data File : BF122338.D  
Acq On : 17 Nov 2020 10:26  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 03:54:48 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110920.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 10 12:25:42 2020  
Response via : Initial Calibration

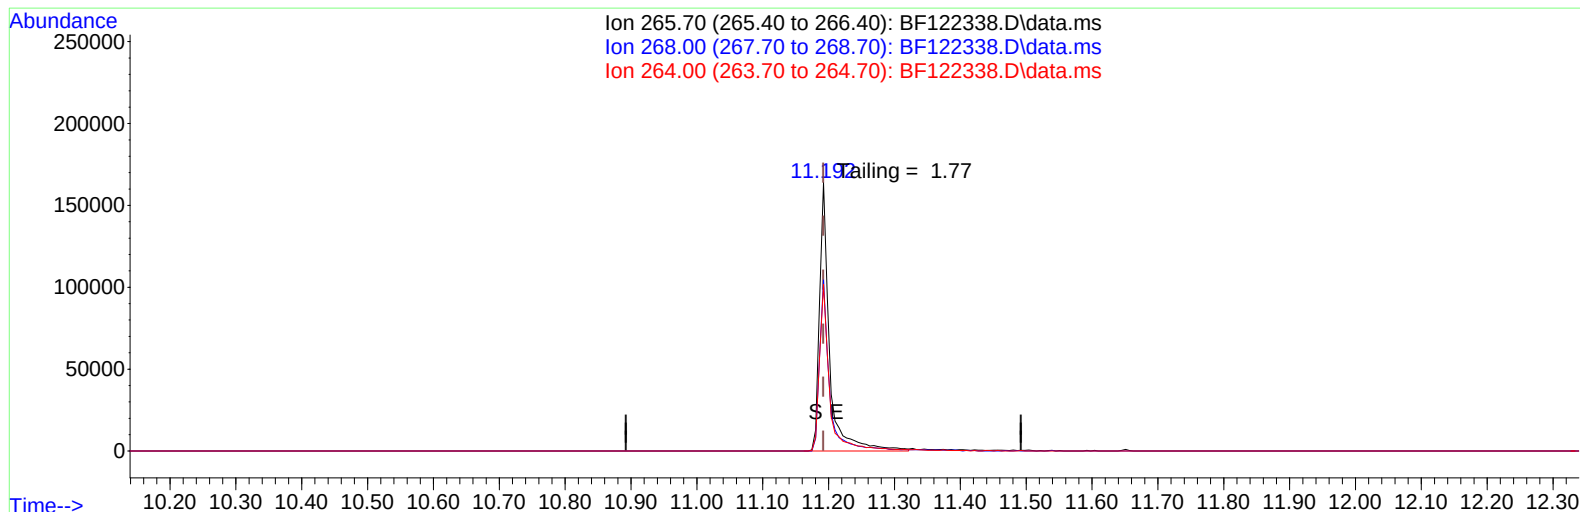

TIC: BF122338.D\data.ms

**(70) Pentachlorophenol (C)**




11.192min (+ 0.000) 31485.84 ng

response 176648

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.50  | 63.74  |
| 264.00 | 62.40  | 61.99  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF111720\  
Data File : BF122338.D  
Acq On : 17 Nov 2020 10:26  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 18 03:54:48 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF110920.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Nov 10 12:25:42 2020  
Response via : Initial Calibration

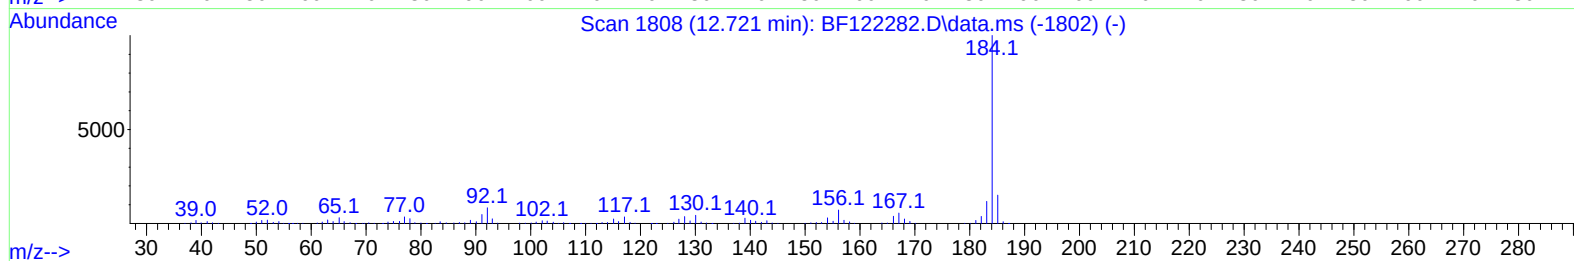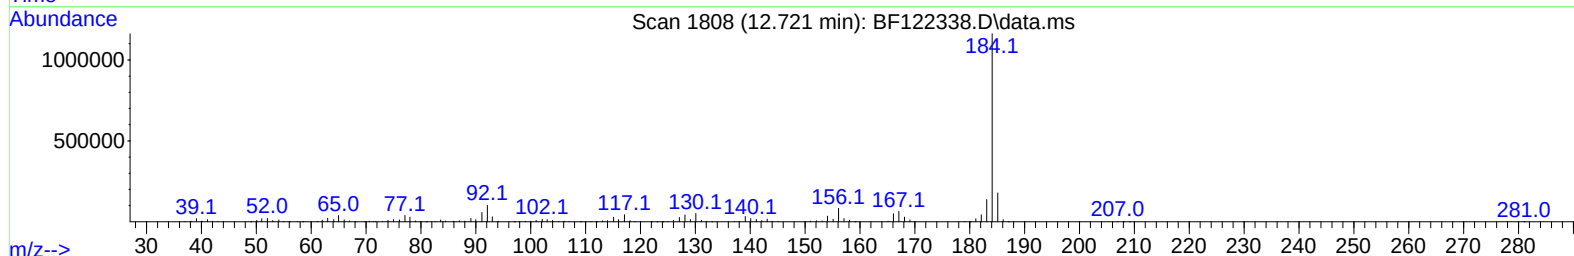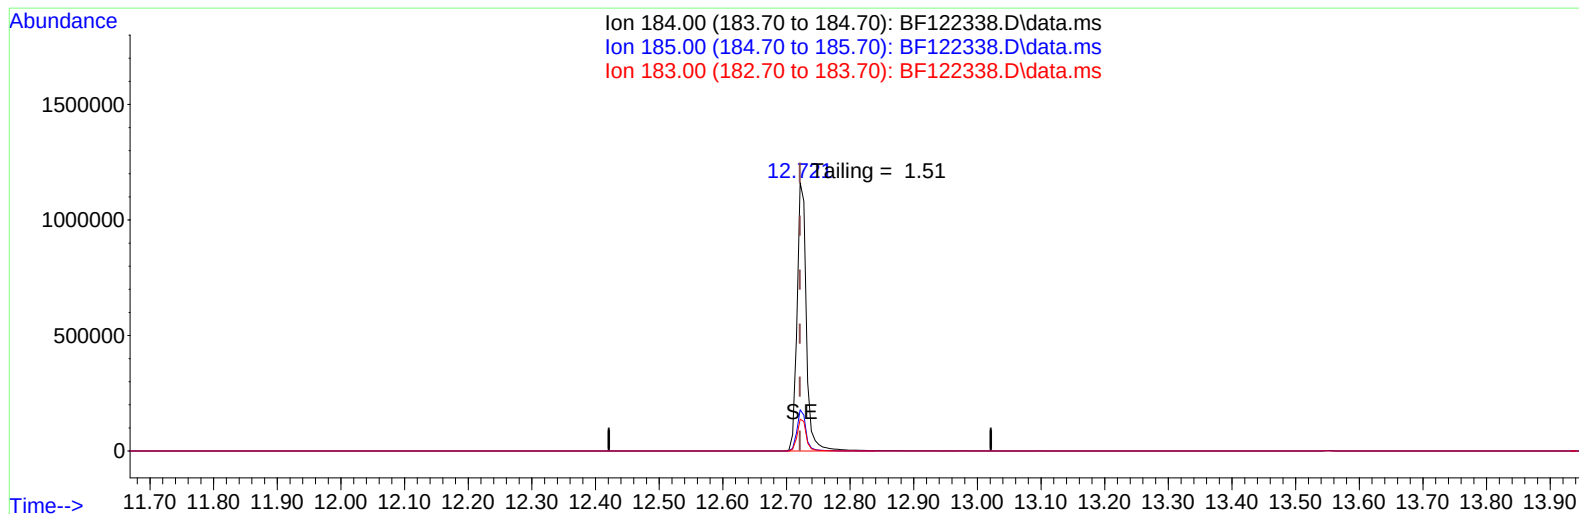

TIC: BF122338.D\data.ms

**(77) Benzidine**

12.721min (+ 0.000) 0.00 ng

response 1192362

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.50  | 15.39  |
| 183.00 | 11.70  | 11.87  |
| 0.00   | 0.00   | 0.00   |