

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
 Data File : BF122348.D
 Acq On : 17 Nov 2020 16:18
 Operator : JU/CG
 Sample : L4723-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RBR-59

Manual Integrations
 APPROVED

mohammad
 11/19/2020 10:28:51 AM

Quant Time: Nov 17 17:19:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 12:25:42 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.863	152	268464	20.00	ng	0.00
21) Naphthalene-d8	8.151	136	1010735	20.00	ng	# 0.00
39) Acenaphthene-d10	9.904	164	534286	20.00	ng	0.00
64) Phenanthrene-d10	11.386	188	1018206	20.00	ng	0.00
76) Chrysene-d12	14.027	240	876278	20.00	ng	0.00
86) Perylene-d12	15.498	264	795177	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	1379971	78.93	ng	0.00
7) Phenol-d6	6.481	99	1766057	77.21	ng	-0.01
23) Nitrobenzene-d5	7.422	82	1072511	64.96	ng	-0.01
42) 2,4,6-Tribromophenol	10.692	330	513612	89.57	ng	0.00
45) 2-Fluorobiphenyl	9.228	172	1574156	46.03	ng	0.00
79) Terphenyl-d14	12.974	244	1645893	39.79	ng	0.00
Target Compounds						Qvalue
50) Dimethylphthalate	9.616	163	446348	11.75	ng	99
71) Phenanthrene	11.410	178	275182	4.76	ng	99
75) Fluoranthene	12.598	202	517148	8.57	ng	99
78) Pyrene	12.827	202	490190	7.96	ng	98
81) Benzo(a)anthracene	14.015	228	203380	3.73	ng	97
83) Chrysene	14.051	228	239676m	4.37	ng	
87) Indeno(1,2,3-cd)pyrene	16.951	276	110478	2.32	ng	94
88) Benzo(b)fluoranthene	15.068	252	270352m	5.25	ng	
90) Benzo(a)pyrene	15.427	252	166072	3.70	ng	99
92) Benzo(g,h,i)perylene	17.386	276	110054	2.83	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111720\
Data File : BF122348.D
Acq On : 17 Nov 2020 16:18
Operator : JU/CG
Sample : L4723-02
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
RBR-59

Manual Integrations
APPROVED


mohammad
11/19/2020 10:28:51 AM

Quant Time: Nov 17 17:19:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 12:25:42 2020
Response via : Initial Calibration



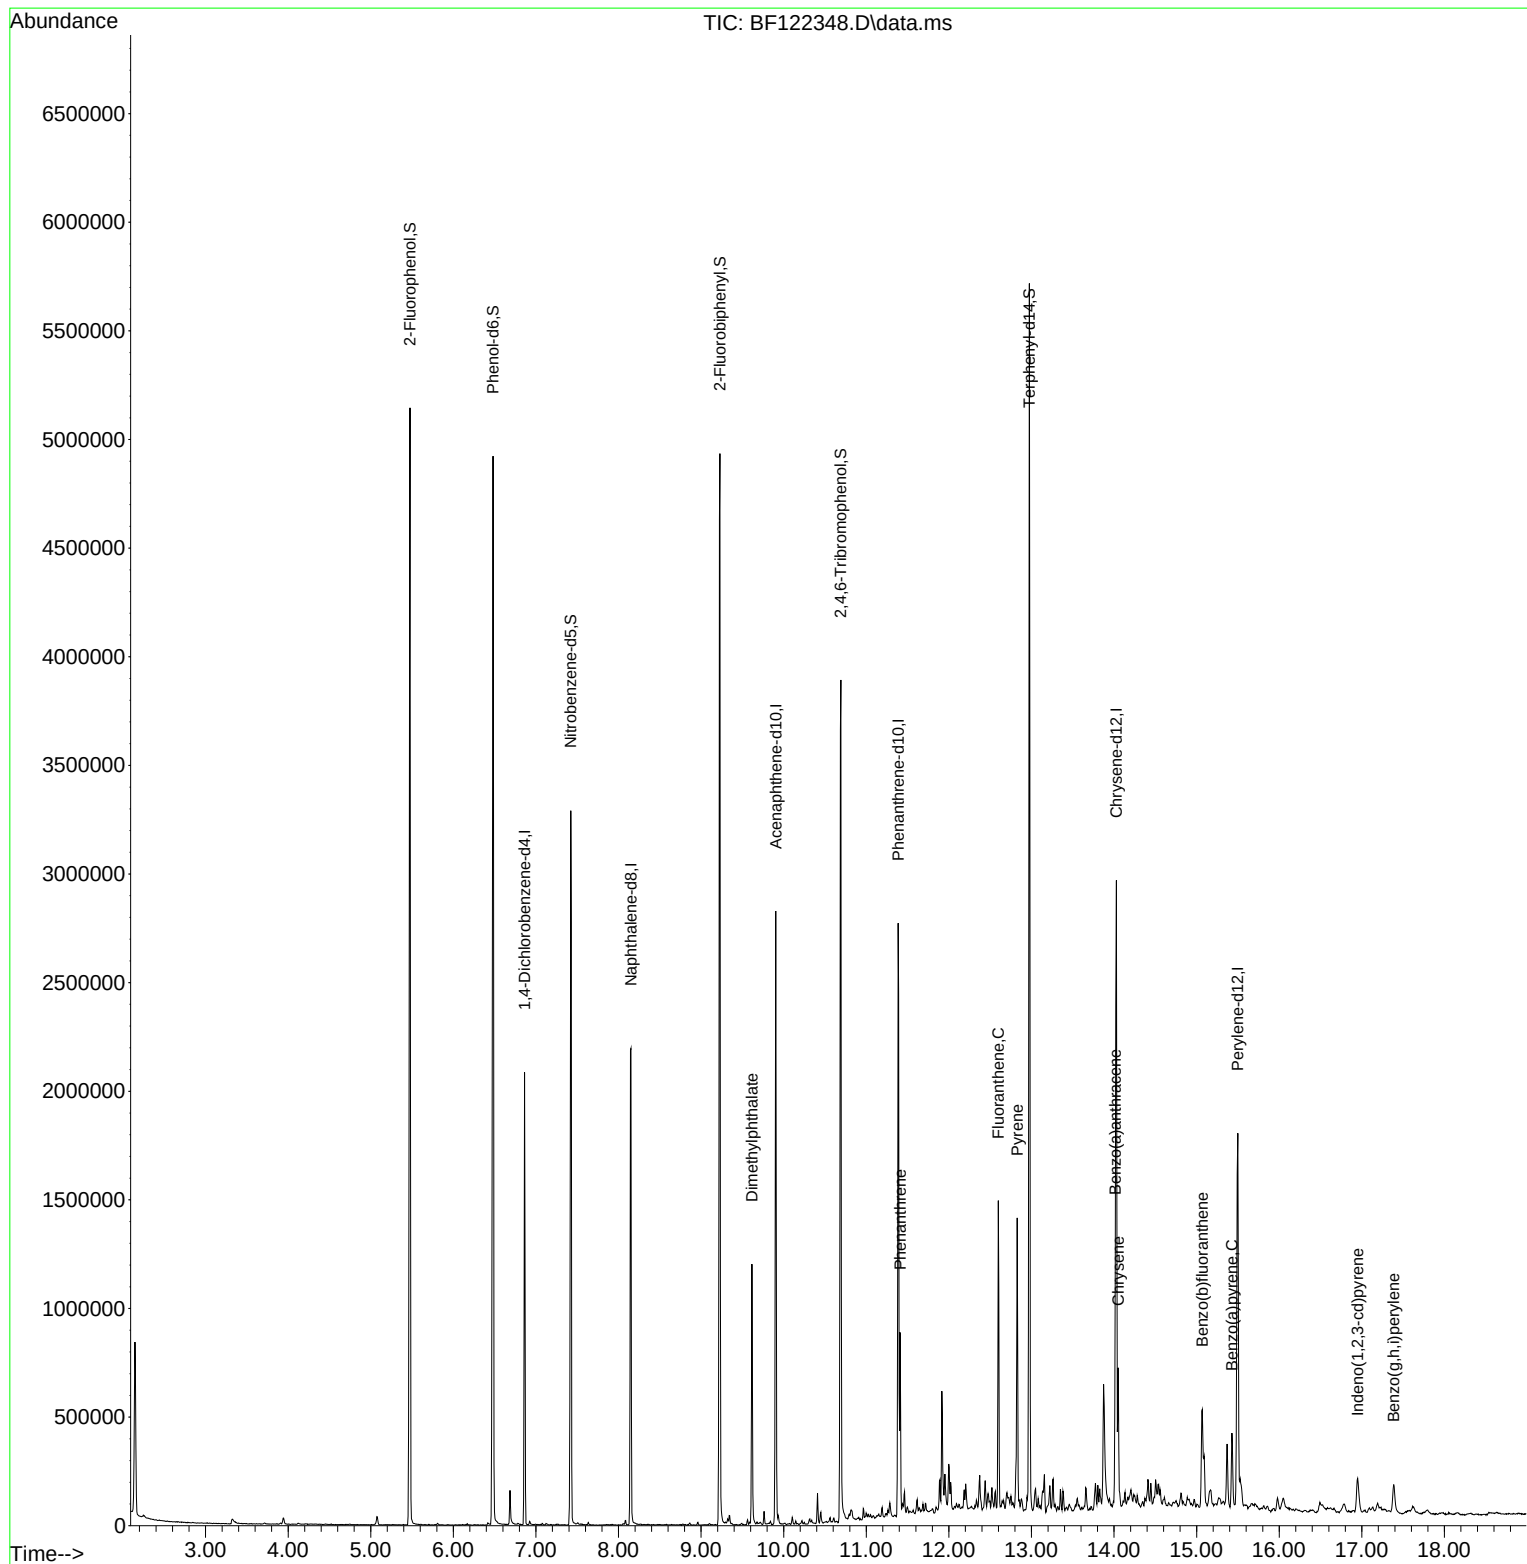





#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.863 min Scan# 812
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18





Tgt Ion:152 Resp: 268464
Ion Ratio Lower Upper
152 100
150 156.5 125.3 187.9
115 60.6 51.9 77.9

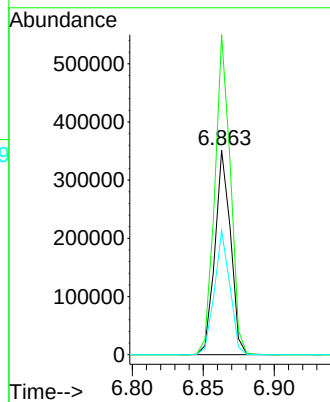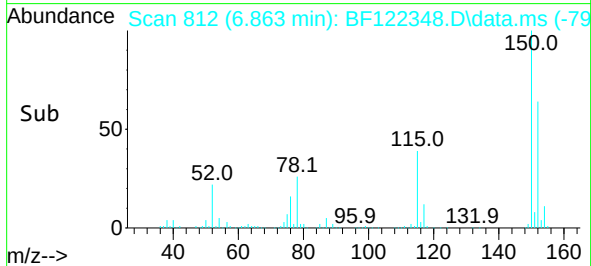

#5
2-Fluorophenol
Concen: 78.93 ng
RT: 5.475 min Scan# 576
Delta R.T. 0.000 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

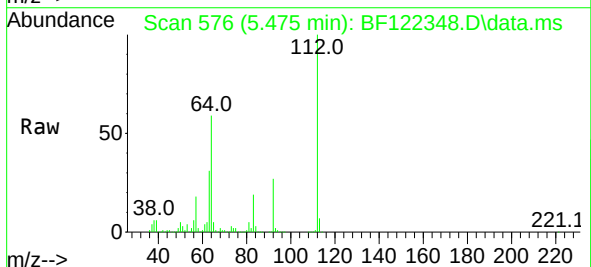


Tgt Ion:112 Resp: 1379971
Ion Ratio Lower Upper
112 100
64 59.2 50.4 75.6
63 30.5 25.8 38.6

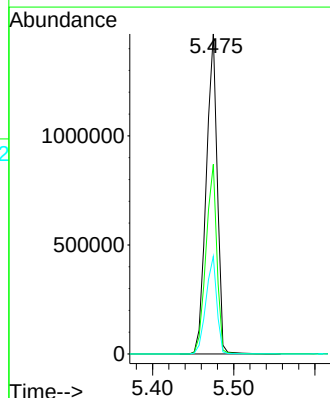


Instrument :
BNA_F
ClientSampled :
RBR-59

Manual Integrations
APPROVED

mohammad
11/19/2020 10:28:51 AM



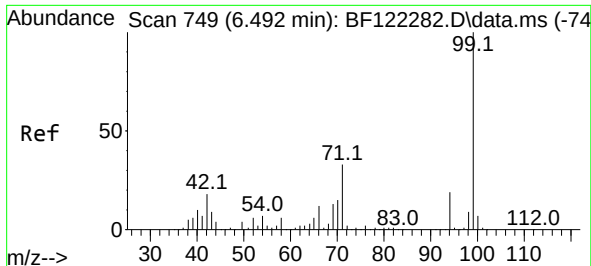


#7
Phenol-d6
Concen: 77.21 ng
RT: 6.481 min Scan# 747
Delta R.T. -0.012 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18




Tgt Ion: 99 Resp: 1766057

Ion	Ratio	Lower	Upper
99	100		
42	19.1	15.9	23.9
71	34.3	27.1	40.7

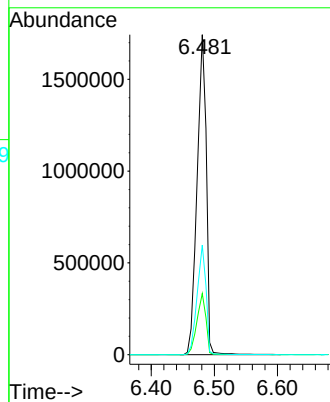
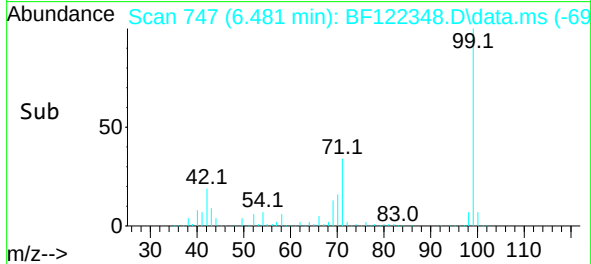


#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.151 min Scan# 1031
Delta R.T. 0.000 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

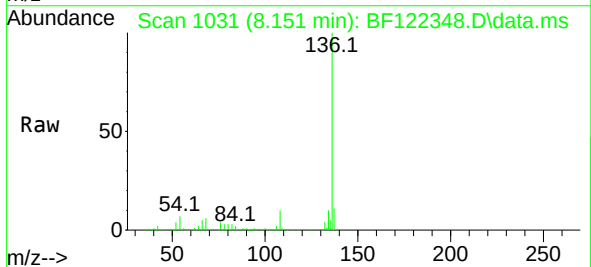

Tgt Ion: 136 Resp: 1010735


Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.6	13.0
54	7.1	7.1	10.7#
68	5.7	5.0	7.4

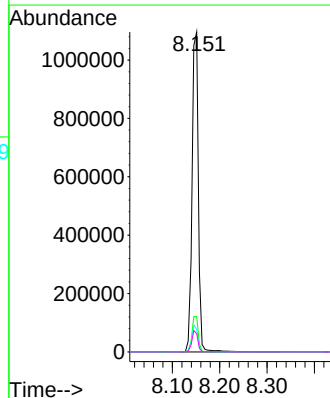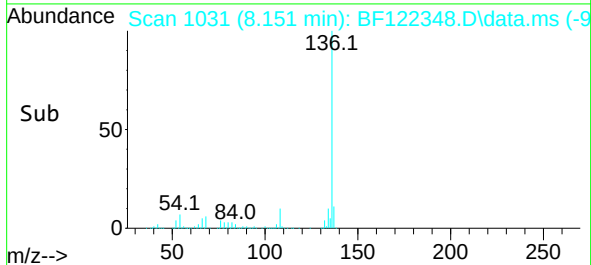

Instrument :
BNA_F
ClientSampleId :
RBR-59

Manual Integrations
APPROVED

mohammad
11/19/2020 10:28:51 AM

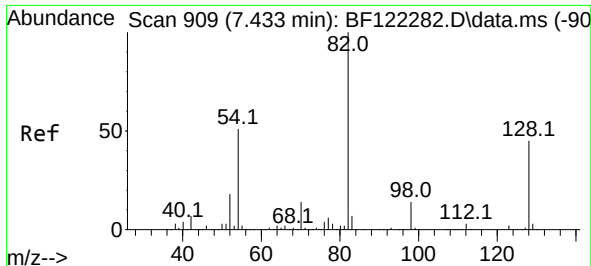

#23
Nitrobenzene-d5
Concen: 64.96 ng
RT: 7.422 min Scan# 907
Delta R.T. -0.012 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18





Tgt Ion: 82 Resp: 1072511

Ion	Ratio	Lower	Upper
82	100		
128	43.4	35.0	52.4
54	50.1	43.9	65.9

Instrument :
BNA_F
ClientSampleId :
RBR-59

Manual Integrations
APPROVED




mohammad
11/19/2020 10:28:51 AM

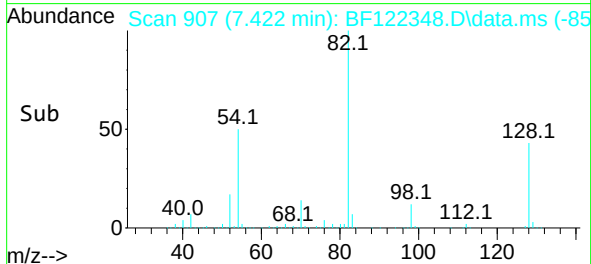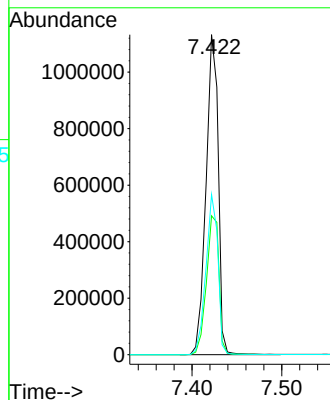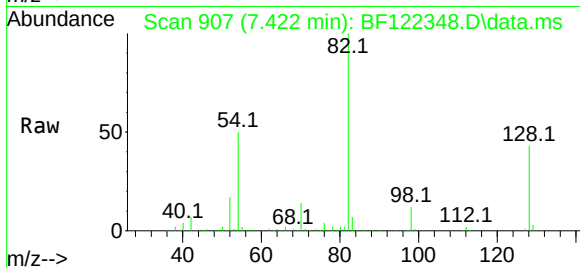


#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.904 min Scan# 1329
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

Tgt Ion: 164 Resp: 534286

Ion	Ratio	Lower	Upper
164	100		
162	101.9	83.2	124.8
160	46.6	37.5	56.3

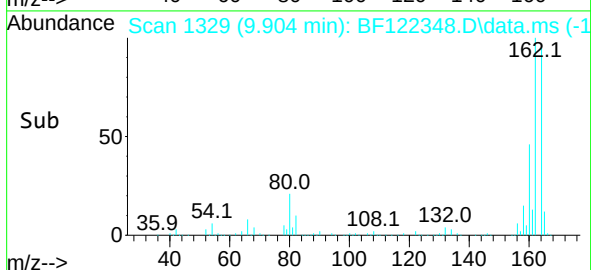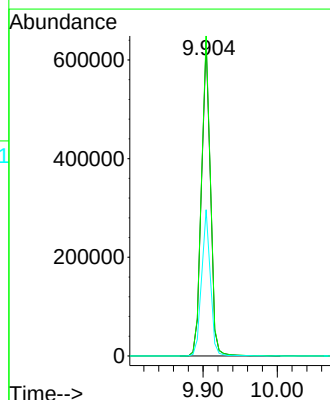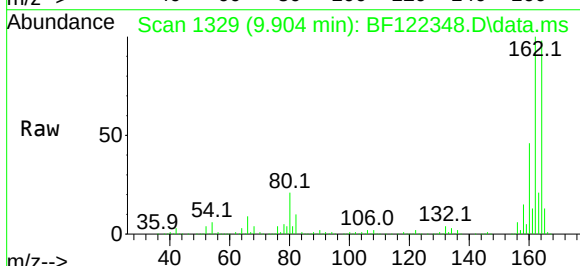

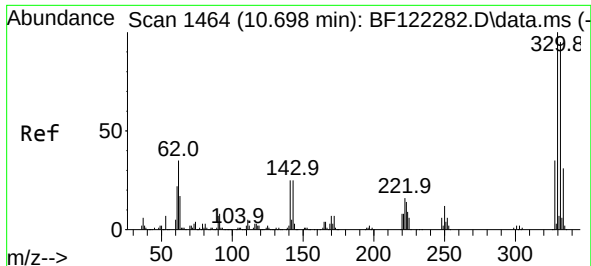





#42
2,4,6-Tribromophenol
Concen: 89.57 ng
RT: 10.692 min Scan# 1463
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

Tgt Ion: 330 Resp: 513612
Ion Ratio Lower Upper
330 100
332 96.5 77.3 115.9
141 30.7 22.3 33.5

Instrument :
BNA_F
ClientSampleId :
RBR-59




Manual Integrations
APPROVED


mohammad
11/19/2020 10:28:51 AM

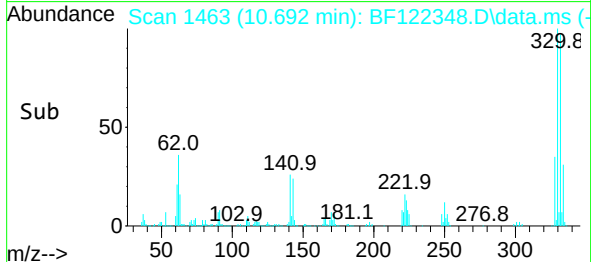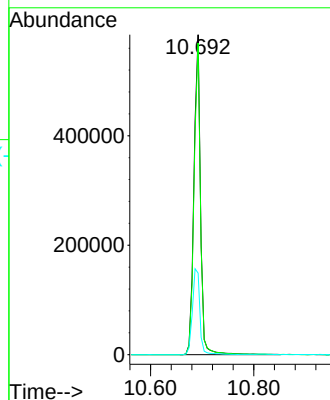

#45
2-Fluorobiphenyl
Concen: 46.03 ng
RT: 9.228 min Scan# 1214
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

Tgt Ion: 172 Resp: 1574156
Ion Ratio Lower Upper
172 100
171 36.5 29.1 43.7
170 24.0 19.8 29.6

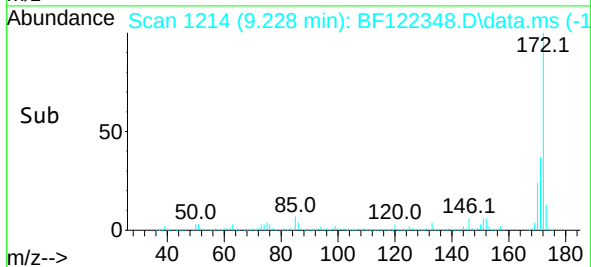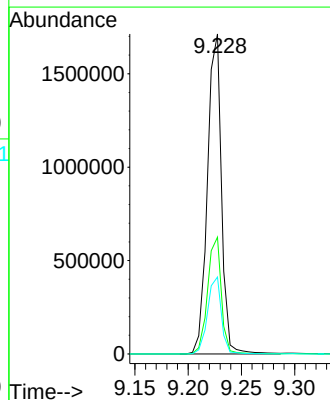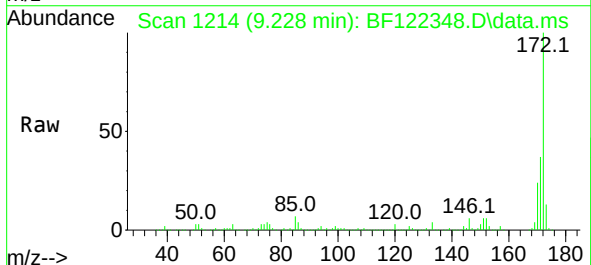







#50
Dimethylphthalate
Concen: 11.75 ng
RT: 9.616 min Scan# 1280
Delta R.T. -0.017 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

Tgt Ion:163 Resp: 446348
Ion Ratio Lower Upper
163 100
194 3.7 3.3 4.9
164 10.4 8.2 12.4

Instrument :
BNA_F
ClientSampleId :
RBR-59




Manual Integrations
APPROVED


mohammad
11/19/2020 10:28:51 AM

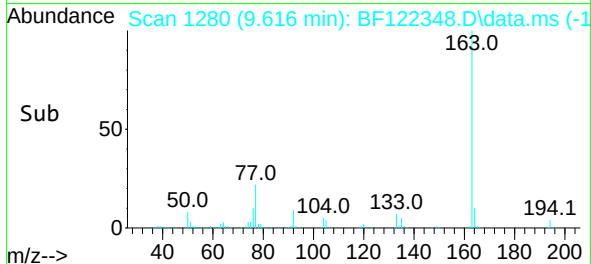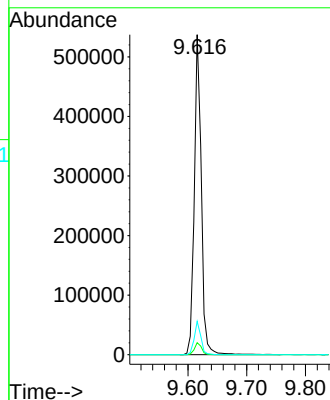

#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.386 min Scan# 1581
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18


Tgt Ion:188 Resp: 1018206
Ion Ratio Lower Upper
188 100
94 10.7 8.3 12.5
80 12.1 9.1 13.7

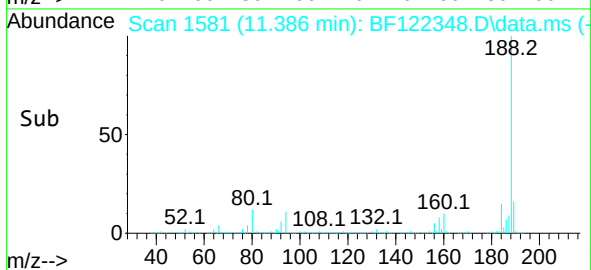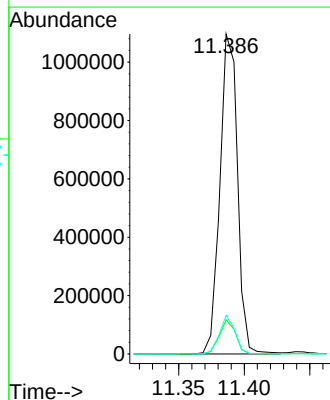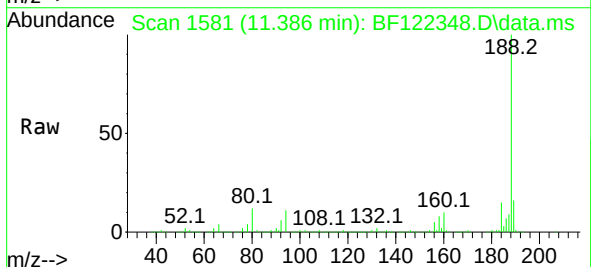

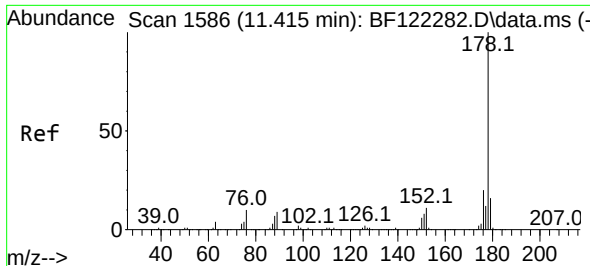

#71
Phenanthrene
Concen: 4.76 ng
RT: 11.410 min Scan# 1585
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18




Instrument :
BNA_F
ClientSampled :
RBR-59

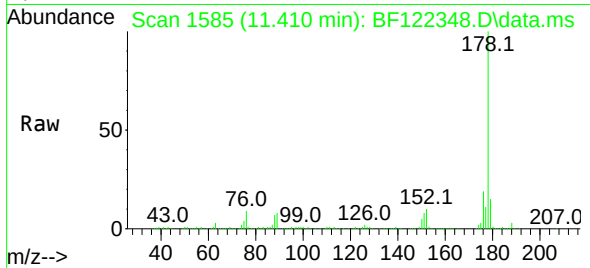


Tgt Ion:178 Resp: 275182
Ion Ratio Lower Upper
178 100
176 19.2 15.9 23.9
179 15.1 12.2 18.4

Manual Integrations
APPROVED



mohammad
11/19/2020 10:28:51 AM

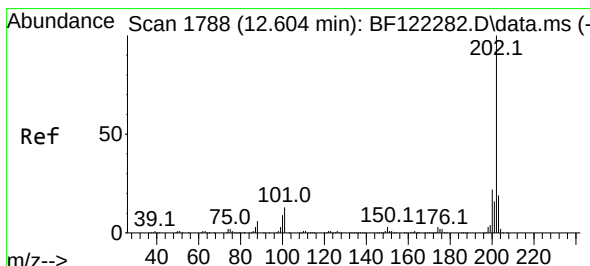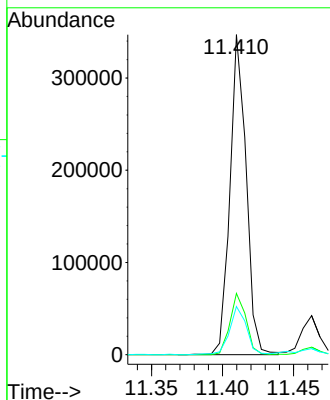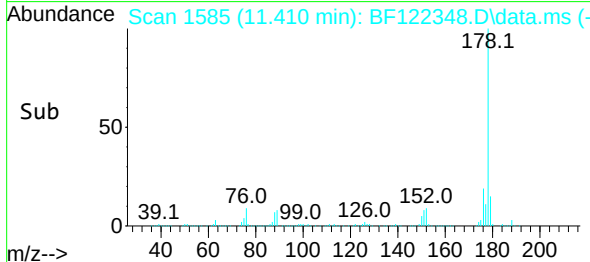


#75
Fluoranthene
Concen: 8.57 ng
RT: 12.598 min Scan# 1787
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

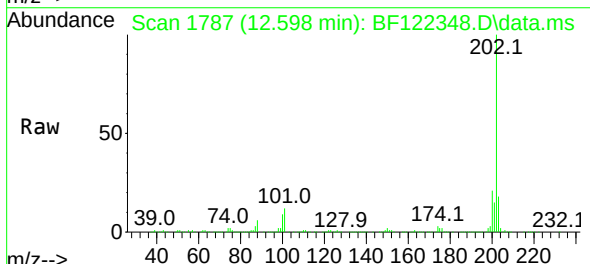


Tgt Ion:202 Resp: 517148
Ion Ratio Lower Upper
202 100
101 12.4 0.0 33.4
203 18.0 0.0 37.9

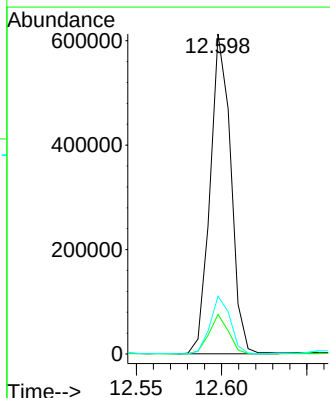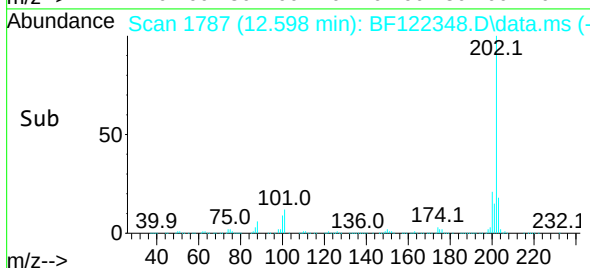

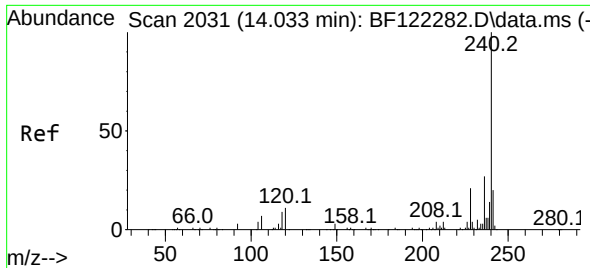

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.027 min Scan# 2030
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18




Instrument :
BNA_F
ClientSampled :
RBR-59

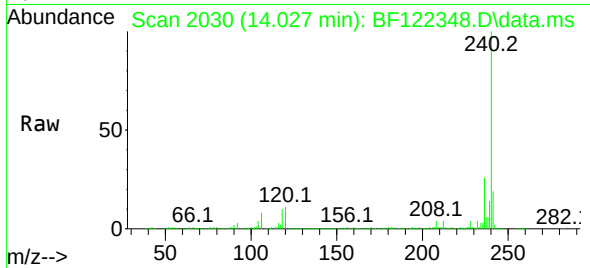


Tgt Ion:240 Resp: 876278
Ion Ratio Lower Upper
240 100
120 10.9 9.2 13.8
236 26.1 20.9 31.3

Manual Integrations
APPROVED



mohammad
11/19/2020 10:28:51 AM

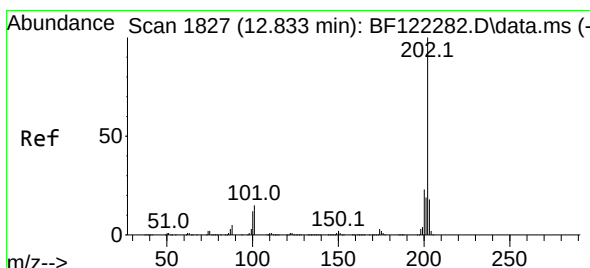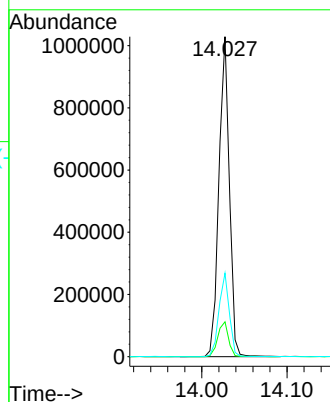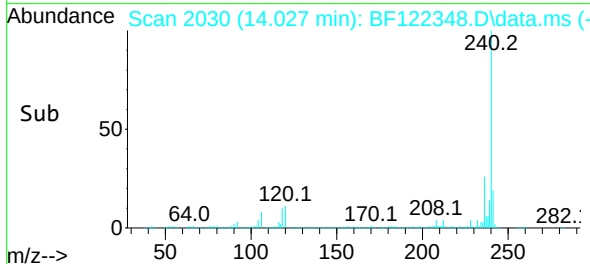


#78
Pyrene
Concen: 7.96 ng
RT: 12.827 min Scan# 1826
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

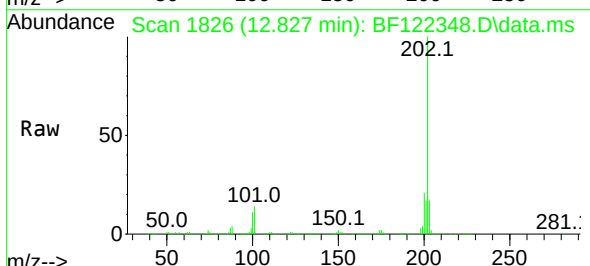


Tgt Ion:202 Resp: 490190
Ion Ratio Lower Upper
202 100
200 21.0 17.4 26.2
203 17.2 14.6 21.8

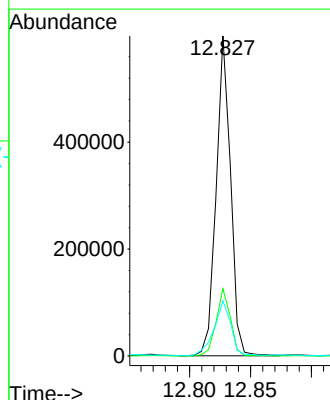
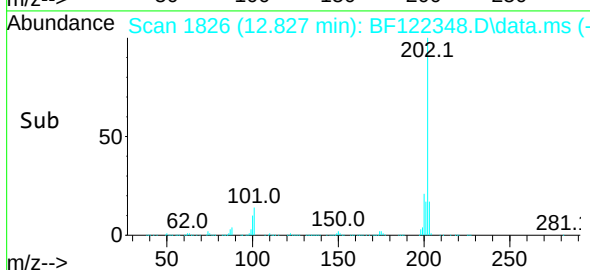


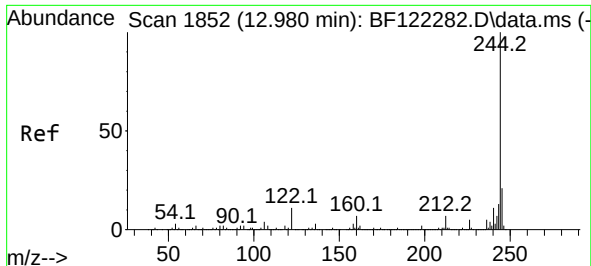

#79
Terphenyl-d14
Concen: 39.79 ng
RT: 12.974 min Scan# 1851
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18




Tgt Ion:244 Resp: 1645893
Ion Ratio Lower Upper
244 100
212 7.1 5.4 8.2
122 11.8 8.1 12.1

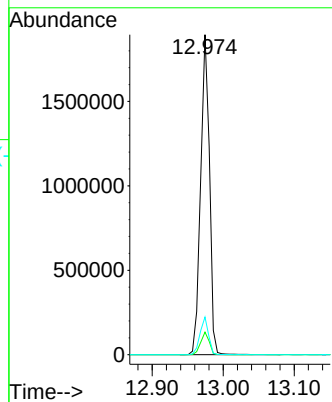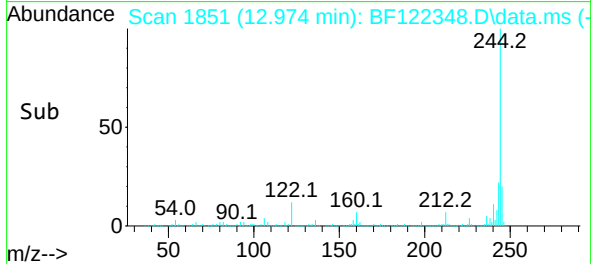


Instrument :
BNA_F
ClientSampled :
RBR-59

Manual Integrations
APPROVED



mohammad
11/19/2020 10:28:51 AM




#81
Benzo(a)anthracene
Concen: 3.73 ng
RT: 14.015 min Scan# 2028
Delta R.T. -0.006 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

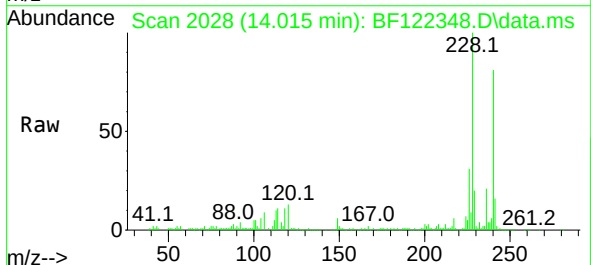

Tgt Ion:228 Resp: 203380
Ion Ratio Lower Upper
228 100
226 30.6 22.3 33.5
229 19.9 16.2 24.4

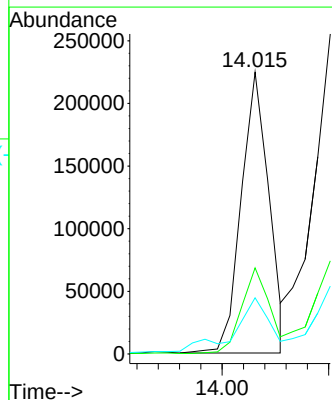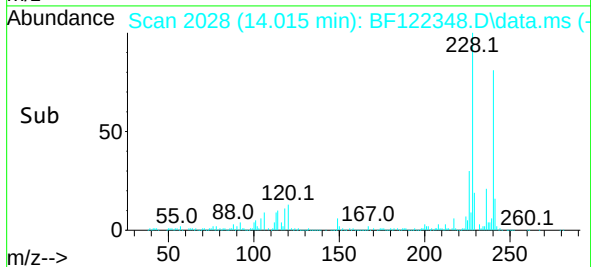







#83
Chrysene
Concen: 4.37 ng m
RT: 14.051 min Scan# 2034
Delta R.T. -0.012 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

Tgt Ion:228 Resp: 239676
Ion Ratio Lower Upper
228 100
226 29.1 24.6 37.0
229 21.2 15.9 23.9

Instrument :
BNA_F
ClientSampled :
RBR-59




Manual Integrations
APPROVED


mohammad
11/19/2020 10:28:51 AM

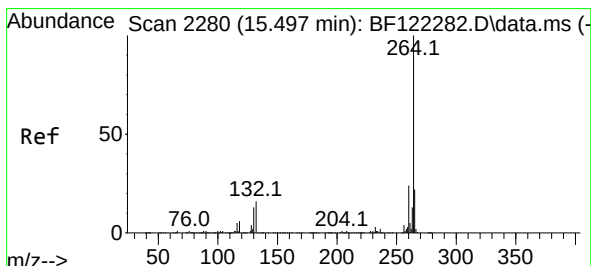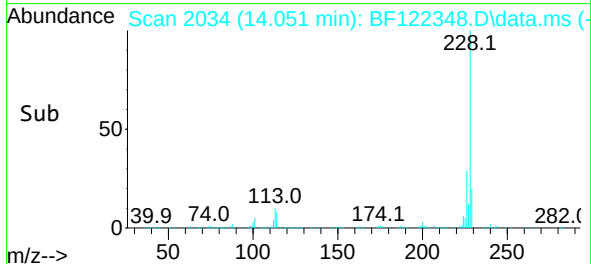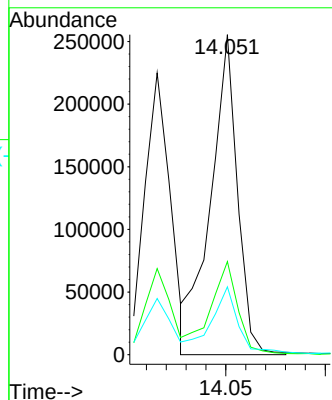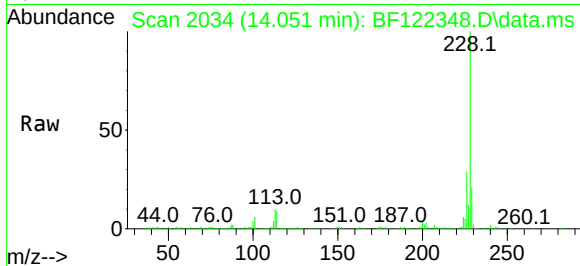


#86
Perylene-d12
Concen: 20.00 ng
RT: 15.498 min Scan# 2280
Delta R.T. 0.000 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

Tgt Ion:264 Resp: 795177
Ion Ratio Lower Upper
264 100
260 23.9 18.7 28.1
265 21.9 17.3 25.9

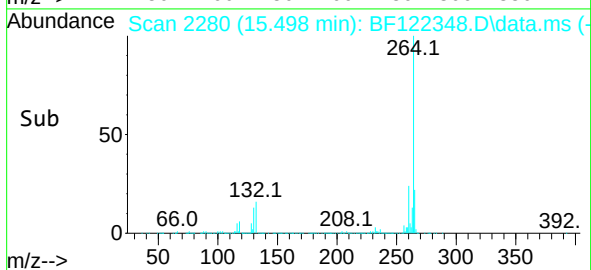
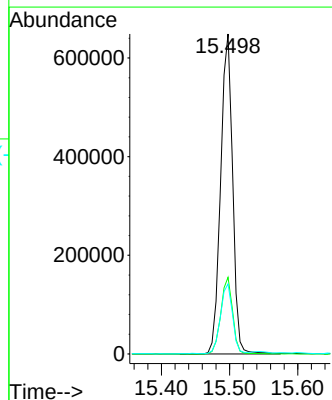
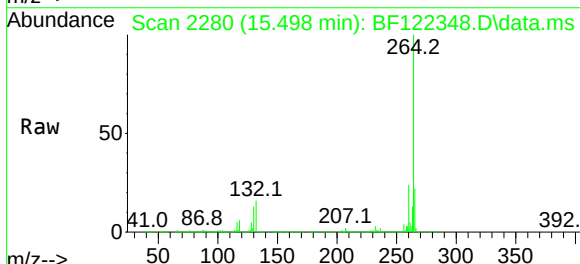





#87
Indeno(1,2,3-cd)pyrene
Concen: 2.32 ng
RT: 16.951 min Scan# 2527
Delta R.T. -0.012 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18





Tgt Ion: 276 Resp: 110478
Ion Ratio Lower Upper
276 100
138 20.5 19.9 29.9
277 23.8 20.4 30.6

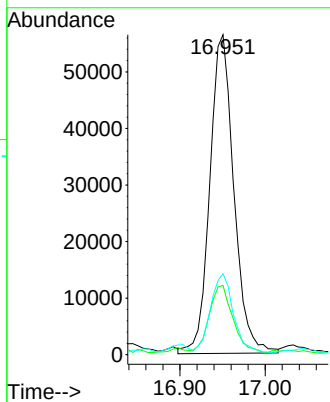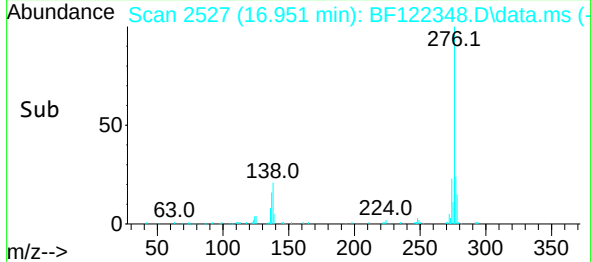

#88
Benzo(b)fluoranthene
Concen: 5.25 ng m
RT: 15.068 min Scan# 2207
Delta R.T. 0.000 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

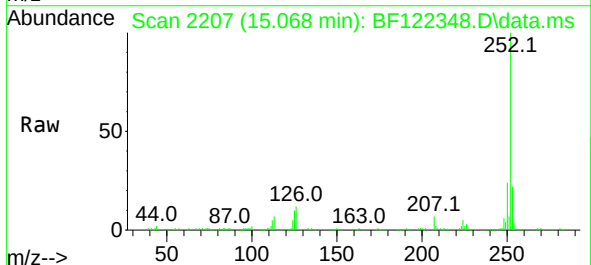


Tgt Ion: 252 Resp: 270352
Ion Ratio Lower Upper
252 100
253 22.3 18.2 27.2
125 9.8 8.0 12.0

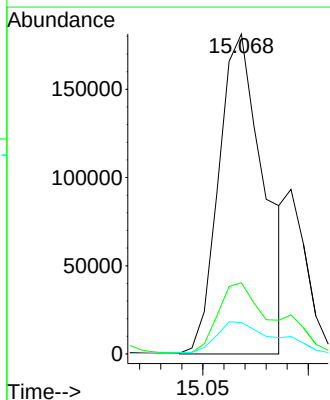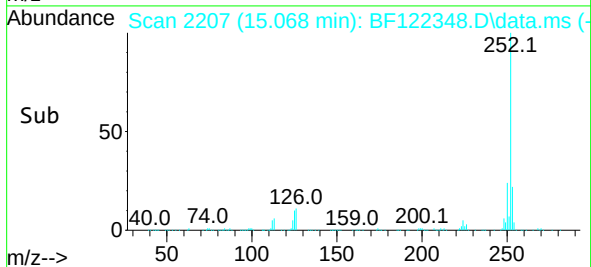

Instrument :
BNA_F
ClientSampled :
RBR-59

Manual Integrations
APPROVED

mohammad
11/19/2020 10:28:51 AM







#90
Benzo(a)pyrene
Concen: 3.70 ng
RT: 15.427 min Scan# 2268
Delta R.T. -0.012 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

Tgt Ion:252 Resp: 166072
Ion Ratio Lower Upper
252 100
253 22.3 17.3 25.9
125 11.2 8.6 13.0

Instrument :
BNA_F
ClientSampled :
RBR-59

Manual Integrations
APPROVED

mohammad
11/19/2020 10:28:51 AM

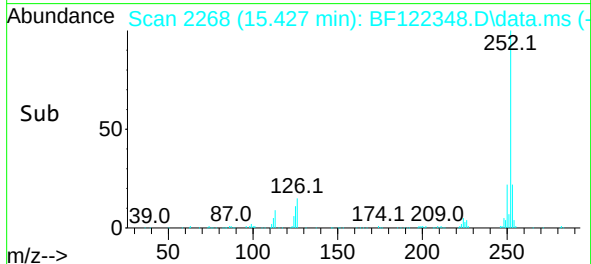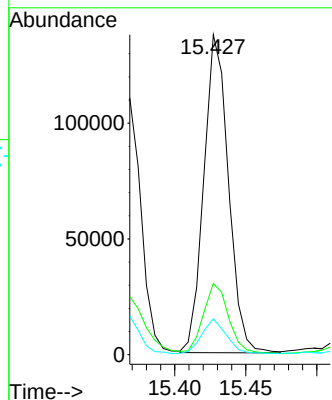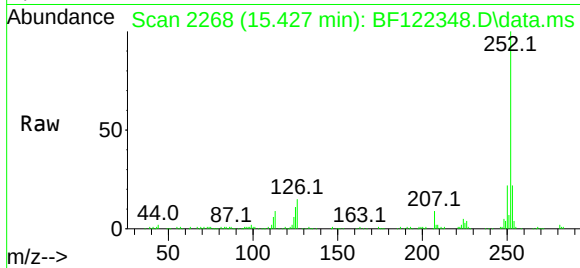

#92
Benzo(g,h,i)perylene
Concen: 2.83 ng
RT: 17.386 min Scan# 2601
Delta R.T. -0.017 min
Lab File: BF122348.D
Acq: 17 Nov 2020 16:18

Tgt Ion:276 Resp: 110054
Ion Ratio Lower Upper
276 100
277 22.3 19.4 29.2
138 21.6 17.8 26.6

